

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101823\
 Data File : PP061033.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2023 15:04
 Operator : YP\AJ
 Sample : 04920-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LSS-B1-COMP-101623

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 16:22:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.552	3.687	50811177	31252967	23.113	23.116
2) SA Decachlor...	10.510	8.754	31037094	25905294	19.819	17.230

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101823\
Data File : PP061033.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2023 15:04
Operator : YP\AJ
Sample : 04920-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LSS-B1-COMP-101623

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 16:22:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

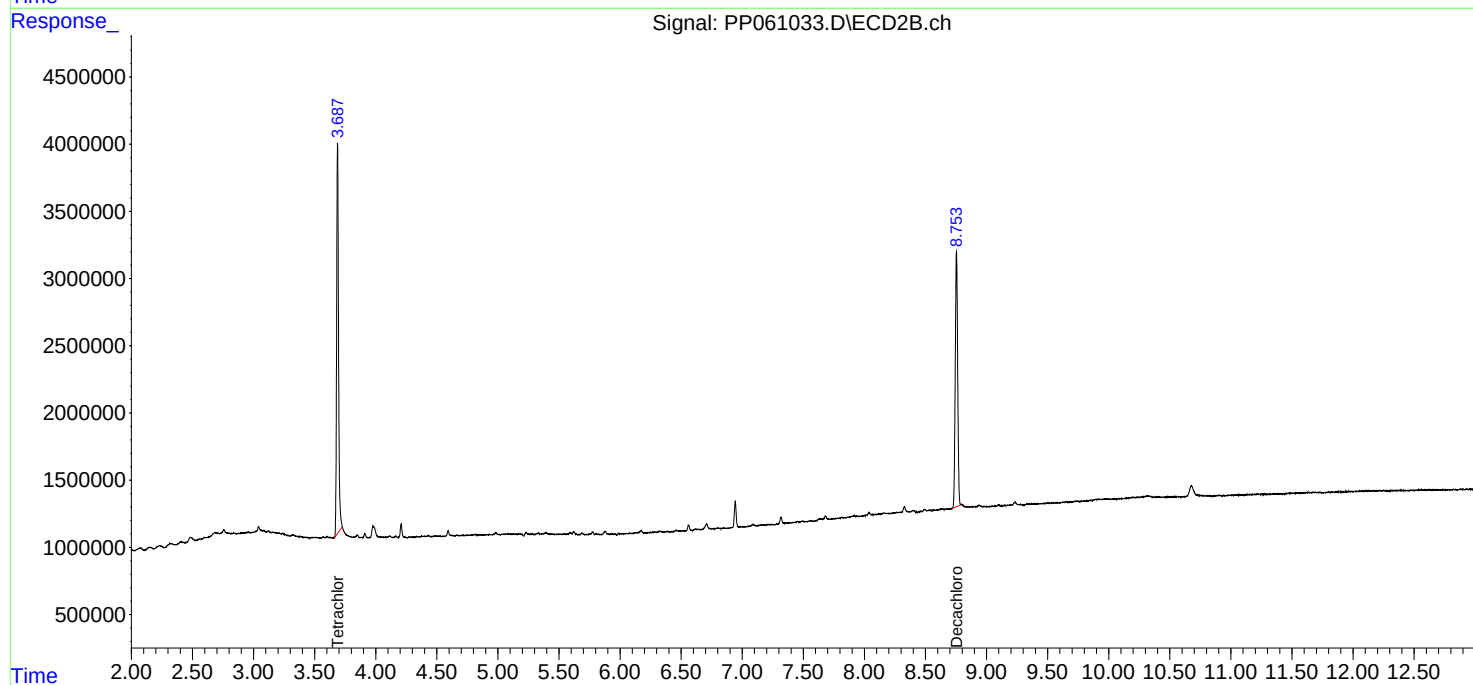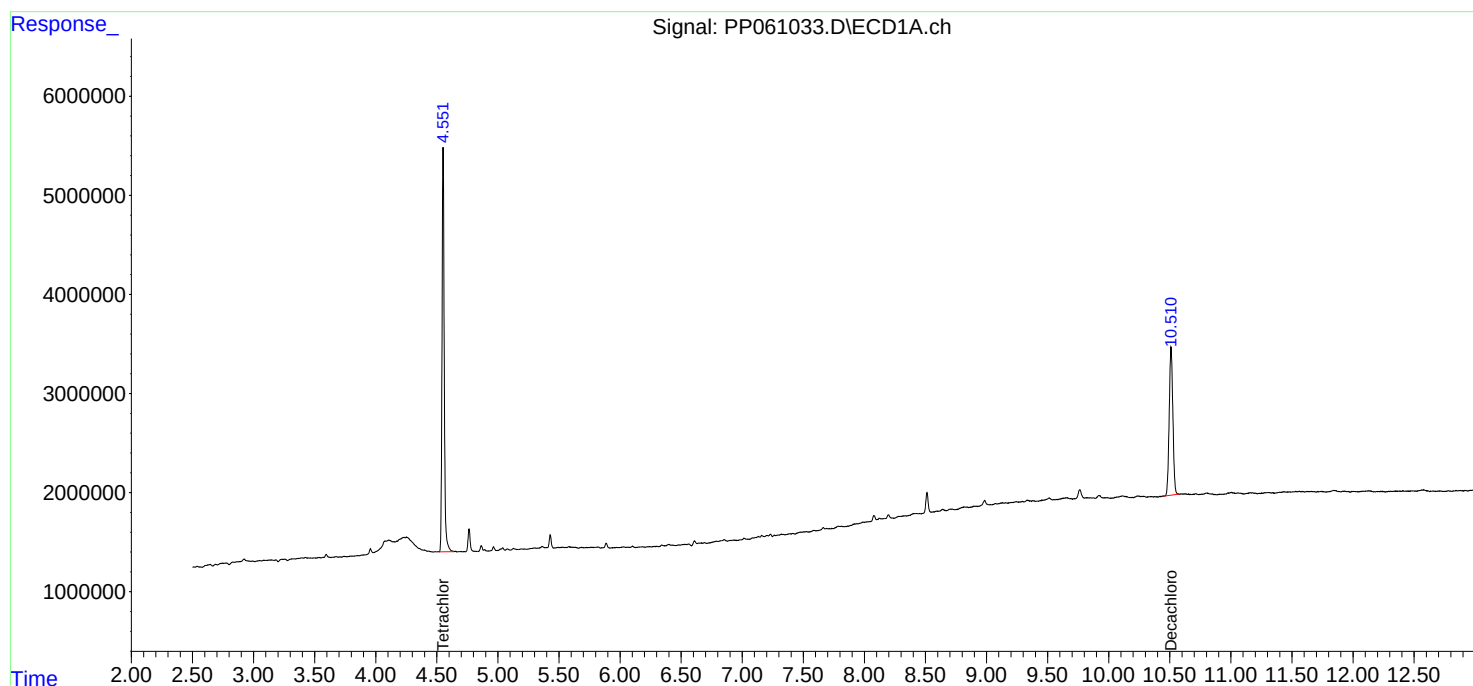


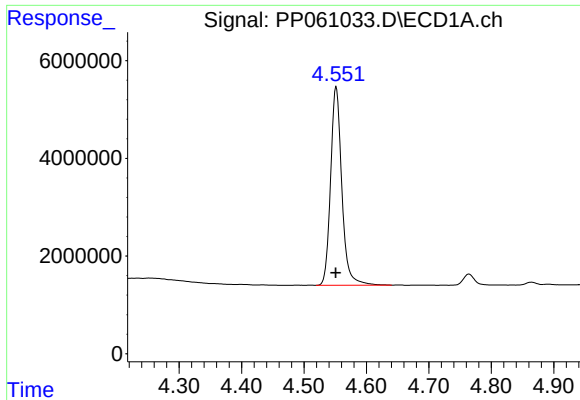

#1 Tetrachloro-m-xylene


R.T.: 4.552 min
Delta R.T.: 0.000 min
Response: 50811177
Conc: 23.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LSS-B1-COMP-101623

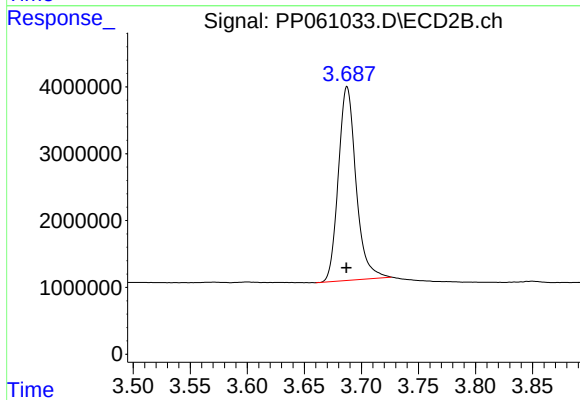


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 31252967
Conc: 23.12 ng/ml

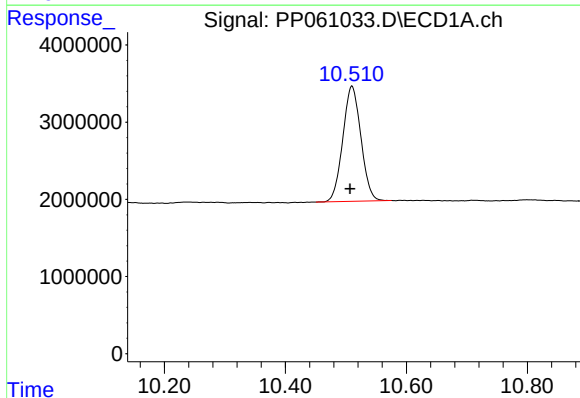

#2 Decachlorobiphenyl

R.T.: 10.510 min
Delta R.T.: 0.003 min
Response: 31037094
Conc: 19.82 ng/ml

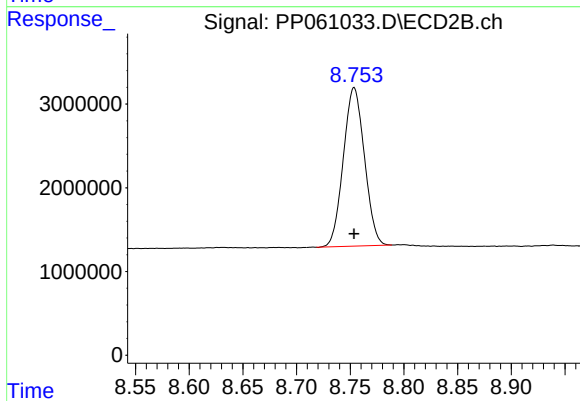

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: 0.000 min
Response: 25905294
Conc: 17.23 ng/ml