

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101823\
 Data File : PP061071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 03:26
 Operator : YP\AJ
 Sample : 04938-15
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 A-8(0-2)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/19/2023
 Supervised By :Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 04:52:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.551	3.687	32365263	25410780	14.723m	18.795 #
2) SA Decachlor...	10.508	8.754	28722937	23698494	18.342	15.762

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101823\
Data File : PP061071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 03:26
Operator : YP\AJ
Sample : 04938-15
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
A-8(0-2)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/19/2023
Supervised By :Ankita Jodhani 10/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 04:52:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

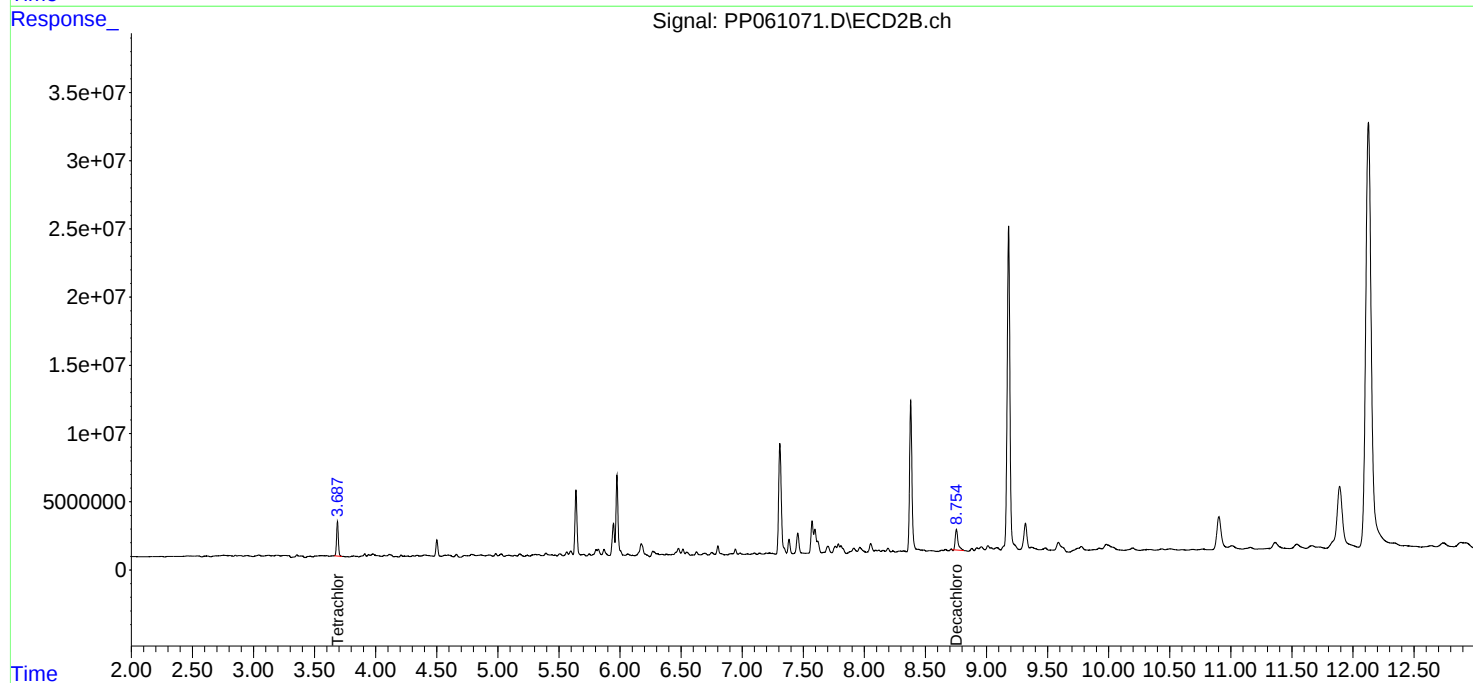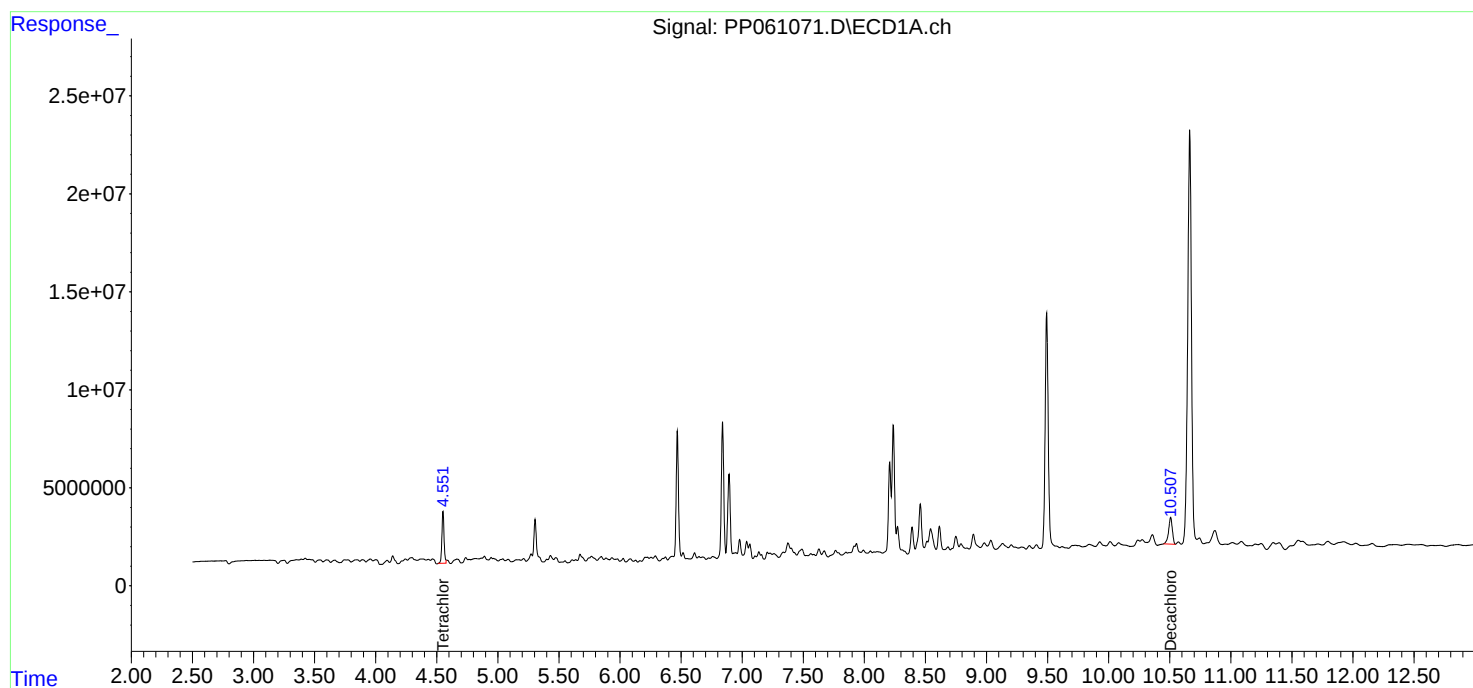

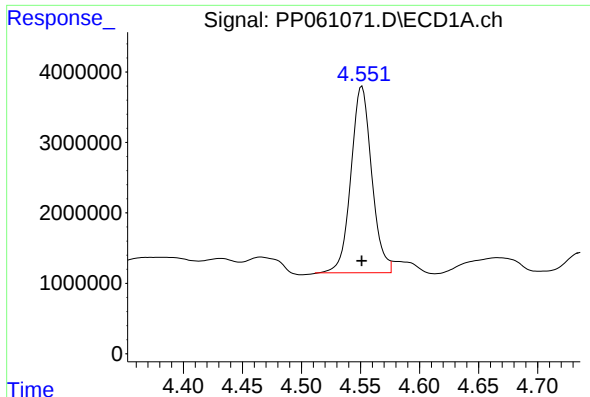


#1 Tetrachloro-m-xylene

R.T.: 4.551 min
Delta R.T.: 0.000 min
Response: 32365263
Conc: 14.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
A-8(0-2)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/19/2023
Supervised By :Ankita Jodhani 10/19/2023

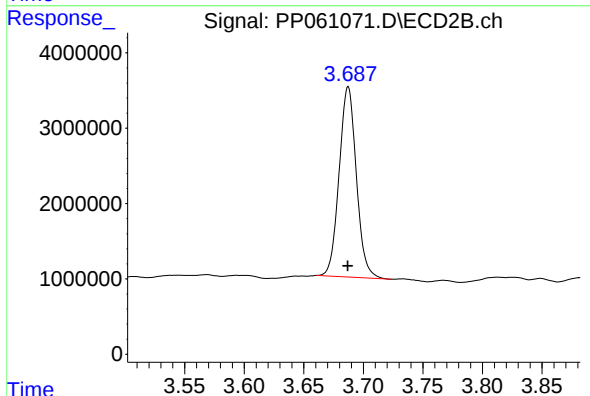


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: 0.000 min
Response: 25410780
Conc: 18.79 ng/ml

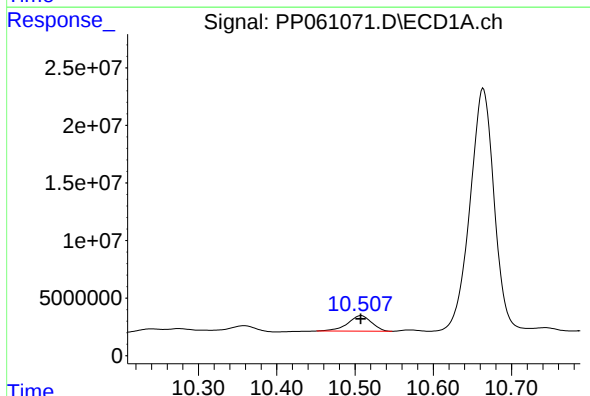

#2 Decachlorobiphenyl

R.T.: 10.508 min
Delta R.T.: 0.000 min
Response: 28722937
Conc: 18.34 ng/ml

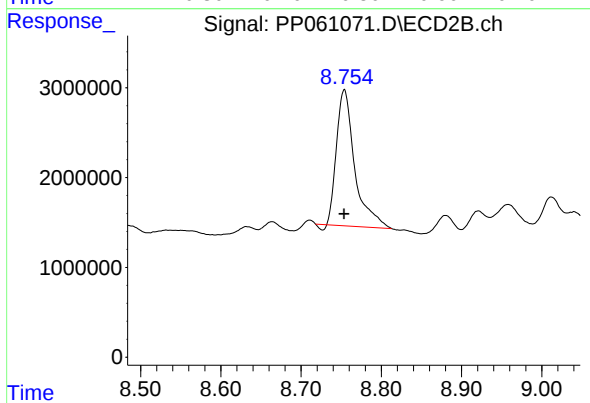

#2 Decachlorobiphenyl

R.T.: 8.754 min
Delta R.T.: 0.000 min
Response: 23698494
Conc: 15.76 ng/ml