

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
 Data File : PP068017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Oct 2024 04:50
 Operator : YP\AJ
 Sample : P4426-35
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRANSFORMER-PAD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 18 07:42:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.752	4.051	10942812	12023430	11.822	11.900
2)	SA Decachlor...	10.660	9.209	22647221	20261392	19.671	18.067
Target Compounds							
3)	L1 AR-1016-1	5.903	5.188	286099	218205	8.652	6.237 #
4)	L1 AR-1016-2	5.903f	5.188	286099	218205	5.866	4.530
5)	L1 AR-1016-3	6.007	5.348	274128	108170	8.699	4.016 #
6)	L1 AR-1016-4	6.095	5.400	259298	117514	10.072	4.879 #
7)	L1 AR-1016-5	0.000	5.617	0	181154	N.D.	5.957 #
8)	L2 AR-1221-1	4.956	0.000	315277	0	24.612	N.D. #
9)	L2 AR-1221-2	5.056	4.361	88348	199162	9.338	19.994 #
10)	L2 AR-1221-3	5.056f	4.441	88348	369008	3.056	11.853 #
11)	L3 AR-1232-1	5.056f	4.441	88348	369008	3.865	15.165 #
12)	L3 AR-1232-2	5.670	5.188	447422	218205	37.972	9.757 #
13)	L3 AR-1232-3	5.903f	5.348	286099	108170	12.844	9.057 #
14)	L3 AR-1232-4	6.095	5.439	259298	115472	22.972	10.014 #
15)	L3 AR-1232-5	6.233f	5.617	103115	181154	11.306	13.468
16)	L4 AR-1242-1	5.903	5.188	286099	218205	10.241	7.505 #
17)	L4 AR-1242-2	5.903f	5.188	286099	218205	7.041	5.435
18)	L4 AR-1242-3	6.007	5.348	274128	108170	10.166	4.809 #
19)	L4 AR-1242-4	6.095	5.439	259298	115472	12.088	4.864 #
20)	L4 AR-1242-5	6.898f	5.967	55436	211990	2.298	7.399 #
21)	L5 AR-1248-1	5.903	5.188	286099	218205	13.355	9.628 #
22)	L5 AR-1248-2	6.233f	5.400	103115	117514	3.067	3.551
23)	L5 AR-1248-3	0.000	5.439	0	115472	N.D.	3.349 #
24)	L5 AR-1248-4	6.770	5.617	38297	181154	0.947	4.423 #
25)	L5 AR-1248-5	6.898f	6.019	55436	141655	1.398	3.783 #
26)	L6 AR-1254-1	6.770	5.967	38297	211990	0.855	3.588 #
27)	L6 AR-1254-2	7.059f	6.120	62849	143970	0.951	2.744 #
28)	L6 AR-1254-3	7.349	6.533	293522	418545	4.226	5.030
29)	L6 AR-1254-4	7.639	6.758	349518	89032	7.004	1.844 #
30)	L6 AR-1254-5	8.056	7.179	360817	236633	6.085	3.217 #
31)	L7 AR-1260-1	7.517	6.686	306086	304660	5.666	5.348
32)	L7 AR-1260-2	7.770	6.847	296869	170616	4.692	2.558 #
34)	L7 AR-1260-4	8.365	7.516	23143	243010	0.384	4.395 #
35)	L7 AR-1260-5	8.712	7.713	60274	257521	0.560	2.106 #
36)	L8 AR-1262-1	8.365	7.218	23143	74279	0.322	0.944 #
37)	L8 AR-1262-2	8.712	7.516	60274	243010	0.496	3.425 #
38)	L8 AR-1262-3	9.046	8.033	1682576	1303749	19.009	22.833
39)	L8 AR-1262-4	9.122	8.104	35826	1008035	0.512	10.037 #
40)	L8 AR-1262-5	0.000	8.603	0	32057	N.D.	0.641 #
41)	L9 AR-1268-1	9.046	8.033	1682576	1303749	11.023	8.192 #
42)	L9 AR-1268-2	9.122	8.104	35826	1008035	0.262	7.040 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
Data File : PP068017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 04:50
Operator : YP\AJ
Sample : P4426-35
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 07:42:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
43)	L9 AR-1268-3	0.000	8.288	0	206213	N.D.	1.617 #
44)	L9 AR-1268-4	0.000	8.603	0	32057	N.D.	0.568 #
45)	L9 AR-1268-5	10.288	8.922	54296	233738	0.145	0.618 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101724\
Data File : PP068017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Oct 2024 04:50
Operator : YP\AJ
Sample : P4426-35
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 18 07:42:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

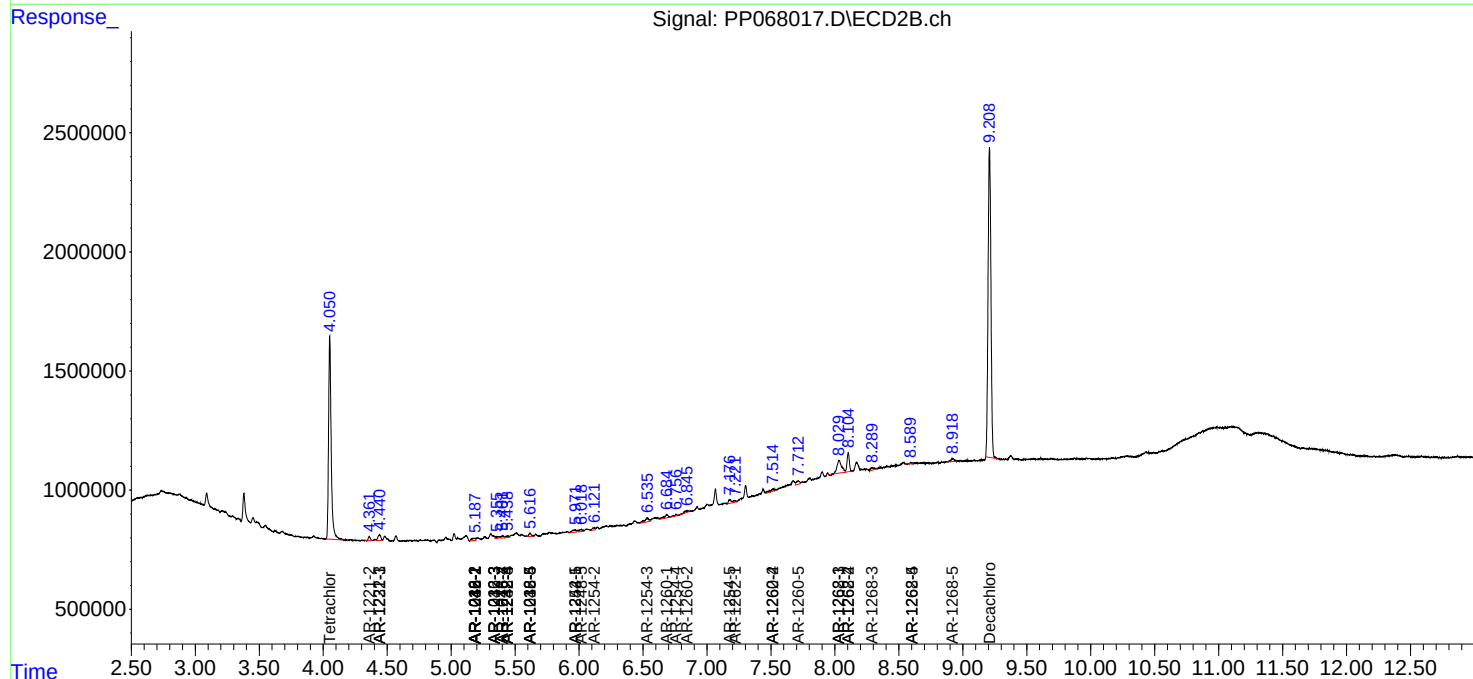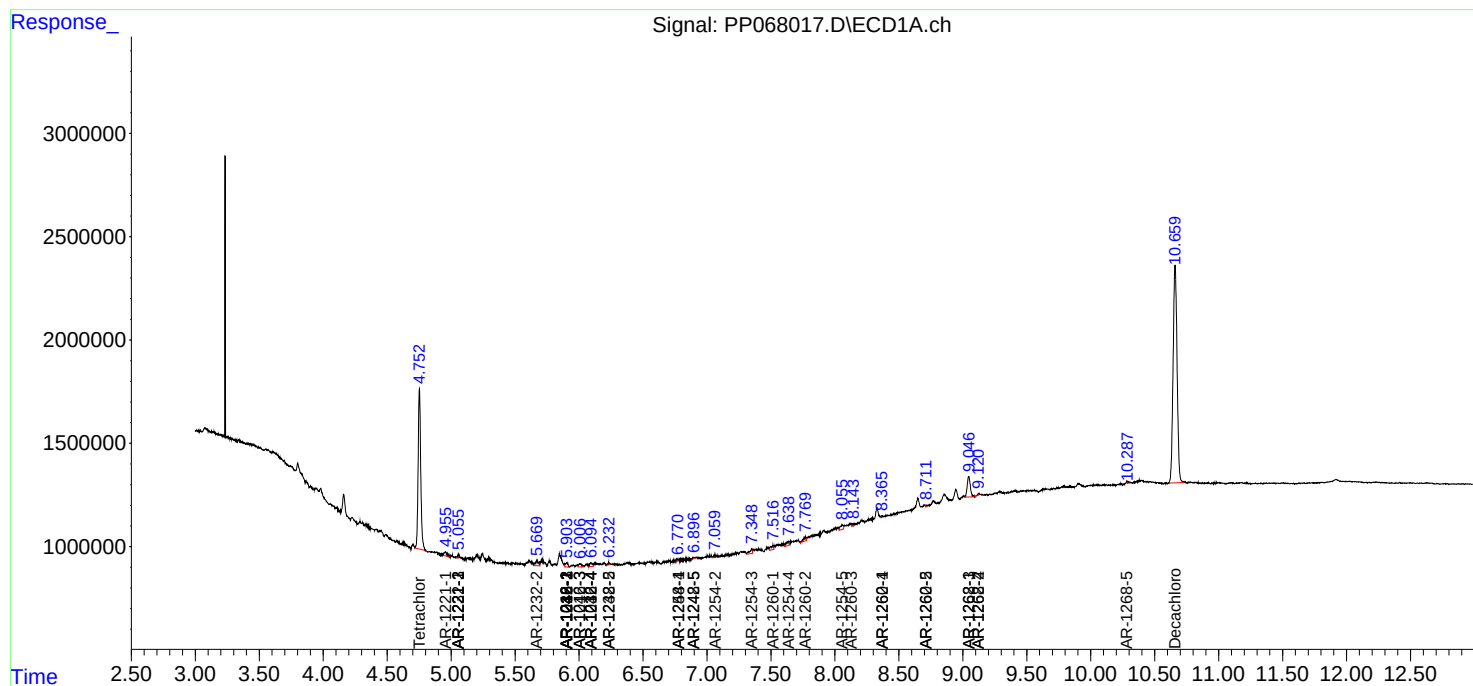


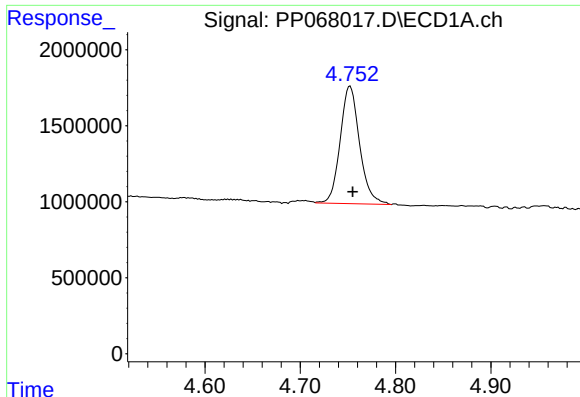

#1 Tetrachloro-m-xylene


R.T.: 4.752 min
Delta R.T.: -0.003 min
Response: 10942812
Conc: 11.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

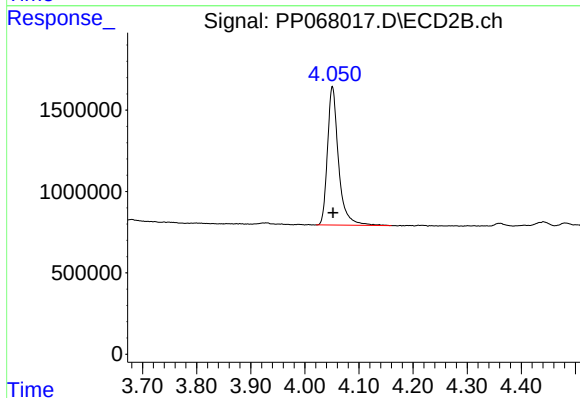


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: -0.001 min
Response: 12023430
Conc: 11.90 ng/ml

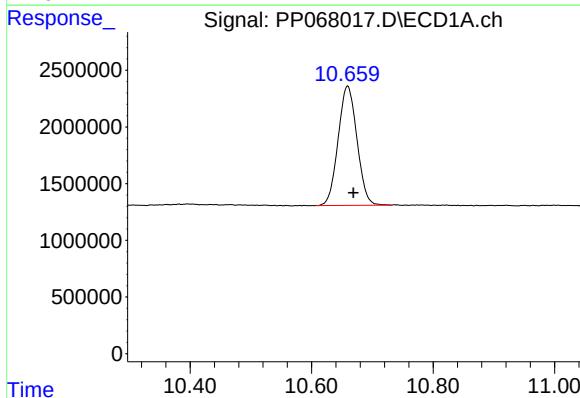


#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: -0.009 min
Response: 22647221
Conc: 19.67 ng/ml

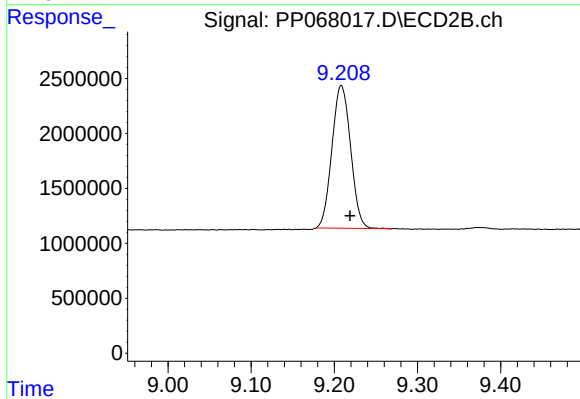

#2 Decachlorobiphenyl


R.T.: 9.209 min
Delta R.T.: -0.011 min
Response: 20261392
Conc: 18.07 ng/ml

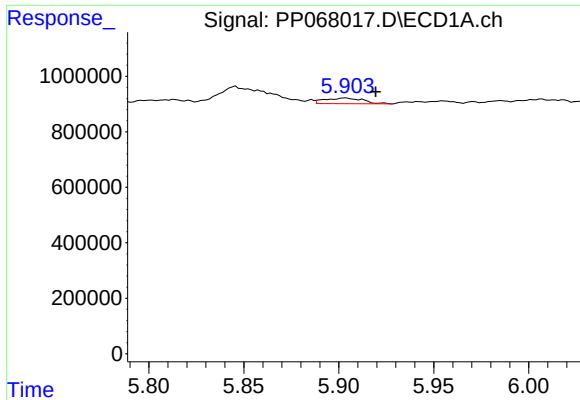

#3 AR-1016-1


R.T.: 5.903 min
Delta R.T.: -0.016 min
Response: 286099
Conc: 8.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

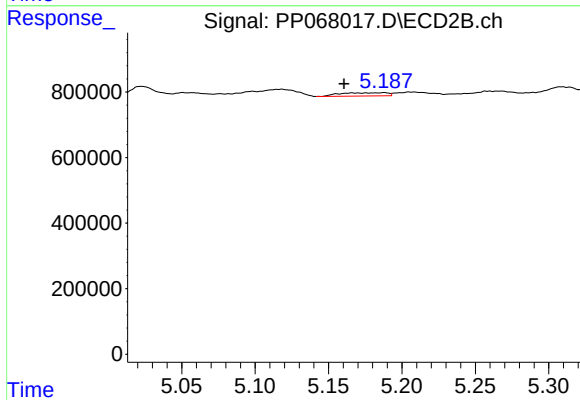


#3 AR-1016-1

R.T.: 5.188 min
Delta R.T.: 0.027 min
Response: 218205
Conc: 6.24 ng/ml

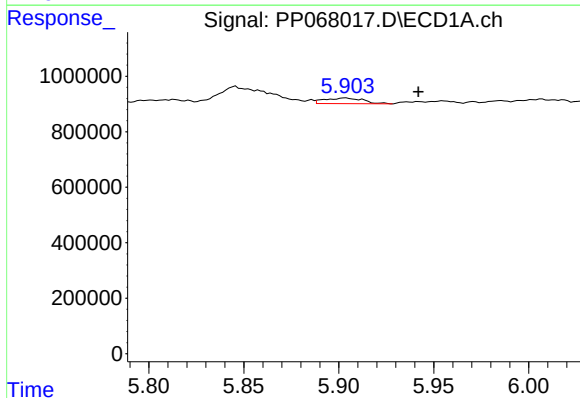


#4 AR-1016-2

R.T.: 5.903 min
Delta R.T.: -0.038 min
Response: 286099
Conc: 5.87 ng/ml

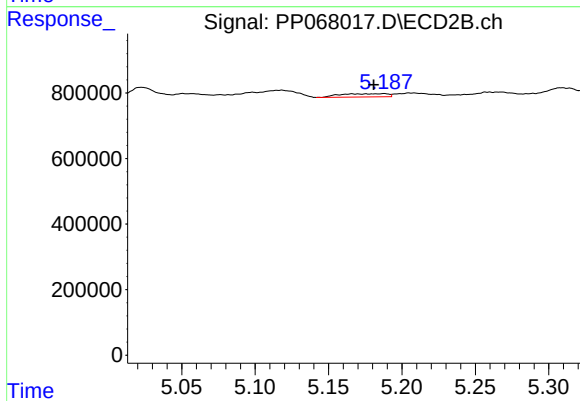

#4 AR-1016-2


R.T.: 5.188 min
Delta R.T.: 0.007 min
Response: 218205
Conc: 4.53 ng/ml

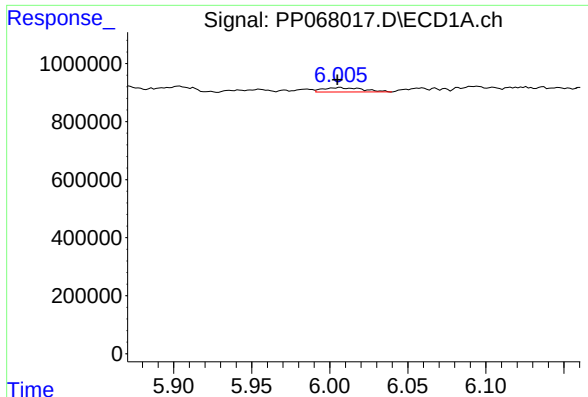

#5 AR-1016-3


R.T.: 6.007 min
Delta R.T.: 0.002 min
Response: 274128
Conc: 8.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

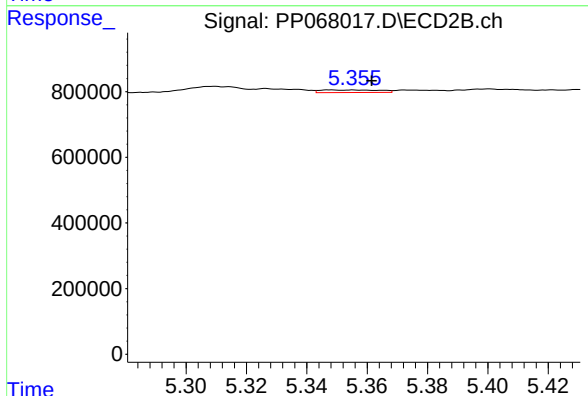


#5 AR-1016-3

R.T.: 5.348 min
Delta R.T.: -0.014 min
Response: 108170
Conc: 4.02 ng/ml

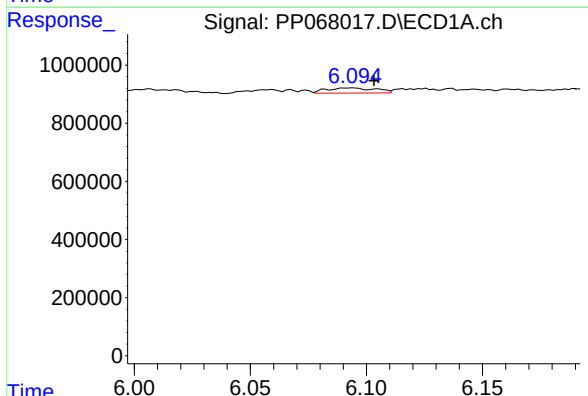


#6 AR-1016-4

R.T.: 6.095 min
Delta R.T.: -0.009 min
Response: 259298
Conc: 10.07 ng/ml

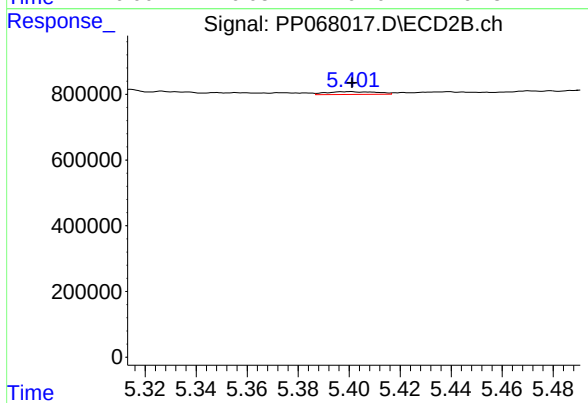

#6 AR-1016-4


R.T.: 5.400 min
Delta R.T.: -0.001 min
Response: 117514
Conc: 4.88 ng/ml

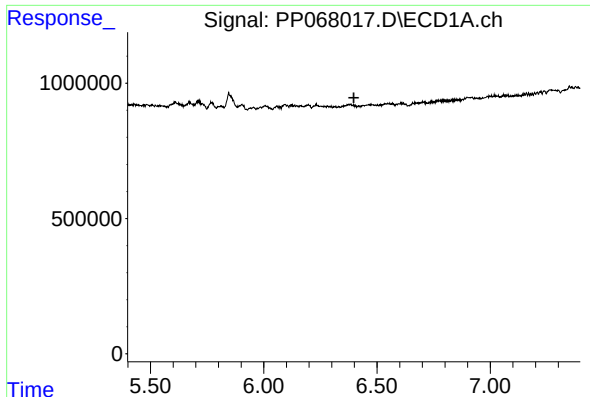

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

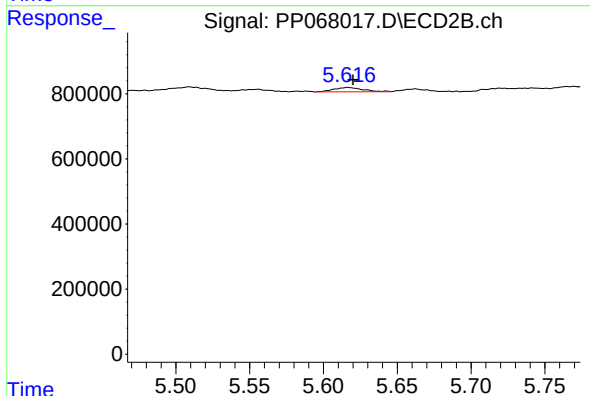


#7 AR-1016-5

R.T.: 5.617 min
Delta R.T.: -0.004 min
Response: 181154
Conc: 5.96 ng/ml

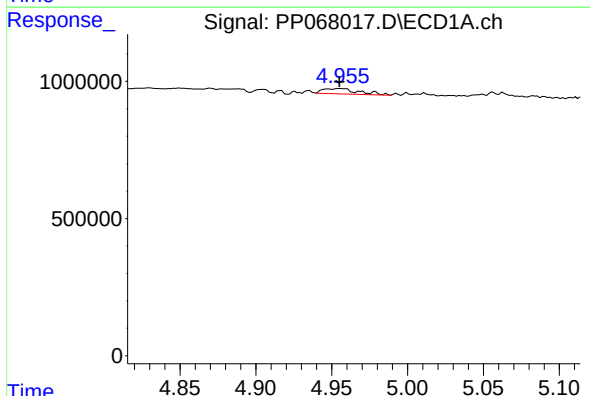


#8 AR-1221-1

R.T.: 4.956 min
Delta R.T.: 0.000 min
Response: 315277
Conc: 24.61 ng/ml

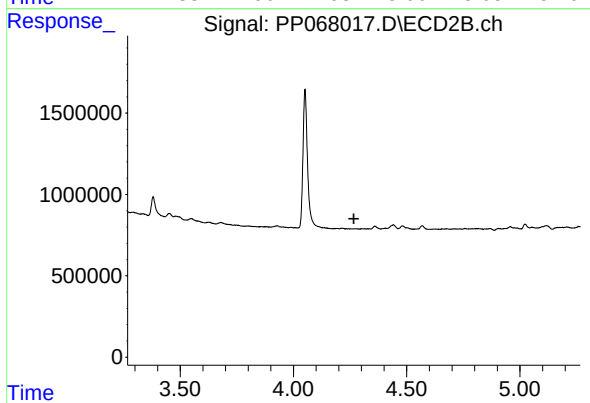

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.267 min
Response: 0
Conc: N.D.

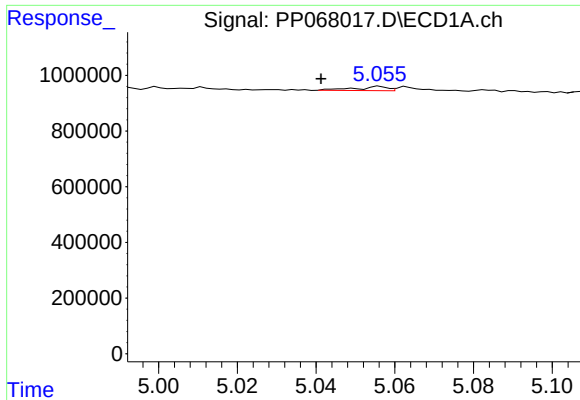

#9 AR-1221-2


R.T.: 5.056 min
Delta R.T.: 0.015 min
Response: 88348
Conc: 9.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

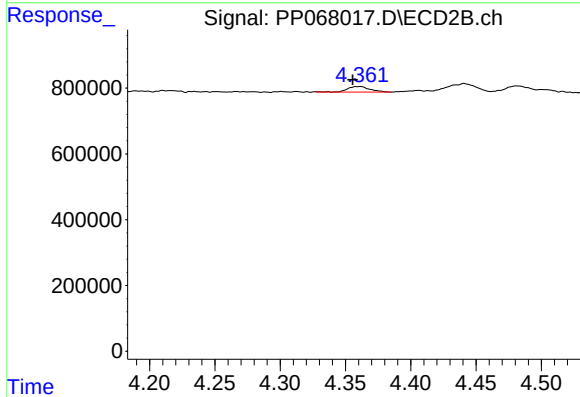


#9 AR-1221-2

R.T.: 4.361 min
Delta R.T.: 0.005 min
Response: 199162
Conc: 19.99 ng/ml

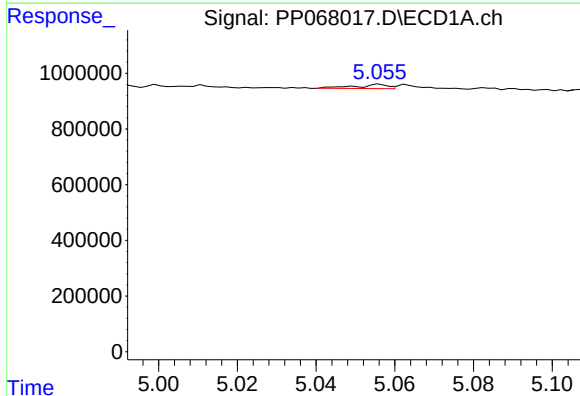


#10 AR-1221-3

R.T.: 5.056 min
Delta R.T.: -0.063 min
Response: 88348
Conc: 3.06 ng/ml

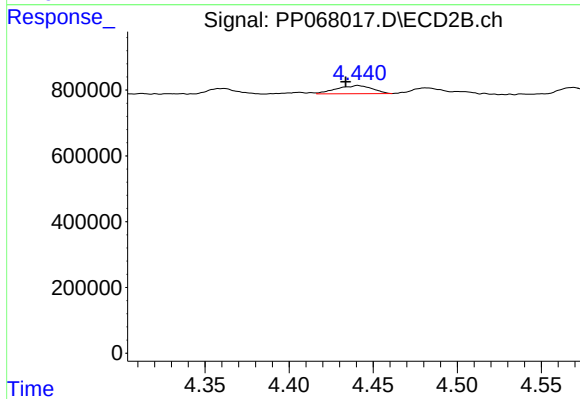

#10 AR-1221-3


R.T.: 4.441 min
Delta R.T.: 0.007 min
Response: 369008
Conc: 11.85 ng/ml

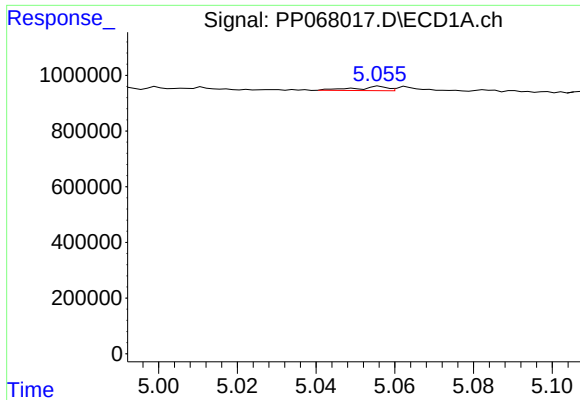

#11 AR-1232-1


R.T.: 5.056 min
Delta R.T.: -0.062 min
Response: 88348
Conc: 3.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

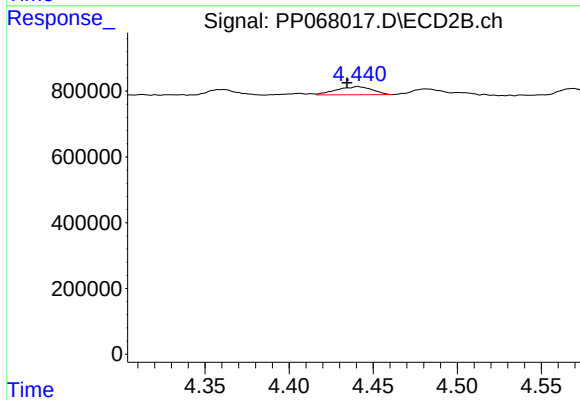


#11 AR-1232-1

R.T.: 4.441 min
Delta R.T.: 0.007 min
Response: 369008
Conc: 15.16 ng/ml

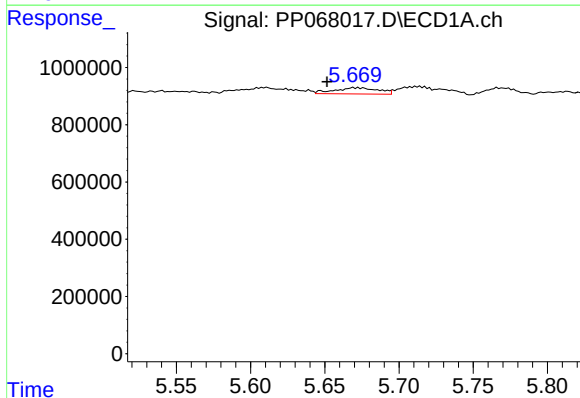


#12 AR-1232-2

R.T.: 5.670 min
Delta R.T.: 0.018 min
Response: 447422
Conc: 37.97 ng/ml

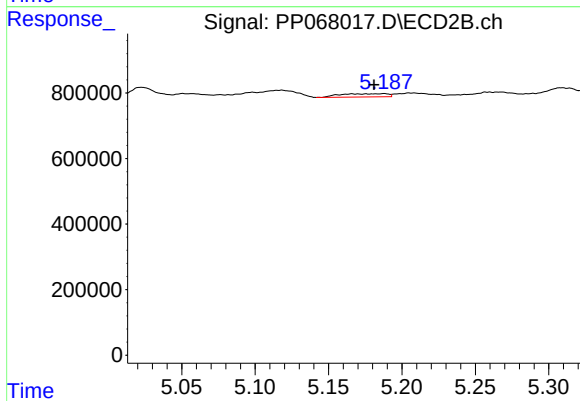

#12 AR-1232-2


R.T.: 5.188 min
Delta R.T.: 0.007 min
Response: 218205
Conc: 9.76 ng/ml

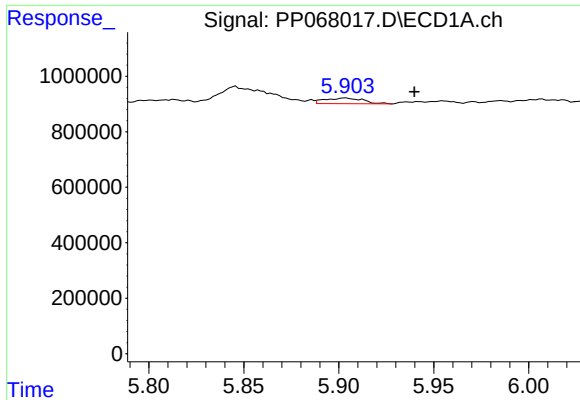

#13 AR-1232-3


R.T.: 5.903 min
Delta R.T.: -0.036 min
Response: 286099
Conc: 12.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

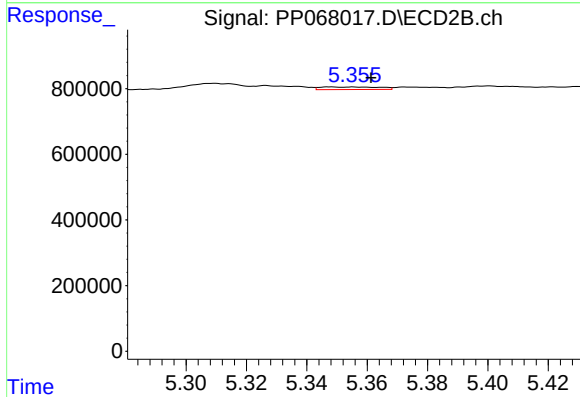


#13 AR-1232-3

R.T.: 5.348 min
Delta R.T.: -0.013 min
Response: 108170
Conc: 9.06 ng/ml

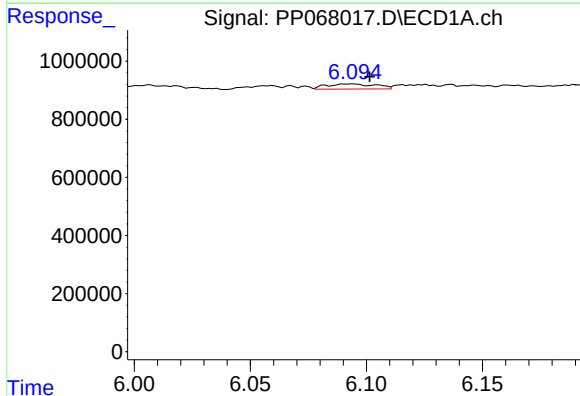


#14 AR-1232-4

R.T.: 6.095 min
Delta R.T.: -0.007 min
Response: 259298
Conc: 22.97 ng/ml

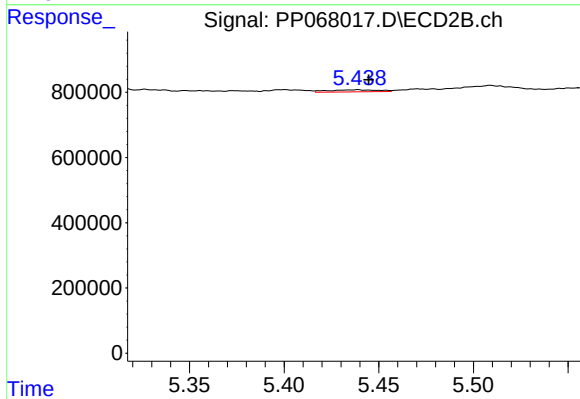

#14 AR-1232-4


R.T.: 5.439 min
Delta R.T.: -0.006 min
Response: 115472
Conc: 10.01 ng/ml

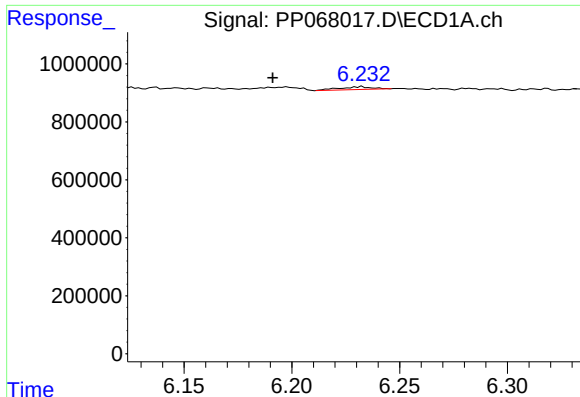

#15 AR-1232-5


R.T.: 6.233 min
Delta R.T.: 0.042 min
Response: 103115
Conc: 11.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

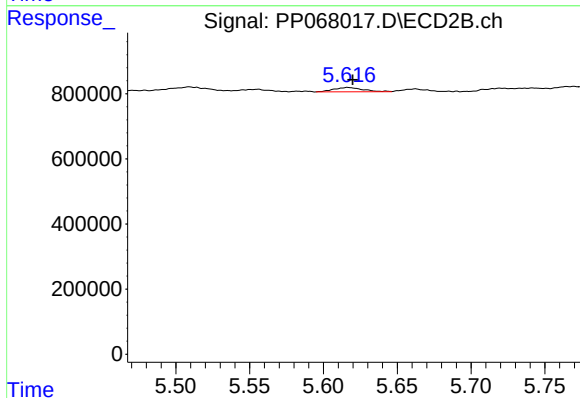


#15 AR-1232-5

R.T.: 5.617 min
Delta R.T.: -0.003 min
Response: 181154
Conc: 13.47 ng/ml

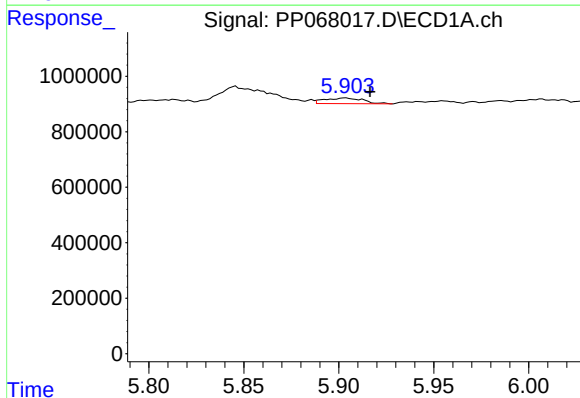


#16 AR-1242-1

R.T.: 5.903 min
Delta R.T.: -0.013 min
Response: 286099
Conc: 10.24 ng/ml

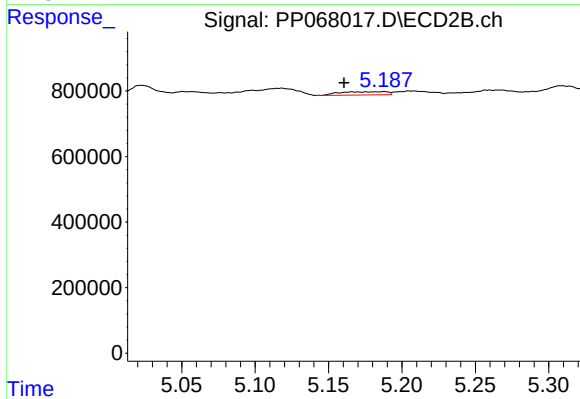

#16 AR-1242-1


R.T.: 5.188 min
Delta R.T.: 0.027 min
Response: 218205
Conc: 7.50 ng/ml

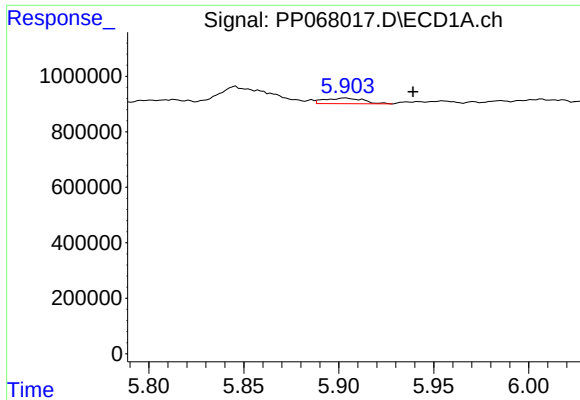

#17 AR-1242-2


R.T.: 5.903 min
Delta R.T.: -0.036 min
Response: 286099
Conc: 7.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

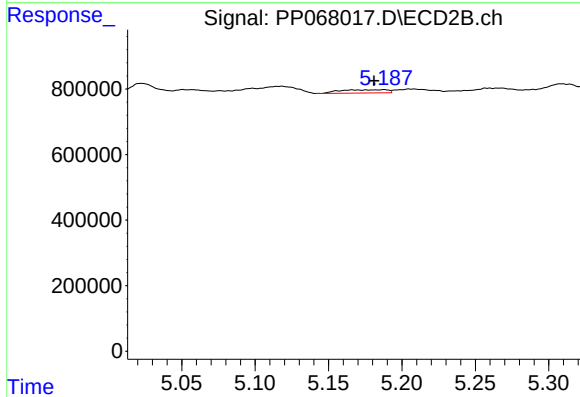


#17 AR-1242-2

R.T.: 5.188 min
Delta R.T.: 0.007 min
Response: 218205
Conc: 5.44 ng/ml

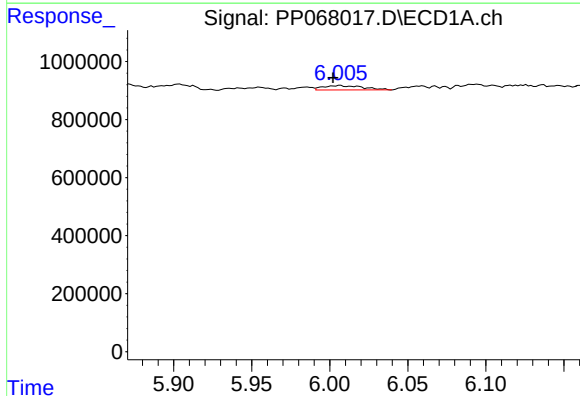


#18 AR-1242-3

R.T.: 6.007 min
Delta R.T.: 0.005 min
Response: 274128
Conc: 10.17 ng/ml

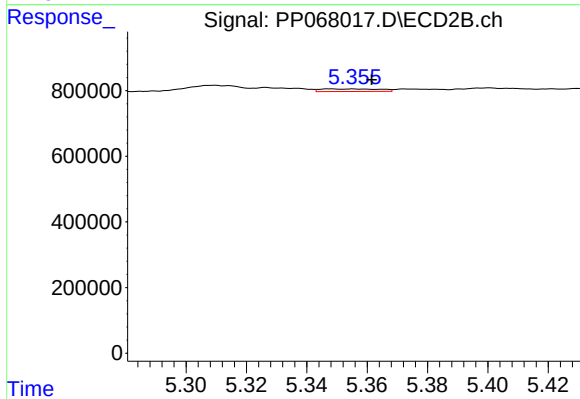

#18 AR-1242-3


R.T.: 5.348 min
Delta R.T.: -0.014 min
Response: 108170
Conc: 4.81 ng/ml

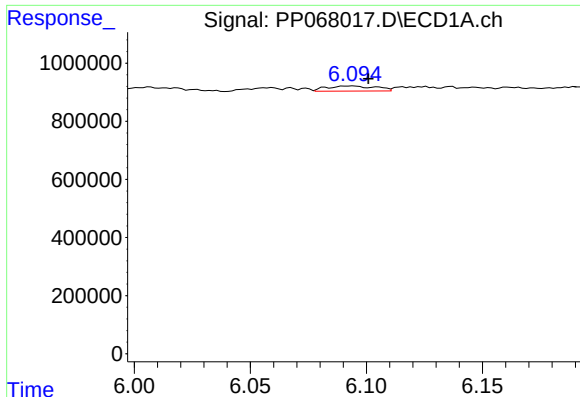

#19 AR-1242-4


R.T.: 6.095 min
Delta R.T.: -0.006 min
Response: 259298
Conc: 12.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

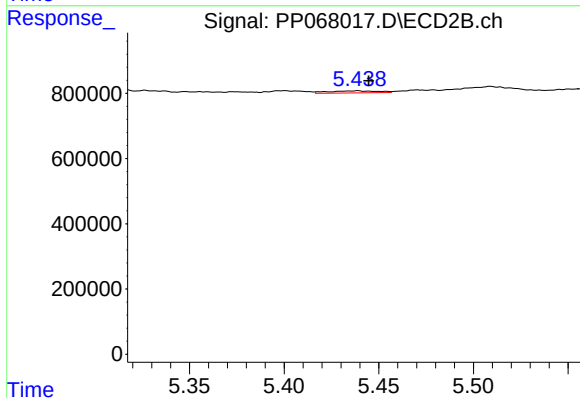


#19 AR-1242-4

R.T.: 5.439 min
Delta R.T.: -0.006 min
Response: 115472
Conc: 4.86 ng/ml

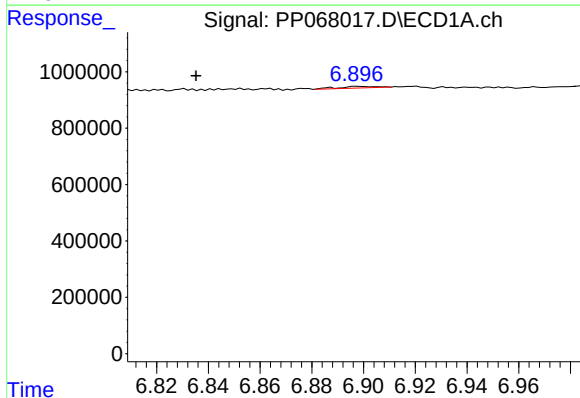


#20 AR-1242-5

R.T.: 6.898 min
Delta R.T.: 0.062 min
Response: 55436
Conc: 2.30 ng/ml

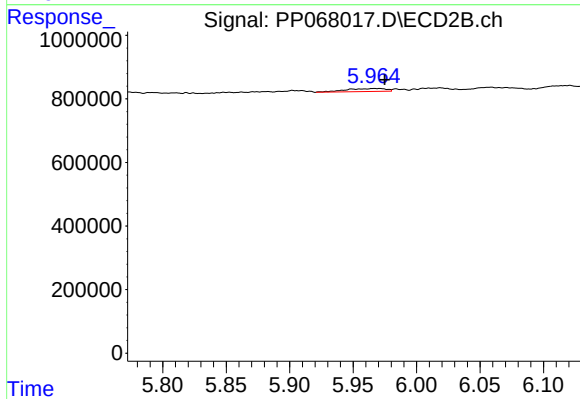

#20 AR-1242-5


R.T.: 5.967 min
Delta R.T.: -0.008 min
Response: 211990
Conc: 7.40 ng/ml

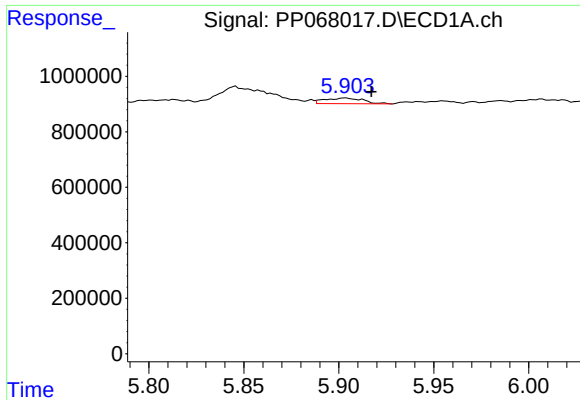

#21 AR-1248-1


R.T.: 5.903 min
Delta R.T.: -0.014 min
Response: 286099
Conc: 13.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

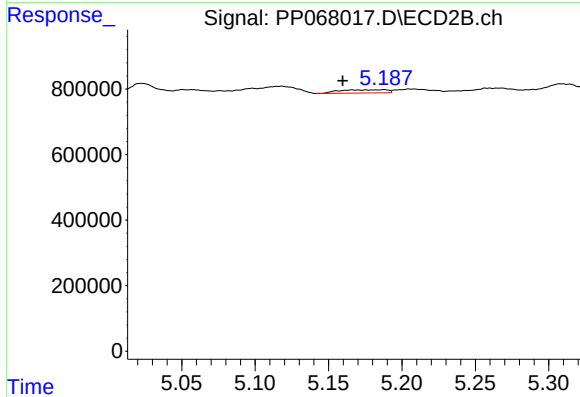


#21 AR-1248-1

R.T.: 5.188 min
Delta R.T.: 0.028 min
Response: 218205
Conc: 9.63 ng/ml

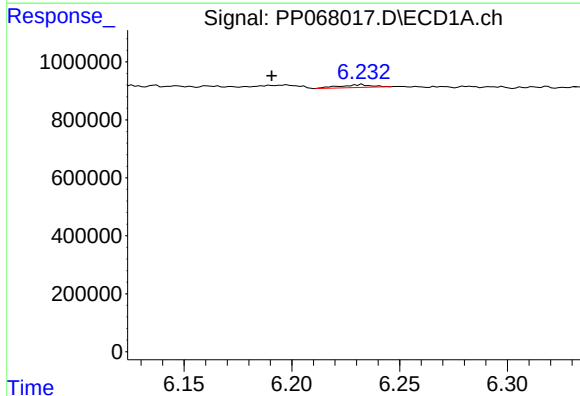


#22 AR-1248-2

R.T.: 6.233 min
Delta R.T.: 0.042 min
Response: 103115
Conc: 3.07 ng/ml

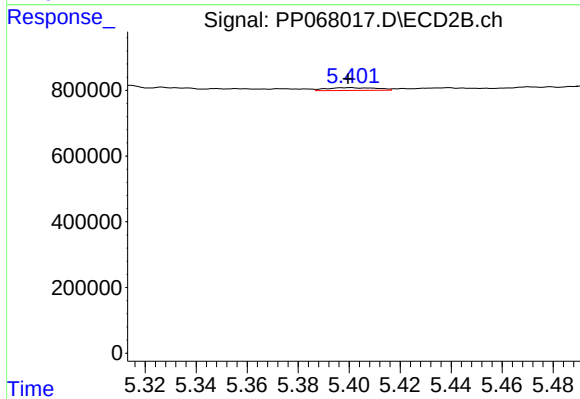

#22 AR-1248-2


R.T.: 5.400 min
Delta R.T.: 0.000 min
Response: 117514
Conc: 3.55 ng/ml

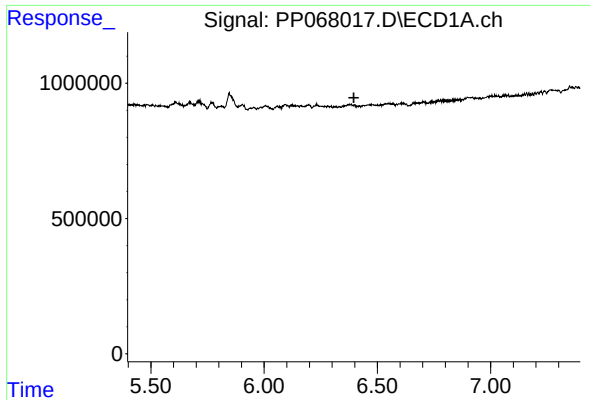

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.396 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

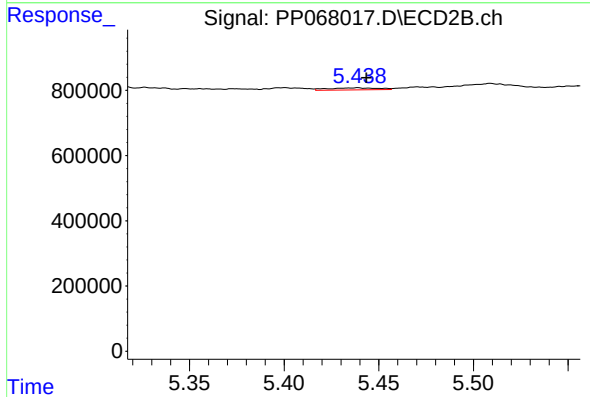


#23 AR-1248-3

R.T.: 5.439 min
Delta R.T.: -0.005 min
Response: 115472
Conc: 3.35 ng/ml

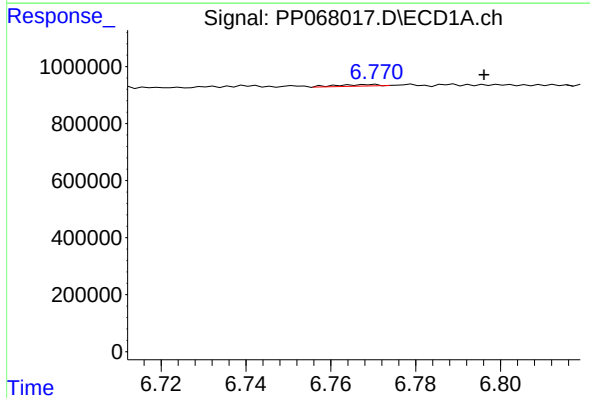


#24 AR-1248-4

R.T.: 6.770 min
Delta R.T.: -0.026 min
Response: 38297
Conc: 0.95 ng/ml

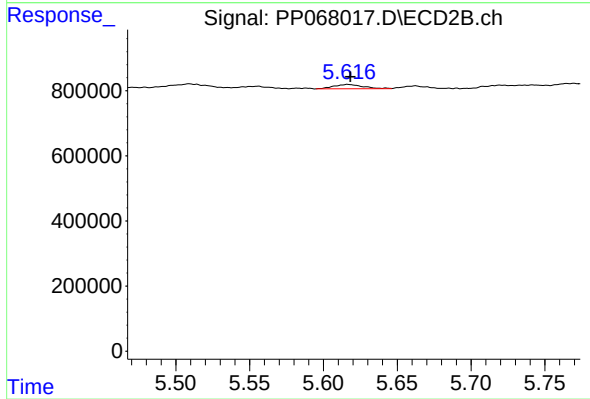

#24 AR-1248-4


R.T.: 5.617 min
Delta R.T.: -0.002 min
Response: 181154
Conc: 4.42 ng/ml

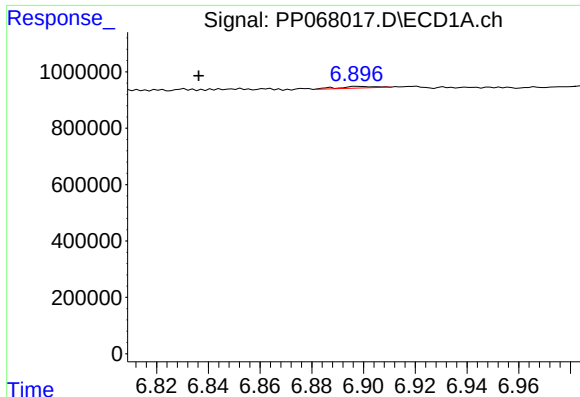

#25 AR-1248-5


R.T.: 6.898 min
Delta R.T.: 0.061 min
Response: 55436
Conc: 1.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

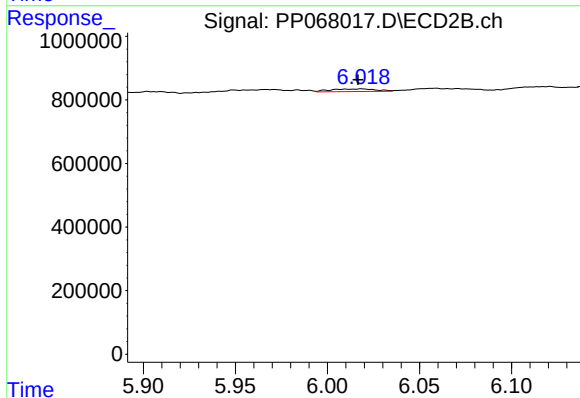


#25 AR-1248-5

R.T.: 6.019 min
Delta R.T.: 0.002 min
Response: 141655
Conc: 3.78 ng/ml

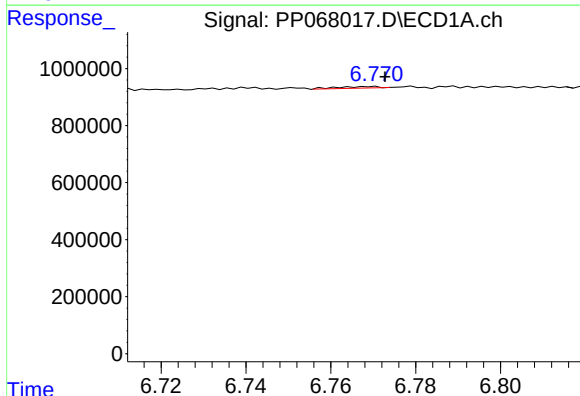


#26 AR-1254-1

R.T.: 6.770 min
Delta R.T.: -0.003 min
Response: 38297
Conc: 0.86 ng/ml

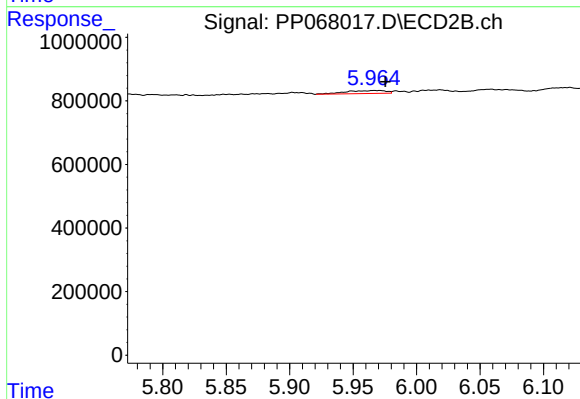

#26 AR-1254-1


R.T.: 5.967 min
Delta R.T.: -0.008 min
Response: 211990
Conc: 3.59 ng/ml

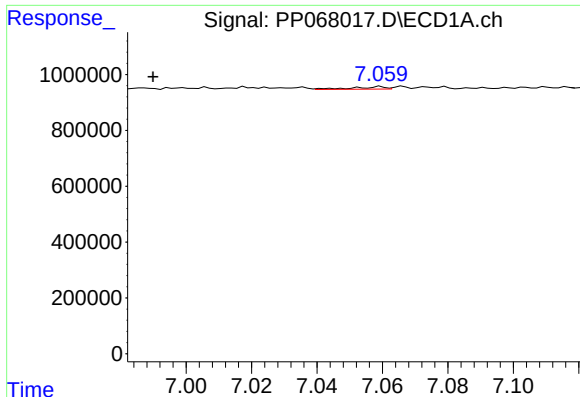

#27 AR-1254-2


R.T.: 7.059 min
Delta R.T.: 0.070 min
Response: 62849
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

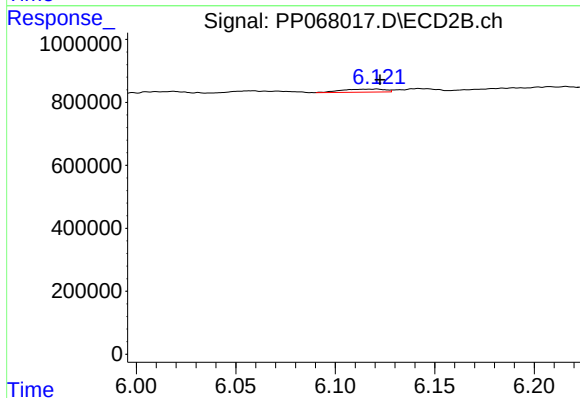


#27 AR-1254-2

R.T.: 6.120 min
Delta R.T.: -0.002 min
Response: 143970
Conc: 2.74 ng/ml

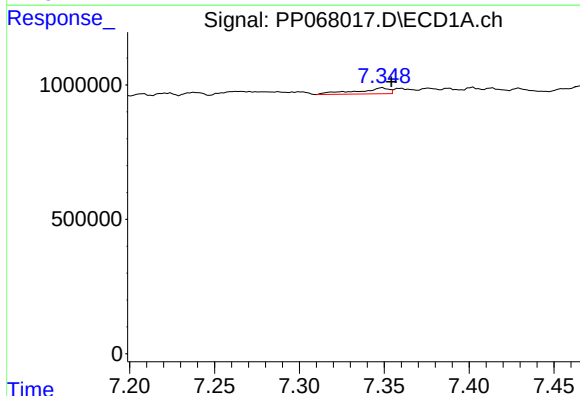


#28 AR-1254-3

R.T.: 7.349 min
Delta R.T.: -0.005 min
Response: 293522
Conc: 4.23 ng/ml

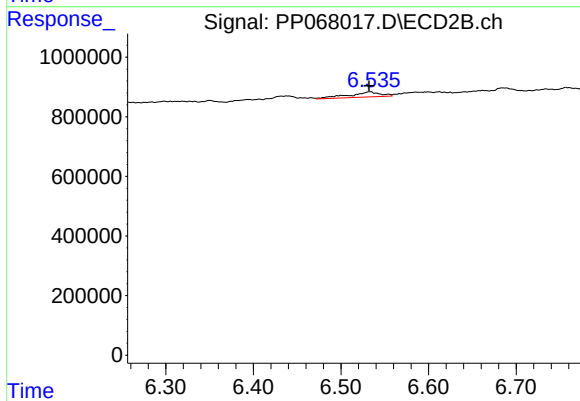

#28 AR-1254-3


R.T.: 6.533 min
Delta R.T.: 0.000 min
Response: 418545
Conc: 5.03 ng/ml

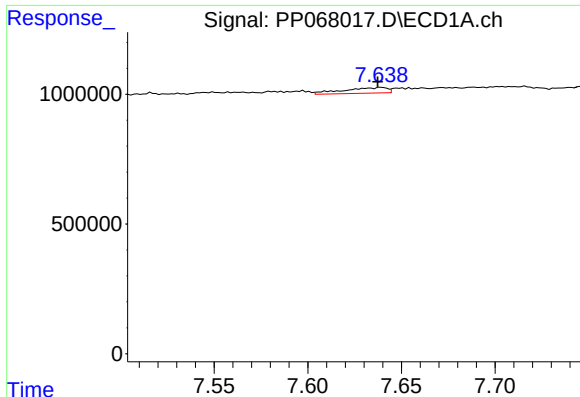

#29 AR-1254-4


R.T.: 7.639 min
Delta R.T.: 0.002 min
Response: 349518
Conc: 7.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

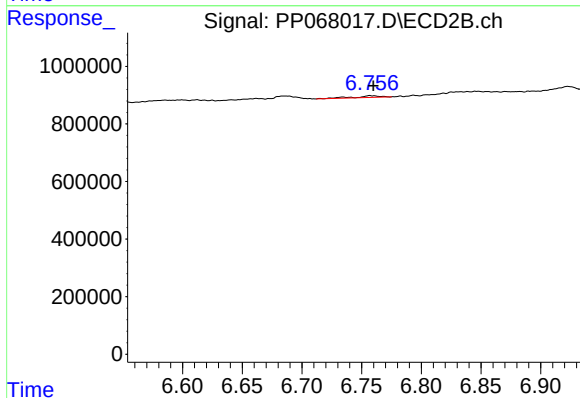


#29 AR-1254-4

R.T.: 6.758 min
Delta R.T.: -0.002 min
Response: 89032
Conc: 1.84 ng/ml

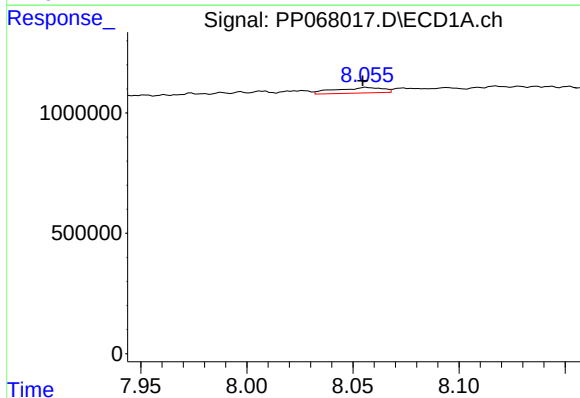


#30 AR-1254-5

R.T.: 8.056 min
Delta R.T.: 0.002 min
Response: 360817
Conc: 6.09 ng/ml

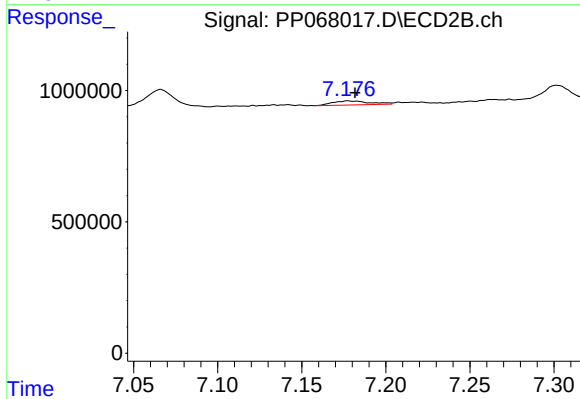

#30 AR-1254-5


R.T.: 7.179 min
Delta R.T.: -0.003 min
Response: 236633
Conc: 3.22 ng/ml

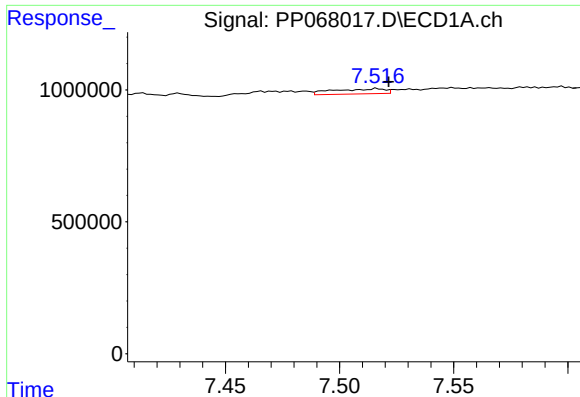

#31 AR-1260-1


R.T.: 7.517 min
Delta R.T.: -0.005 min
Response: 306086
Conc: 5.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

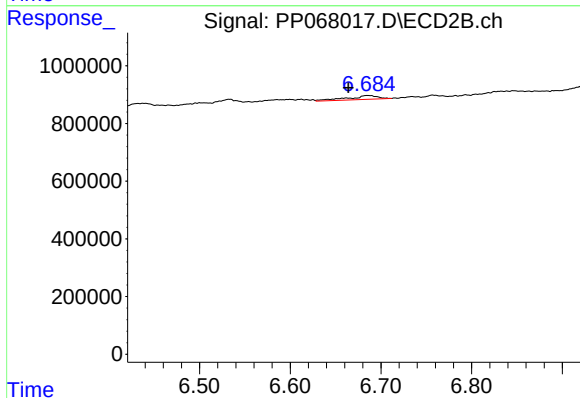


#31 AR-1260-1

R.T.: 6.686 min
Delta R.T.: 0.022 min
Response: 304660
Conc: 5.35 ng/ml

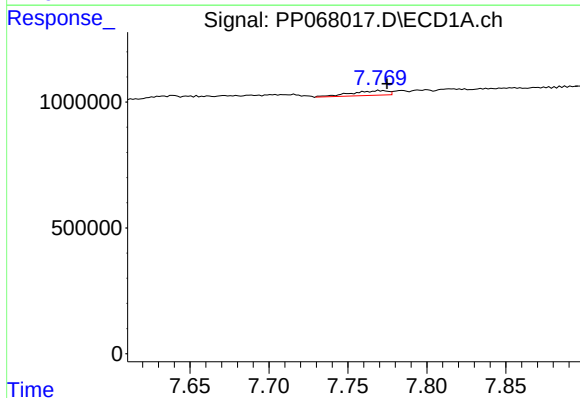


#32 AR-1260-2

R.T.: 7.770 min
Delta R.T.: -0.005 min
Response: 296869
Conc: 4.69 ng/ml

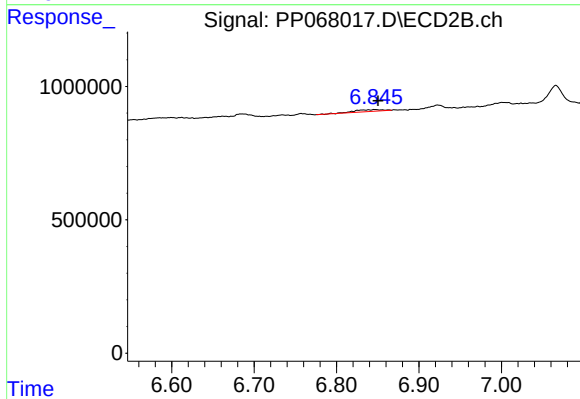

#32 AR-1260-2


R.T.: 6.847 min
Delta R.T.: -0.003 min
Response: 170616
Conc: 2.56 ng/ml

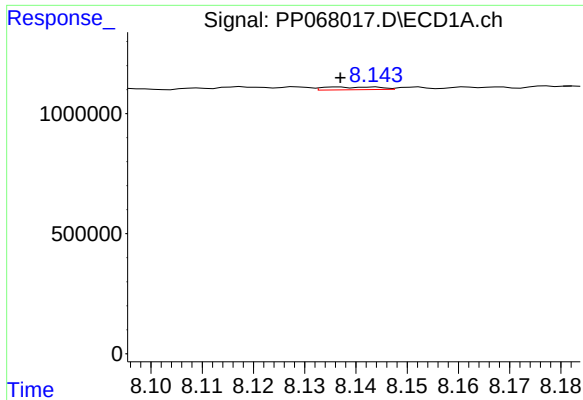

#33 AR-1260-3


R.T.: 8.136 min
Delta R.T.: 0.000 min
Response: 85234
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

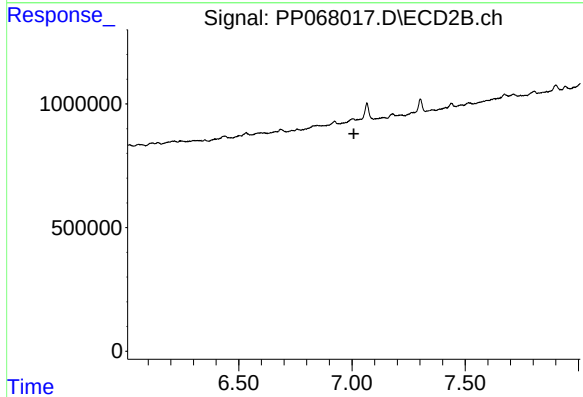


#33 AR-1260-3

R.T.: 7.004 min
Delta R.T.: -0.005 min
Response: -180732
Conc: N.D.

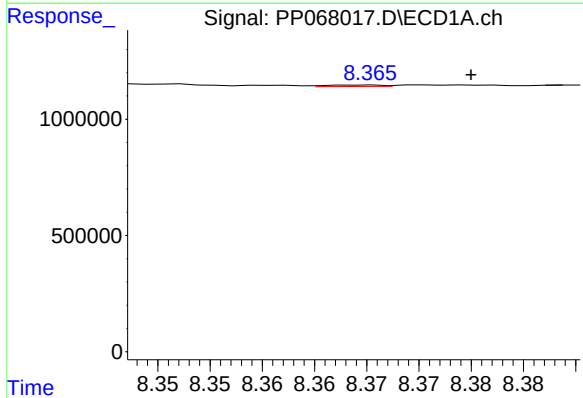


#34 AR-1260-4

R.T.: 8.365 min
Delta R.T.: -0.010 min
Response: 23143
Conc: 0.38 ng/ml

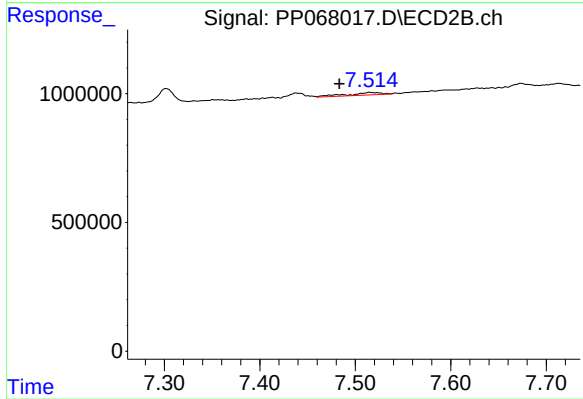

#34 AR-1260-4


R.T.: 7.516 min
Delta R.T.: 0.032 min
Response: 243010
Conc: 4.39 ng/ml

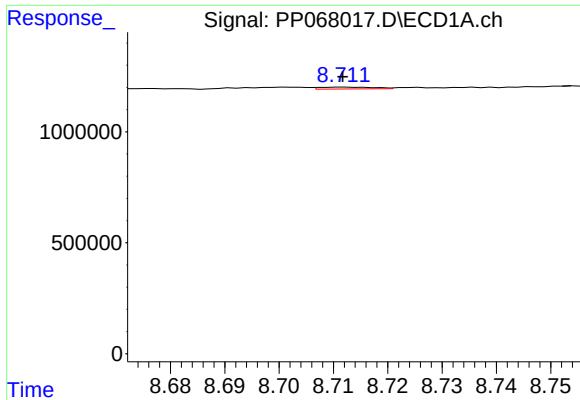

#35 AR-1260-5


R.T.: 8.712 min
Delta R.T.: 0.000 min
Response: 60274
Conc: 0.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

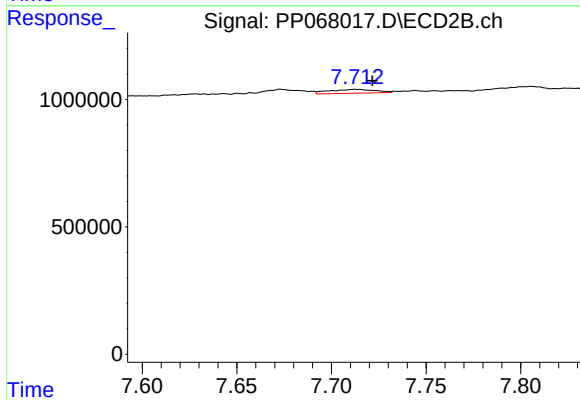


#35 AR-1260-5

R.T.: 7.713 min
Delta R.T.: -0.008 min
Response: 257521
Conc: 2.11 ng/ml

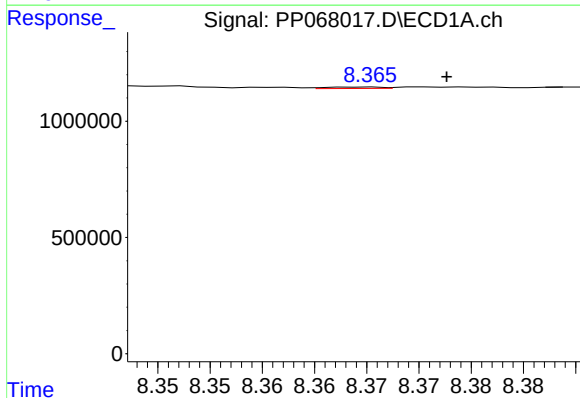


#36 AR-1262-1

R.T.: 8.365 min
Delta R.T.: -0.008 min
Response: 23143
Conc: 0.32 ng/ml

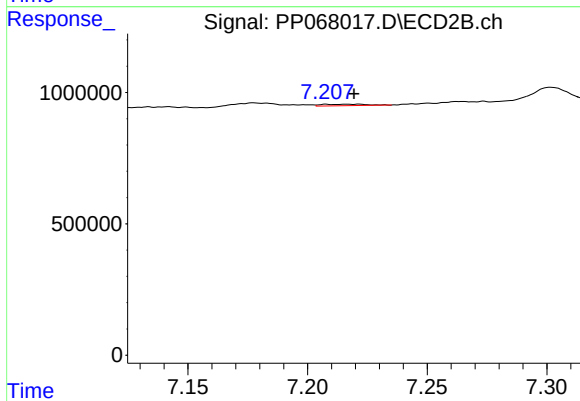

#36 AR-1262-1


R.T.: 7.218 min
Delta R.T.: -0.002 min
Response: 74279
Conc: 0.94 ng/ml

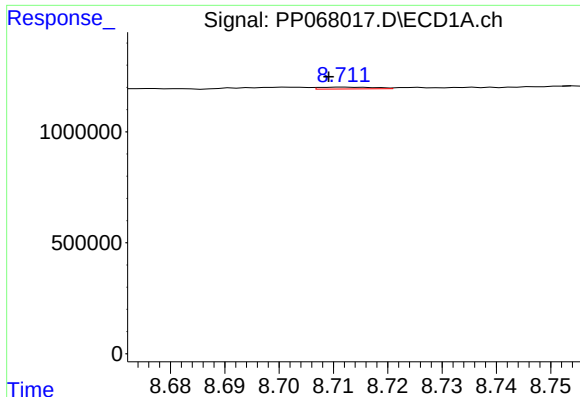

#37 AR-1262-2


R.T.: 8.712 min
Delta R.T.: 0.003 min
Response: 60274
Conc: 0.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

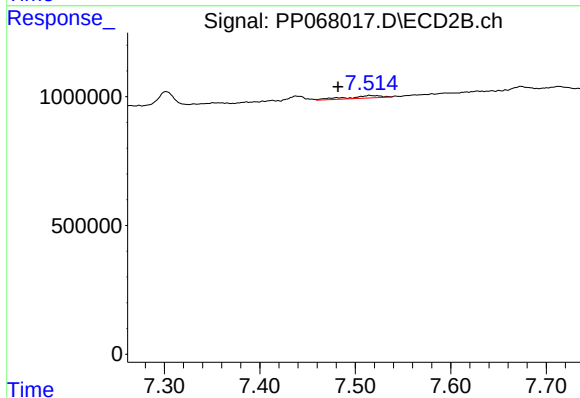


#37 AR-1262-2

R.T.: 7.516 min
Delta R.T.: 0.034 min
Response: 243010
Conc: 3.42 ng/ml

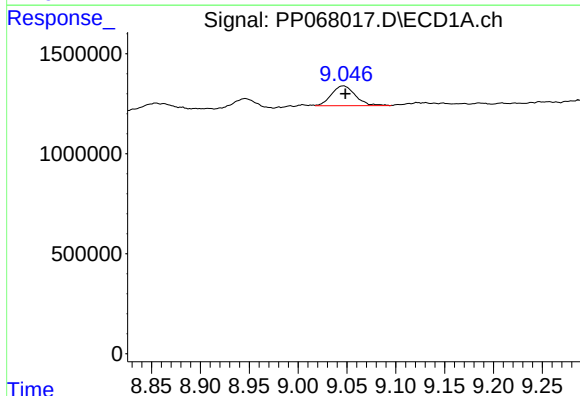


#38 AR-1262-3

R.T.: 9.046 min
Delta R.T.: -0.002 min
Response: 1682576
Conc: 19.01 ng/ml

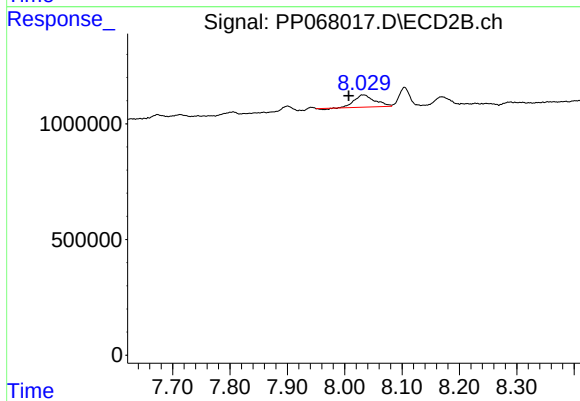

#38 AR-1262-3


R.T.: 8.033 min
Delta R.T.: 0.026 min
Response: 1303749
Conc: 22.83 ng/ml

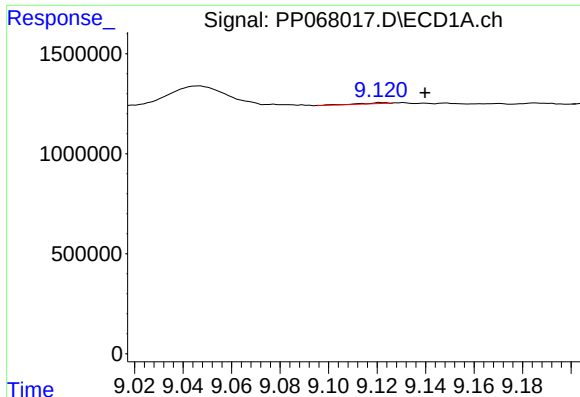

#39 AR-1262-4


R.T.: 9.122 min
Delta R.T.: -0.018 min
Response: 35826
Conc: 0.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

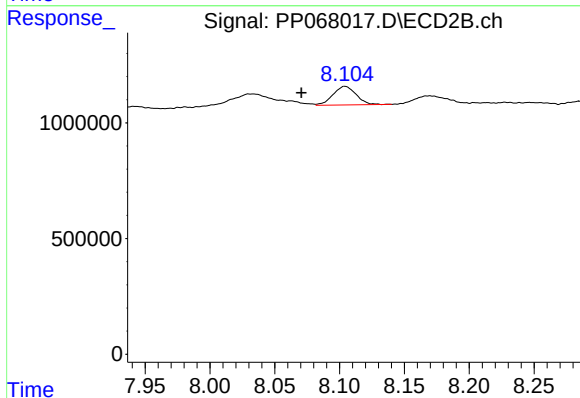


#39 AR-1262-4

R.T.: 8.104 min
Delta R.T.: 0.034 min
Response: 1008035
Conc: 10.04 ng/ml

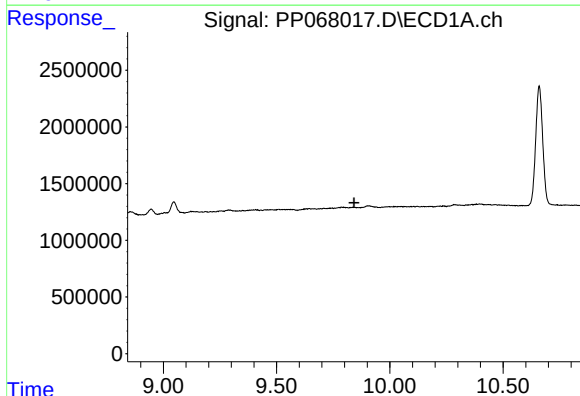


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.842 min
Response: 0
Conc: N.D.

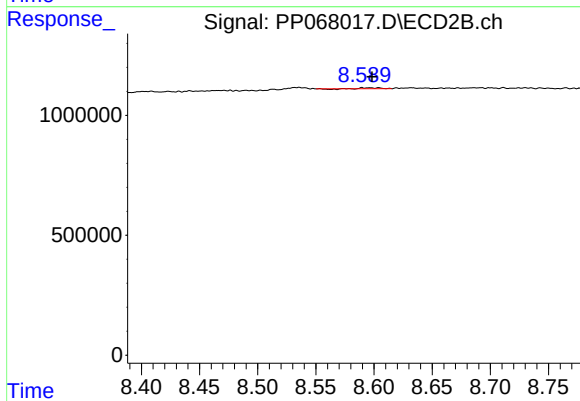

#40 AR-1262-5


R.T.: 8.603 min
Delta R.T.: 0.005 min
Response: 32057
Conc: 0.64 ng/ml

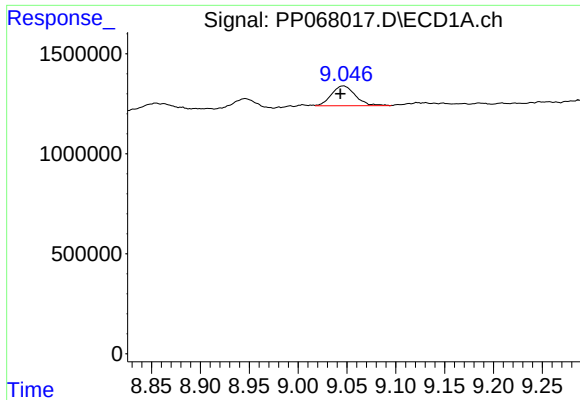

#41 AR-1268-1


R.T.: 9.046 min
Delta R.T.: 0.003 min
Response: 1682576
Conc: 11.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

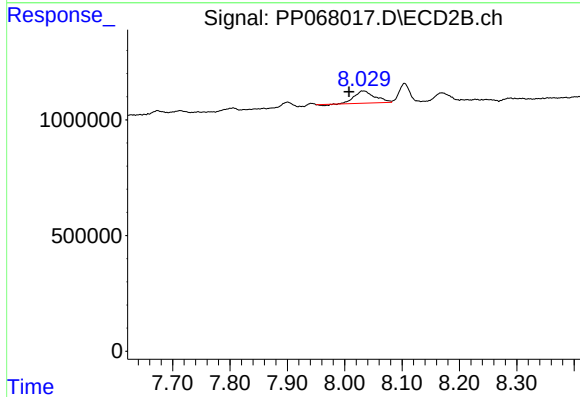


#41 AR-1268-1

R.T.: 8.033 min
Delta R.T.: 0.025 min
Response: 1303749
Conc: 8.19 ng/ml

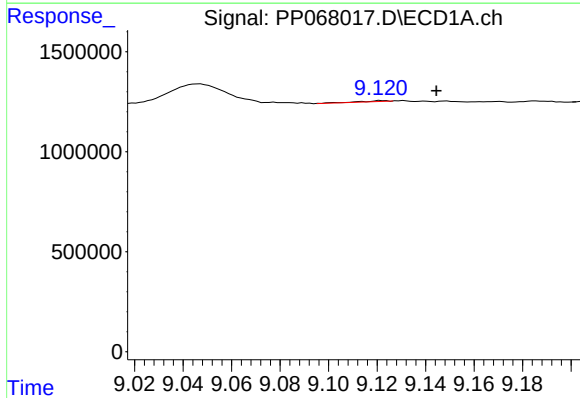


#42 AR-1268-2

R.T.: 9.122 min
Delta R.T.: -0.022 min
Response: 35826
Conc: 0.26 ng/ml

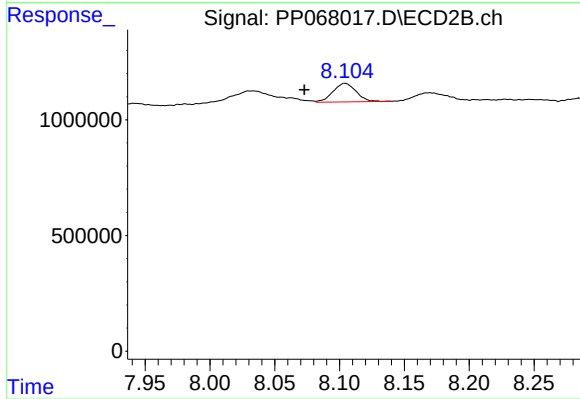

#42 AR-1268-2


R.T.: 8.104 min
Delta R.T.: 0.031 min
Response: 1008035
Conc: 7.04 ng/ml

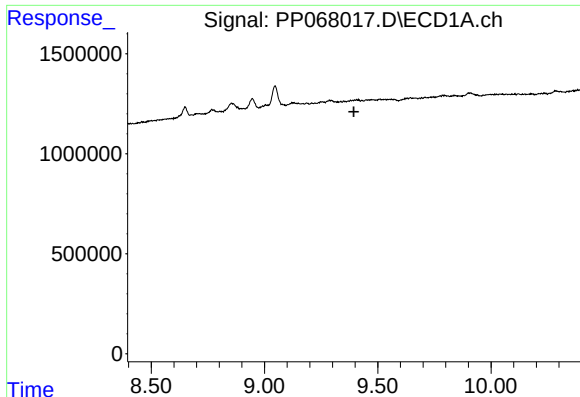

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

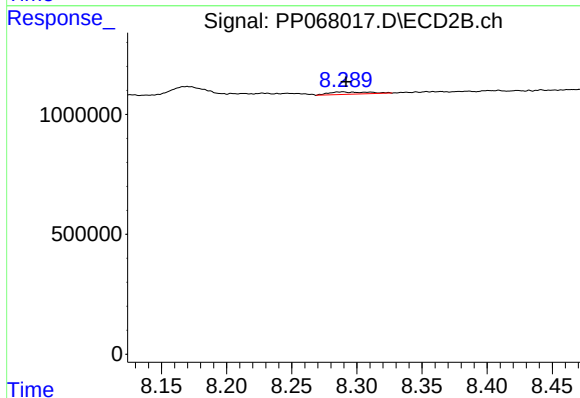


#43 AR-1268-3

R.T.: 8.288 min
Delta R.T.: -0.004 min
Response: 206213
Conc: 1.62 ng/ml

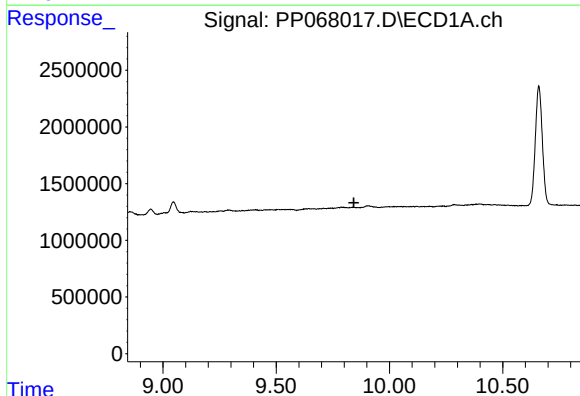


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.843 min
Response: 0
Conc: N.D.

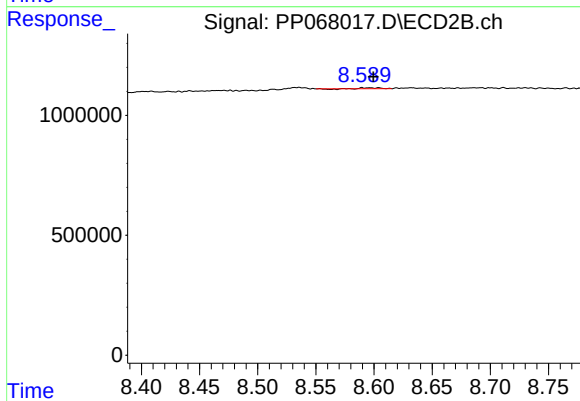

#44 AR-1268-4


R.T.: 8.603 min
Delta R.T.: 0.003 min
Response: 32057
Conc: 0.57 ng/ml

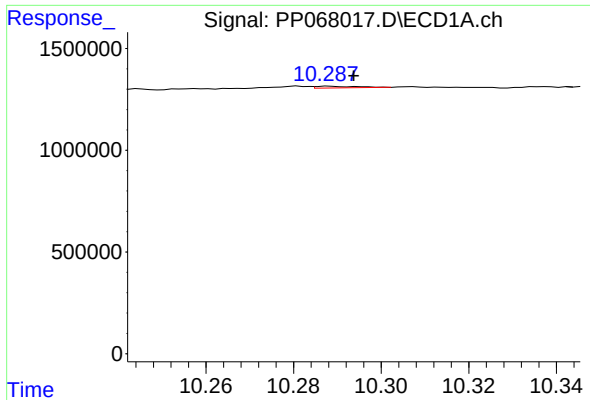

#45 AR-1268-5

R.T.: 10.288 min
Delta R.T.: -0.006 min
Response: 54296
Conc: 0.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRANSFORMER-PAD

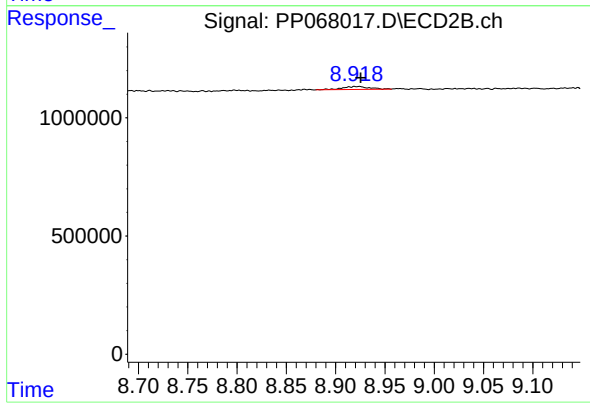

#45 AR-1268-5

R.T.: 8.922 min
Delta R.T.: -0.003 min
Response: 233738
Conc: 0.62 ng/ml