

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101921\
 Data File : PP040242.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2021 23:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:12:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.892	3.980	747651	416110	24.619	24.613
2)	SA Decachlor...	10.911	9.306	633627	535668	25.636	25.240
Target Compounds							
10)	L2 AR-1221-3	0.000	4.419	0	7626	N.D.	14.082 #
11)	L3 AR-1232-1	0.000	4.419	0	7626	N.D.	18.776 #
20)	L4 AR-1242-5	0.000	6.145f	0	22841	N.D.	47.888 #
25)	L5 AR-1248-5	0.000	6.145f	0	22841	N.D.	36.613 #
26)	L6 AR-1254-1	7.136	6.145f	-757	22841	N.D.	23.841 #
28)	L6 AR-1254-3	7.758f	0.000	18499	0	12.985	N.D. #
32)	L7 AR-1260-2	8.193f	7.015f	58592	15505	42.869	13.094 #
33)	L7 AR-1260-3	0.000	7.189	0	15569	N.D.	13.178 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101921\
Data File : PP040242.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2021 23:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:12:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

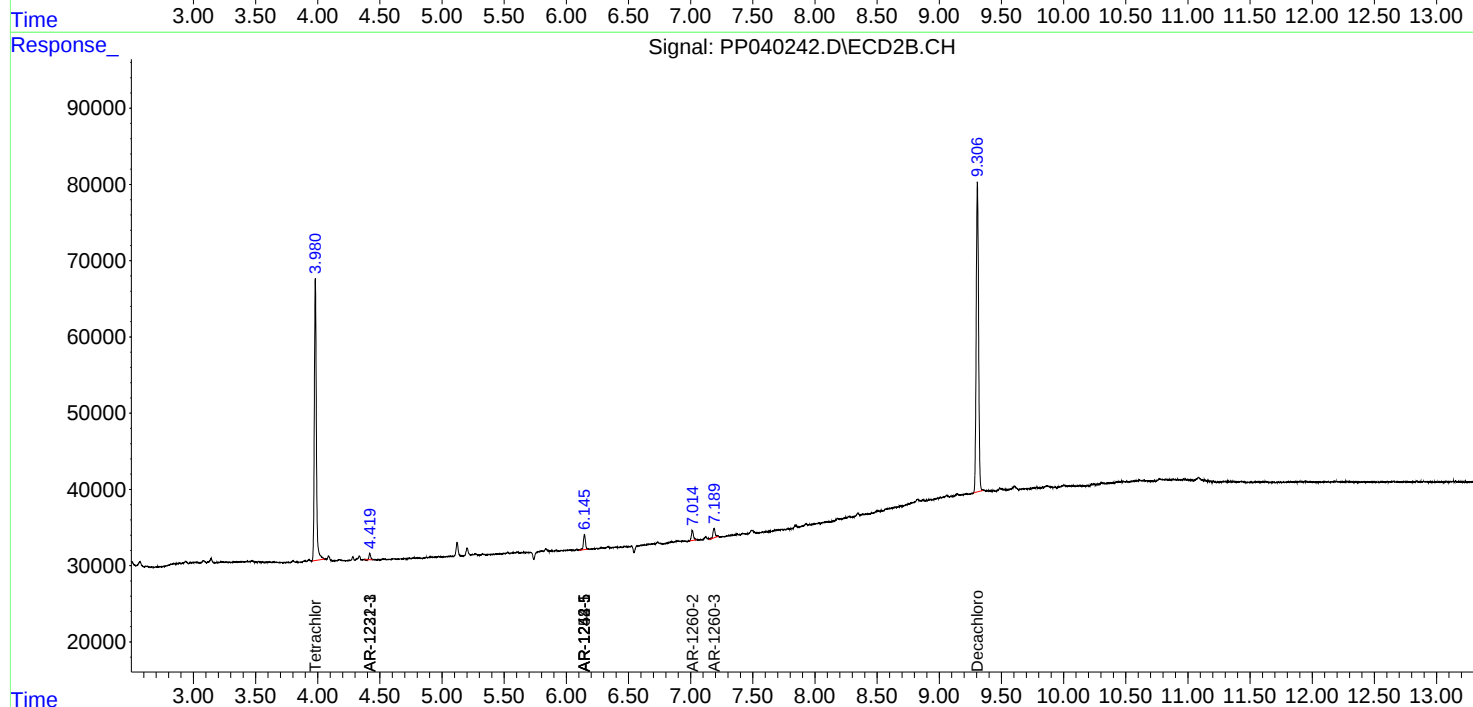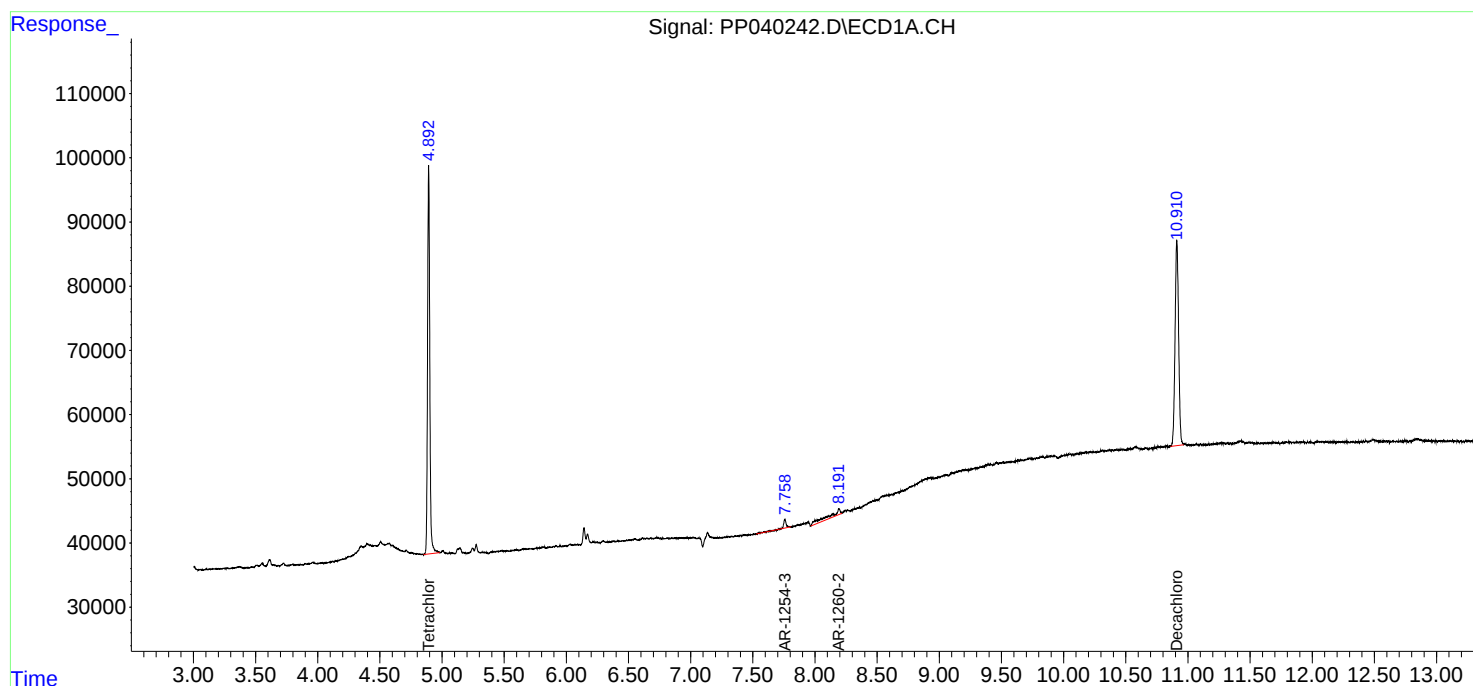


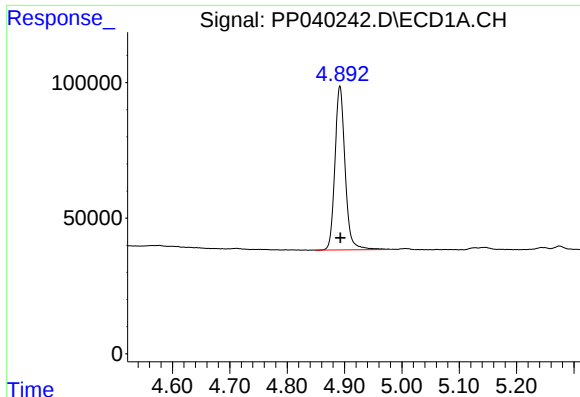

#1 Tetrachloro-m-xylene


R.T.: 4.892 min
Delta R.T.: 0.000 min
Response: 747651
Conc: 24.62 ng/ml

Instrument :
ECD_P
ClientSampleId :

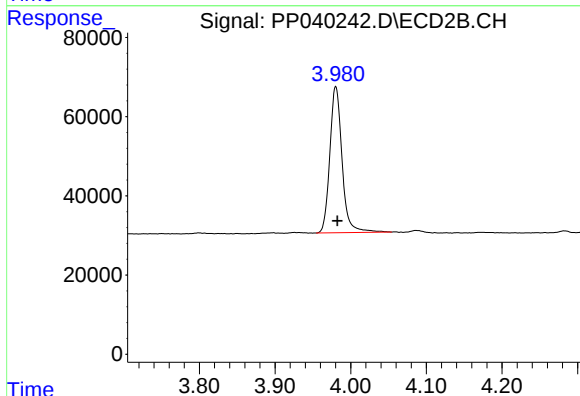


#1 Tetrachloro-m-xylene

R.T.: 3.980 min
Delta R.T.: -0.002 min
Response: 416110
Conc: 24.61 ng/ml

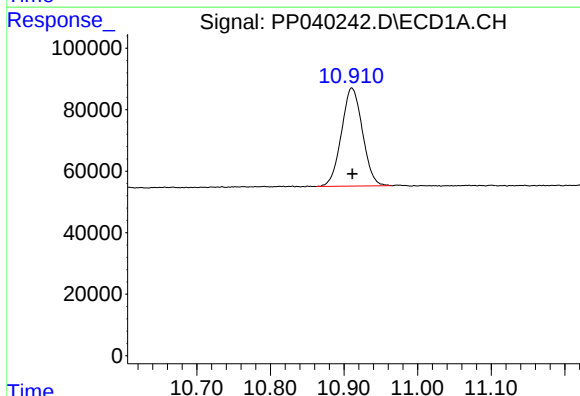


#2 Decachlorobiphenyl

R.T.: 10.911 min
Delta R.T.: 0.000 min
Response: 633627
Conc: 25.64 ng/ml

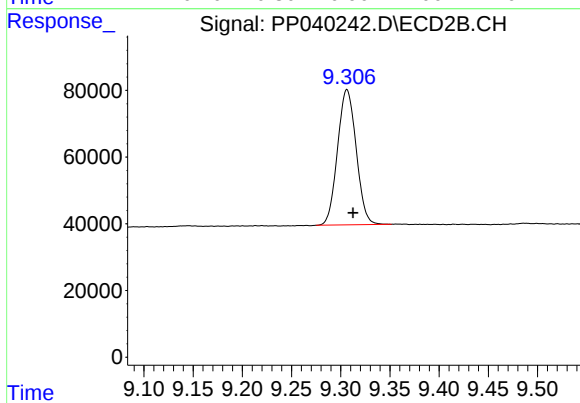

#2 Decachlorobiphenyl


R.T.: 9.306 min
Delta R.T.: -0.006 min
Response: 535668
Conc: 25.24 ng/ml

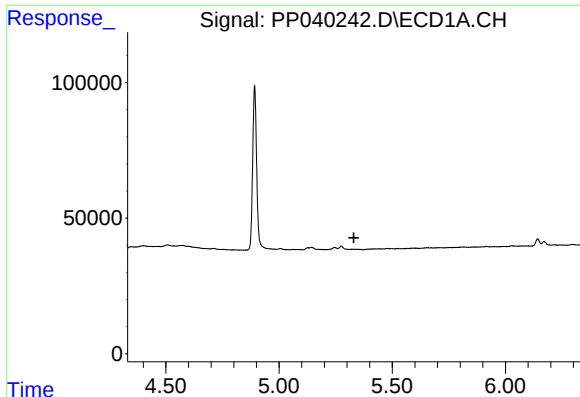

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

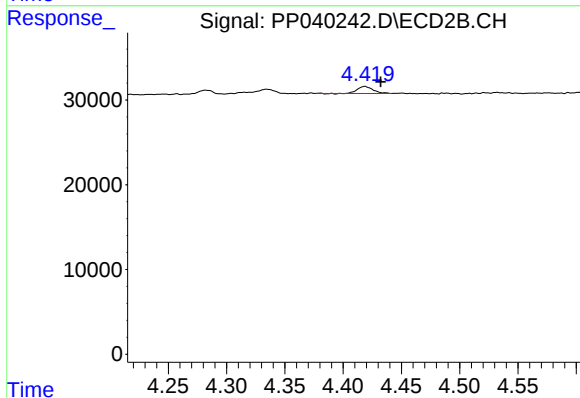


#10 AR-1221-3

R.T.: 4.419 min
Delta R.T.: -0.013 min
Response: 7626
Conc: 14.08 ng/ml

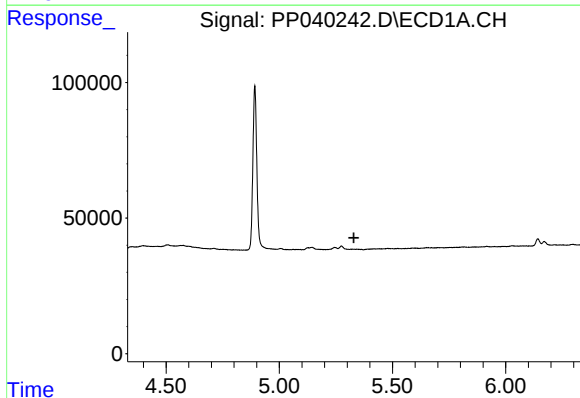


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.330 min
Response: 0
Conc: N.D.

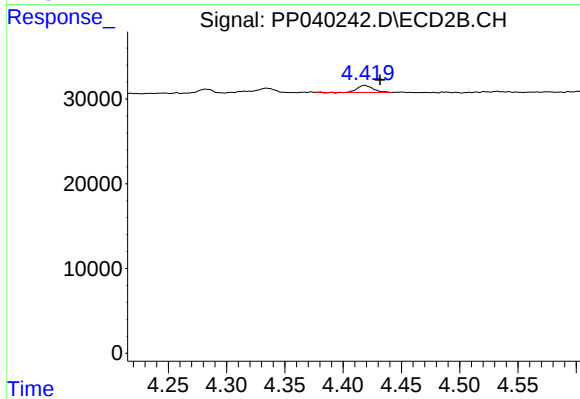

#11 AR-1232-1


R.T.: 4.419 min
Delta R.T.: -0.013 min
Response: 7626
Conc: 18.78 ng/ml

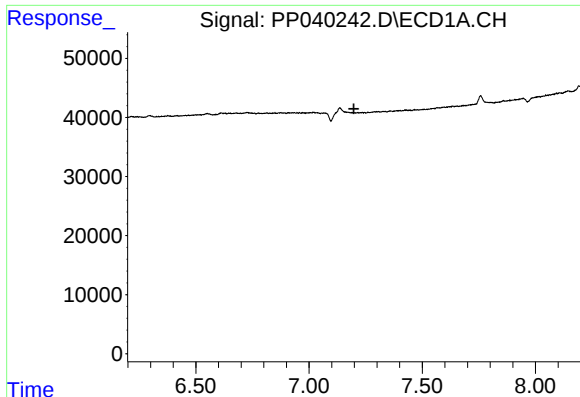

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

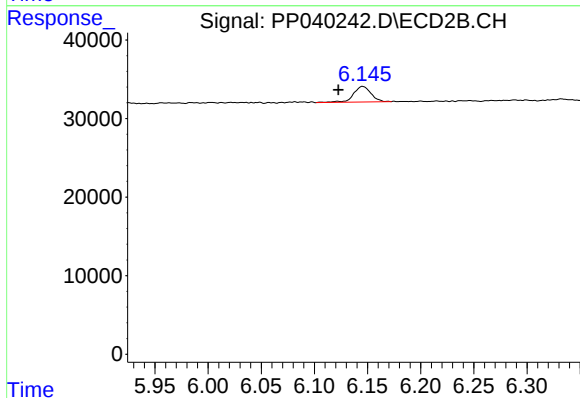


#20 AR-1242-5

R.T.: 6.145 min
Delta R.T.: 0.023 min
Response: 22841
Conc: 47.89 ng/ml

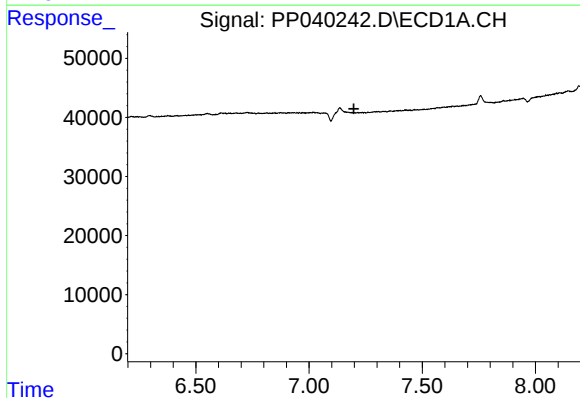


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

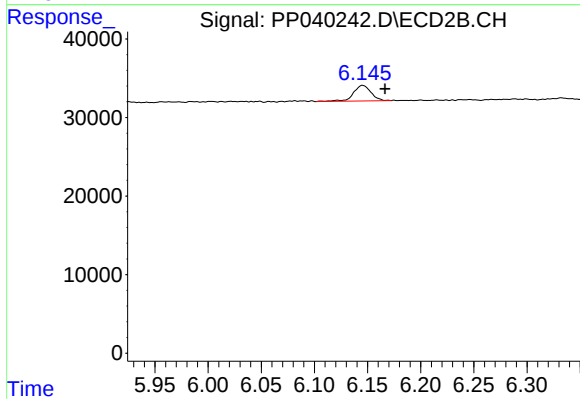

#25 AR-1248-5


R.T.: 6.145 min
Delta R.T.: -0.021 min
Response: 22841
Conc: 36.61 ng/ml

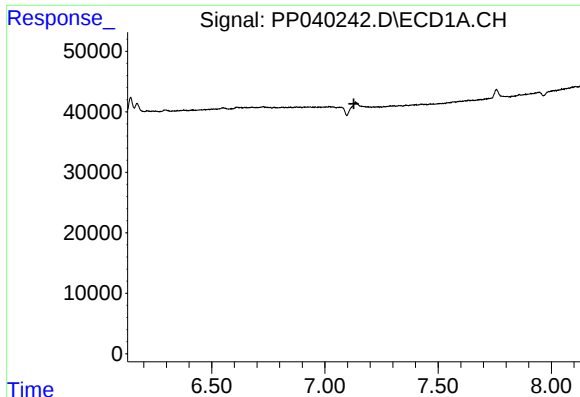

#26 AR-1254-1


R.T.: 7.136 min
Delta R.T.: 0.008 min
Response: -757
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

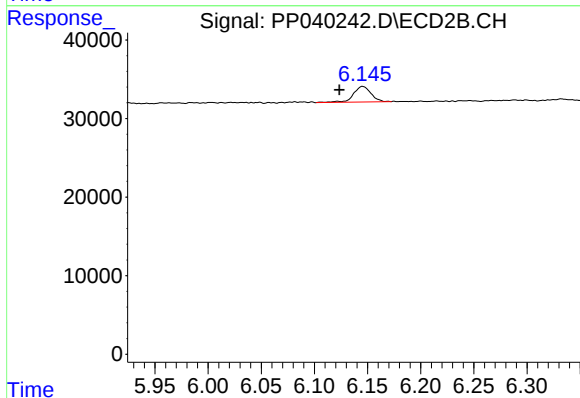


#26 AR-1254-1

R.T.: 6.145 min
Delta R.T.: 0.022 min
Response: 22841
Conc: 23.84 ng/ml

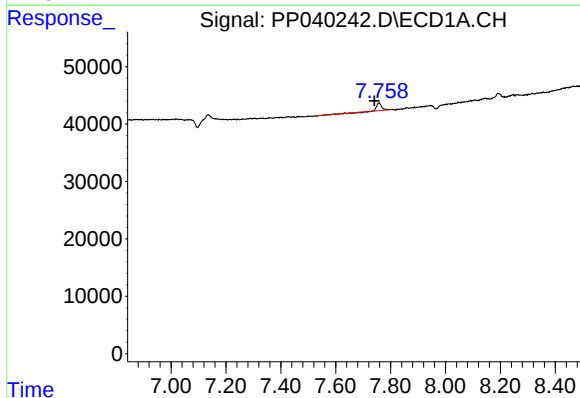


#28 AR-1254-3

R.T.: 7.758 min
Delta R.T.: 0.017 min
Response: 18499
Conc: 12.99 ng/ml

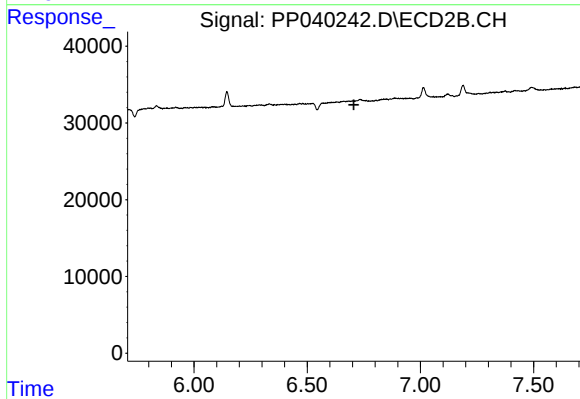

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

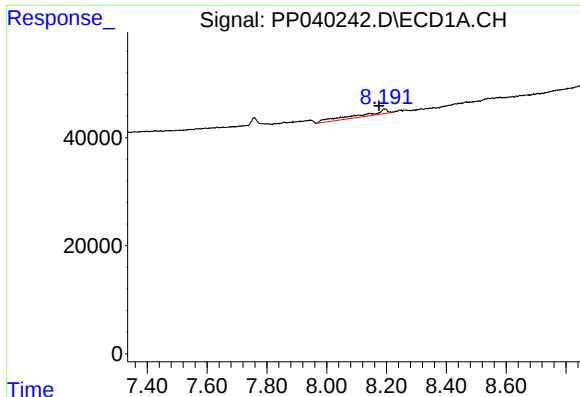

#32 AR-1260-2


R.T.: 8.193 min
Delta R.T.: 0.018 min
Response: 58592
Conc: 42.87 ng/ml

Instrument :
ECD_P
ClientSampleId :

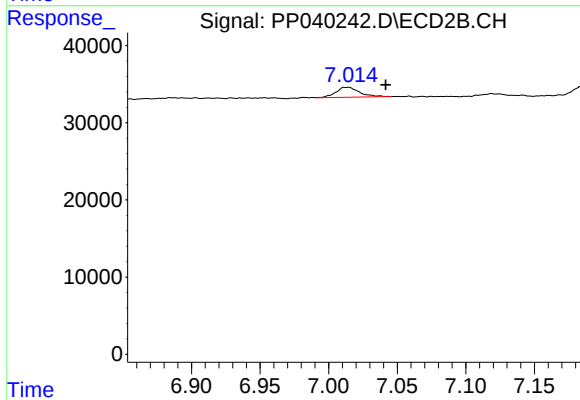


#32 AR-1260-2

R.T.: 7.015 min
Delta R.T.: -0.027 min
Response: 15505
Conc: 13.09 ng/ml

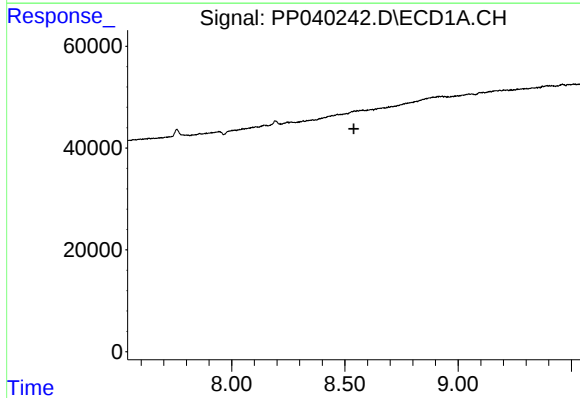

#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

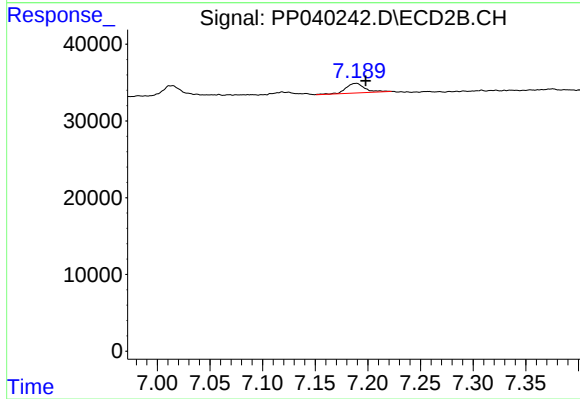

#33 AR-1260-3

R.T.: 7.189 min
Delta R.T.: -0.009 min
Response: 15569
Conc: 13.18 ng/ml