

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101921\
 Data File : PP040218.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2021 15:34
 Operator : AJ\MA
 Sample : M4269-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RT-2664

Manual Integrations
 APPROVED

mohammad
 10/20/2021 1:31:36 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:56:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.892	3.982	451872	273995	14.880m	16.207
2) SA Decachlor...	10.908	9.305	593591	488839	24.016	23.034

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101921\
Data File : PP040218.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2021 15:34
Operator : AJ\MA
Sample : M4269-03
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RT-2664


Manual Integrations
APPROVED

mohammad
10/20/2021 1:31:36 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:56:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

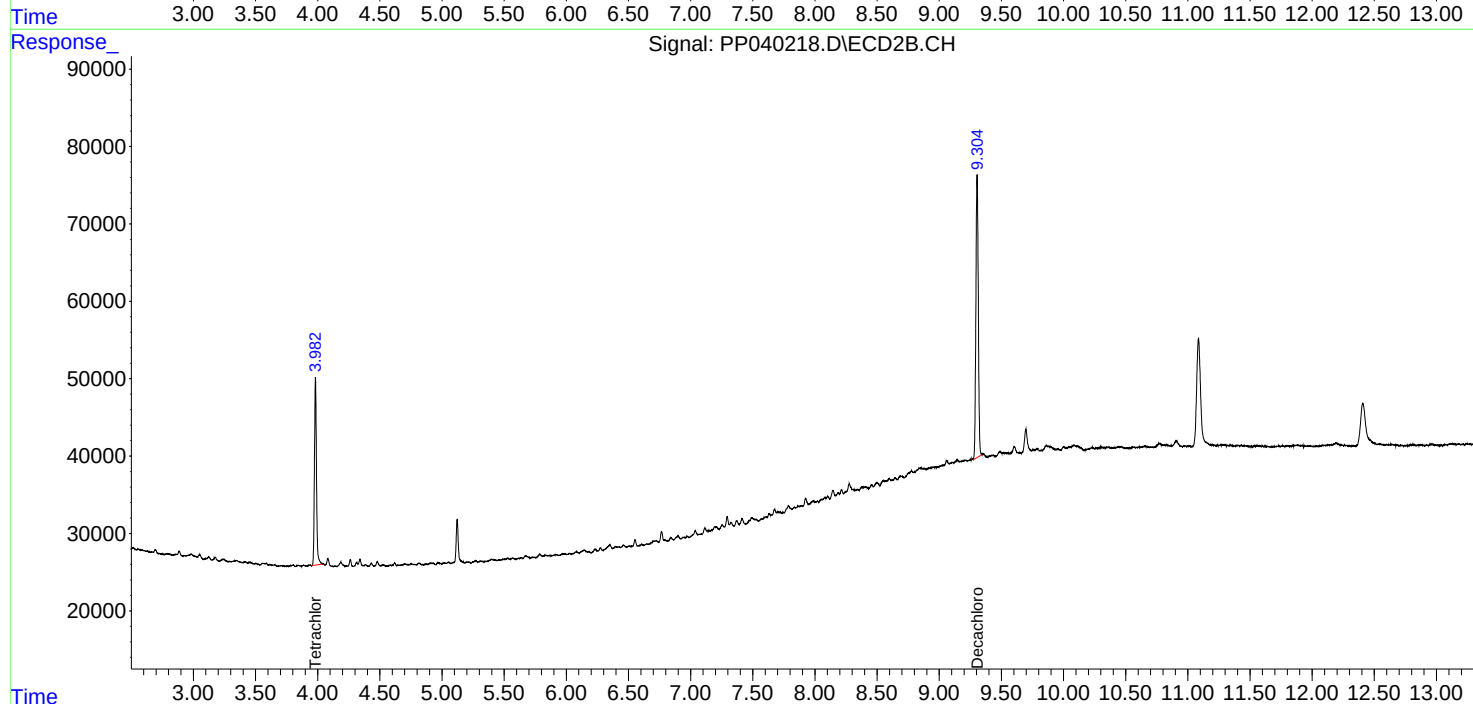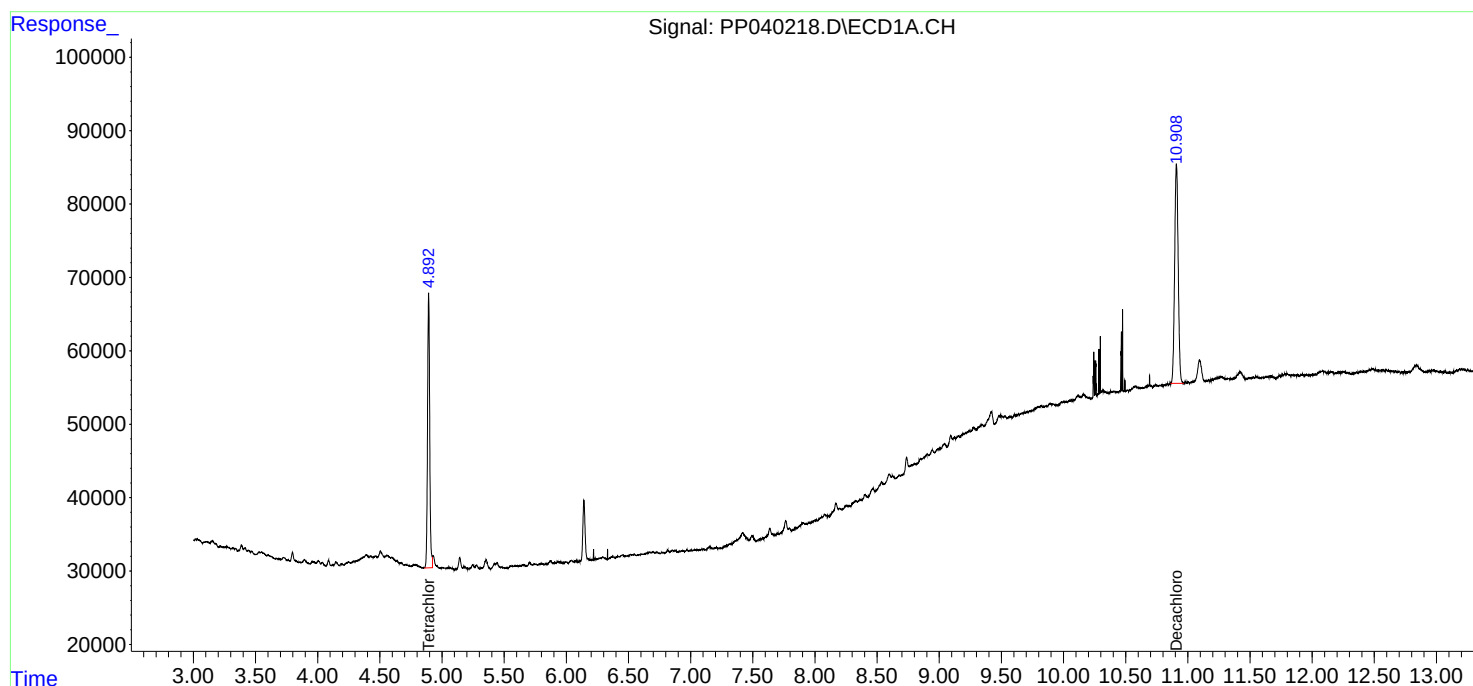

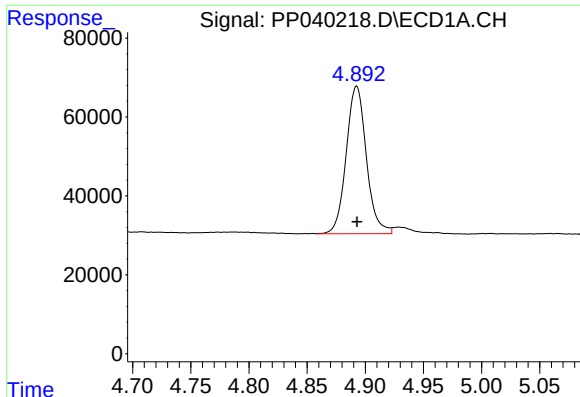


#1 Tetrachloro-m-xylene

R.T.: 4.892 min
Delta R.T.: 0.000 min
Response: 451872
Conc: 14.88 ng/ml m

Instrument :
ECD_P
ClientSampleId :
RT-2664


Manual Integrations
APPROVED

mohammad
10/20/2021 1:31:36 PM

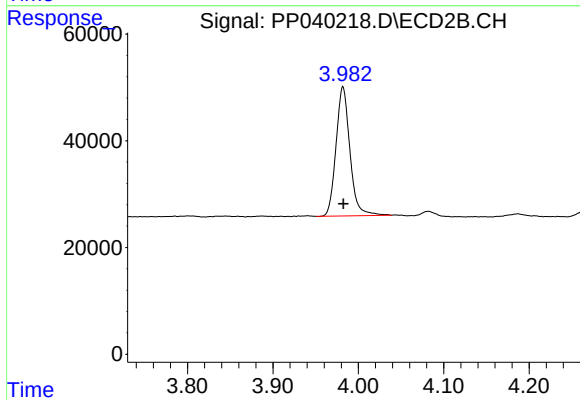


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 273995
Conc: 16.21 ng/ml

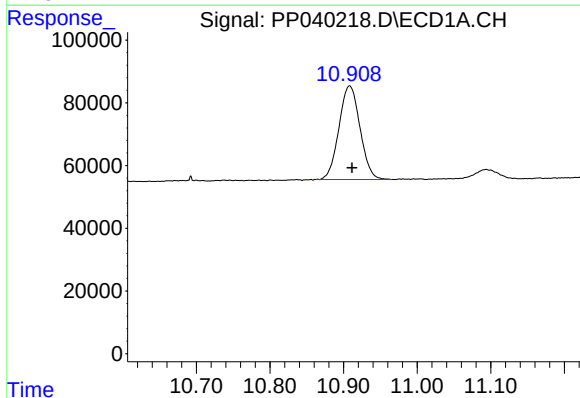

#2 Decachlorobiphenyl

R.T.: 10.908 min
Delta R.T.: -0.003 min
Response: 593591
Conc: 24.02 ng/ml

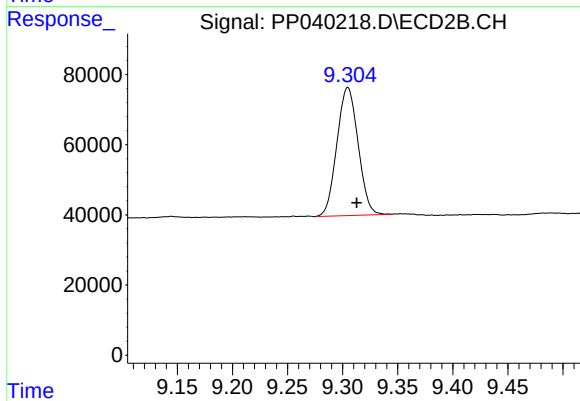

#2 Decachlorobiphenyl

R.T.: 9.305 min
Delta R.T.: -0.008 min
Response: 488839
Conc: 23.03 ng/ml