

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101921\
 Data File : PP040243.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Oct 2021 23:27
 Operator : AJ\MA
 Sample : PB140041BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB140041BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 02:13:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.891	3.979	732532	392737	24.122	23.231
2)	SA Decachlor...	10.909	9.304	599421	516831	24.252	24.353

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101921\
Data File : PP040243.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Oct 2021 23:27
Operator : AJ\MA
Sample : PB140041BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB140041BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 02:13:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

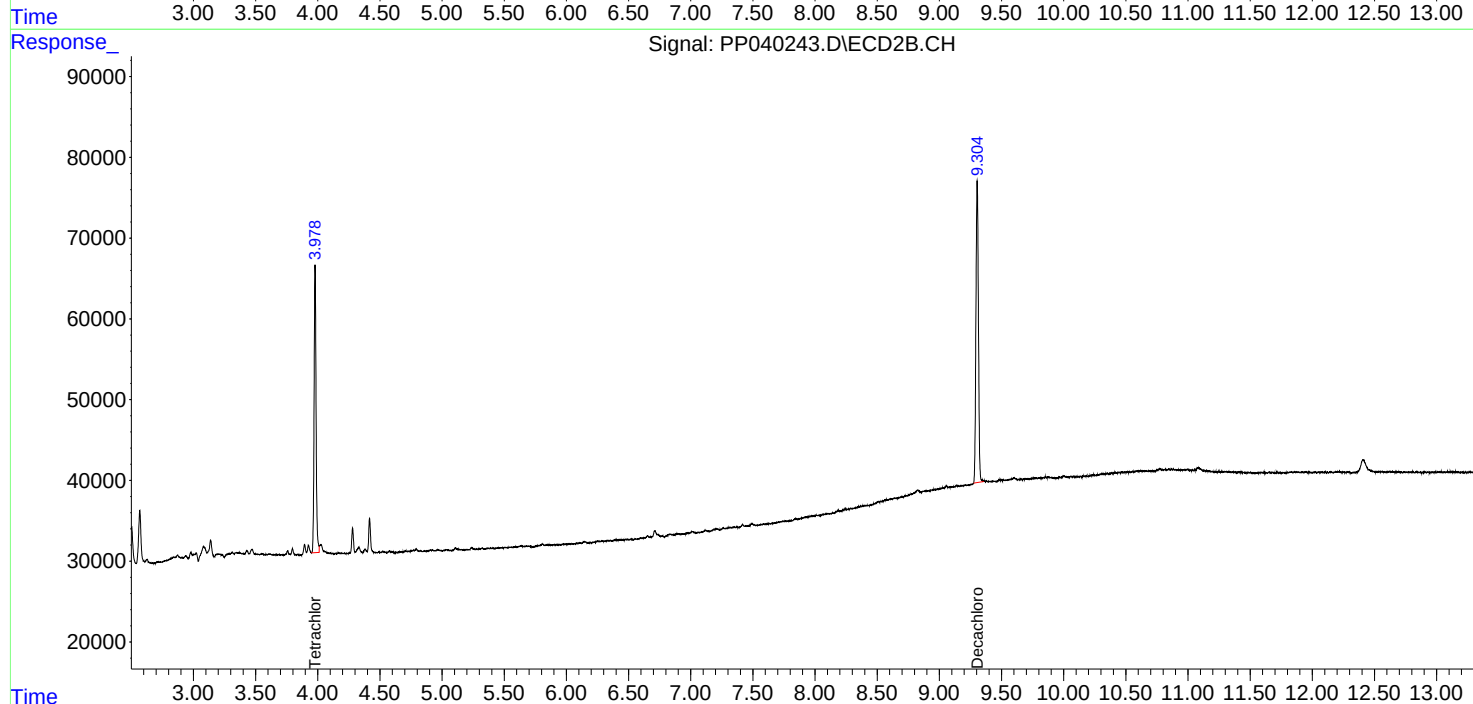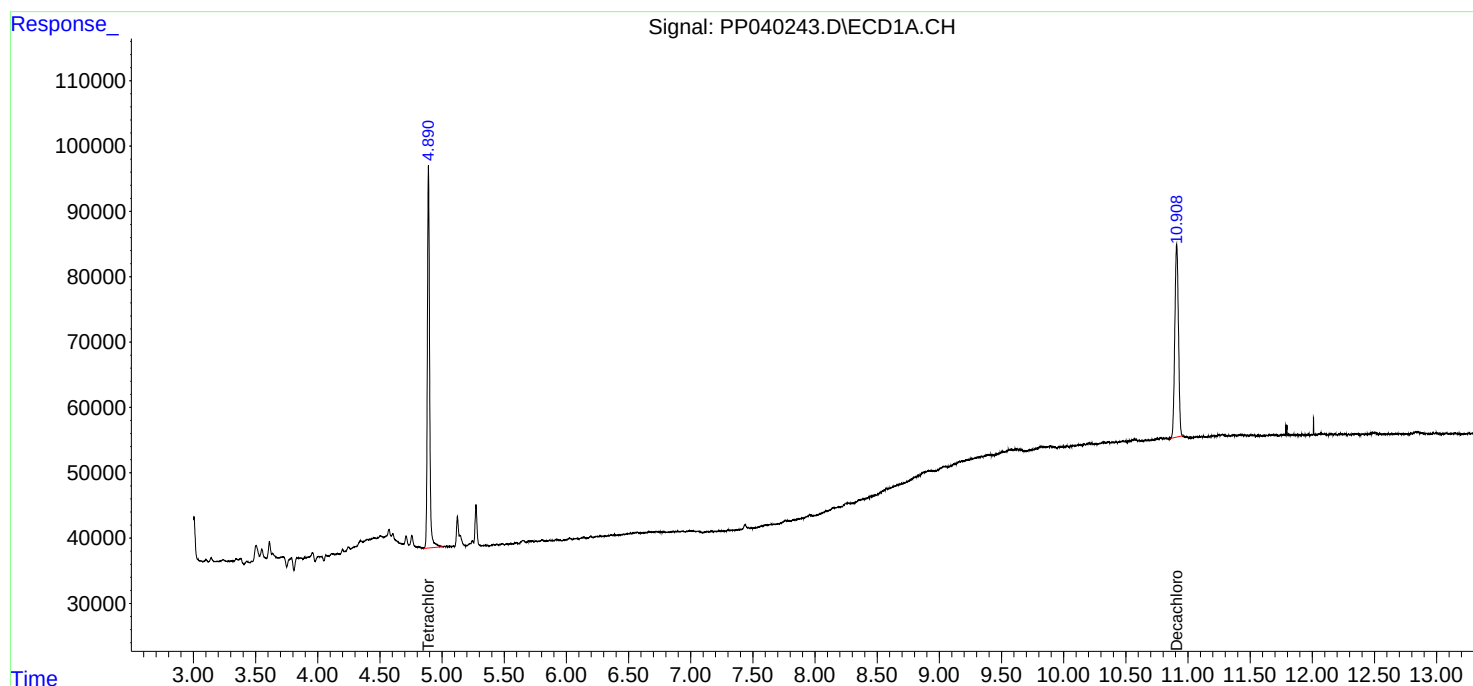


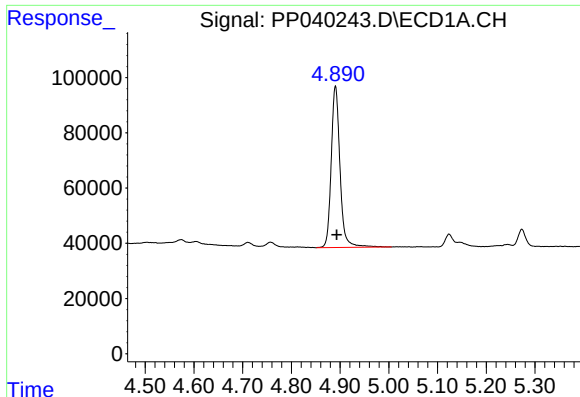

#1 Tetrachloro-m-xylene


R.T.: 4.891 min
Delta R.T.: -0.002 min
Response: 732532
Conc: 24.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB140041BL

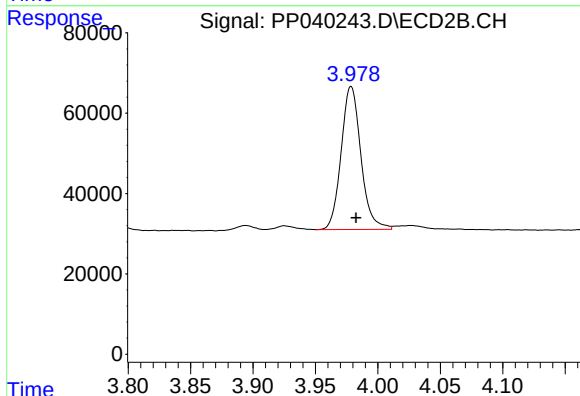


#1 Tetrachloro-m-xylene

R.T.: 3.979 min
Delta R.T.: -0.004 min
Response: 392737
Conc: 23.23 ng/ml

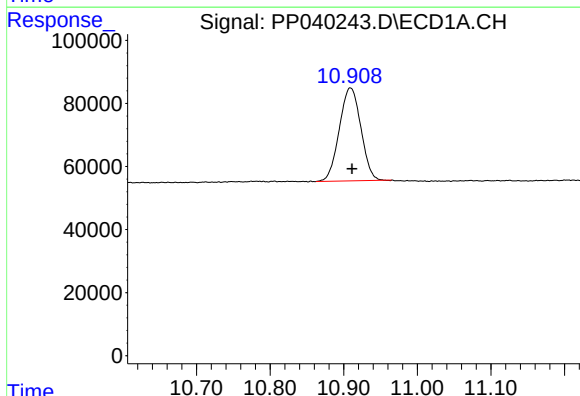

#2 Decachlorobiphenyl

R.T.: 10.909 min
Delta R.T.: -0.002 min
Response: 599421
Conc: 24.25 ng/ml

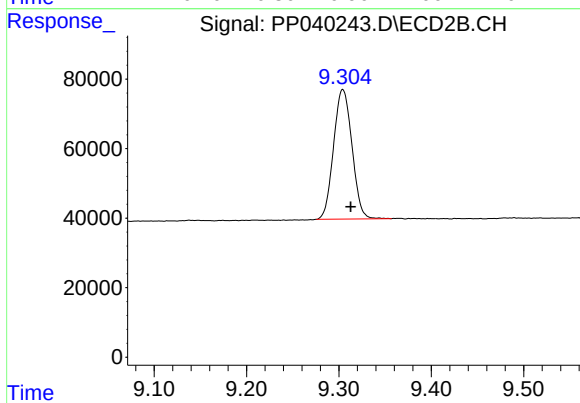

#2 Decachlorobiphenyl

R.T.: 9.304 min
Delta R.T.: -0.009 min
Response: 516831
Conc: 24.35 ng/ml