

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101922\
 Data File : PP052465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2022 11:07
 Operator : YP\AJ
 Sample : N5110-01 (Sig #1); N5110-01RE (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MANSFIELD-OILY-Water

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/20/2022
 Supervised By :Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 12:49:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 12 05:20:17 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.672	14012353	8689944	8.915m	7.585
2) SA Decachlor...	10.240	8.764	9591793	7432744	6.911	6.652

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101922\
Data File : PP052465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2022 11:07
Operator : YP\AJ
Sample : N5110-01 (Sig #1); N5110-01RE (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MANSFIELD-OILY-Water


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/20/2022
Supervised By :Ankita Jodhani 10/20/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 12:49:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101122.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 12 05:20:17 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

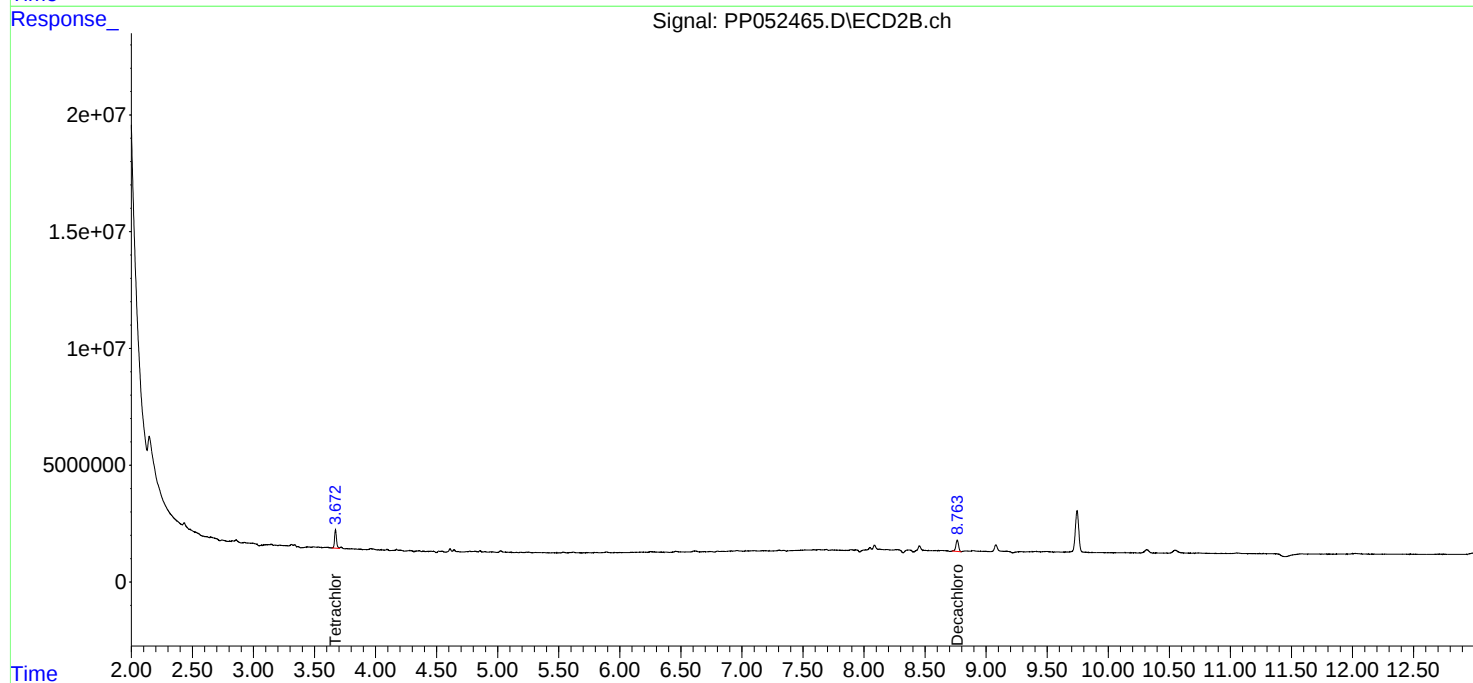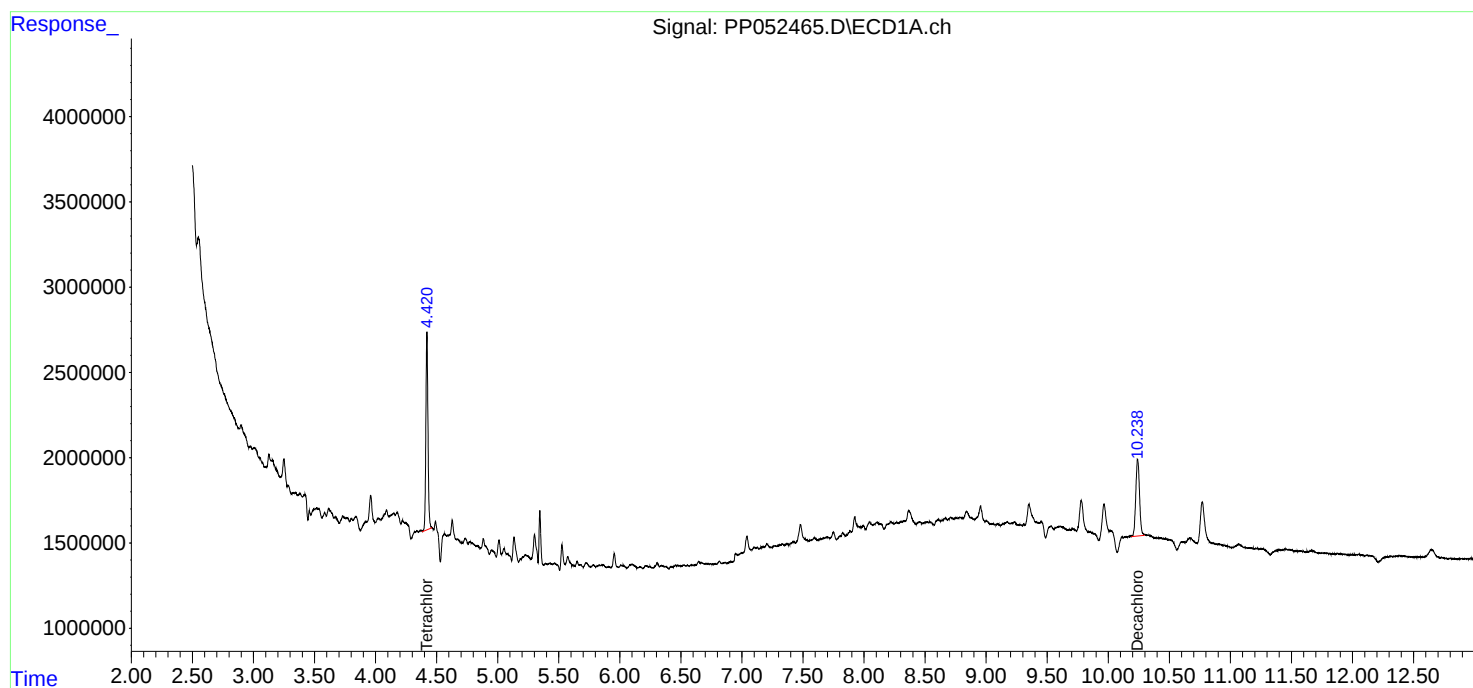

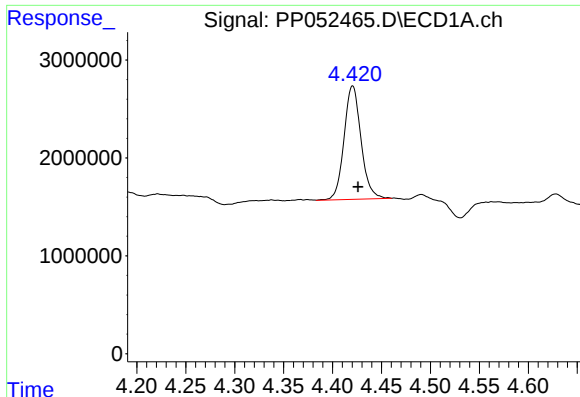


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.006 min
Response: 14012353
Conc: 8.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MANSFIELD-OILY-Water


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/20/2022
Supervised By :Ankita Jodhani 10/20/2022

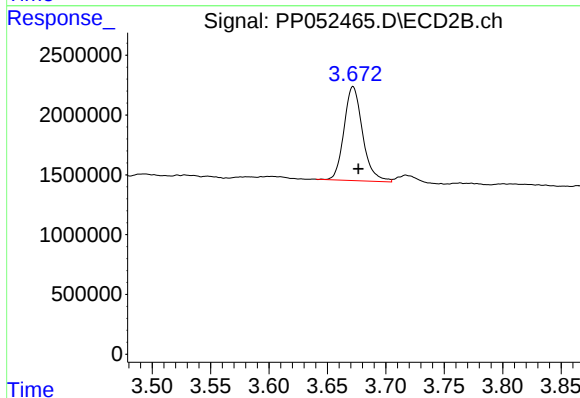


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.005 min
Response: 8689944
Conc: 7.59 ng/ml

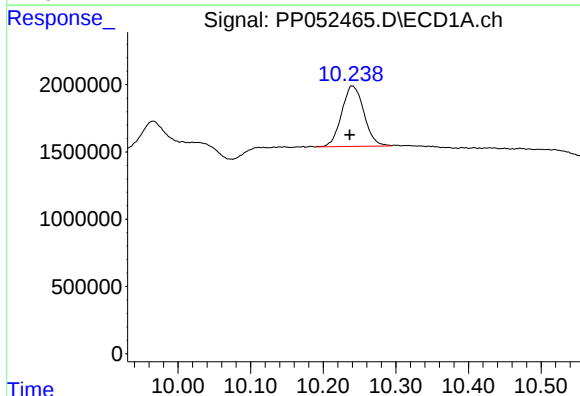

#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: 0.003 min
Response: 9591793
Conc: 6.91 ng/ml

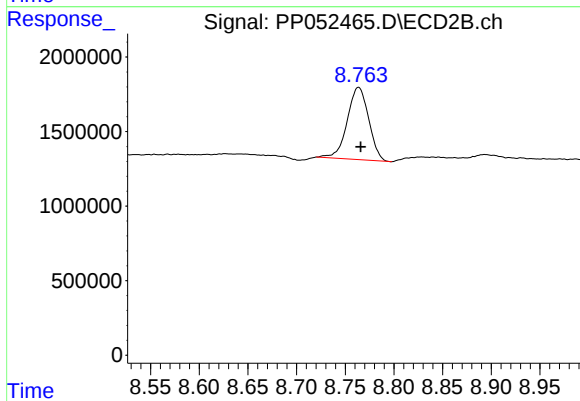

#2 Decachlorobiphenyl

R.T.: 8.764 min
Delta R.T.: -0.002 min
Response: 7432744
Conc: 6.65 ng/ml