

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101923\
 Data File : PP061101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 13:29
 Operator : YP\AJ
 Sample : 04843-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/20/2023
 Supervised By :Ankita Jodhani 10/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 19 19:03:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.556	3.695	33389044	18533649	15.188	13.708m
2) SA Decachlor...	10.513	8.757	33377888	24401060	21.314	16.229

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101923\
Data File : PP061101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 13:29
Operator : YP\AJ
Sample : 04843-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/20/2023
Supervised By :Ankita Jodhani 10/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 19 19:03:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

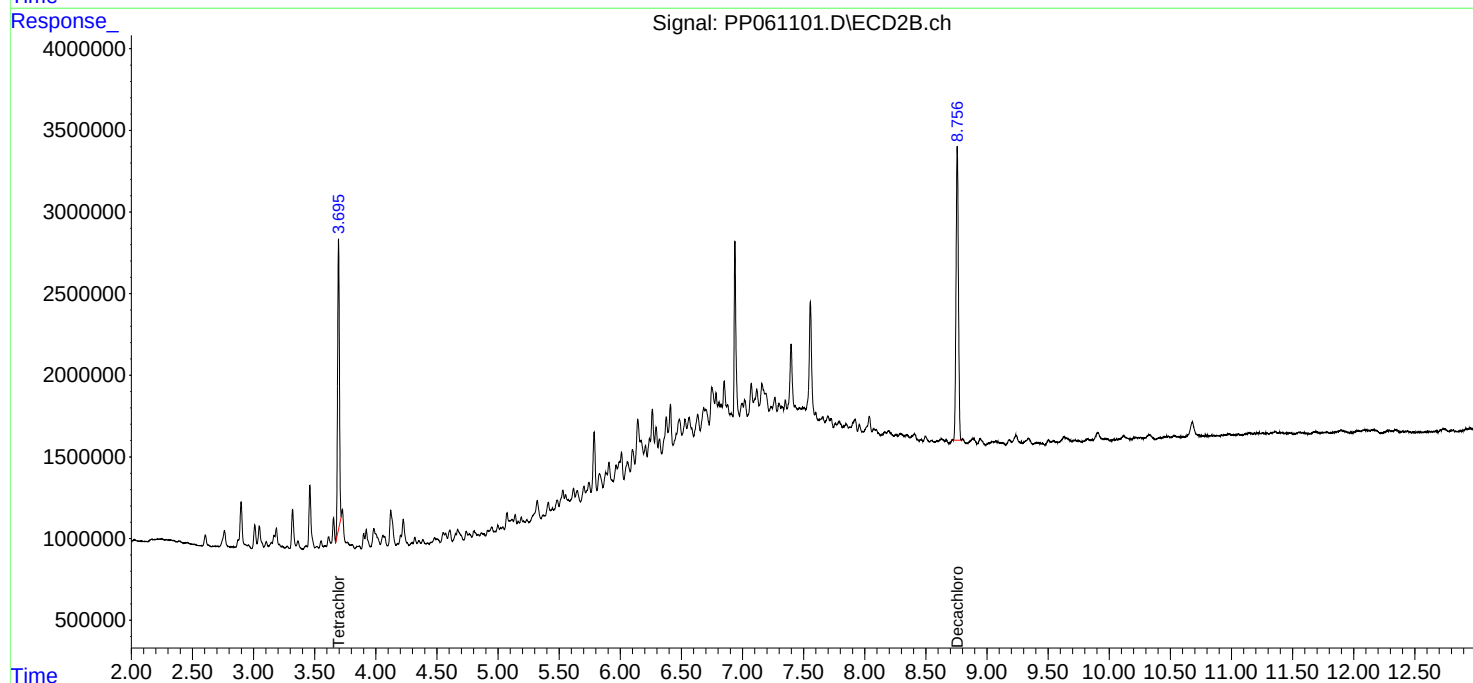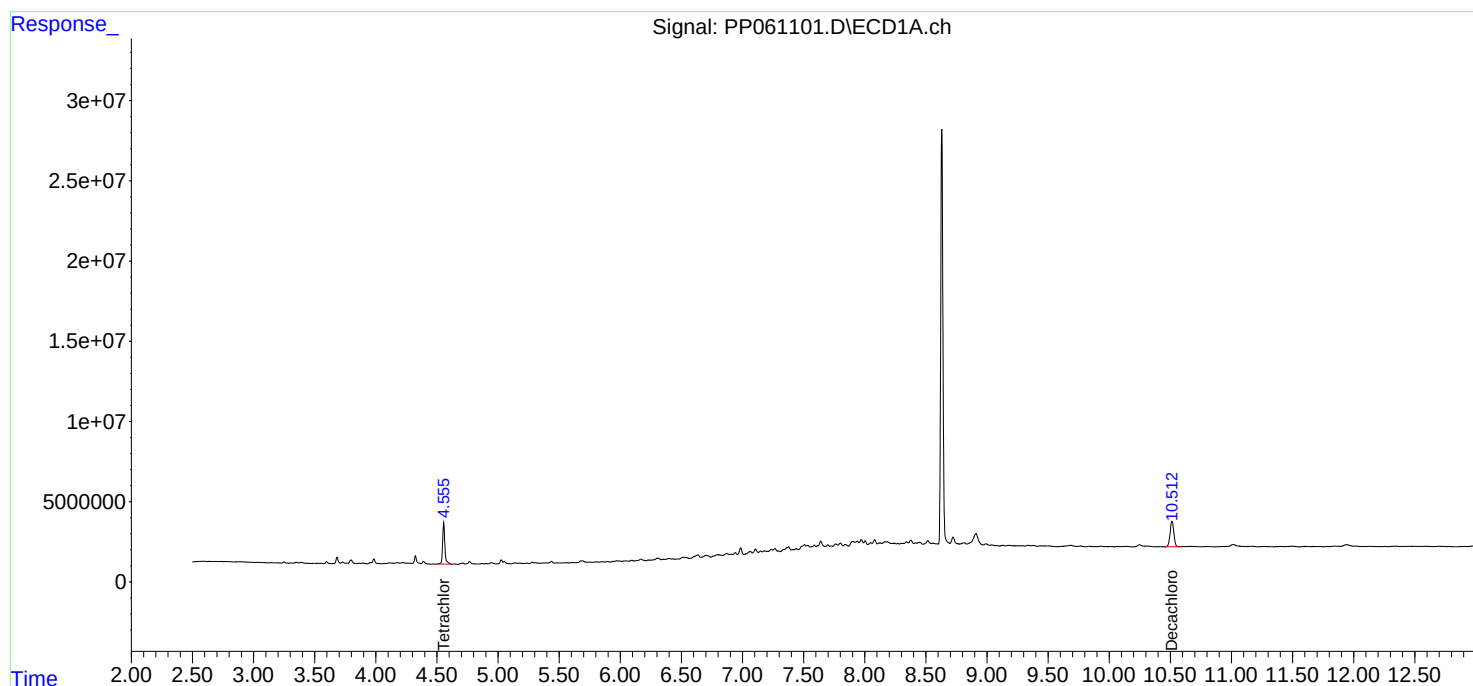

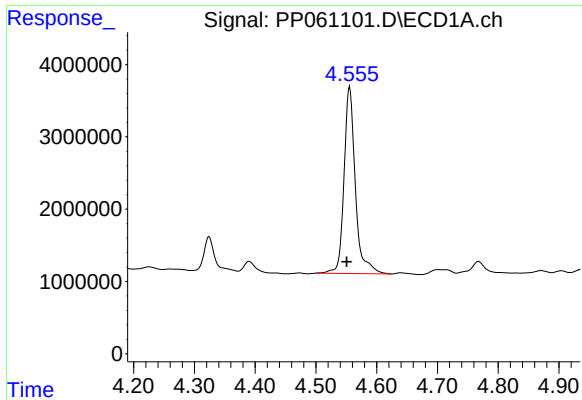


#1 Tetrachloro-m-xylene

R.T.: 4.556 min
Delta R.T.: 0.005 min
Response: 33389044
Conc: 15.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/20/2023
Supervised By :Ankita Jodhani 10/20/2023

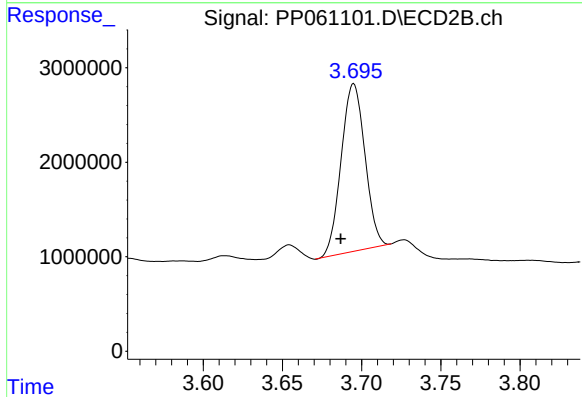


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.008 min
Response: 18533649
Conc: 13.71 ng/ml m

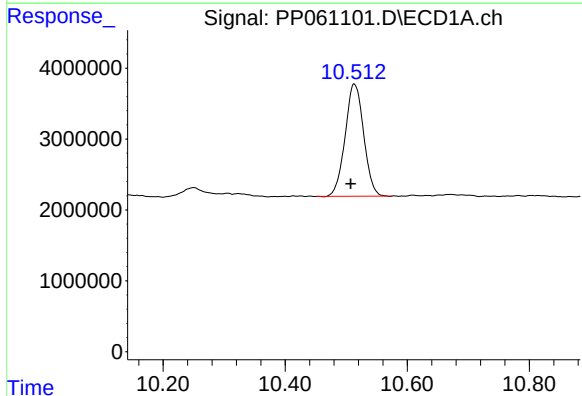

#2 Decachlorobiphenyl

R.T.: 10.513 min
Delta R.T.: 0.006 min
Response: 33377888
Conc: 21.31 ng/ml

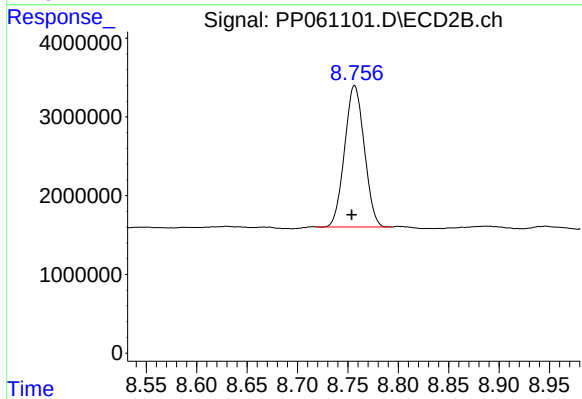

#2 Decachlorobiphenyl

R.T.: 8.757 min
Delta R.T.: 0.003 min
Response: 24401060
Conc: 16.23 ng/ml