

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101923\
 Data File : PP061116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Oct 2023 18:12
 Operator : YP\AJ
 Sample : 04945-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PAT-2-101823

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/20/2023
 Supervised By :Ankita Jodhani 10/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 01:06:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.555	3.692	54469574	35449549	24.778	26.220m
2) SA Decachlor...	10.516	8.760	39851337	32169825	25.448	21.396

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP101923\
Data File : PP061116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Oct 2023 18:12
Operator : YP\AJ
Sample : 04945-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PAT-2-101823


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/20/2023
Supervised By :Ankita Jodhani 10/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 01:06:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

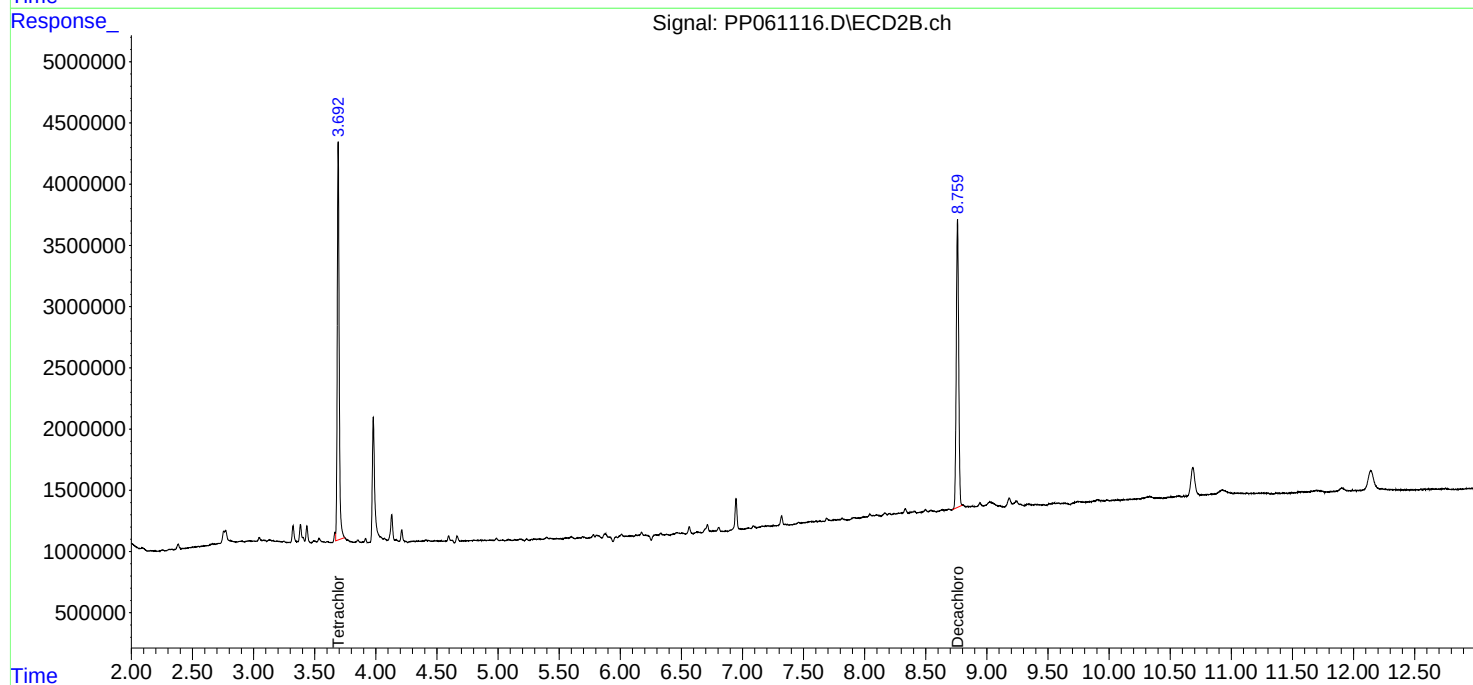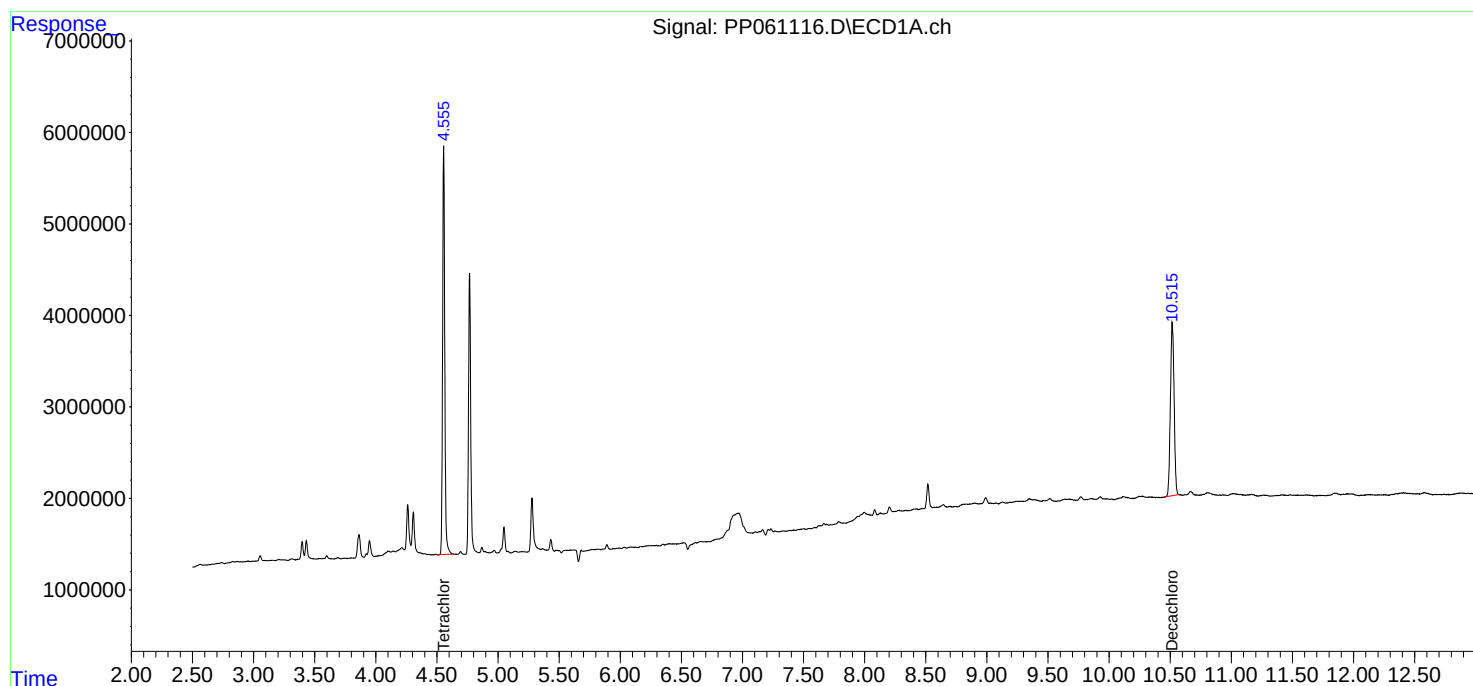

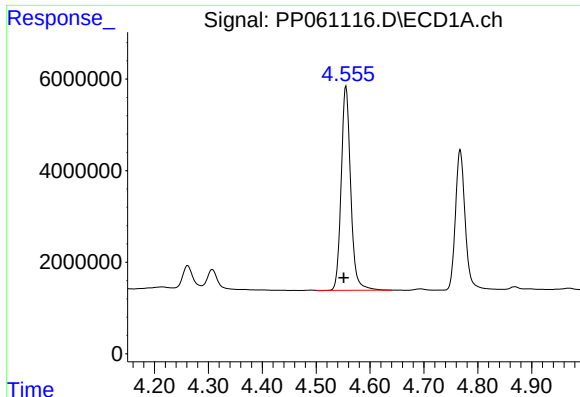

#1 Tetrachloro-m-xylene

R.T.: 4.555 min
Delta R.T.: 0.004 min
Response: 54469574
Conc: 24.78 ng/ml

Instrument :

ECD_P


ClientSampleId :

PAT-2-101823

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/20/2023
Supervised By :Ankita Jodhani 10/20/2023

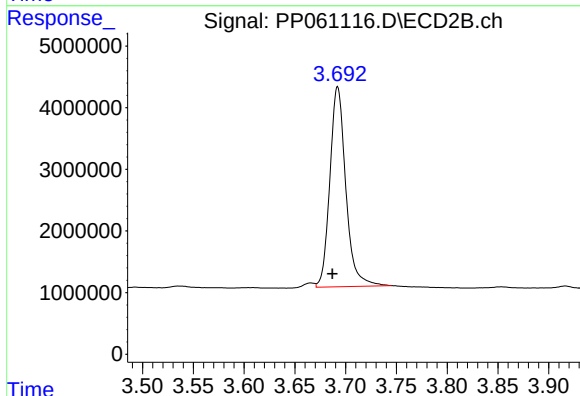


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: 0.005 min
Response: 35449549
Conc: 26.22 ng/ml m

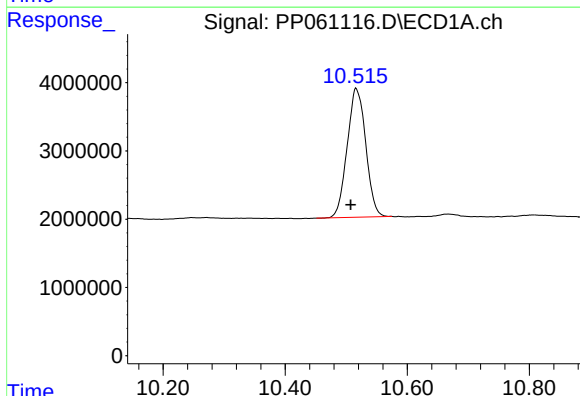

#2 Decachlorobiphenyl

R.T.: 10.516 min
Delta R.T.: 0.009 min
Response: 39851337
Conc: 25.45 ng/ml

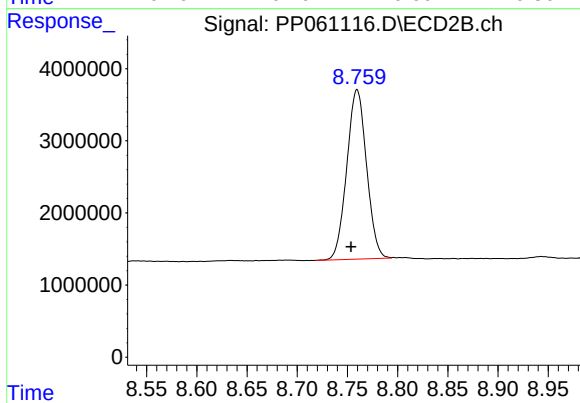

#2 Decachlorobiphenyl

R.T.: 8.760 min
Delta R.T.: 0.006 min
Response: 32169825
Conc: 21.40 ng/ml