

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102021\
 Data File : PP040272.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2021 19:23
 Operator : AJ\MA
 Sample : M4284-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 20878-SOLID

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 02:10:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.891	3.978	548552	312203	18.063	18.467
2) SA Decachlor...	10.907	9.303	231544	206927	9.368	9.750

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102021\
Data File : PP040272.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2021 19:23
Operator : AJ\MA
Sample : M4284-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
20878-SOLID

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 02:10:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

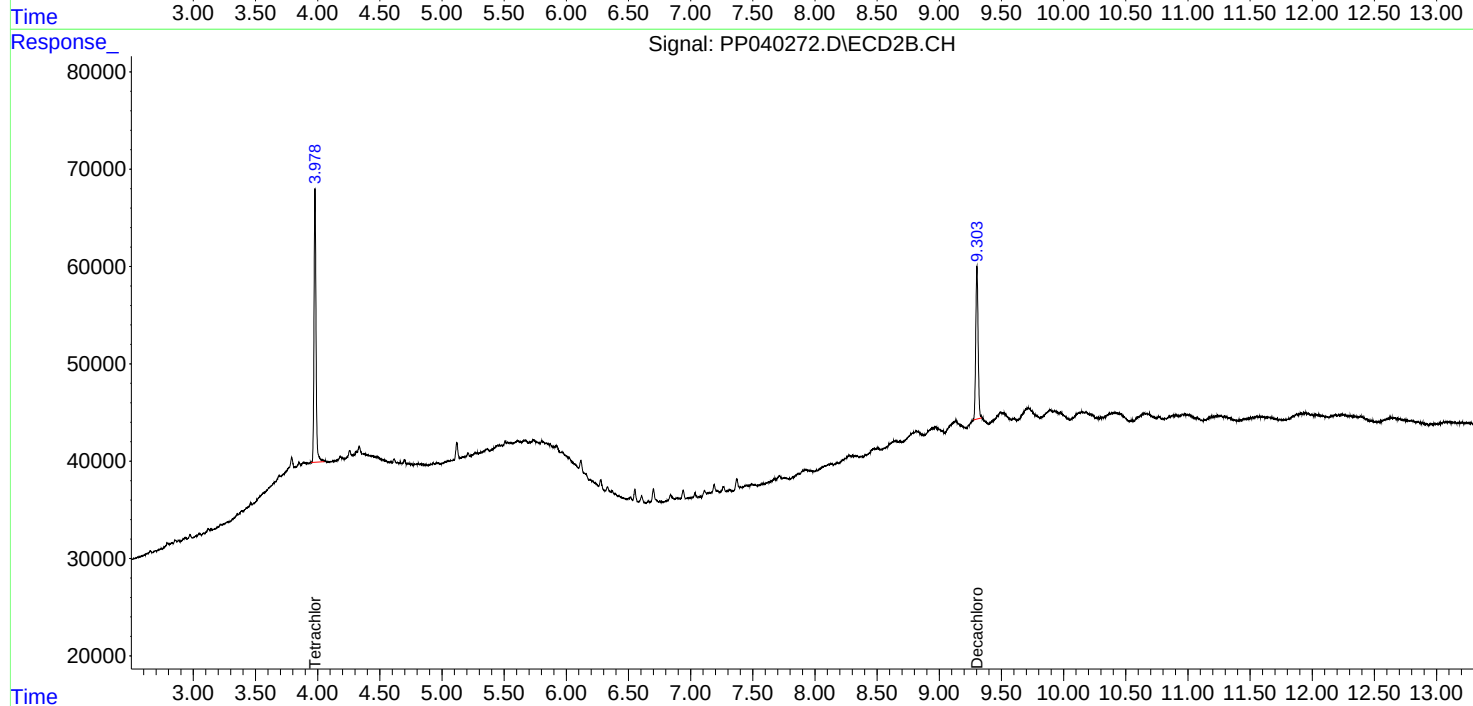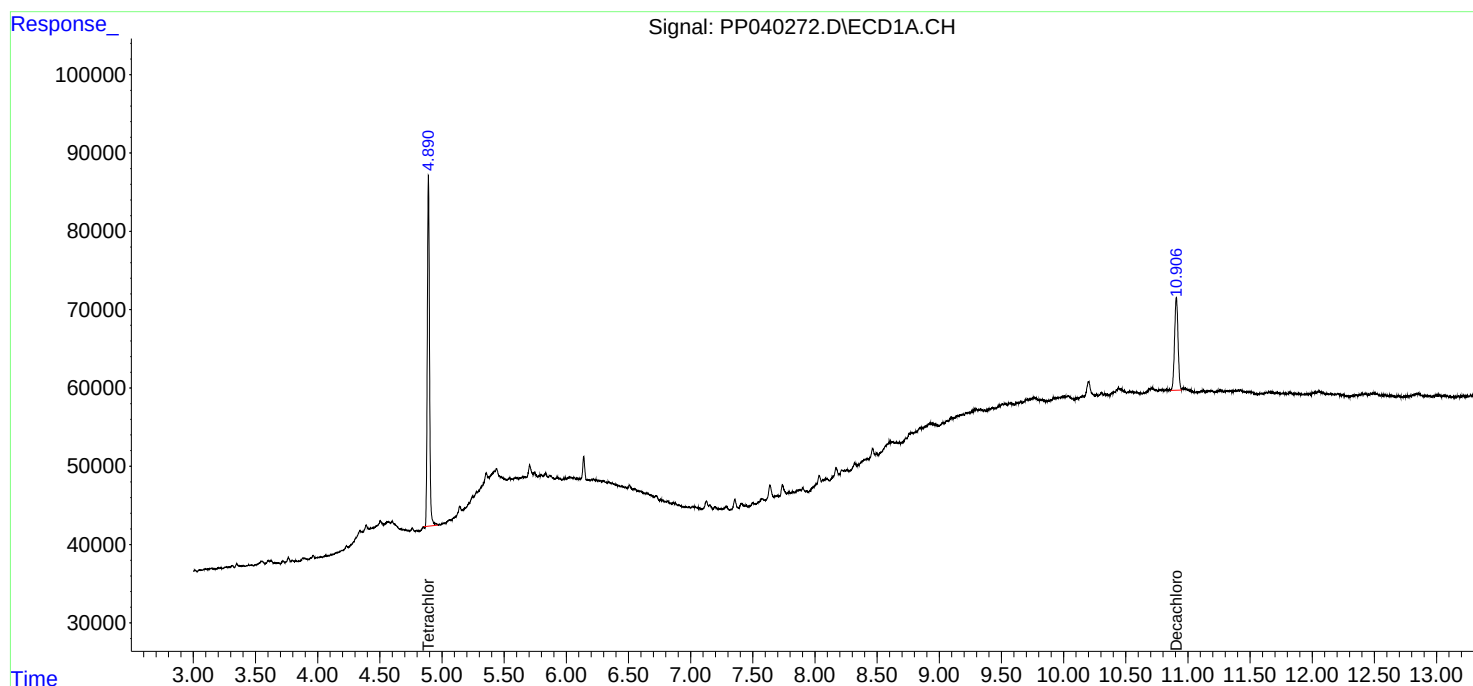


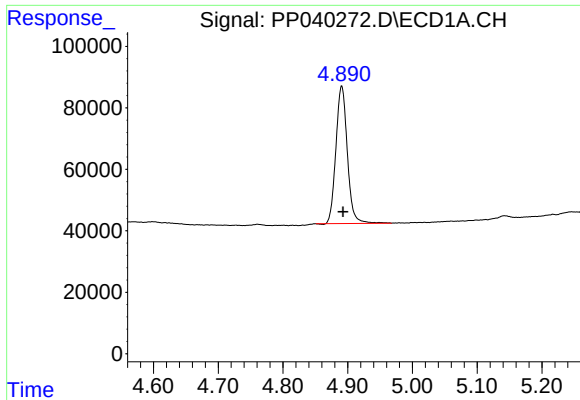

#1 Tetrachloro-m-xylene


R.T.: 4.891 min
Delta R.T.: -0.002 min
Response: 548552
Conc: 18.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
20878-SOLID

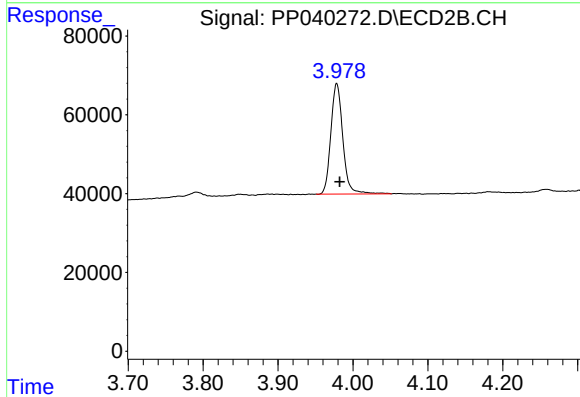


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.004 min
Response: 312203
Conc: 18.47 ng/ml

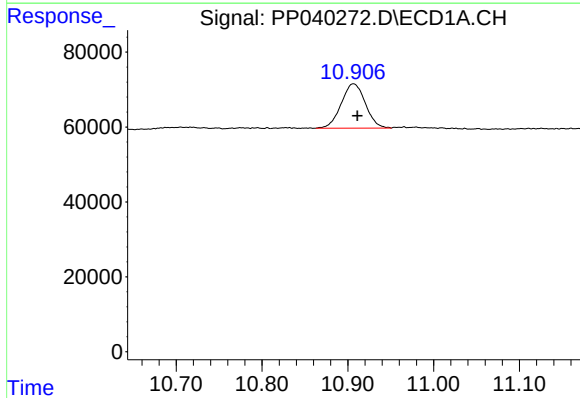

#2 Decachlorobiphenyl

R.T.: 10.907 min
Delta R.T.: -0.005 min
Response: 231544
Conc: 9.37 ng/ml

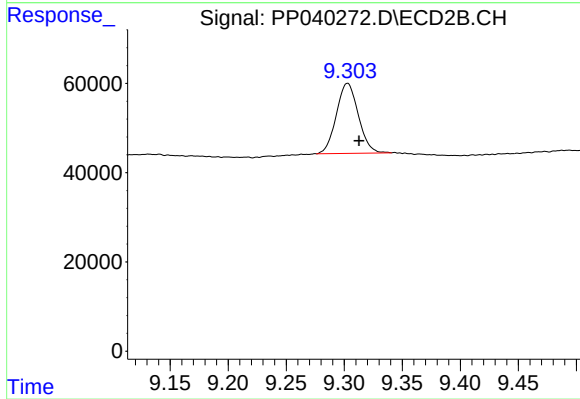

#2 Decachlorobiphenyl

R.T.: 9.303 min
Delta R.T.: -0.010 min
Response: 206927
Conc: 9.75 ng/ml