

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102021\
 Data File : PP040274.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Oct 2021 19:57
 Operator : AJ\MA
 Sample : M4284-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 16943

Manual Integrations
 APPROVED

mohammad
 10/21/2021 1:44:02 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 02:11:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.891	3.978	530261	311137	17.461	18.404m
2)	SA Decachlor...	10.910	9.307	412631	323875	16.694	15.261

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102021\
Data File : PP040274.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Oct 2021 19:57
Operator : AJ\MA
Sample : M4284-04
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
16943


Manual Integrations
APPROVED

mohammad
10/21/2021 1:44:02 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 02:11:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

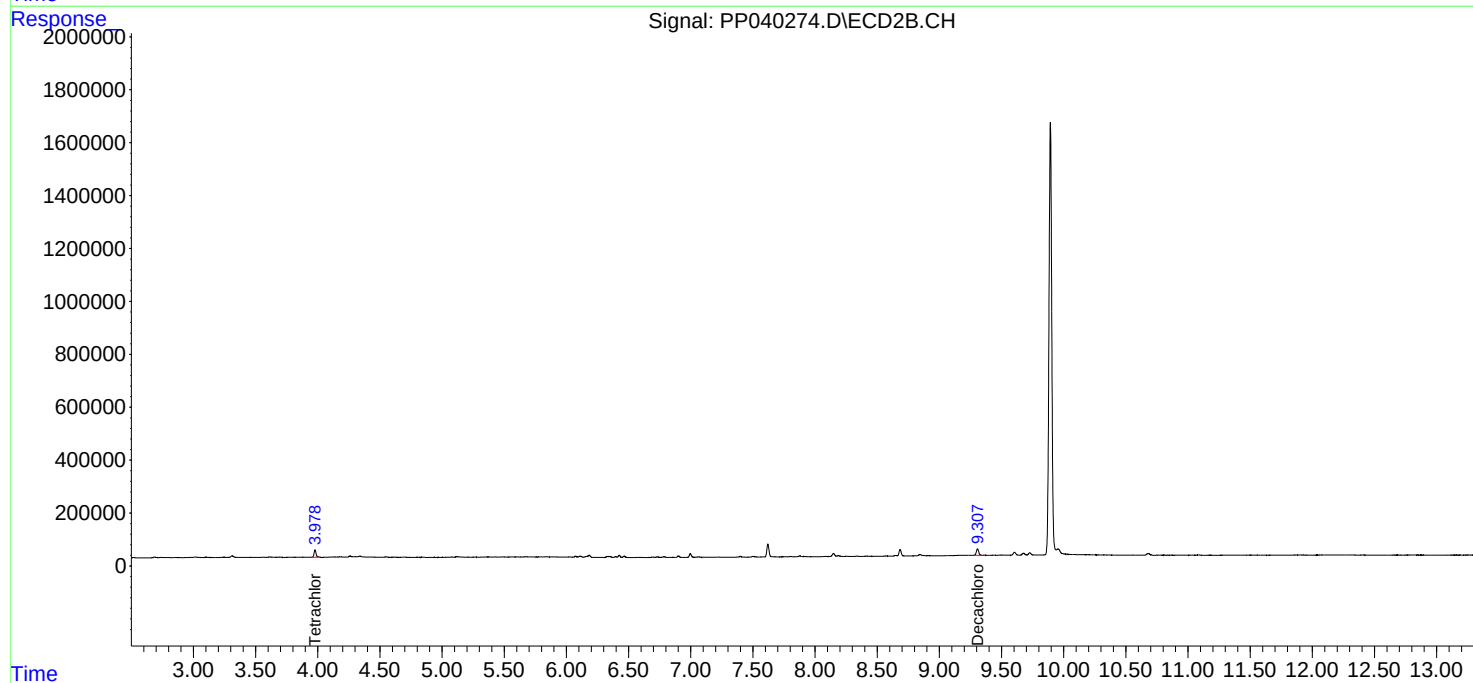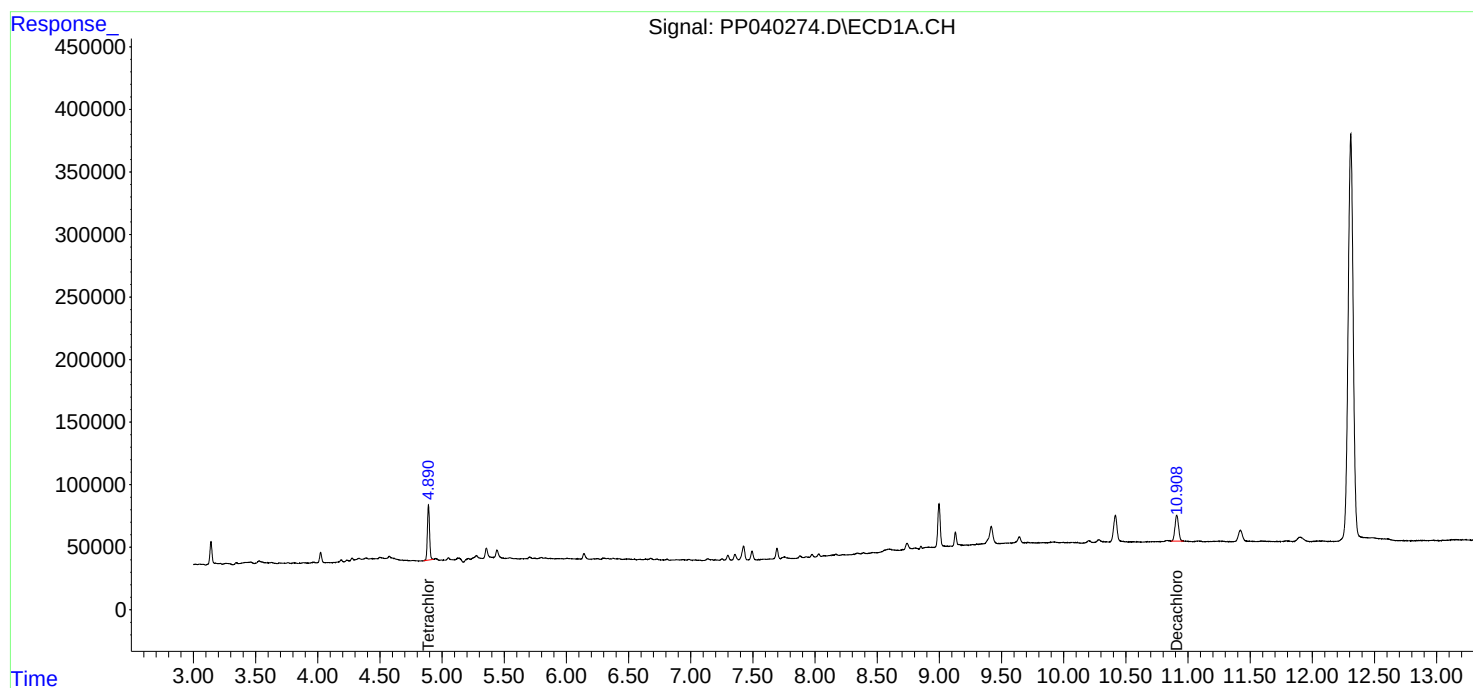

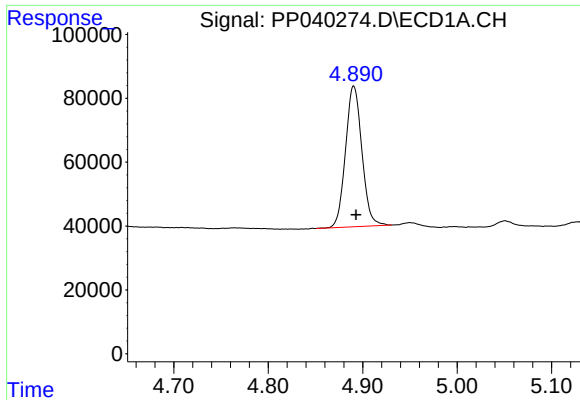


#1 Tetrachloro-m-xylene

R.T.: 4.891 min
Delta R.T.: -0.002 min
Response: 530261
Conc: 17.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
16943


Manual Integrations
APPROVED

mohammad
10/21/2021 1:44:02 PM

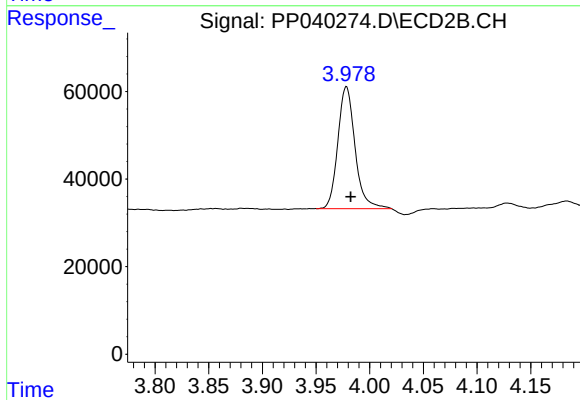


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.004 min
Response: 311137
Conc: 18.40 ng/ml m

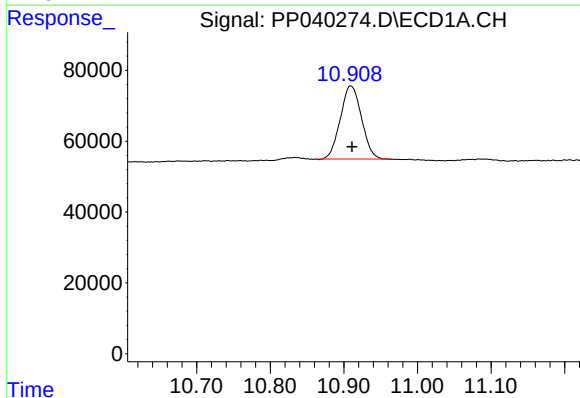

#2 Decachlorobiphenyl

R.T.: 10.910 min
Delta R.T.: -0.002 min
Response: 412631
Conc: 16.69 ng/ml

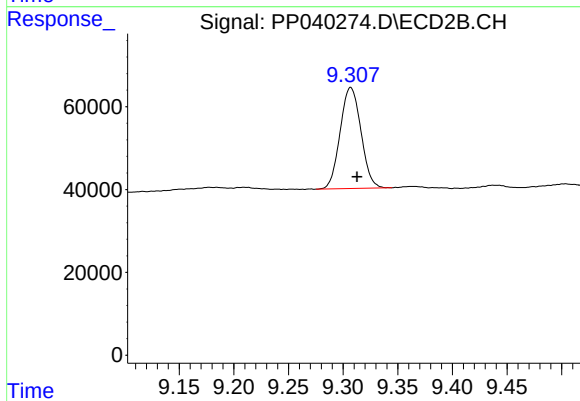

#2 Decachlorobiphenyl

R.T.: 9.307 min
Delta R.T.: -0.006 min
Response: 323875
Conc: 15.26 ng/ml