

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
 Data File : PP061137.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 17:04
 Operator : YP\AJ
 Sample : 04979-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GAS-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2023
 Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 20 18:18:17 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.558	3.694	38979320	23288325	17.731m	17.225
2) SA Decachlor...	10.532	8.767	13541253	10849508	8.647m	7.216

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
Data File : PP061137.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 17:04
Operator : YP\AJ
Sample : 04979-04
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GAS-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 20 18:18:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

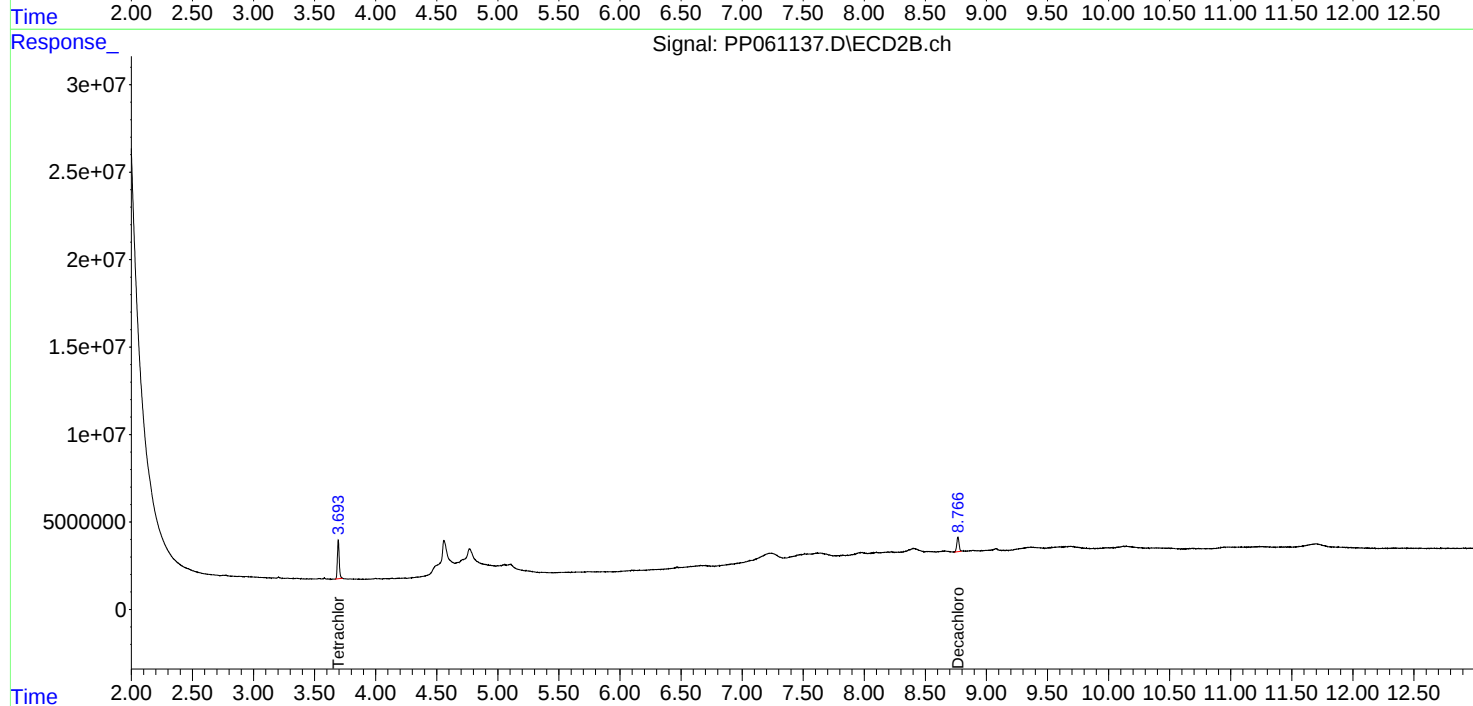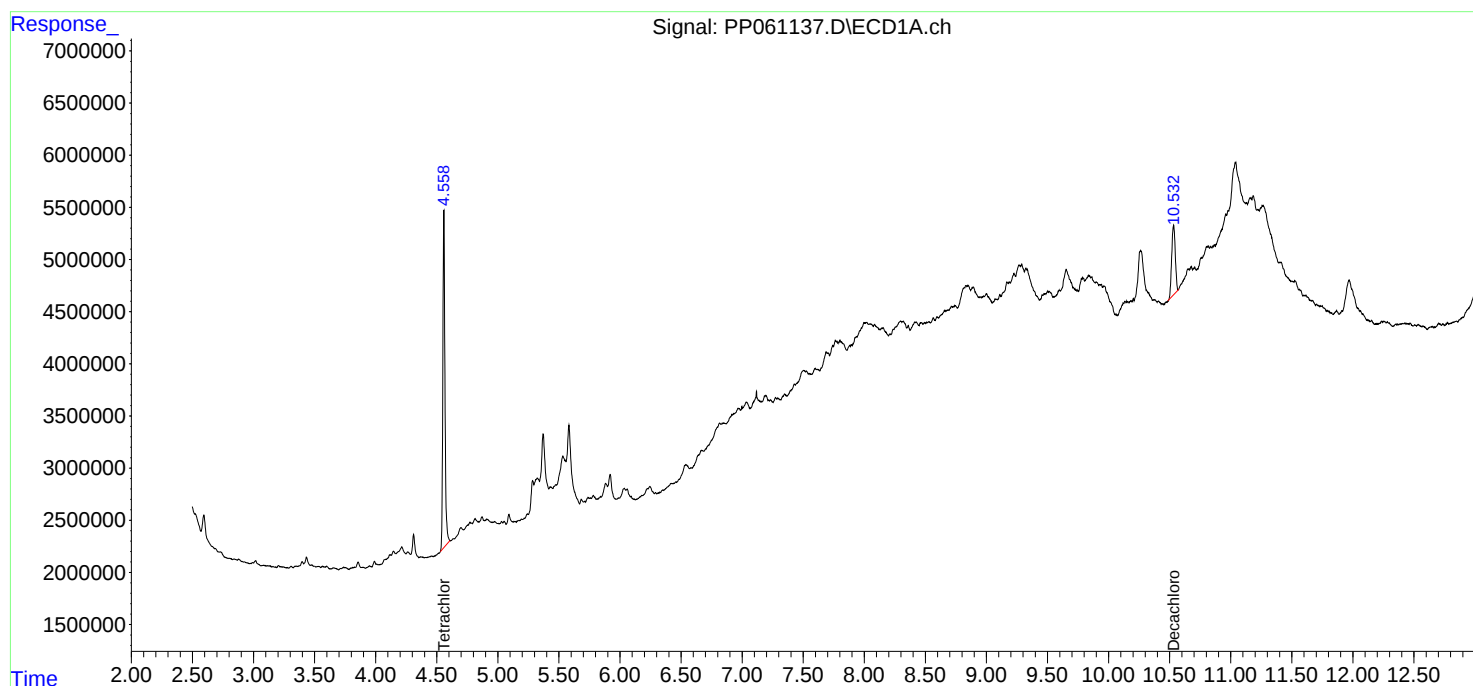

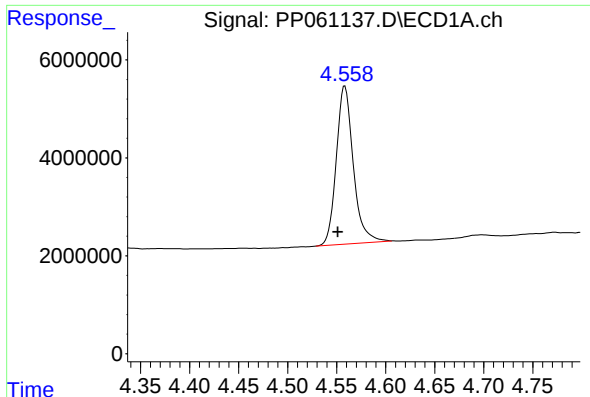


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: 0.007 min
Response: 38979320
Conc: 17.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
GAS-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

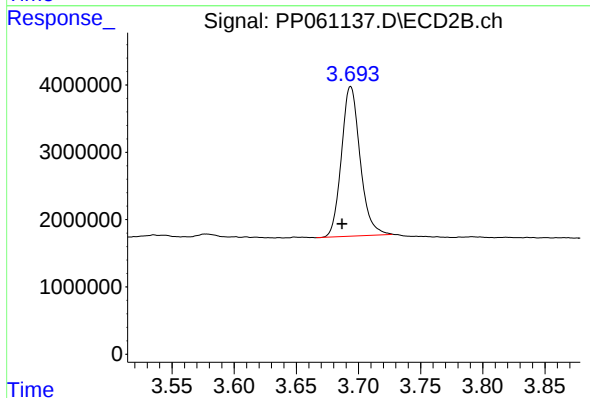


#1 Tetrachloro-m-xylene

R.T.: 3.694 min
Delta R.T.: 0.007 min
Response: 23288325
Conc: 17.23 ng/ml

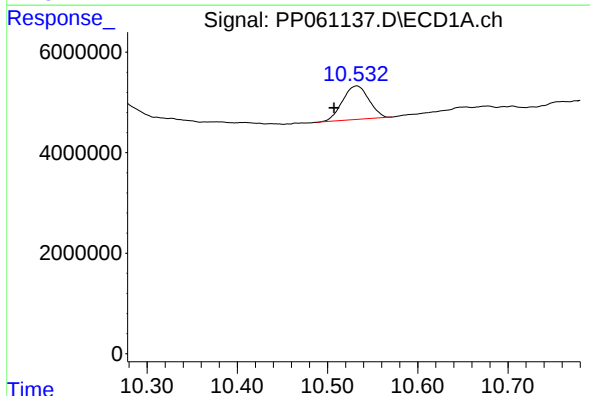

#2 Decachlorobiphenyl

R.T.: 10.532 min
Delta R.T.: 0.024 min
Response: 13541253
Conc: 8.65 ng/ml m

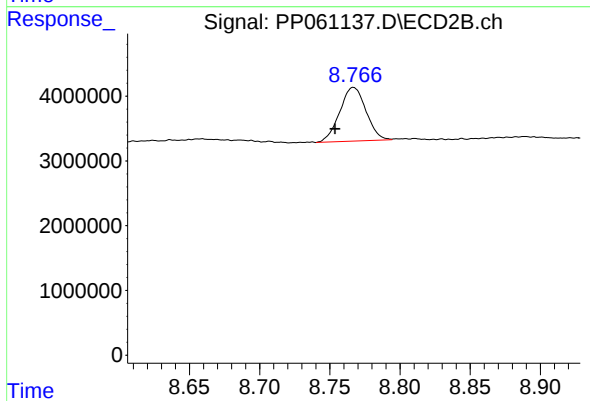

#2 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: 0.013 min
Response: 10849508
Conc: 7.22 ng/ml