

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
 Data File : PP061146.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Oct 2023 19:52
 Operator : YP\AJ
 Sample : 04974-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2023
 Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 00:49:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	3.693	53047900	32148009	24.131	23.778
2)	SA Decachlor...	10.530	8.766	38975490	28457323	24.889	18.927
Target Compounds							
26)	L6 AR-1254-1	6.621	5.604	5358244	4967351	67.749	64.293
27)	L6 AR-1254-2	6.842	5.752	10109286	4809731	84.861	69.418
28)	L6 AR-1254-3	7.213	6.159	9147416	8325589	74.770	73.579m
29)	L6 AR-1254-4	7.502	6.390	6212327	4907409	70.579	71.423
30)	L6 AR-1254-5	7.925	6.812	9329854	10521341	93.956m	98.359

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
Data File : PP061146.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Oct 2023 19:52
Operator : YP\AJ
Sample : 04974-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 00:49:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

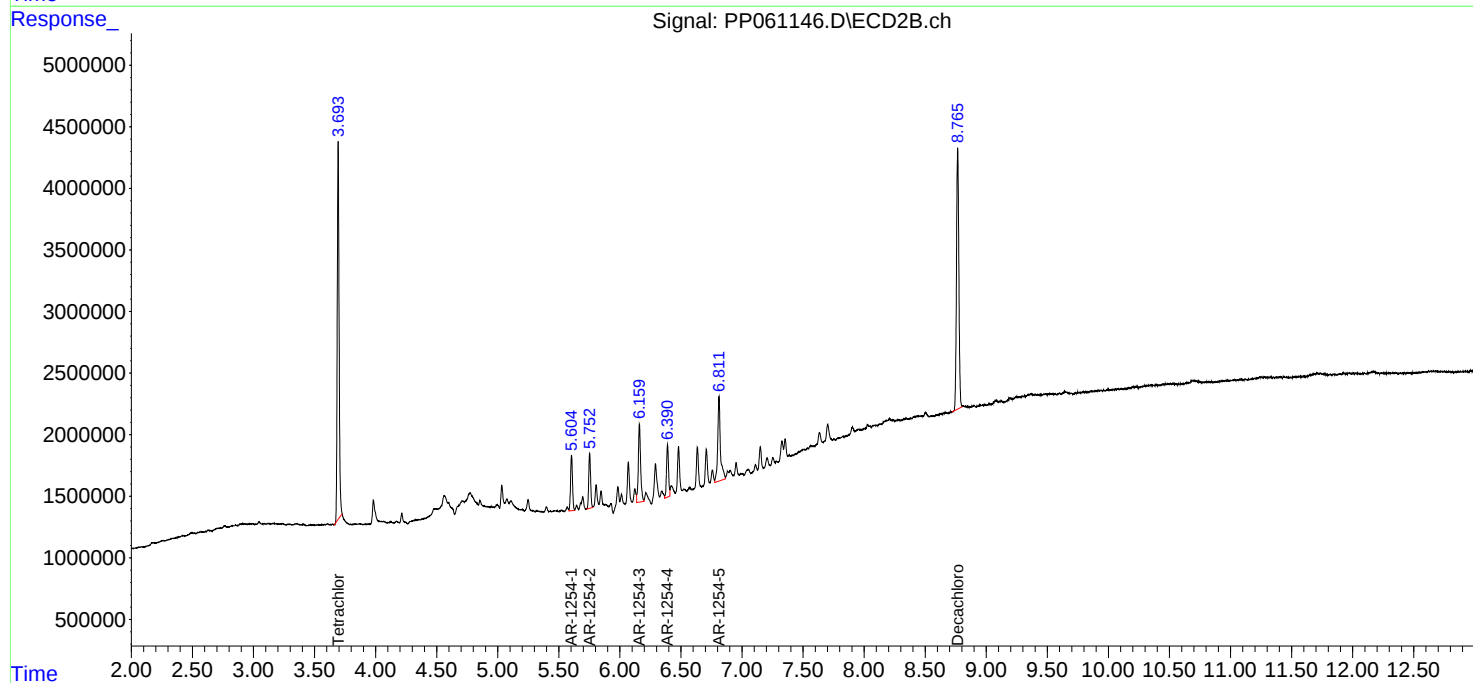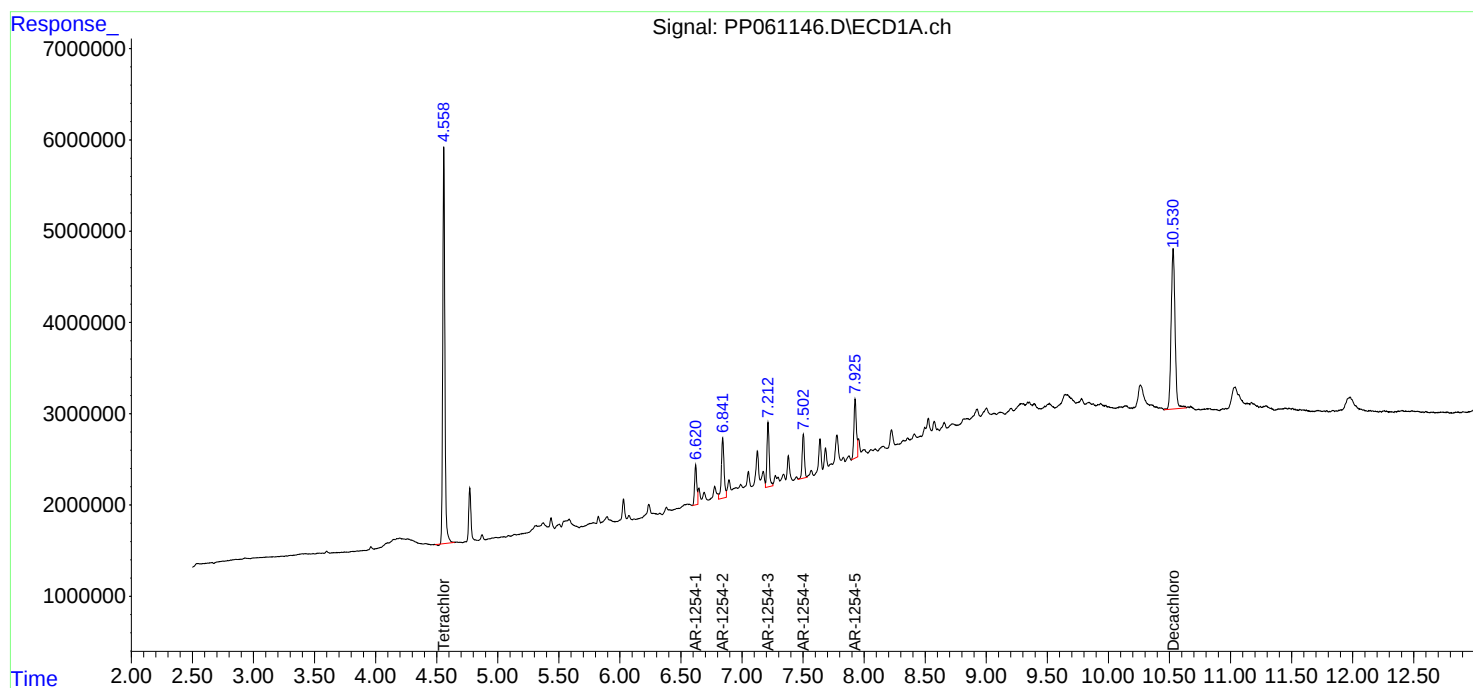

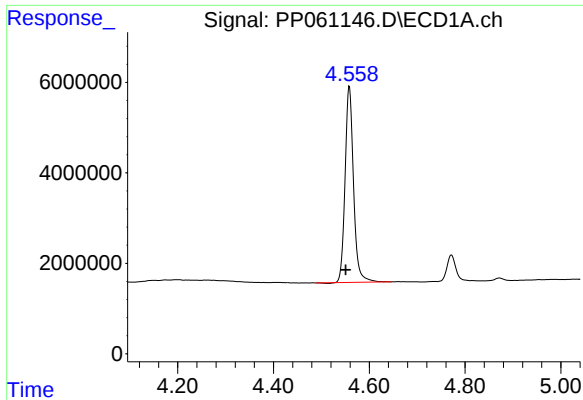


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: 0.007 min
Response: 53047900
Conc: 24.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

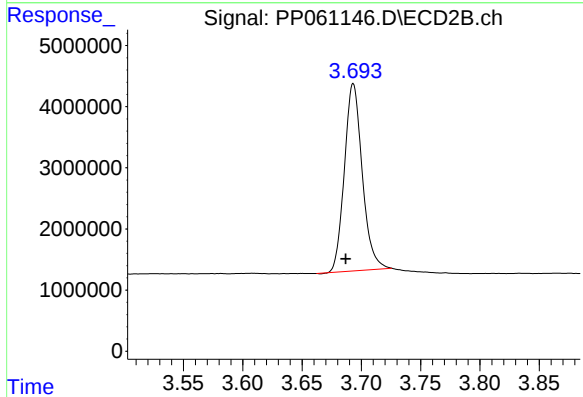


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.006 min
Response: 32148009
Conc: 23.78 ng/ml

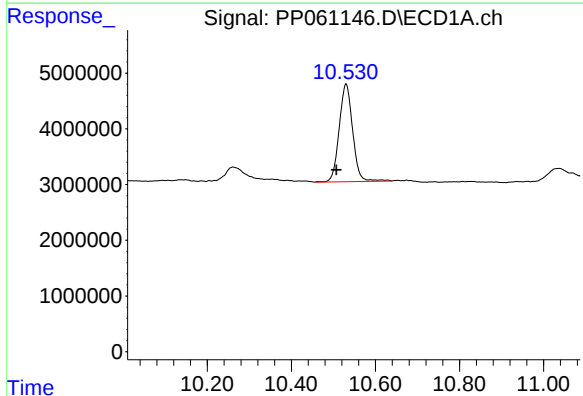


#2 Decachlorobiphenyl

R.T.: 10.530 min
Delta R.T.: 0.023 min
Response: 38975490
Conc: 24.89 ng/ml

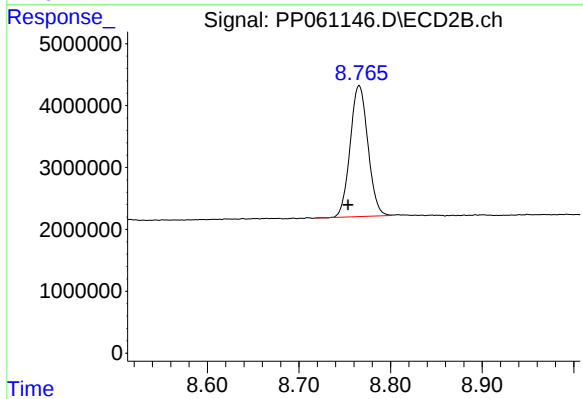

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: 0.012 min
Response: 28457323
Conc: 18.93 ng/ml

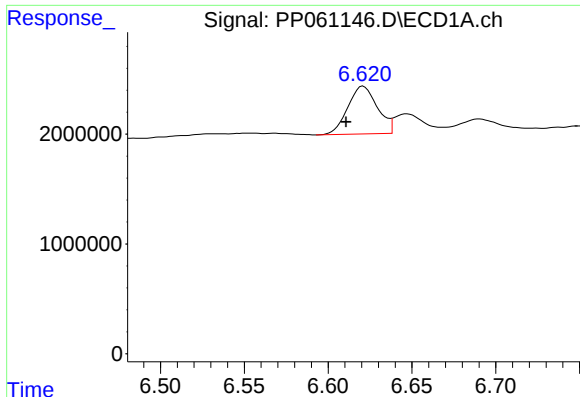


#26 AR-1254-1

R.T.: 6.621 min
Delta R.T.: 0.010 min
Response: 5358244
Conc: 67.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

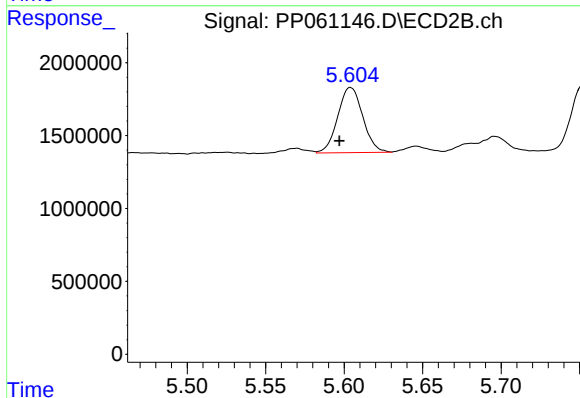


#26 AR-1254-1

R.T.: 5.604 min
Delta R.T.: 0.007 min
Response: 4967351
Conc: 64.29 ng/ml

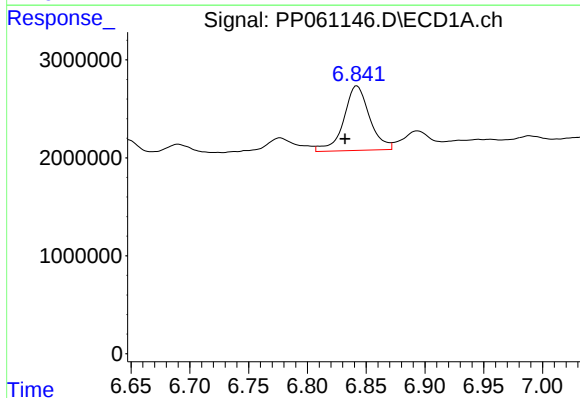


#27 AR-1254-2

R.T.: 6.842 min
Delta R.T.: 0.010 min
Response: 10109286
Conc: 84.86 ng/ml

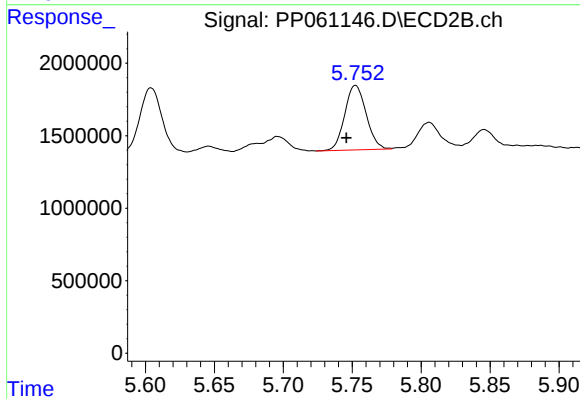

#27 AR-1254-2

R.T.: 5.752 min
Delta R.T.: 0.007 min
Response: 4809731
Conc: 69.42 ng/ml

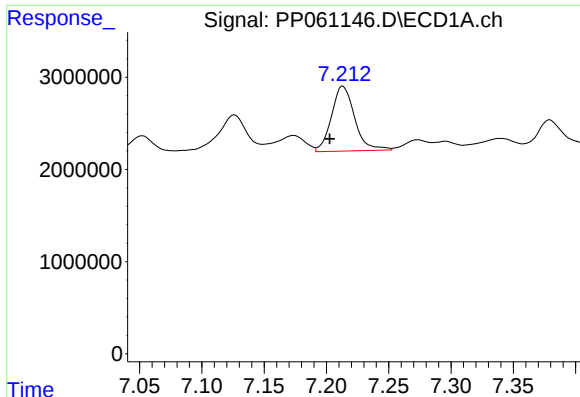


#28 AR-1254-3

R.T.: 7.213 min
Delta R.T.: 0.011 min
Response: 9147416
Conc: 74.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

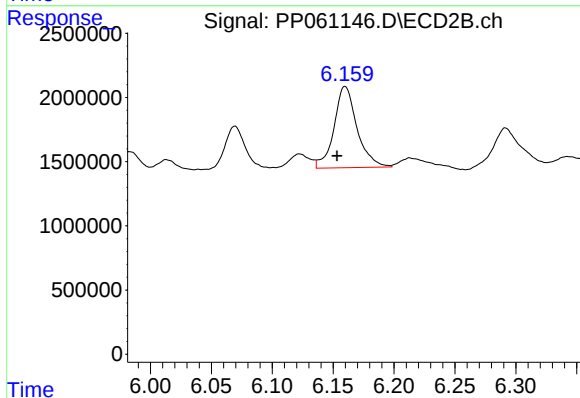


#28 AR-1254-3

R.T.: 6.159 min
Delta R.T.: 0.006 min
Response: 8325589
Conc: 73.58 ng/ml m

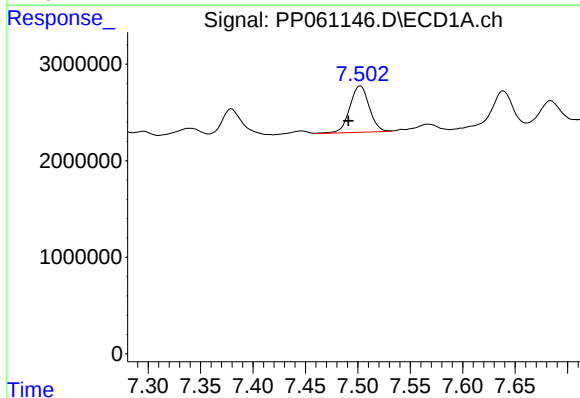


#29 AR-1254-4

R.T.: 7.502 min
Delta R.T.: 0.011 min
Response: 6212327
Conc: 70.58 ng/ml

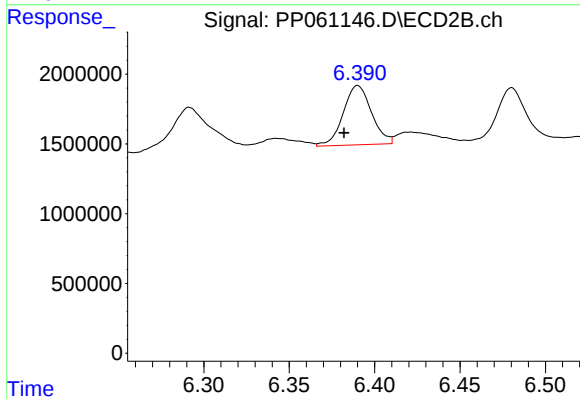

#29 AR-1254-4

R.T.: 6.390 min
Delta R.T.: 0.008 min
Response: 4907409
Conc: 71.42 ng/ml

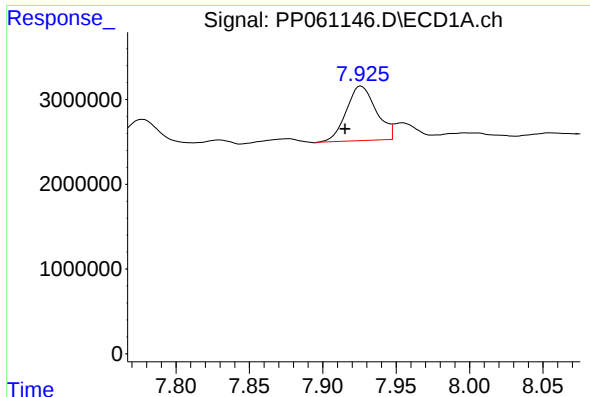


#30 AR-1254-5

R.T.: 7.925 min
Delta R.T.: 0.010 min
Response: 9329854
Conc: 93.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

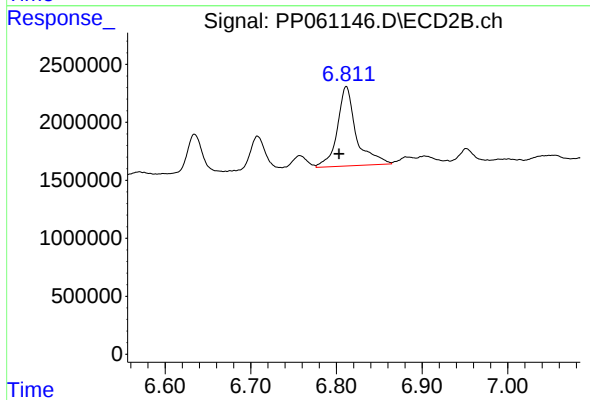

#30 AR-1254-5

R.T.: 6.812 min
Delta R.T.: 0.008 min
Response: 10521341
Conc: 98.36 ng/ml