

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
 Data File : PP061166.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2023 01:43
 Operator : YP\AJ
 Sample : 04909-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LCOL-12

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2023
 Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 02:43:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.565	3.704	155.3E6	66943938	70.637m	49.515 #
2) SA Decachlor...	10.510	8.800f	30455556	72338500	19.448m	48.112m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
Data File : PP061166.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2023 01:43
Operator : YP\AJ
Sample : 04909-01
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LCOL-12


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 02:43:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

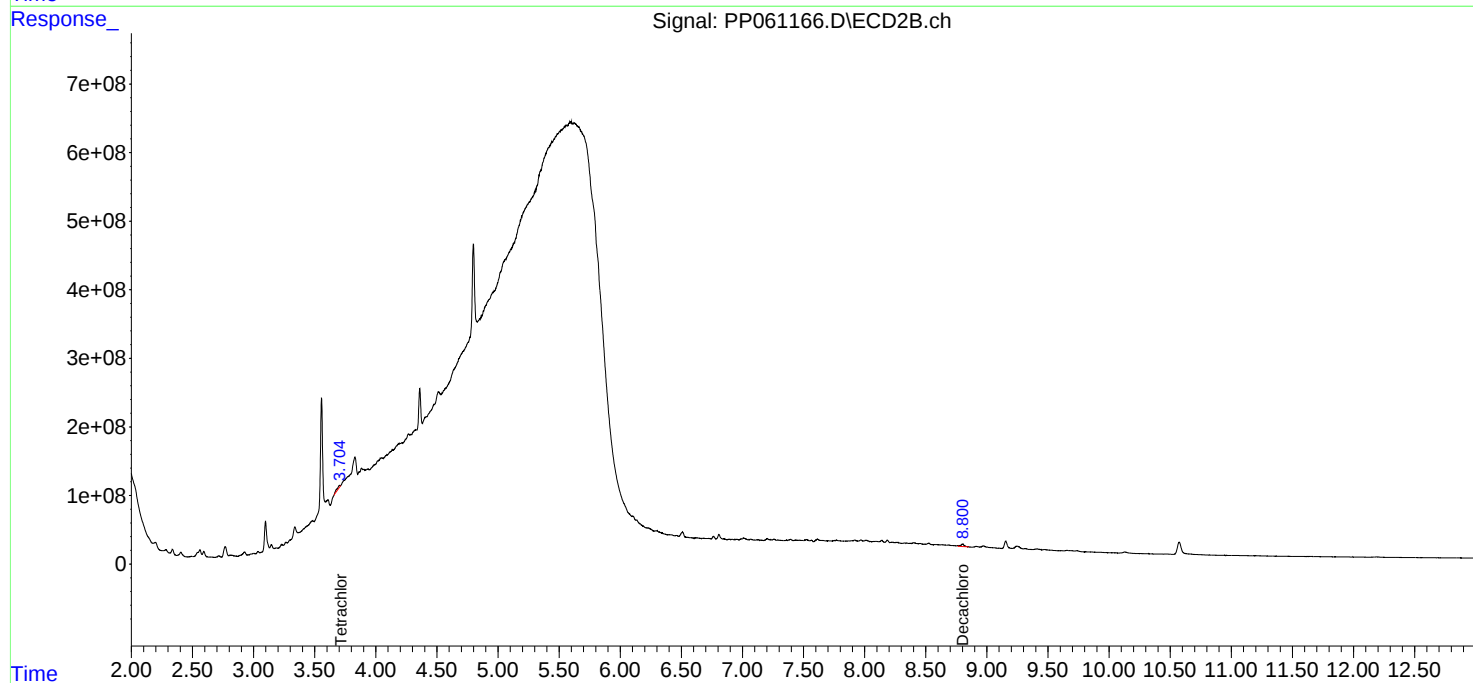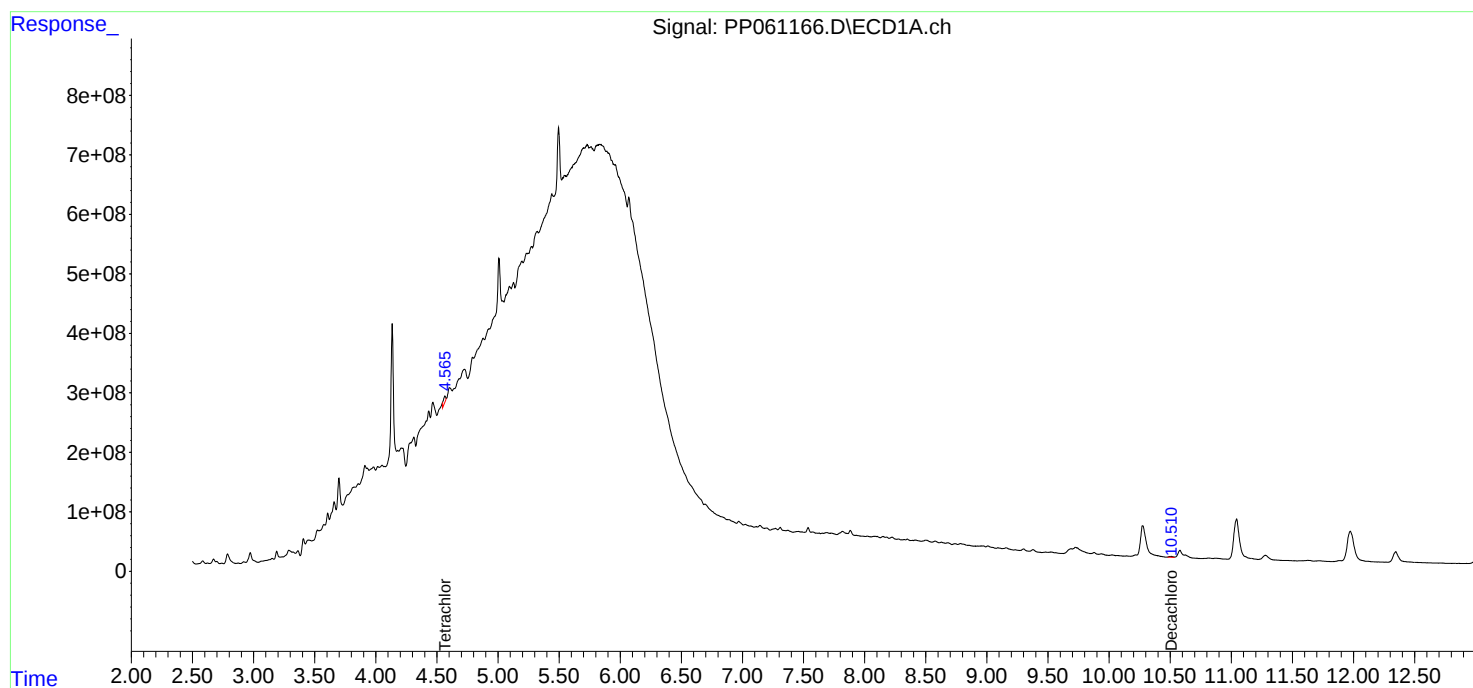

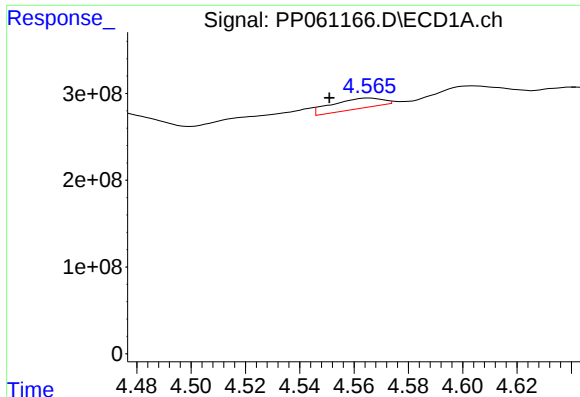


#1 Tetrachloro-m-xylene

R.T.: 4.565 min
Delta R.T.: 0.014 min
Response: 155284238
Conc: 70.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
LCOL-12


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

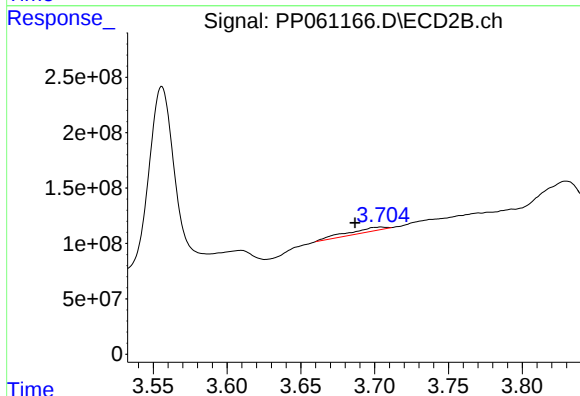


#1 Tetrachloro-m-xylene

R.T.: 3.704 min
Delta R.T.: 0.018 min
Response: 66943938
Conc: 49.51 ng/ml

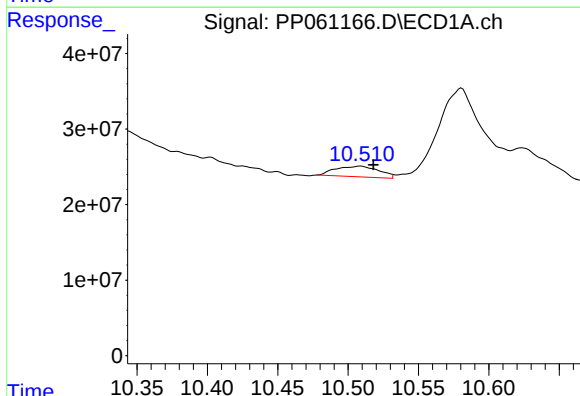

#2 Decachlorobiphenyl

R.T.: 10.510 min
Delta R.T.: -0.008 min
Response: 30455556
Conc: 19.45 ng/ml m

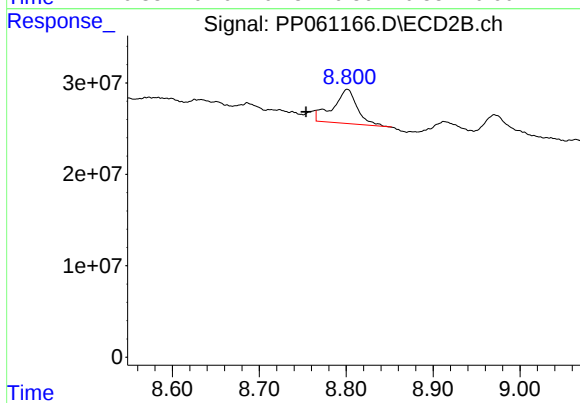

#2 Decachlorobiphenyl

R.T.: 8.800 min
Delta R.T.: 0.047 min
Response: 72338500
Conc: 48.11 ng/ml m