

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
 Data File : PP061167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2023 03:33
 Operator : YP\AJ
 Sample : 04909-01RE
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LCOL-12RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2023
 Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 04:27:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.577f	3.703	168.3E6	65935517	76.577m	48.769 #
2) SA Decachlor...	10.553f	8.780f	35173329	3927543	22.461m	2.612 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102023\
Data File : PP061167.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2023 03:33
Operator : YP\AJ
Sample : 04909-01RE
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LCOL-12RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 04:27:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

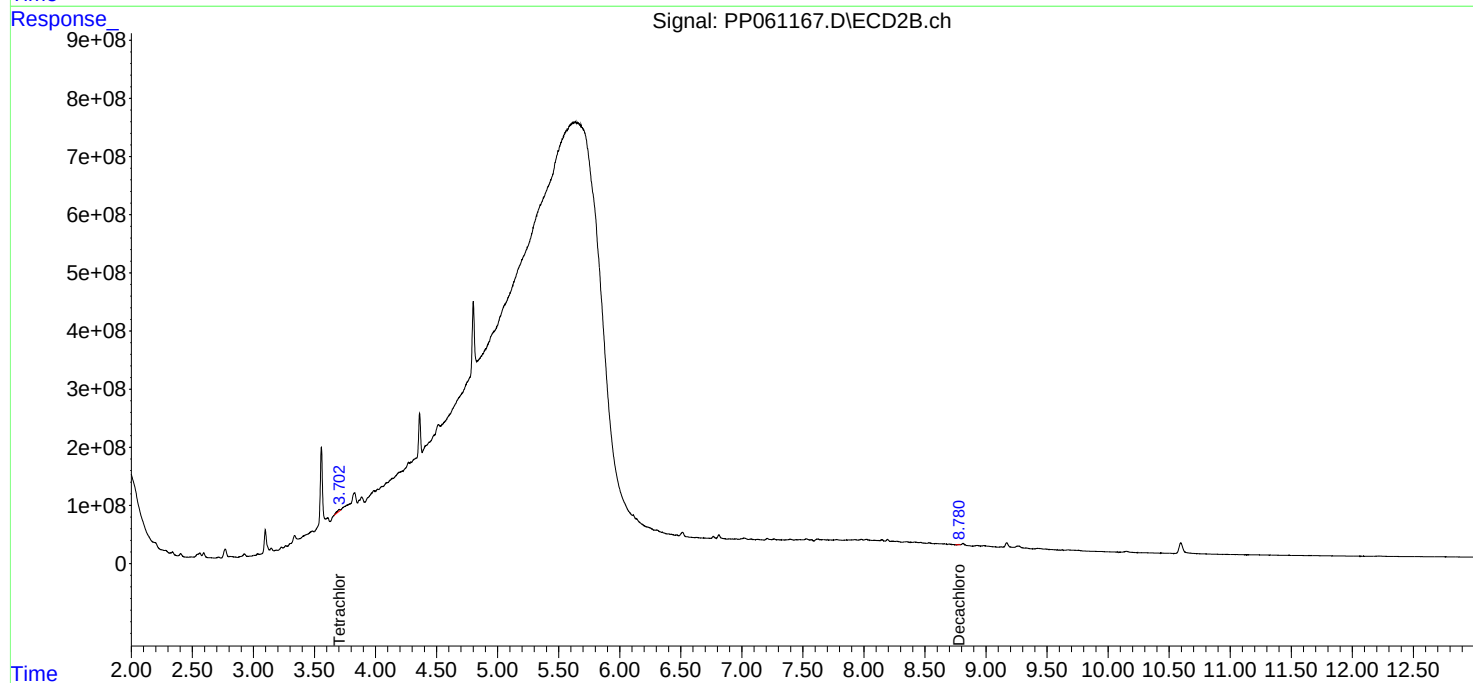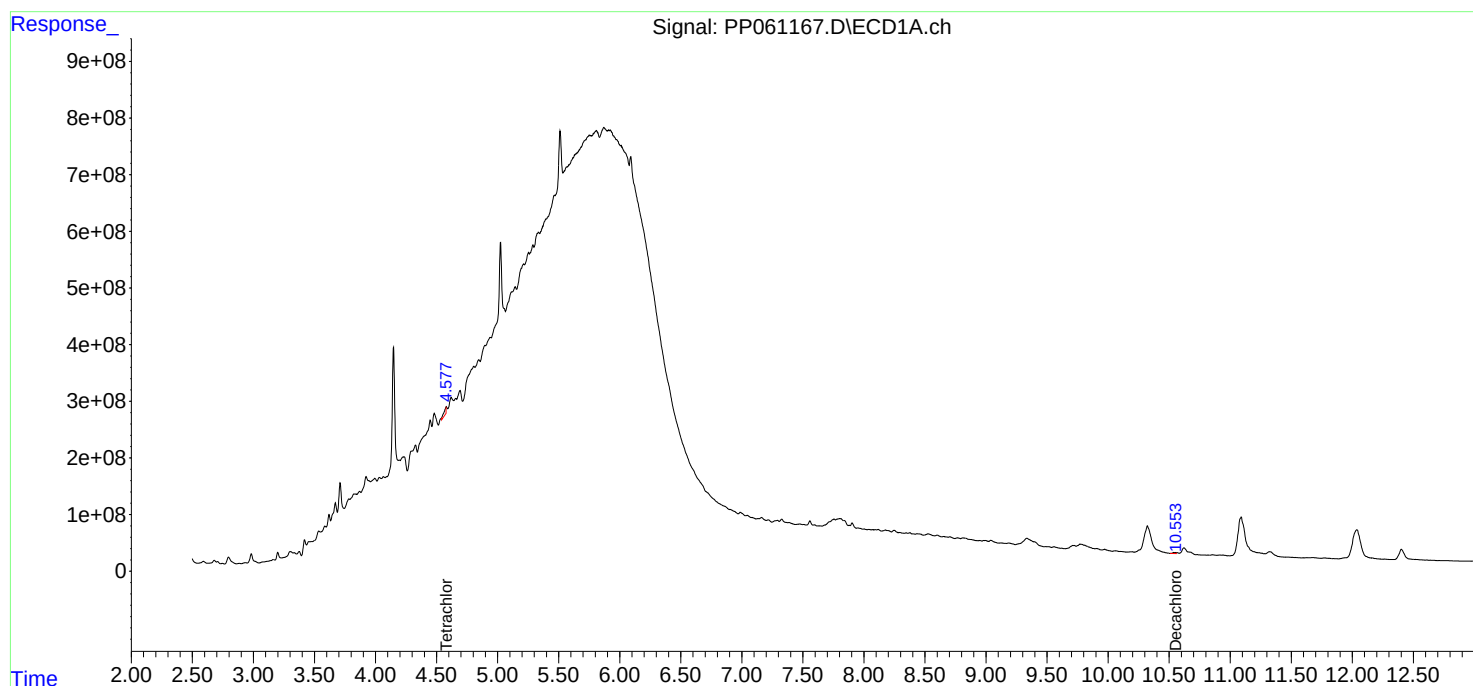

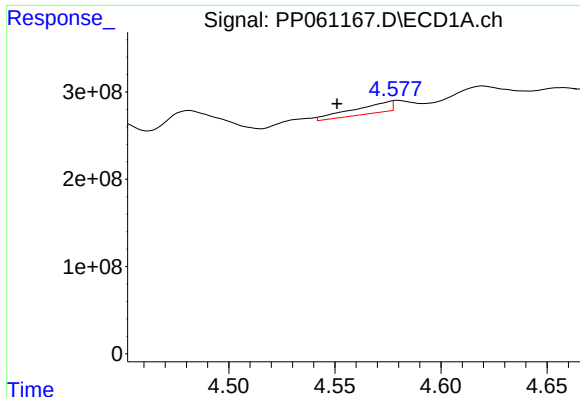


#1 Tetrachloro-m-xylene

R.T.: 4.577 min
Delta R.T.: 0.026 min
Response: 168341684
Conc: 76.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LCOL-12RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2023
Supervised By :Ankita Jodhani 10/23/2023

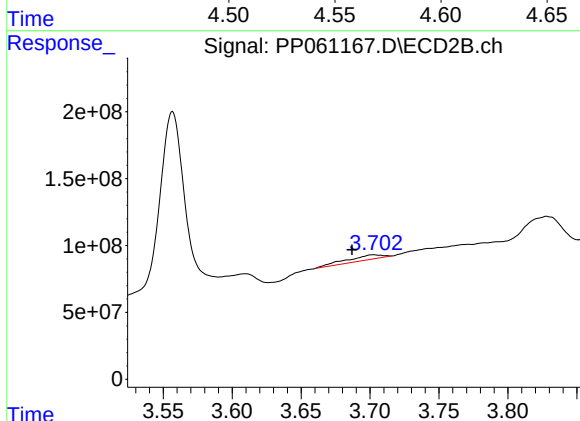


#1 Tetrachloro-m-xylene

R.T.: 3.703 min
Delta R.T.: 0.016 min
Response: 65935517
Conc: 48.77 ng/ml

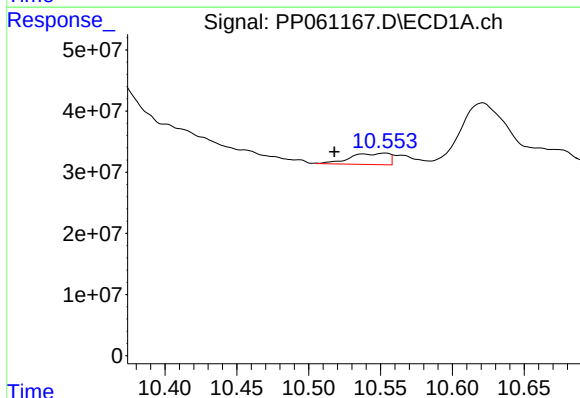

#2 Decachlorobiphenyl

R.T.: 10.553 min
Delta R.T.: 0.035 min
Response: 35173329
Conc: 22.46 ng/ml m

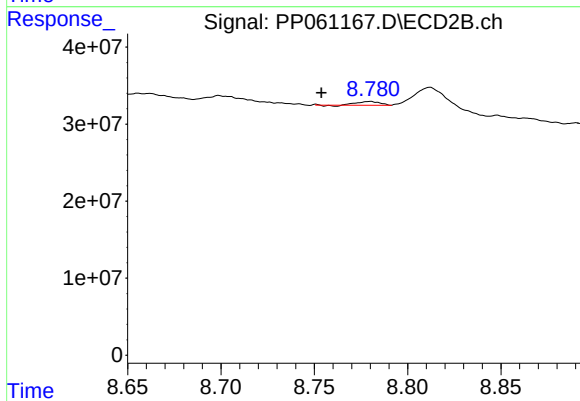

#2 Decachlorobiphenyl

R.T.: 8.780 min
Delta R.T.: 0.026 min
Response: 3927543
Conc: 2.61 ng/ml