

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102121\
 Data File : PP040327.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2021 14:51
 Operator : AJ\MA
 Sample : M4290-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 21 16:40:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.890	3.977	693127	389764	22.824	23.055
2) SA Decachlor...	10.906	9.301	572335	474348	23.156	22.351
Target Compounds						
9) L2 AR-1221-2	0.000	4.333	0	12129	N.D.	72.105 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102121\
Data File : PP040327.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2021 14:51
Operator : AJ\MA
Sample : M4290-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 21 16:40:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

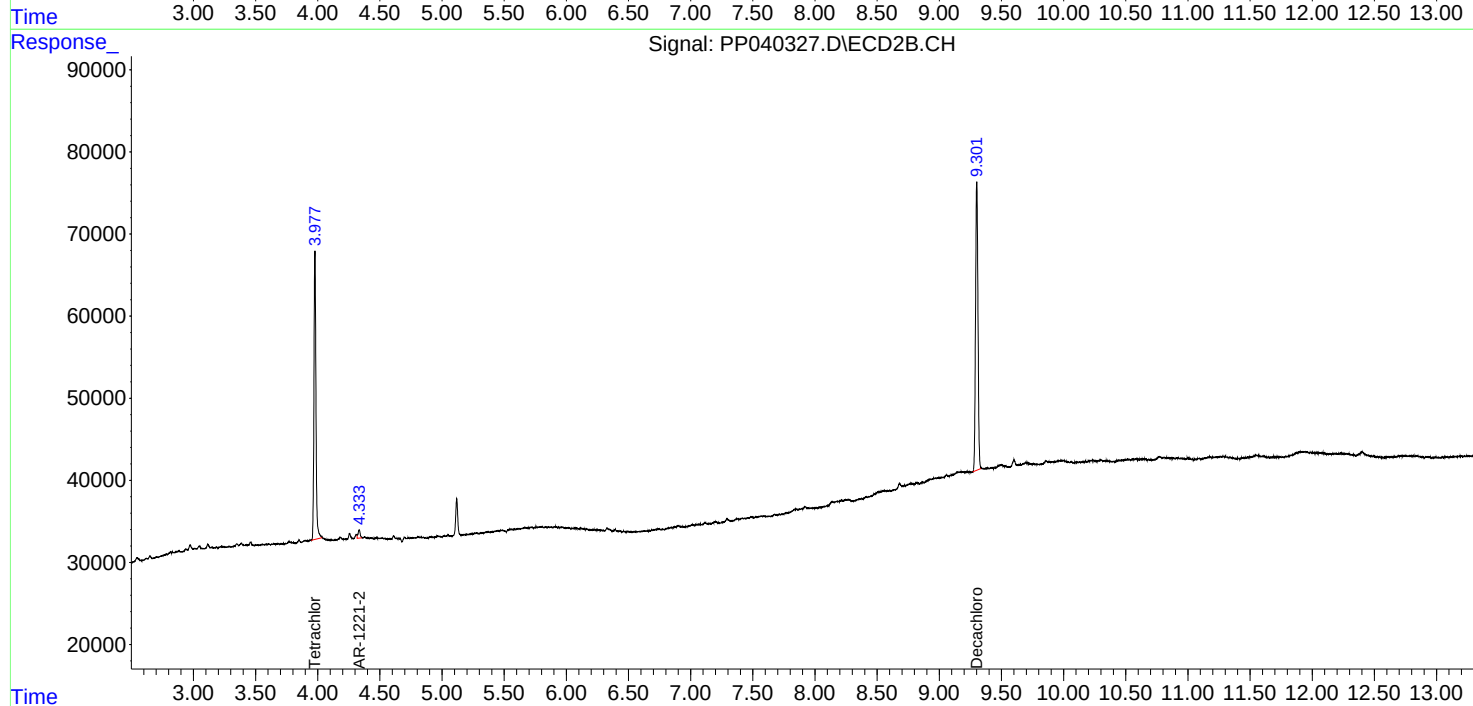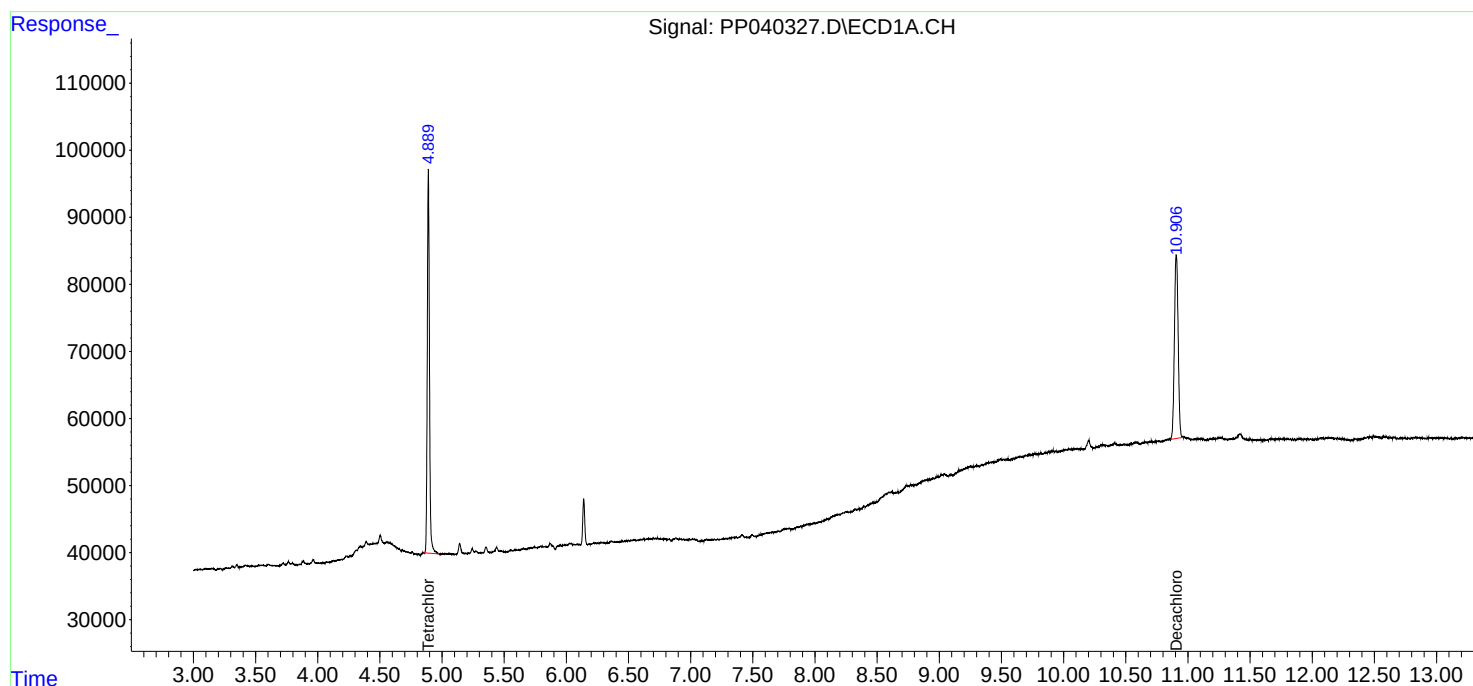


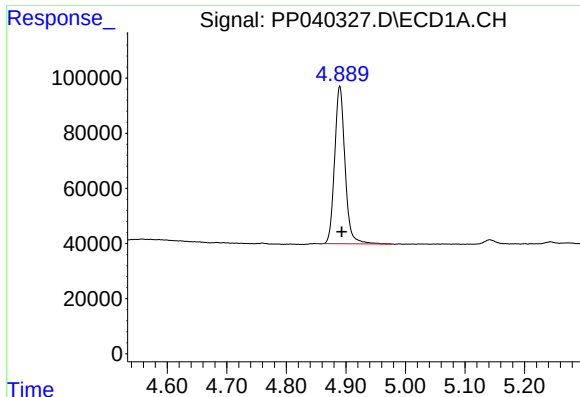

#1 Tetrachloro-m-xylene


R.T.: 4.890 min
Delta R.T.: -0.003 min
Response: 693127
Conc: 22.82 ng/ml

Instrument :
ECD_P
ClientSampleId :

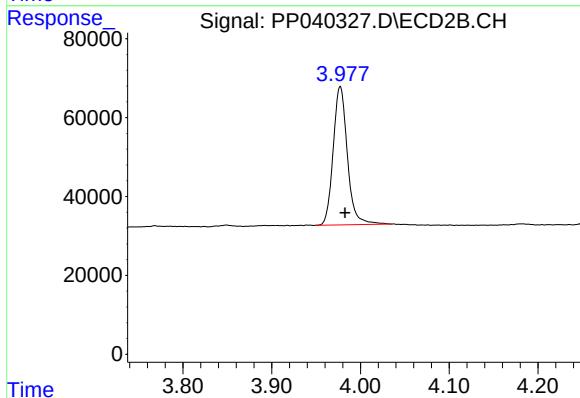


#1 Tetrachloro-m-xylene

R.T.: 3.977 min
Delta R.T.: -0.005 min
Response: 389764
Conc: 23.05 ng/ml

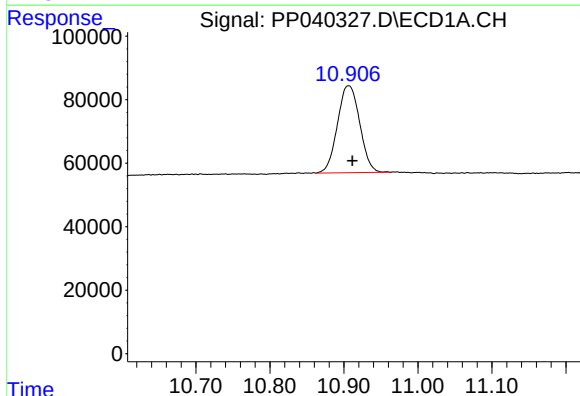


#2 Decachlorobiphenyl

R.T.: 10.906 min
Delta R.T.: -0.005 min
Response: 572335
Conc: 23.16 ng/ml

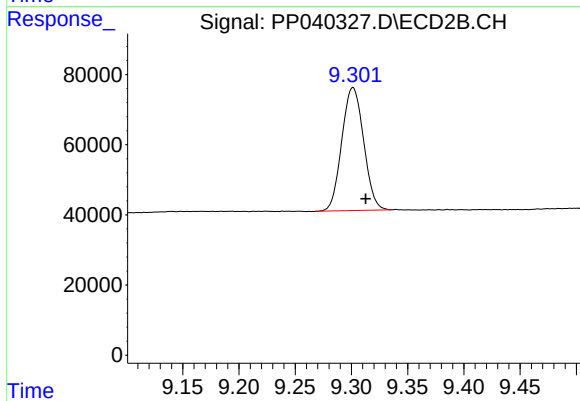

#2 Decachlorobiphenyl


R.T.: 9.301 min
Delta R.T.: -0.011 min
Response: 474348
Conc: 22.35 ng/ml

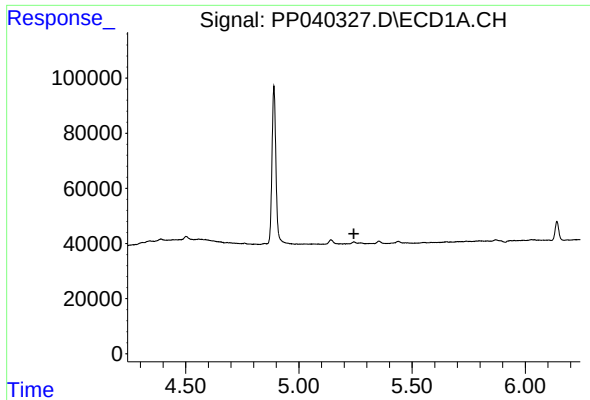

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.243 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

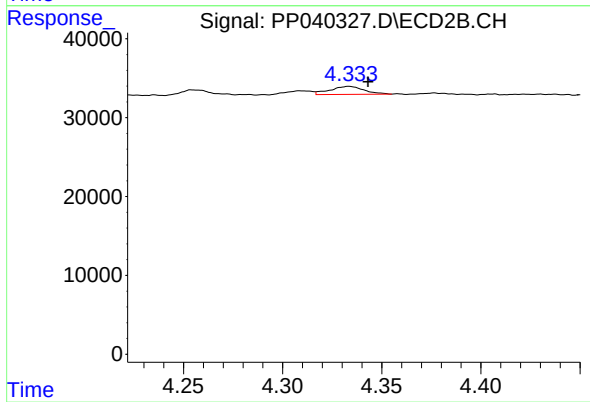

#9 AR-1221-2

R.T.: 4.333 min
Delta R.T.: -0.010 min
Response: 12129
Conc: 72.10 ng/ml