

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102121\
 Data File : PP040349.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Oct 2021 21:28
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 01:35:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.891	3.978	619222	356149	20.390	21.066
2)	SA Decachlor...	10.909	9.303	564495	486010	22.839	22.900
Target Compounds							
10)	L2 AR-1221-3	0.000	4.416f	0	15189	N.D.	28.048 #
11)	L3 AR-1232-1	0.000	4.416f	0	15189	N.D.	37.397 #
20)	L4 AR-1242-5	0.000	6.144f	0	33803	N.D.	70.870 #
24)	L5 AR-1248-4	7.135f	0.000	1678	0	1.823	N.D. #
25)	L5 AR-1248-5	0.000	6.144f	0	33803	N.D.	54.185 #
26)	L6 AR-1254-1	7.135	6.144f	1678	33803	1.809	35.283 #
28)	L6 AR-1254-3	7.756f	0.000	27488	0	19.295	N.D. #
32)	L7 AR-1260-2	0.000	7.012f	0	24248	N.D.	20.478 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102121\
Data File : PP040349.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Oct 2021 21:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 01:35:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

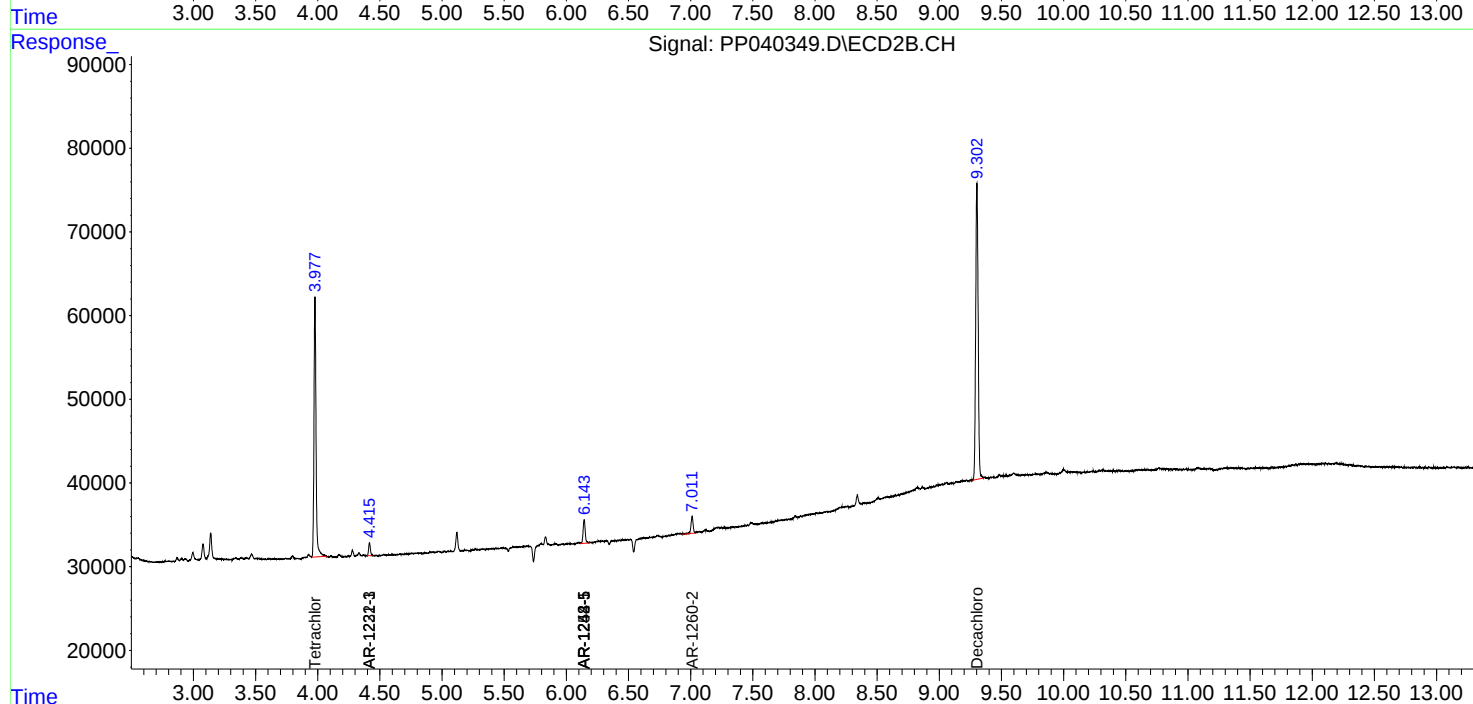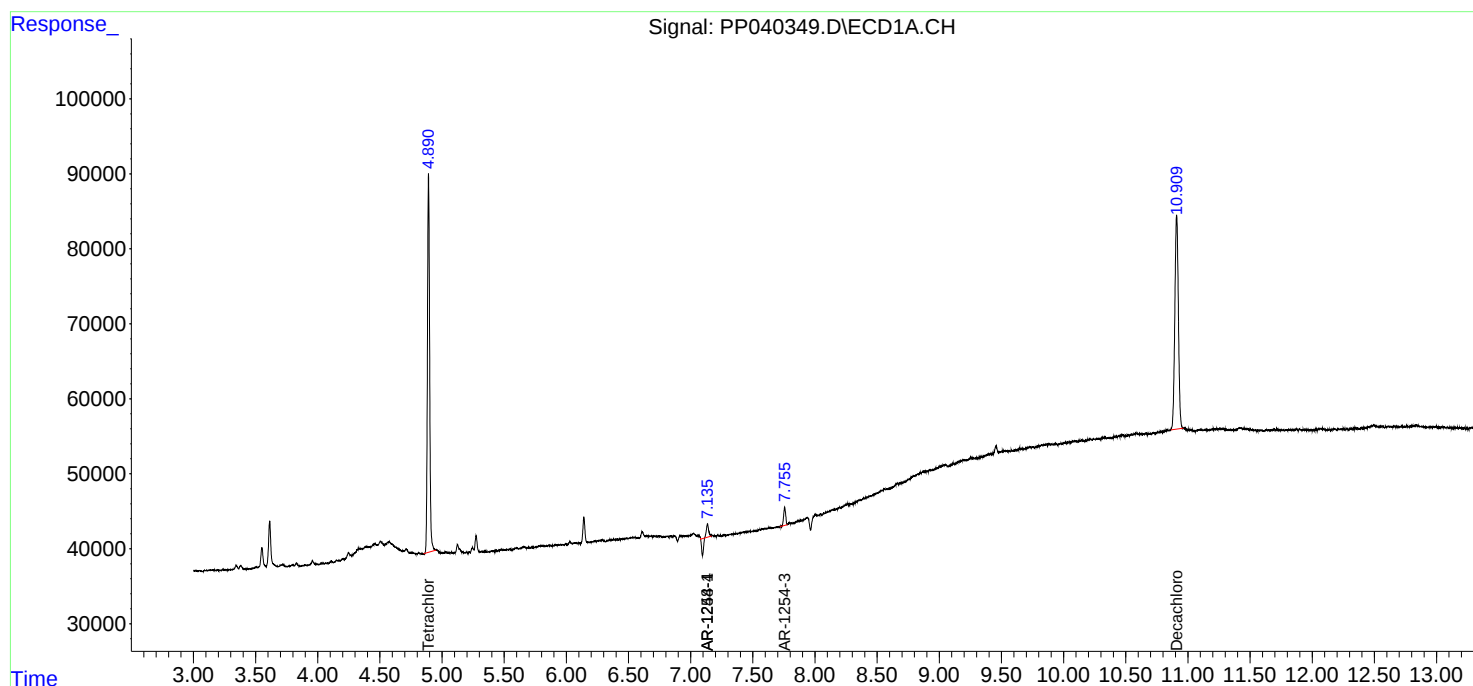


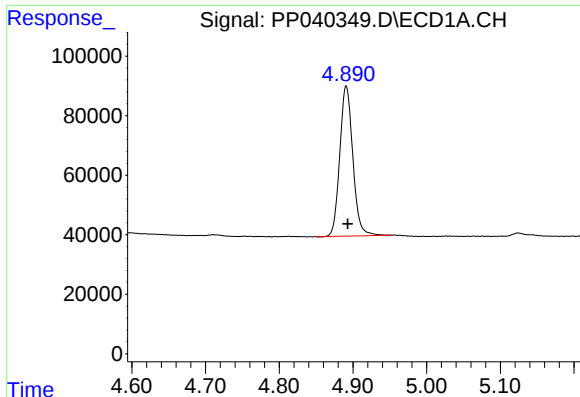

#1 Tetrachloro-m-xylene


R.T.: 4.891 min
Delta R.T.: -0.002 min
Response: 619222
Conc: 20.39 ng/ml

Instrument :
ECD_P
ClientSampleId :

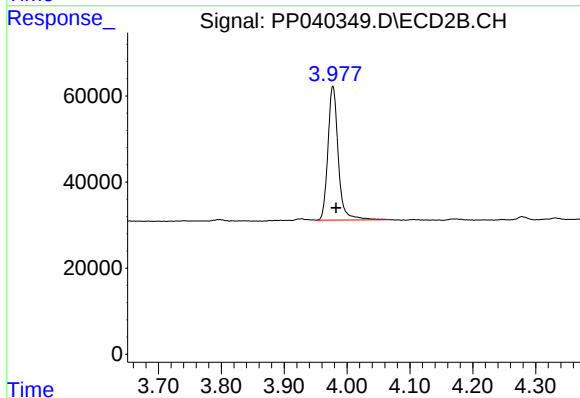


#1 Tetrachloro-m-xylene

R.T.: 3.978 min
Delta R.T.: -0.005 min
Response: 356149
Conc: 21.07 ng/ml

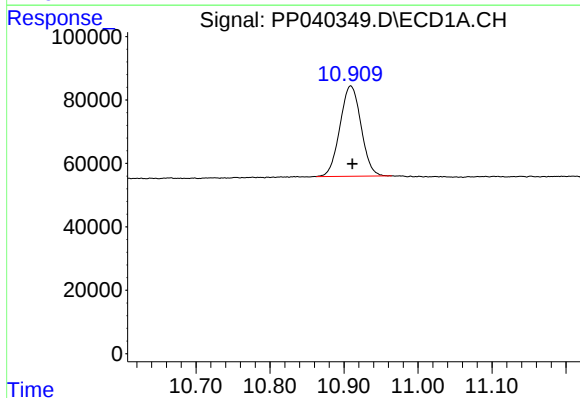


#2 Decachlorobiphenyl

R.T.: 10.909 min
Delta R.T.: -0.002 min
Response: 564495
Conc: 22.84 ng/ml

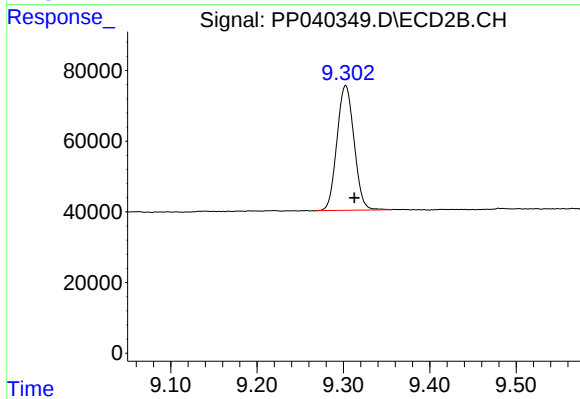

#2 Decachlorobiphenyl


R.T.: 9.303 min
Delta R.T.: -0.010 min
Response: 486010
Conc: 22.90 ng/ml

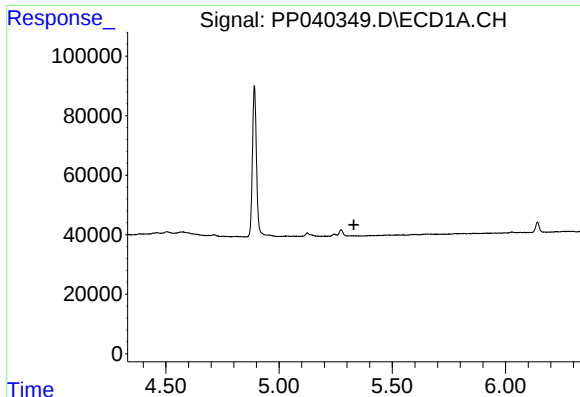

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T.: 5.331 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

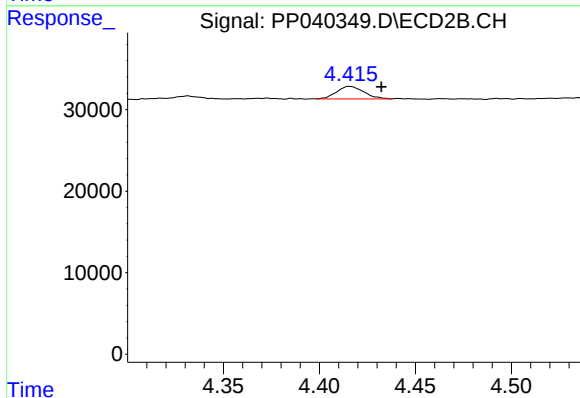


#10 AR-1221-3

R.T.: 4.416 min
Delta R.T.: -0.017 min
Response: 15189
Conc: 28.05 ng/ml

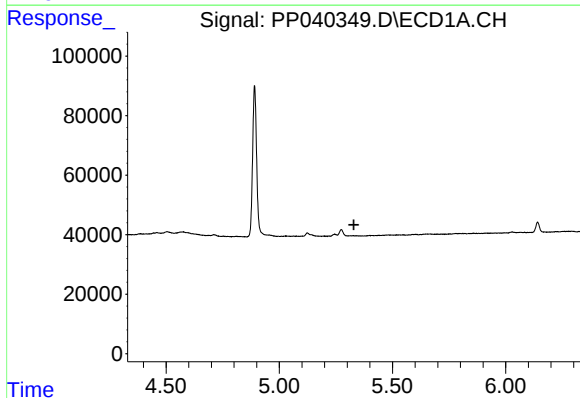


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T.: 5.330 min
Response: 0
Conc: N.D.

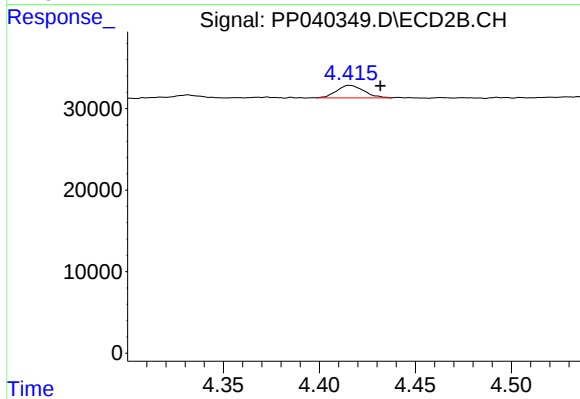

#11 AR-1232-1


R.T.: 4.416 min
Delta R.T.: -0.016 min
Response: 15189
Conc: 37.40 ng/ml

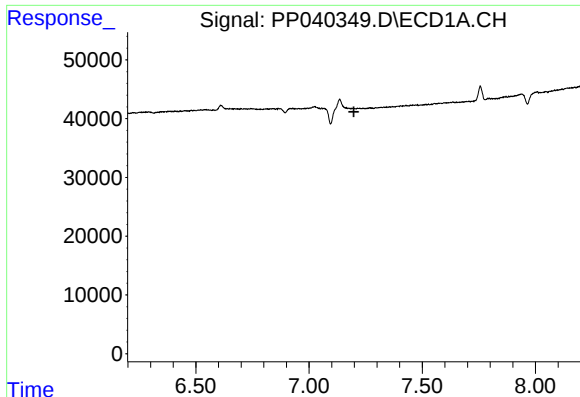

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

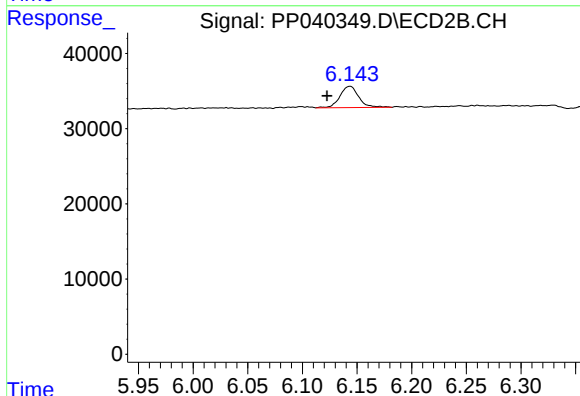


#20 AR-1242-5

R.T.: 6.144 min
Delta R.T.: 0.021 min
Response: 33803
Conc: 70.87 ng/ml

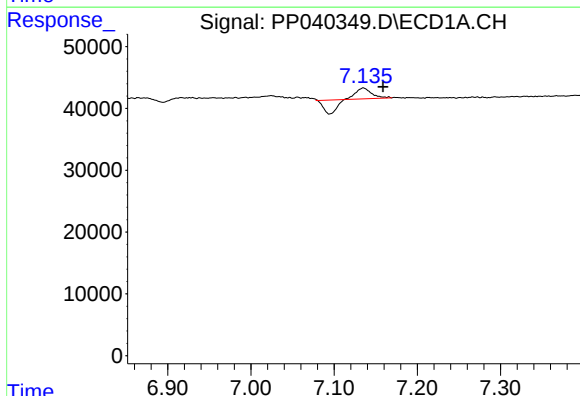


#24 AR-1248-4

R.T.: 7.135 min
Delta R.T.: -0.024 min
Response: 1678
Conc: 1.82 ng/ml

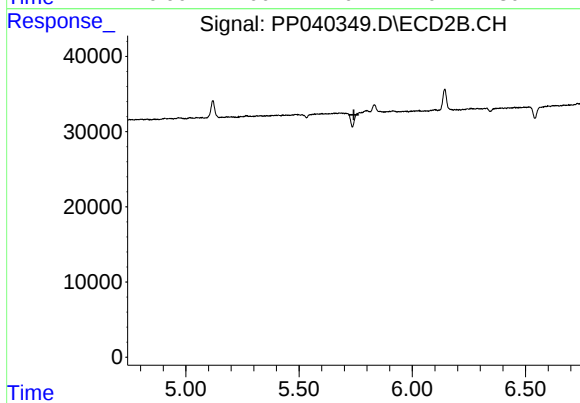

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 5.742 min
Response: 0
Conc: N.D.

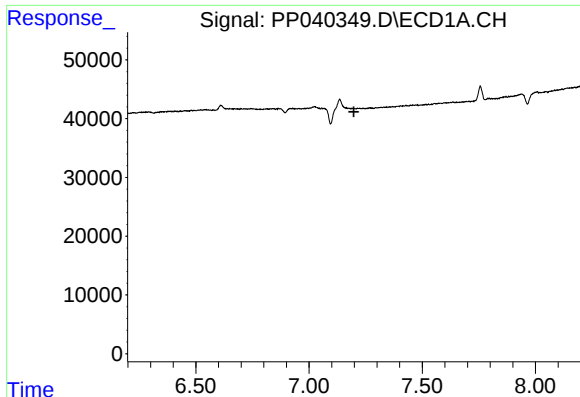

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.198 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

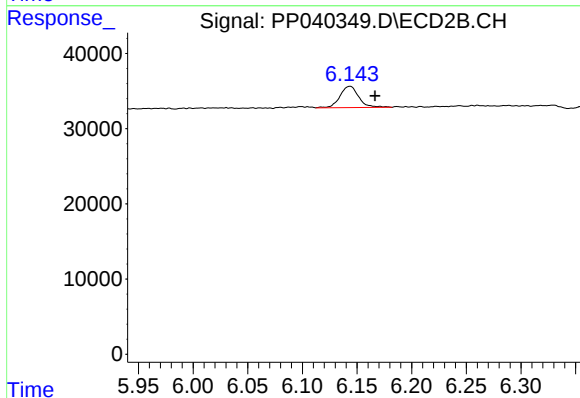


#25 AR-1248-5

R.T.: 6.144 min
Delta R.T.: -0.023 min
Response: 33803
Conc: 54.18 ng/ml

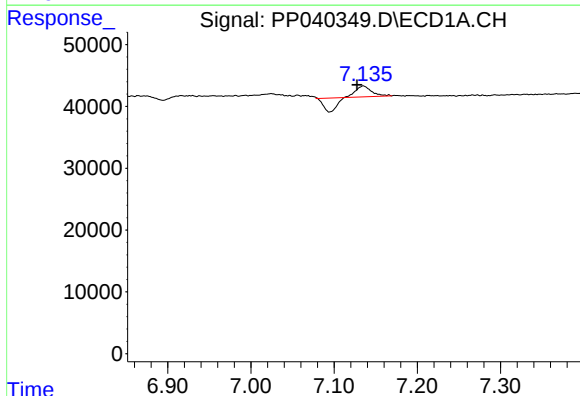


#26 AR-1254-1

R.T.: 7.135 min
Delta R.T.: 0.007 min
Response: 1678
Conc: 1.81 ng/ml

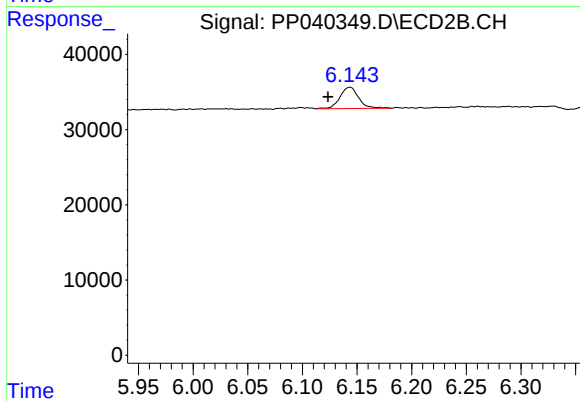

#26 AR-1254-1


R.T.: 6.144 min
Delta R.T.: 0.020 min
Response: 33803
Conc: 35.28 ng/ml

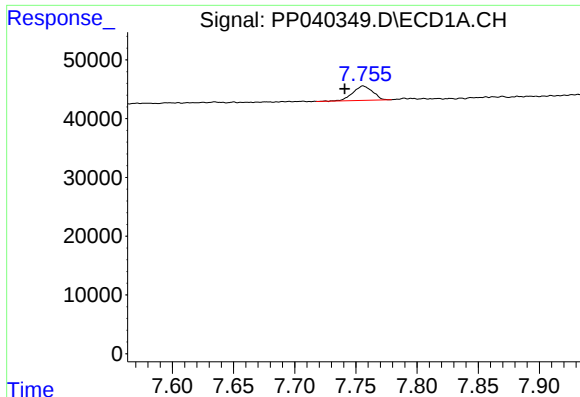

#28 AR-1254-3


R.T.: 7.756 min
Delta R.T.: 0.015 min
Response: 27488
Conc: 19.29 ng/ml

Instrument :
ECD_P
ClientSampleId :

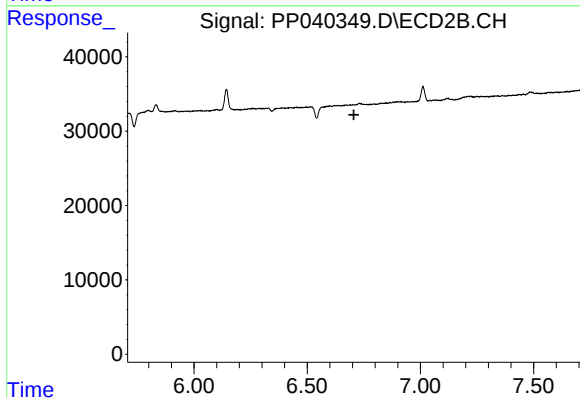


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.706 min
Response: 0
Conc: N.D.

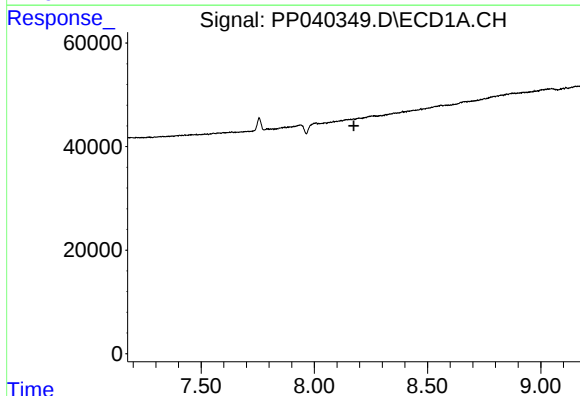

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.175 min
Response: 0
Conc: N.D.

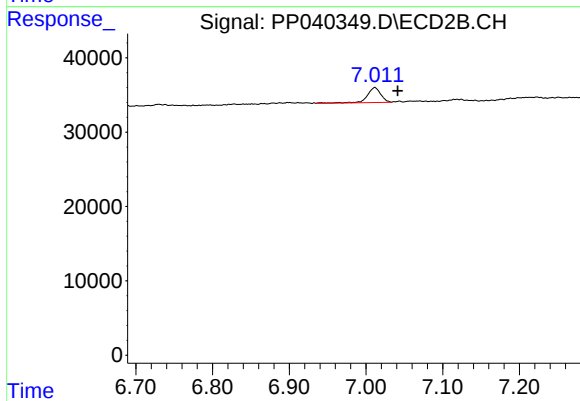

#32 AR-1260-2

R.T.: 7.012 min
Delta R.T.: -0.030 min
Response: 24248
Conc: 20.48 ng/ml