

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102121\  
 Data File : PP040324.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 21 Oct 2021 14:01  
 Operator : AJ\MA  
 Sample : M4146-03  
 Misc :  
 ALS Vial : 12 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 20-SB-3-20211007-24.0-24.5

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 21 16:39:26 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP101221.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 13 08:03:59 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|--------|--------|--------|--------|
| -----                       |        |       |        |        |        |        |
| System Monitoring Compounds |        |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.890  | 3.978 | 663930 | 366207 | 21.863 | 21.661 |
| 2) SA Decachlor...          | 10.907 | 9.302 | 544514 | 476337 | 22.030 | 22.445 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102121\  
Data File : PP040324.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 21 Oct 2021 14:01  
Operator : AJ\MA  
Sample : M4146-03  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
20-SB-3-20211007-24.0-24.5

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 21 16:39:26 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP101221.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 13 08:03:59 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

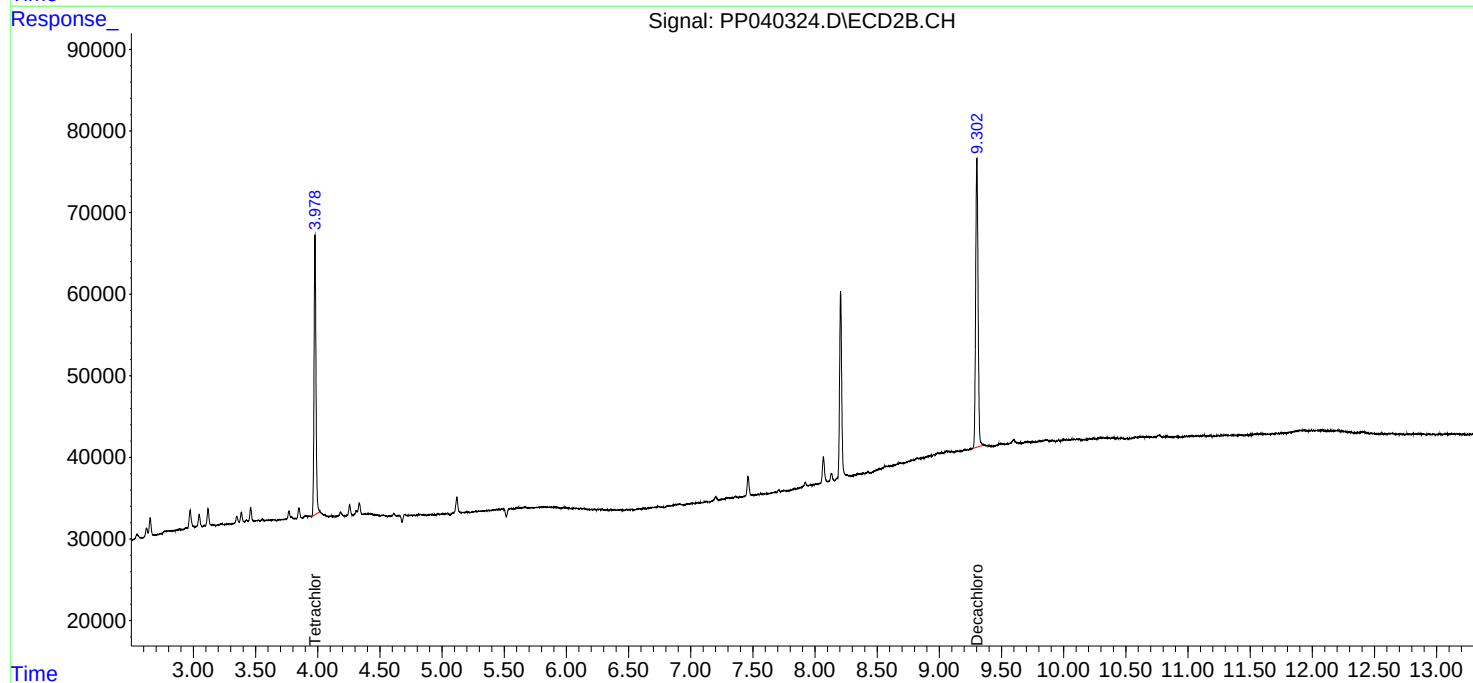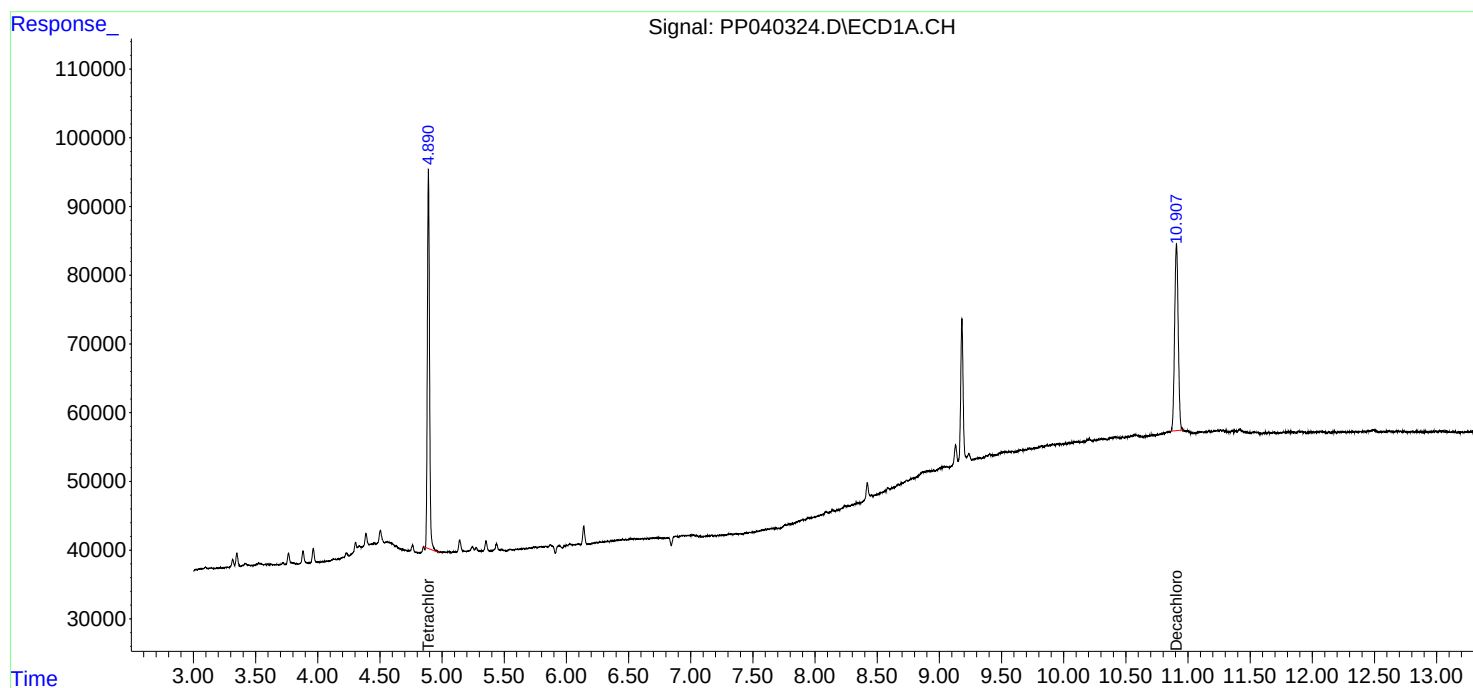


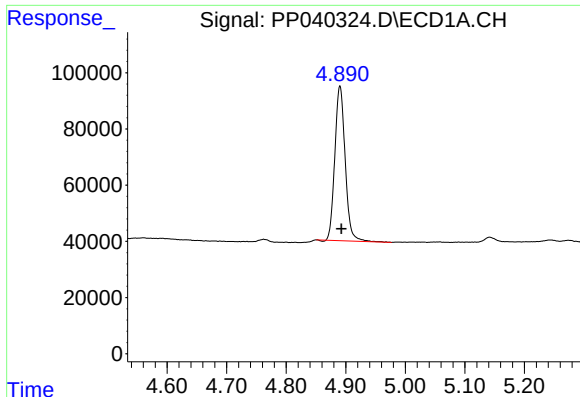

#1 Tetrachloro-m-xylene


R.T.: 4.890 min  
Delta R.T.: -0.003 min  
Response: 663930  
Conc: 21.86 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
20-SB-3-20211007-24.0-24.5

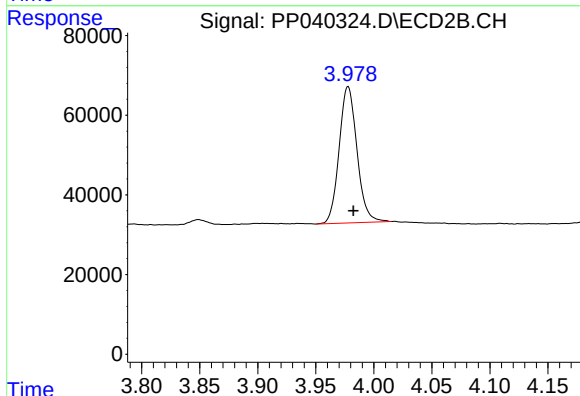


#1 Tetrachloro-m-xylene

R.T.: 3.978 min  
Delta R.T.: -0.005 min  
Response: 366207  
Conc: 21.66 ng/ml

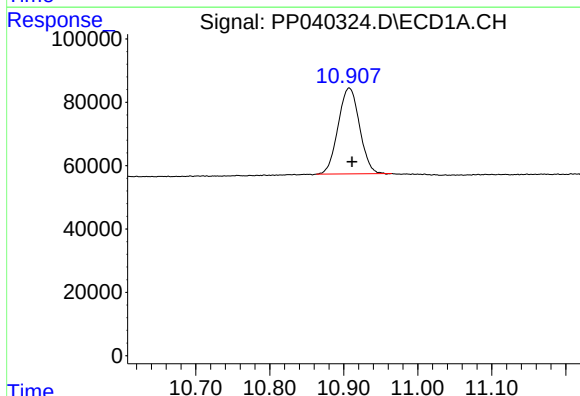

#2 Decachlorobiphenyl

R.T.: 10.907 min  
Delta R.T.: -0.004 min  
Response: 544514  
Conc: 22.03 ng/ml

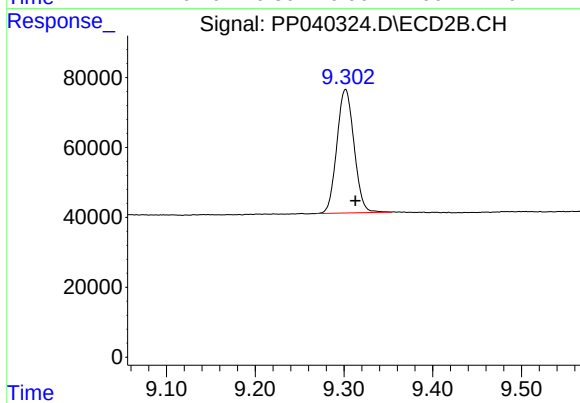

#2 Decachlorobiphenyl

R.T.: 9.302 min  
Delta R.T.: -0.011 min  
Response: 476337  
Conc: 22.44 ng/ml