

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102124\
 Data File : PP068110.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Oct 2024 20:27
 Operator : YP\AJ
 Sample : P4457-10 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC260234LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :Ankita Jodhani 10/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 04:15:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.755	4.052	1876776	1721817	2.028m	1.704m
2) SA Decachlor...	10.667	9.209	2384937	1642596	2.072m	1.465m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102124\
Data File : PP068110.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Oct 2024 20:27
Operator : YP\AJ
Sample : P4457-10 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC260234LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :Ankita Jodhani 10/22/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 04:15:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

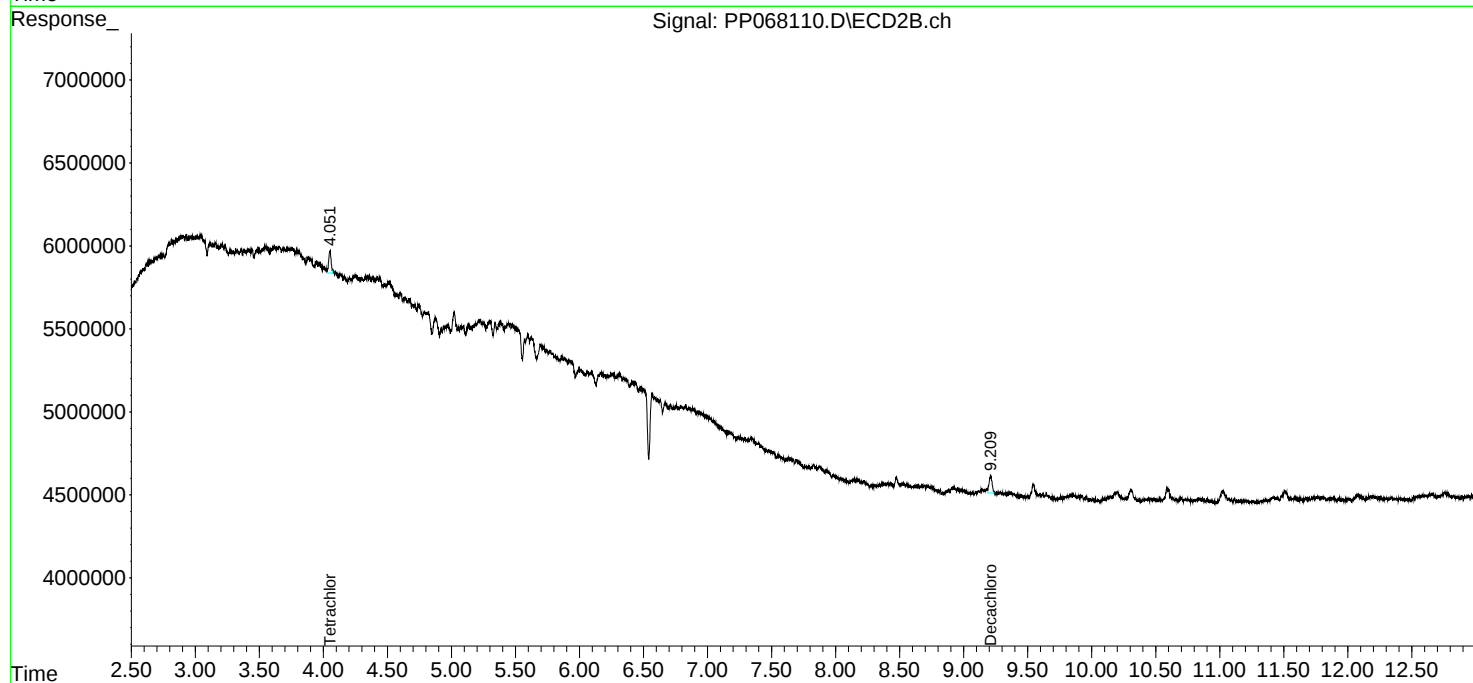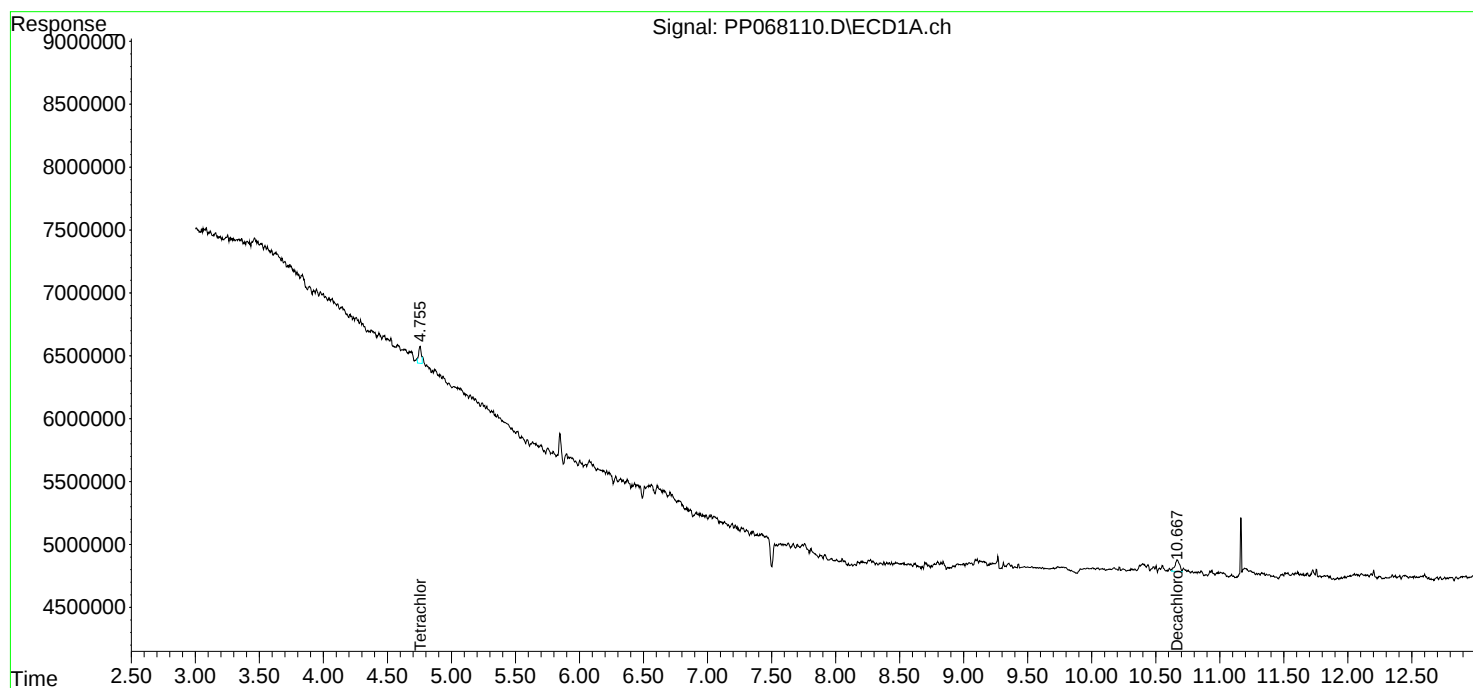

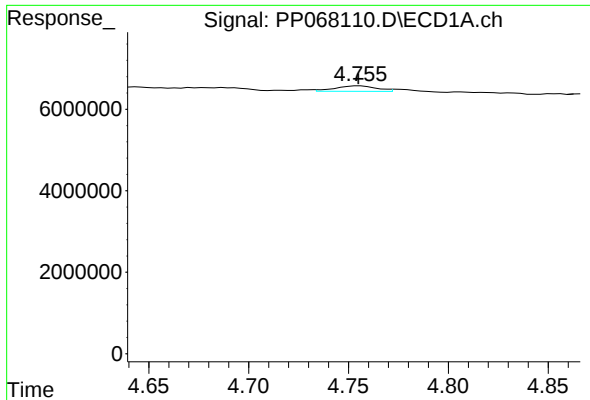


#1 Tetrachloro-m-xylene

R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 1876776
Conc: 2.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC260234LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :Ankita Jodhani 10/22/2024

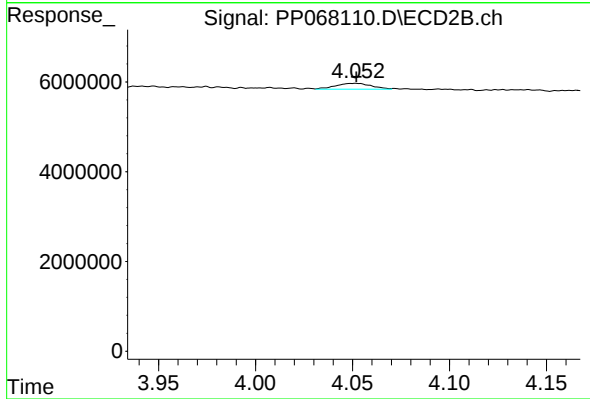


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 1721817
Conc: 1.70 ng/ml m

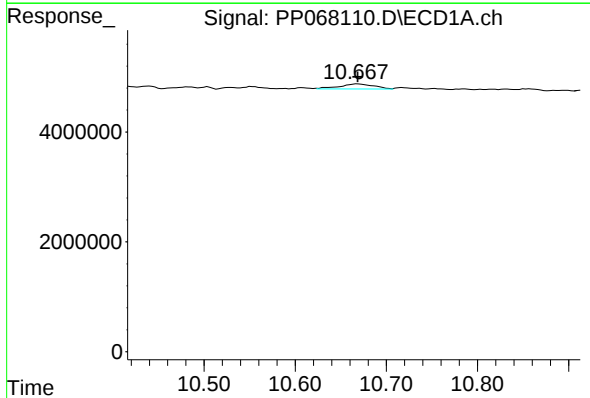

#2 Decachlorobiphenyl

R.T.: 10.667 min
Delta R.T.: -0.002 min
Response: 2384937
Conc: 2.07 ng/ml m

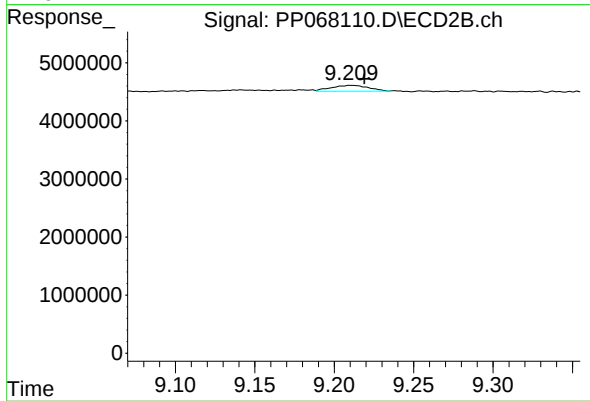

#2 Decachlorobiphenyl

R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 1642596
Conc: 1.46 ng/ml m