

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102220\
 Data File : PP030774.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 15:26
 Operator : DD\AJ
 Sample : MDL-AR1221-S-1
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1221-S-1

Manual Integrations
 APPROVED

Ankita
 10/24/2020 9:49:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 08:09:50 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 22 12:07:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.804	4.089	1115792	1031961	16.814	16.629
2)	SA Decachlor...	10.687	9.431	635176	647861	17.450	17.349
Target Compounds							
8)	L2 AR-1221-1	5.053	4.350	20457	20134	31.787m	35.506m
9)	L2 AR-1221-2	5.150	4.446	28817	20606	62.019m	49.429
10)	L2 AR-1221-3	5.233	4.539	44530	34728	29.959	25.282

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102220\
Data File : PP030774.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 15:26
Operator : DD\AJ
Sample : MDL-AR1221-S-1
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
MDL-AR1221-S-1


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 08:09:50 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 22 12:07:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

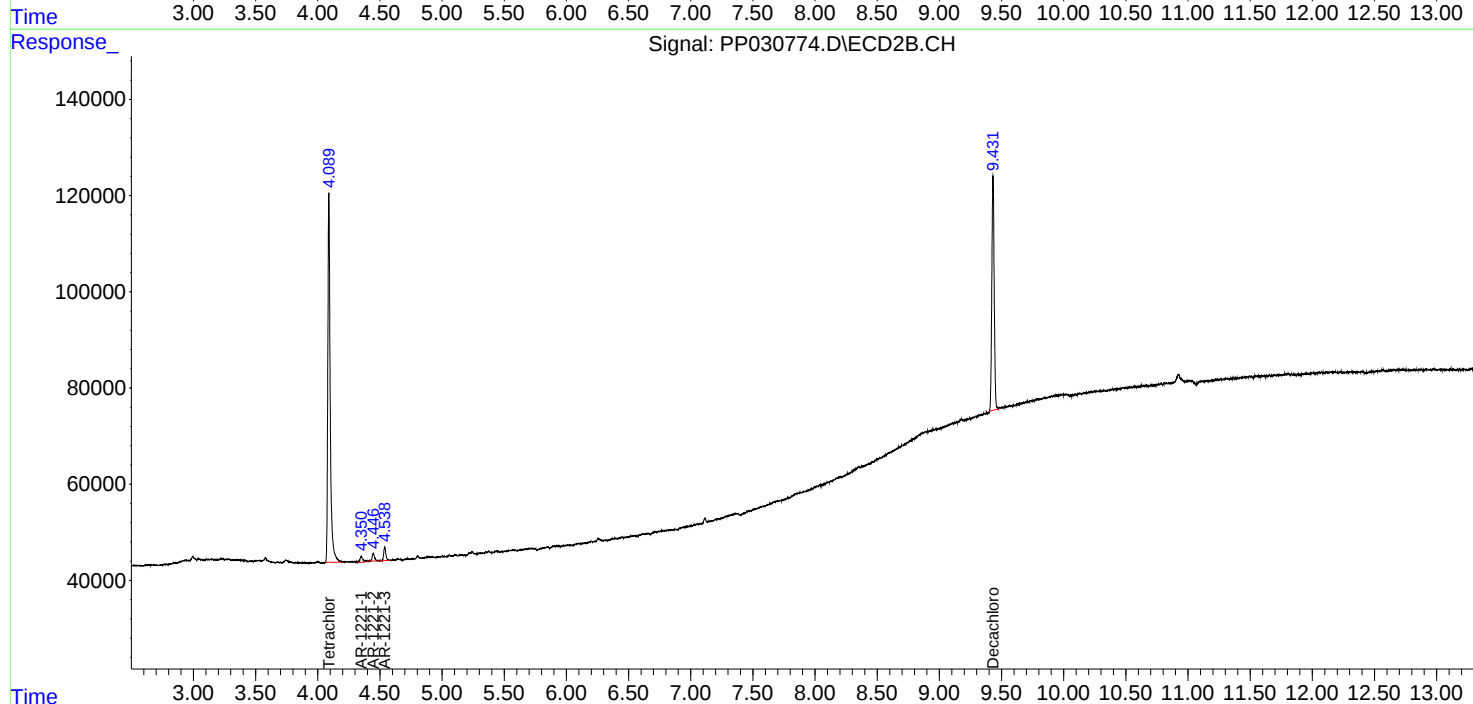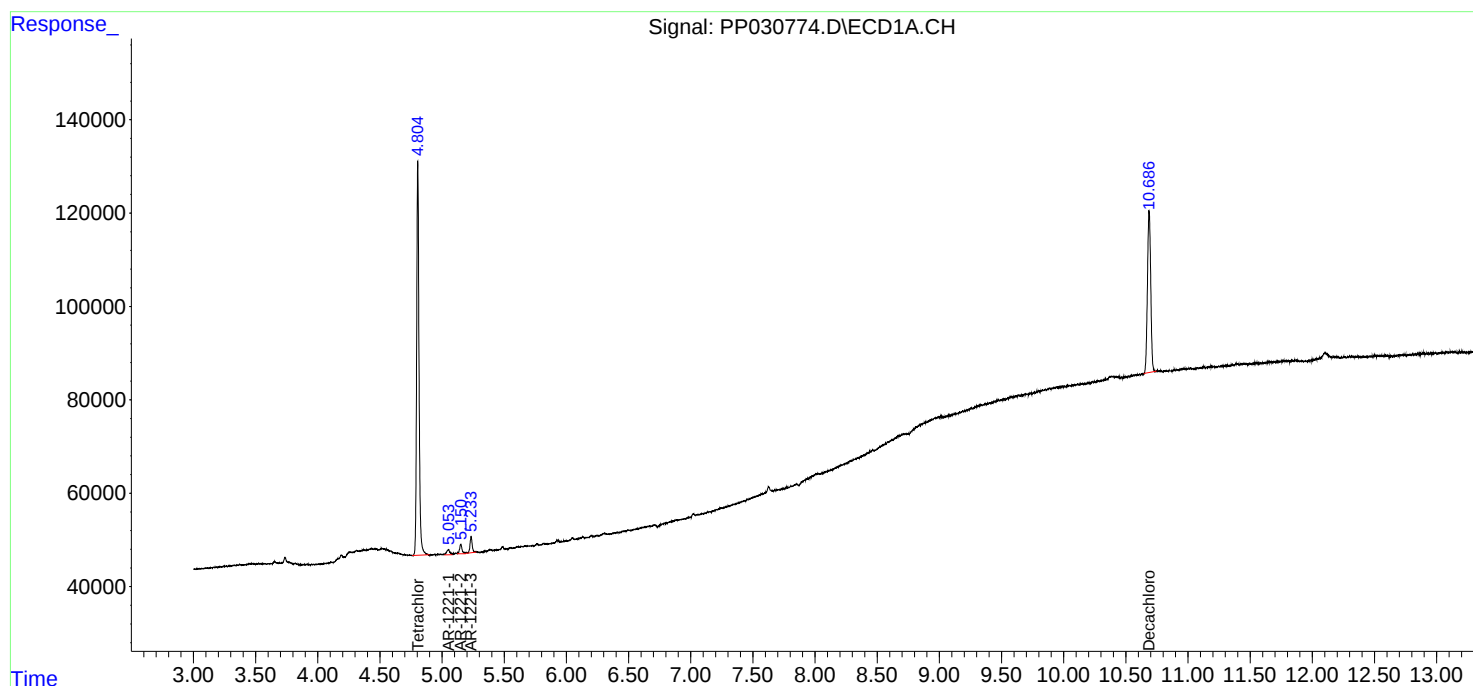

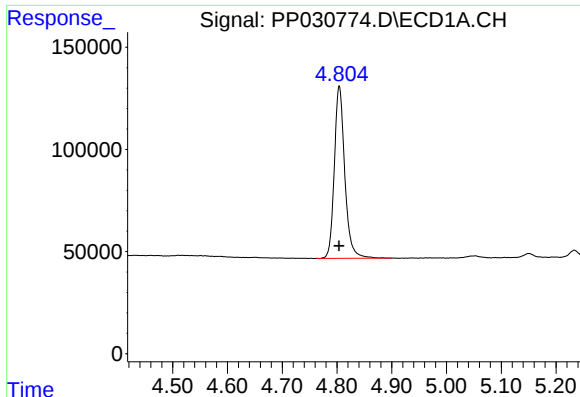


#1 Tetrachloro-m-xylene

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1115792
Conc: 16.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-1


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:05 AM

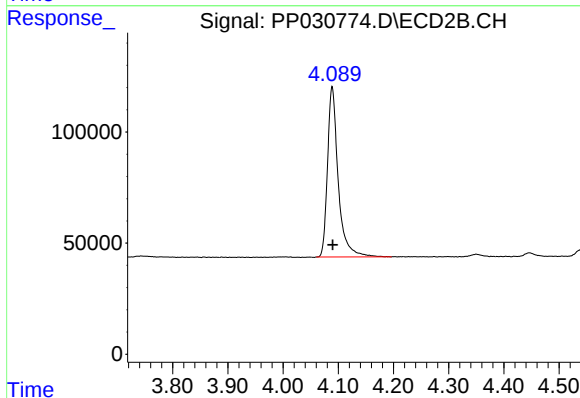


#1 Tetrachloro-m-xylene

R.T.: 4.089 min
Delta R.T.: -0.001 min
Response: 1031961
Conc: 16.63 ng/ml

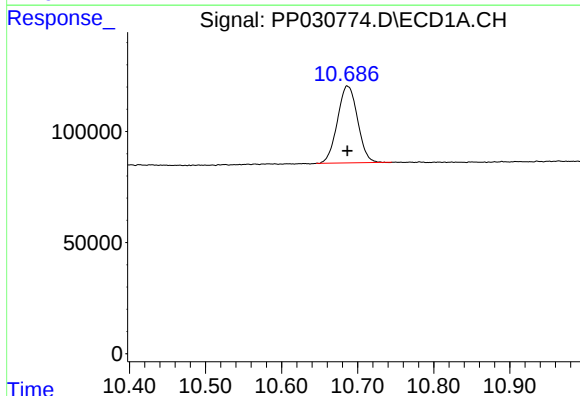


#2 Decachlorobiphenyl

R.T.: 10.687 min
Delta R.T.: 0.000 min
Response: 635176
Conc: 17.45 ng/ml

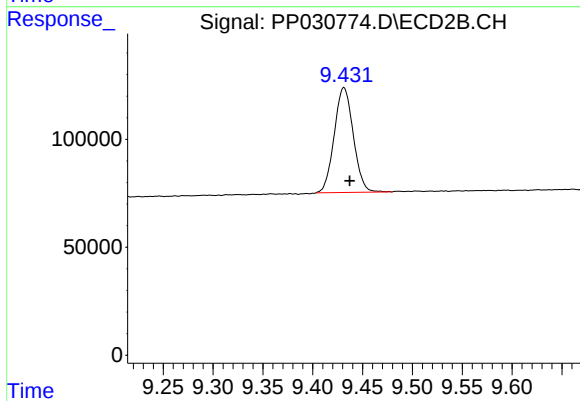

#2 Decachlorobiphenyl

R.T.: 9.431 min
Delta R.T.: -0.006 min
Response: 647861
Conc: 17.35 ng/ml

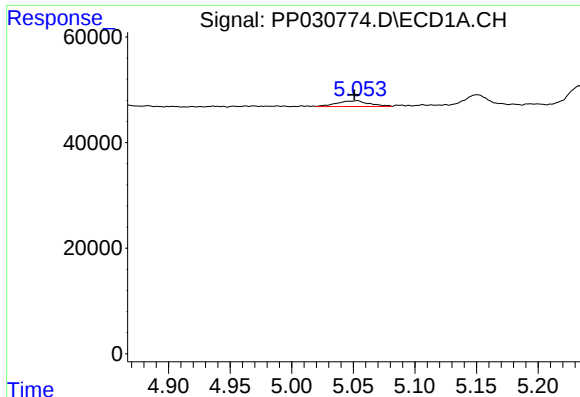


#8 AR-1221-1

R.T.: 5.053 min
Delta R.T.: 0.002 min
Response: 20457
Conc: 31.79 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-1


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:05 AM

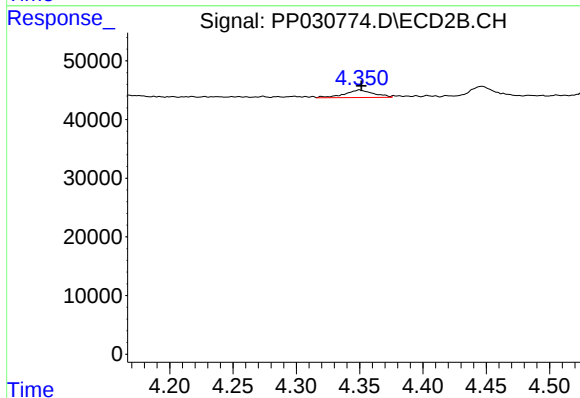


#8 AR-1221-1

R.T.: 4.350 min
Delta R.T.: -0.002 min
Response: 20134
Conc: 35.51 ng/ml m

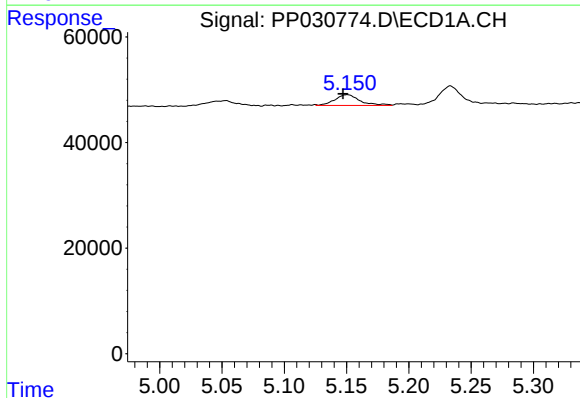


#9 AR-1221-2

R.T.: 5.150 min
Delta R.T.: 0.003 min
Response: 28817
Conc: 62.02 ng/ml m

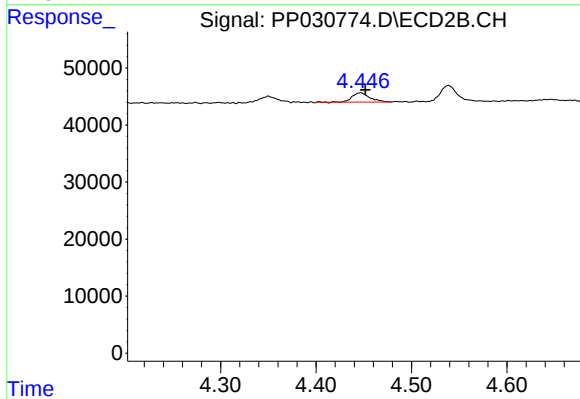

#9 AR-1221-2

R.T.: 4.446 min
Delta R.T.: -0.005 min
Response: 20606
Conc: 49.43 ng/ml

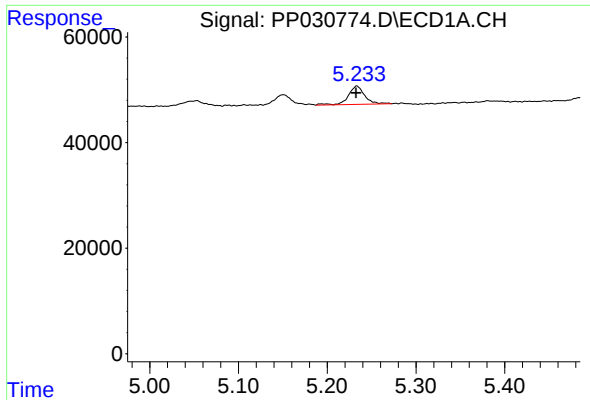


#10 AR-1221-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 44530
Conc: 29.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-1

Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:05 AM

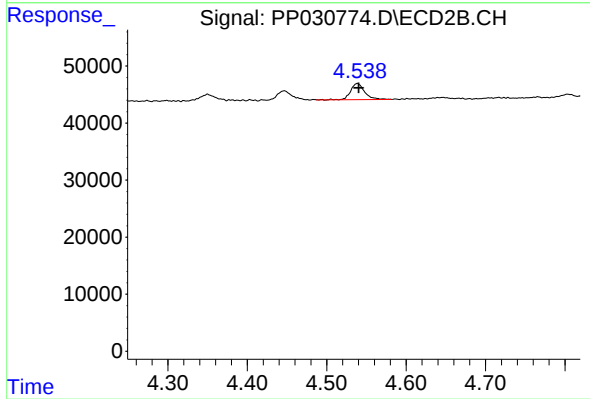

#10 AR-1221-3

R.T.: 4.539 min
Delta R.T.: -0.002 min
Response: 34728
Conc: 25.28 ng/ml