

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102220\
 Data File : PP030775.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 15:42
 Operator : DD\AJ
 Sample : MDL-AR1221-S-2
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1221-S-2

Manual Integrations
 APPROVED

Ankita
 10/24/2020 9:49:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 08:10:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 22 12:07:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.804	4.089	1142581	1077098	17.218	17.357
2)	SA Decachlor...	10.688	9.431	638515	642264	17.542	17.199
Target Compounds							
8)	L2 AR-1221-1	5.048	4.351	19863	17640	30.864m	31.109m
9)	L2 AR-1221-2	5.150	4.446	31155	23744	67.051	56.955
10)	L2 AR-1221-3	5.233	4.538	43220	36816	29.078	26.801

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102220\
Data File : PP030775.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 15:42
Operator : DD\AJ
Sample : MDL-AR1221-S-2
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
MDL-AR1221-S-2


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 08:10:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 22 12:07:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

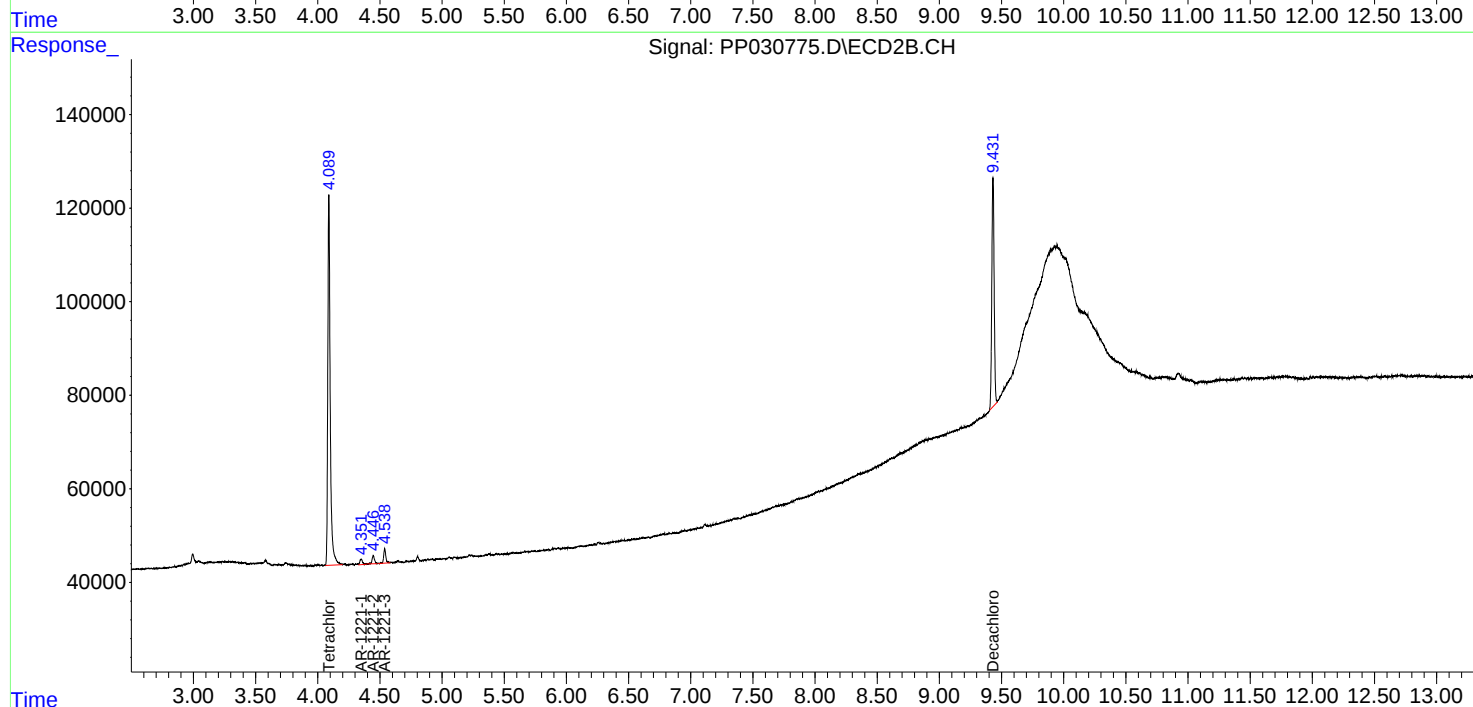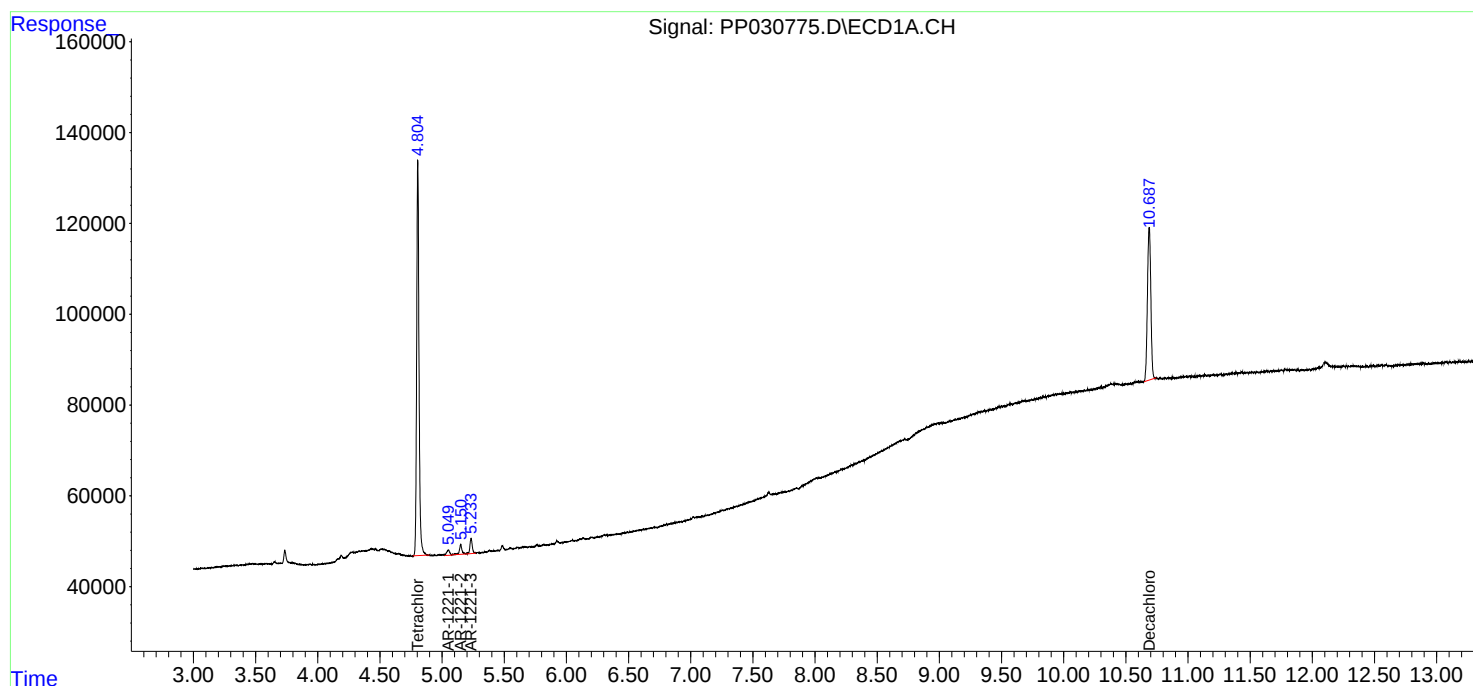

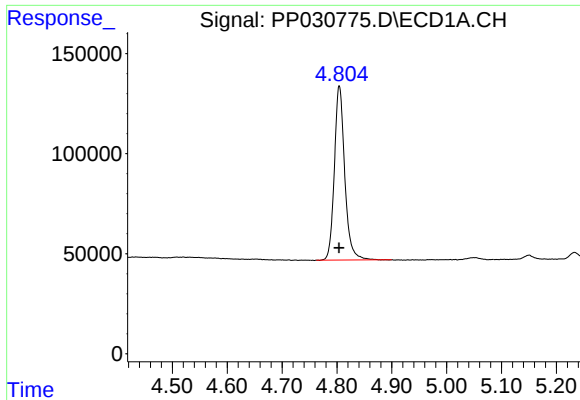


#1 Tetrachloro-m-xylene

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1142581
Conc: 17.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-2


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:08 AM

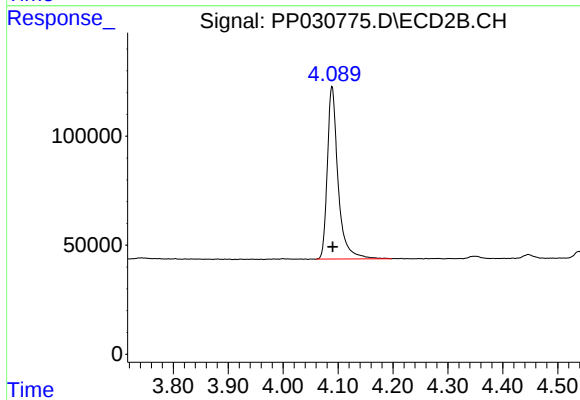


#1 Tetrachloro-m-xylene

R.T.: 4.089 min
Delta R.T.: -0.001 min
Response: 1077098
Conc: 17.36 ng/ml

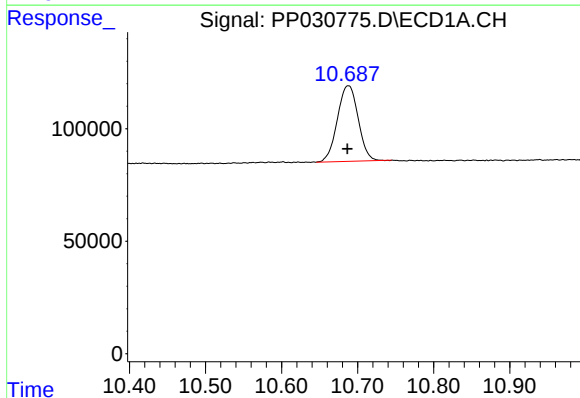


#2 Decachlorobiphenyl

R.T.: 10.688 min
Delta R.T.: 0.000 min
Response: 638515
Conc: 17.54 ng/ml

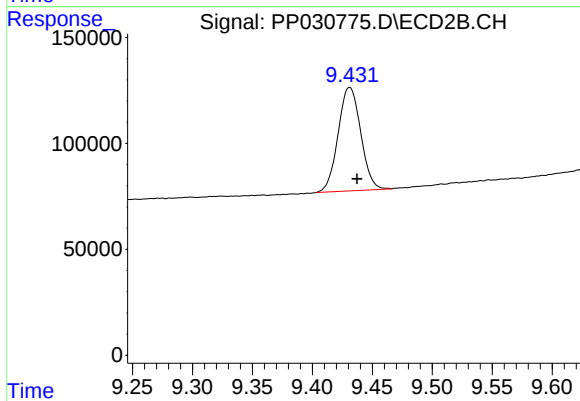

#2 Decachlorobiphenyl

R.T.: 9.431 min
Delta R.T.: -0.006 min
Response: 642264
Conc: 17.20 ng/ml

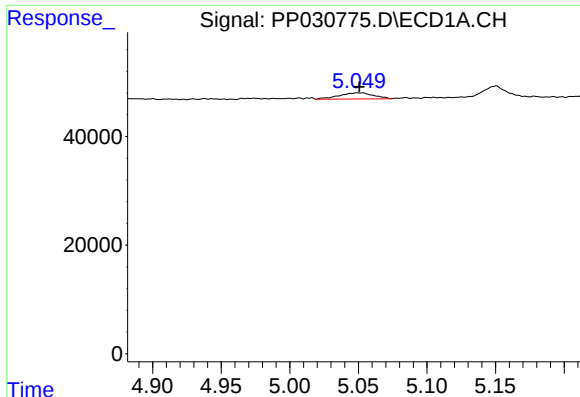


#8 AR-1221-1

R.T.: 5.048 min
Delta R.T.: -0.002 min
Response: 19863
Conc: 30.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-2


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:08 AM

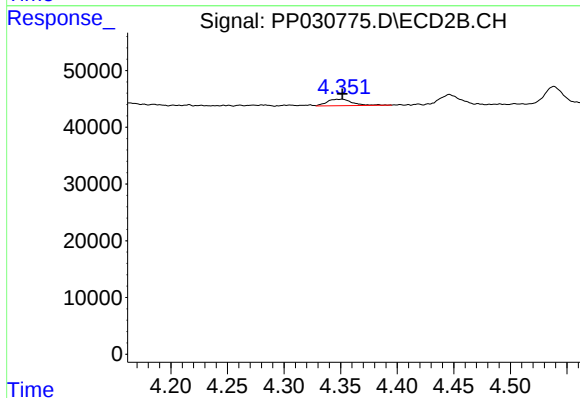


#8 AR-1221-1

R.T.: 4.351 min
Delta R.T.: 0.000 min
Response: 17640
Conc: 31.11 ng/ml m

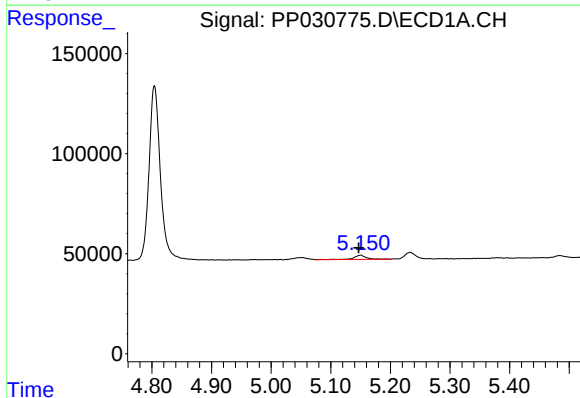


#9 AR-1221-2

R.T.: 5.150 min
Delta R.T.: 0.003 min
Response: 31155
Conc: 67.05 ng/ml

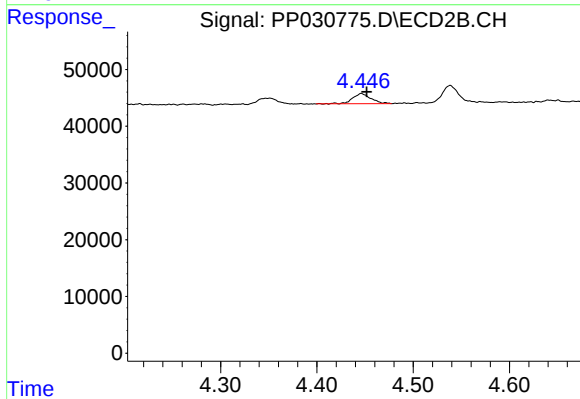

#9 AR-1221-2

R.T.: 4.446 min
Delta R.T.: -0.006 min
Response: 23744
Conc: 56.96 ng/ml

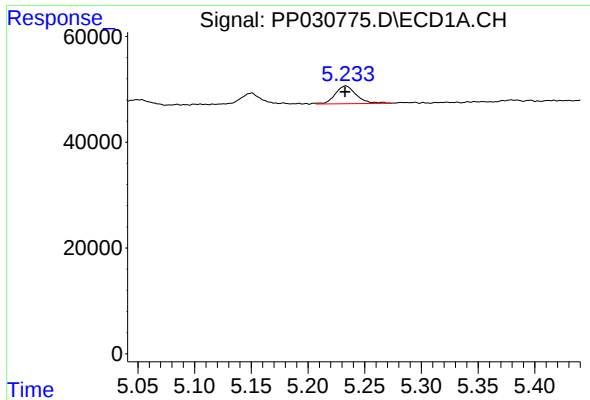


#10 AR-1221-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 43220
Conc: 29.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-2

Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:08 AM

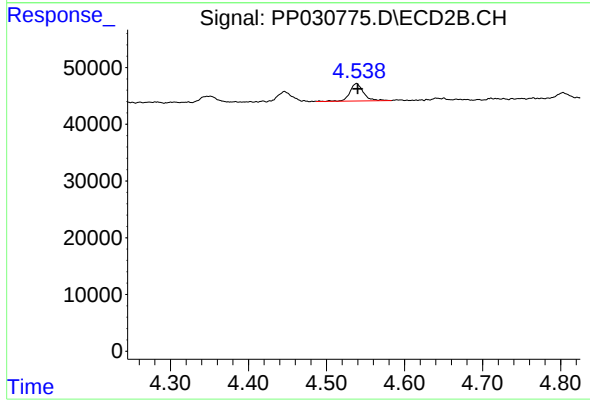

#10 AR-1221-3

R.T.: 4.538 min
Delta R.T.: -0.002 min
Response: 36816
Conc: 26.80 ng/ml