

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102220\
 Data File : PP030776.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2020 15:59
 Operator : DD\AJ
 Sample : MDL-AR1221-S-3
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-AR1221-S-3

Manual Integrations
 APPROVED

Ankita
 10/24/2020 9:49:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 08:10:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 22 12:07:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.804	4.088	1178973	1083188	17.766	17.455
2)	SA Decachlor...	10.687	9.430	622961	621235	17.114	16.636
Target Compounds							
8)	L2 AR-1221-1	5.047	4.350	18367	14710	28.539m	25.942m
9)	L2 AR-1221-2	5.148	4.447	28302	21624	60.912	51.870
10)	L2 AR-1221-3	5.233	4.538	43413	34690	29.207	25.254

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102220\
Data File : PP030776.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2020 15:59
Operator : DD\AJ
Sample : MDL-AR1221-S-3
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-3


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 08:10:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 22 12:07:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

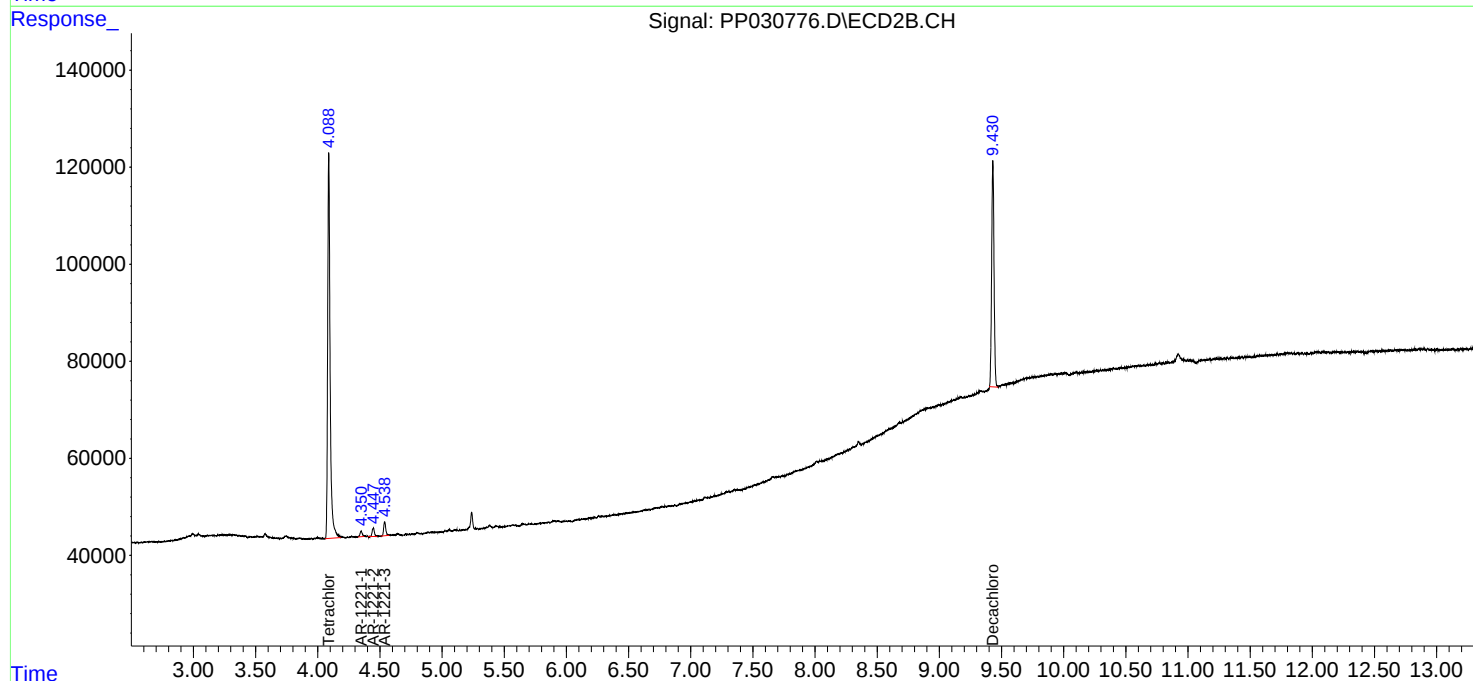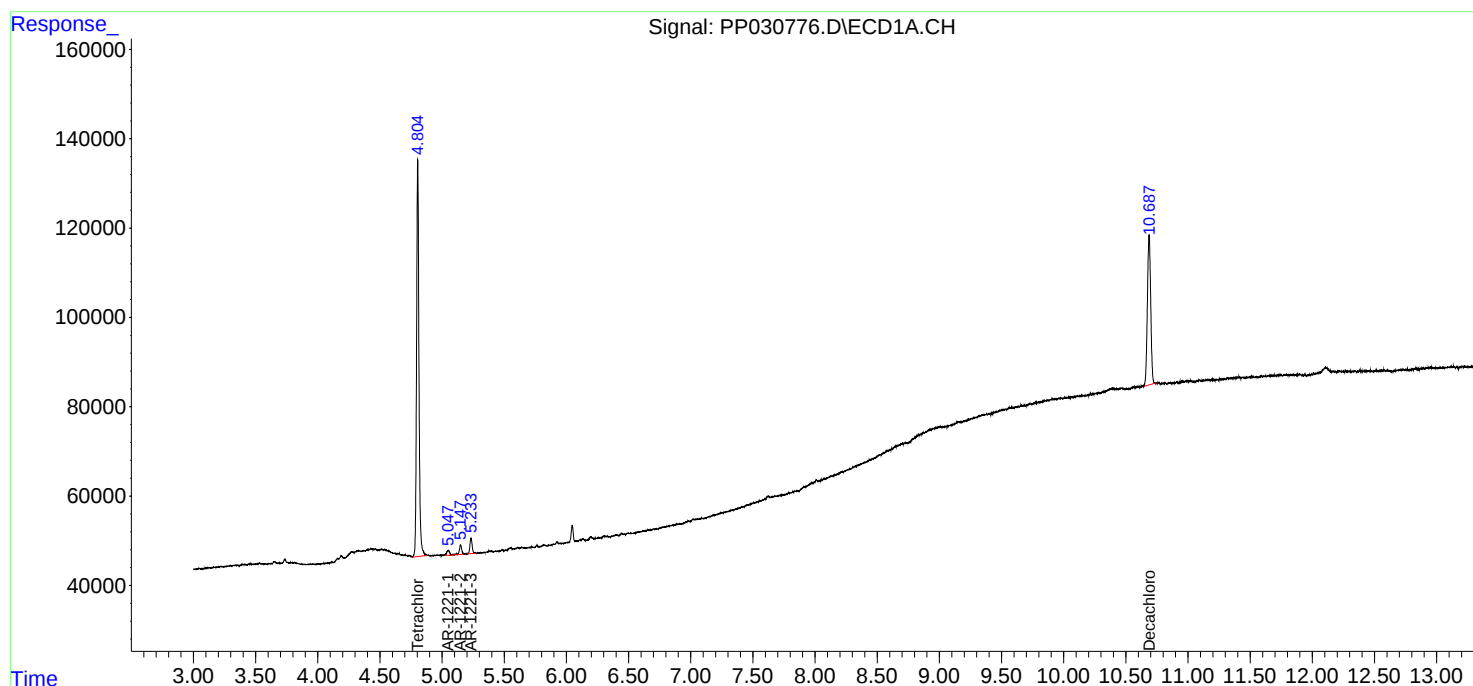

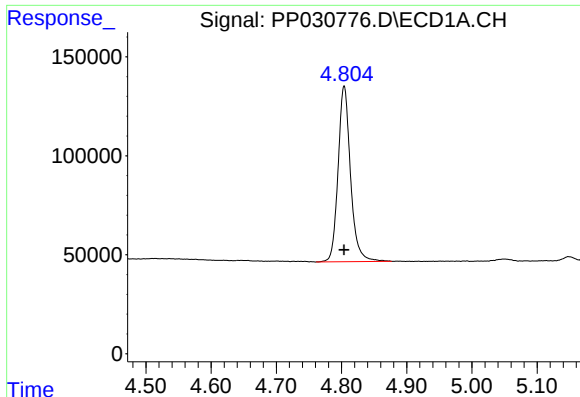


#1 Tetrachloro-m-xylene

R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1178973
Conc: 17.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-3


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:11 AM

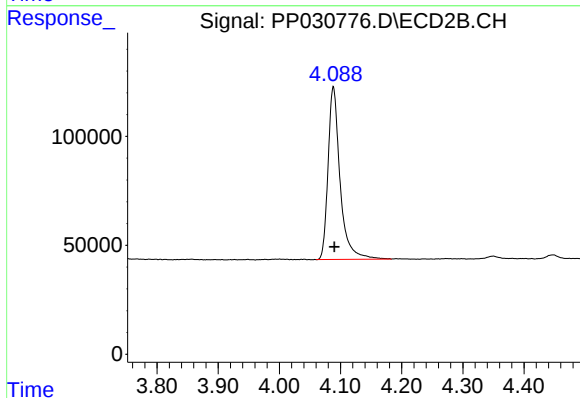


#1 Tetrachloro-m-xylene

R.T.: 4.088 min
Delta R.T.: -0.002 min
Response: 1083188
Conc: 17.45 ng/ml

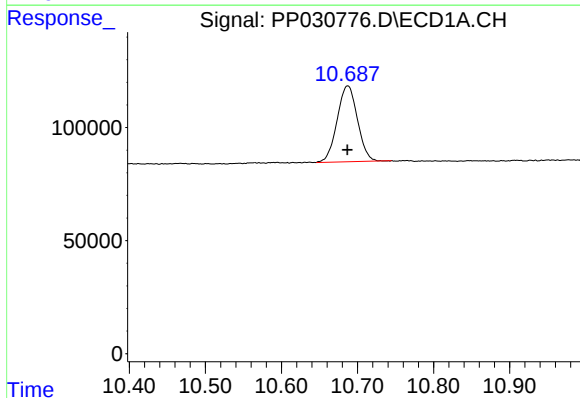


#2 Decachlorobiphenyl

R.T.: 10.687 min
Delta R.T.: 0.000 min
Response: 622961
Conc: 17.11 ng/ml

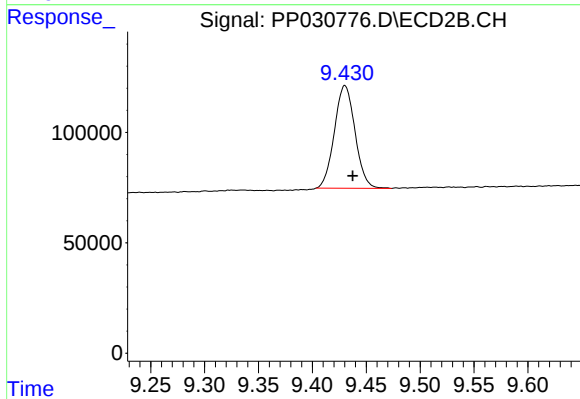

#2 Decachlorobiphenyl

R.T.: 9.430 min
Delta R.T.: -0.007 min
Response: 621235
Conc: 16.64 ng/ml

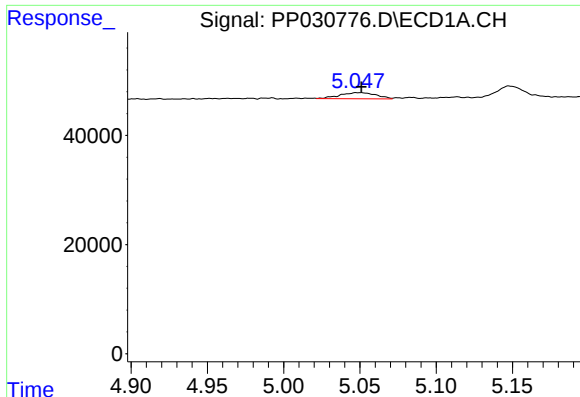


#8 AR-1221-1

R.T.: 5.047 min
Delta R.T.: -0.004 min
Response: 18367
Conc: 28.54 ng/ml m

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-3


Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:11 AM

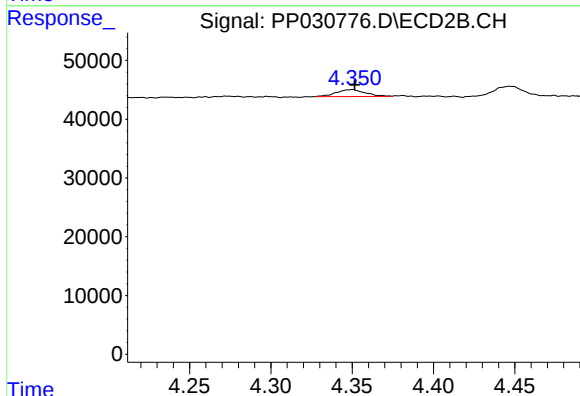


#8 AR-1221-1

R.T.: 4.350 min
Delta R.T.: -0.002 min
Response: 14710
Conc: 25.94 ng/ml m

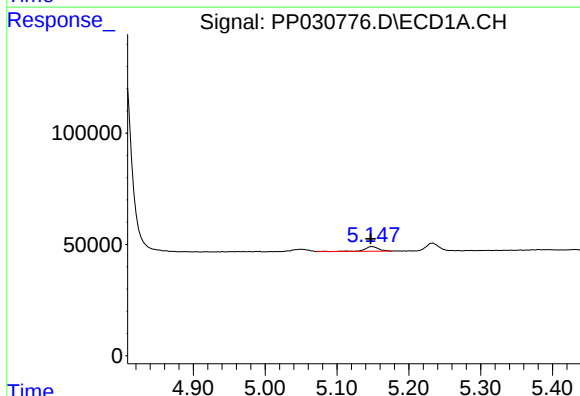


#9 AR-1221-2

R.T.: 5.148 min
Delta R.T.: 0.001 min
Response: 28302
Conc: 60.91 ng/ml

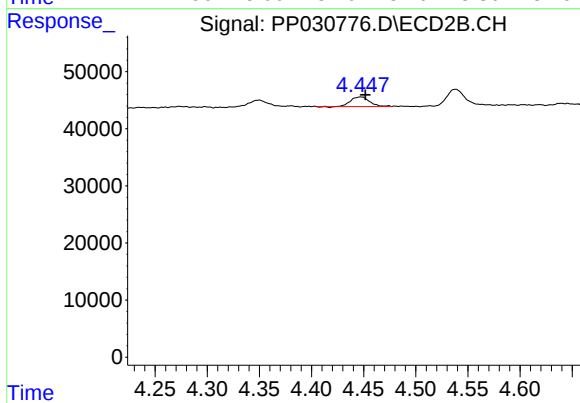

#9 AR-1221-2

R.T.: 4.447 min
Delta R.T.: -0.004 min
Response: 21624
Conc: 51.87 ng/ml

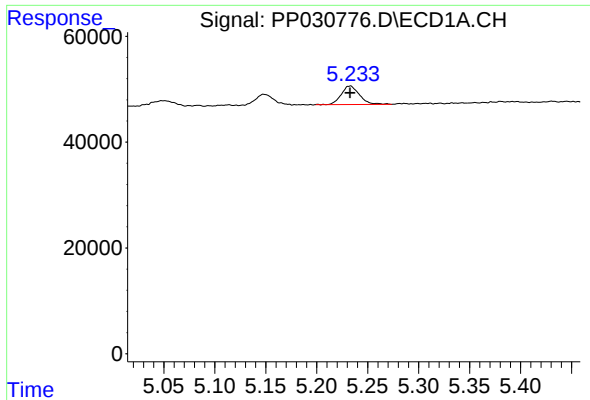


#10 AR-1221-3

R.T.: 5.233 min
Delta R.T.: 0.000 min
Response: 43413
Conc: 29.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-AR1221-S-3

Manual Integrations
APPROVED

Ankita
10/24/2020 9:49:11 AM

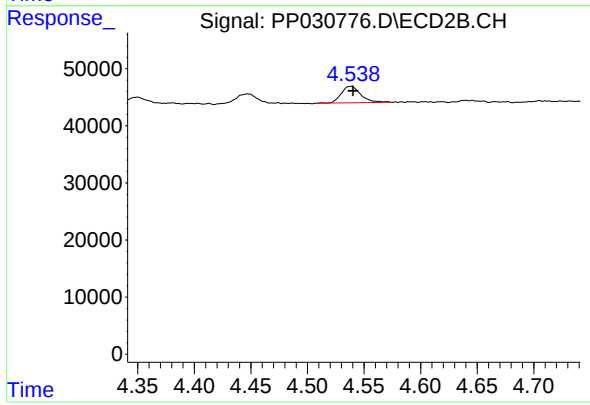

#10 AR-1221-3

R.T.: 4.538 min
Delta R.T.: -0.002 min
Response: 34690
Conc: 25.25 ng/ml