

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102220\  
 Data File : PP030782.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 22 Oct 2020 17:39  
 Operator : DD\AJ  
 Sample : MDL-PCB-BL-W-10  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 MDL-PCB-BL-W-10

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 23 08:11:15 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PP102120.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Oct 22 12:07:08 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|---------|--------|--------|
| -----                       |        |       |         |         |        |        |
| System Monitoring Compounds |        |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.804  | 4.087 | 1274089 | 1169566 | 19.200 | 18.847 |
| 2) SA Decachlor...          | 10.687 | 9.429 | 730282  | 743542  | 20.063 | 19.911 |

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102220\  
Data File : PP030782.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 22 Oct 2020 17:39  
Operator : DD\AJ  
Sample : MDL-PCB-BL-W-10  
Misc :  
ALS Vial : 16 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-PCB-BL-W-10

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 23 08:11:15 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PP102120.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Oct 22 12:07:08 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

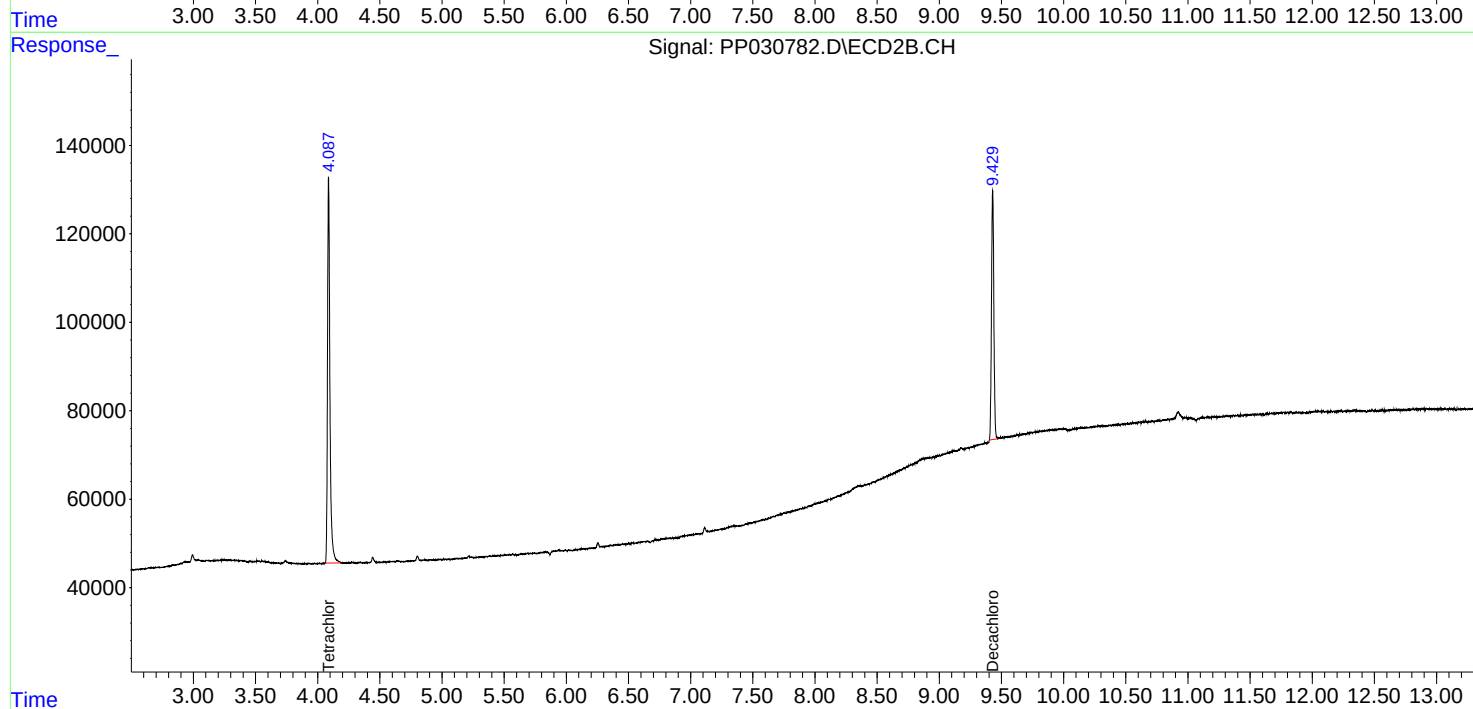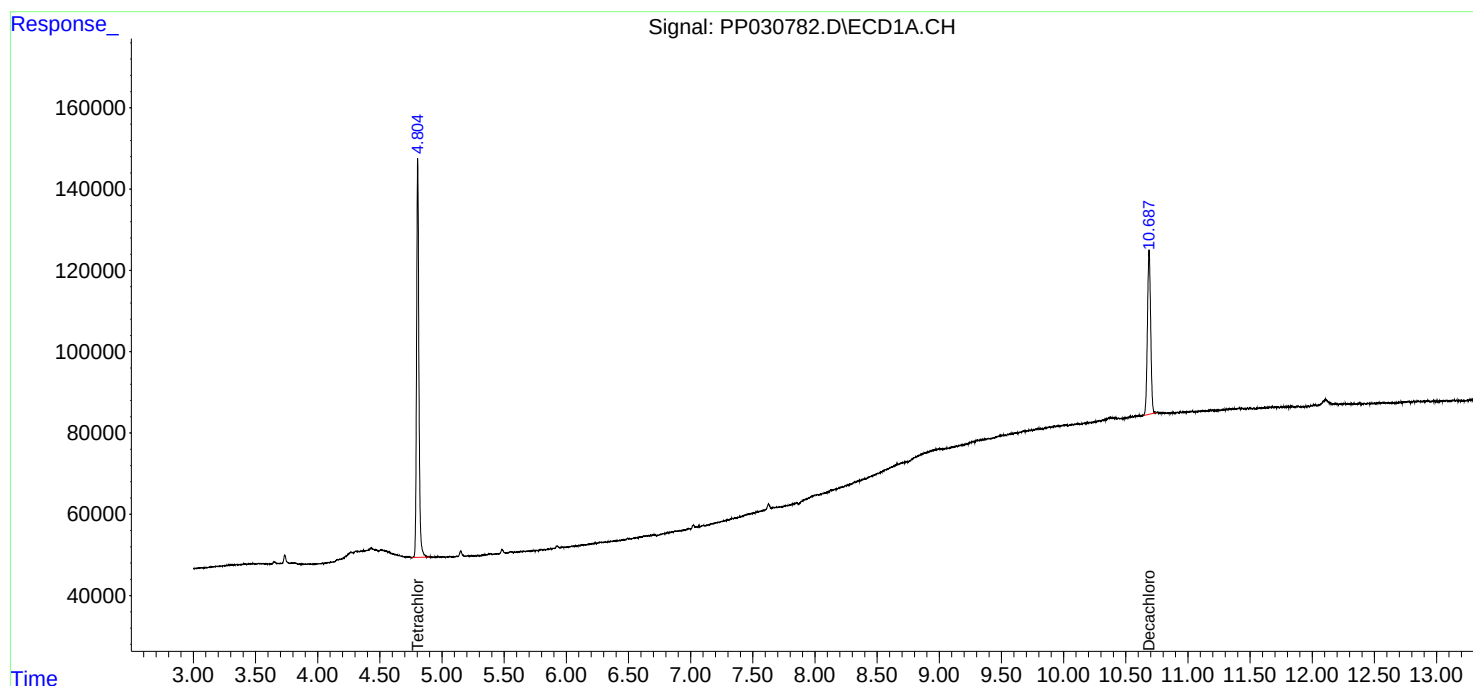


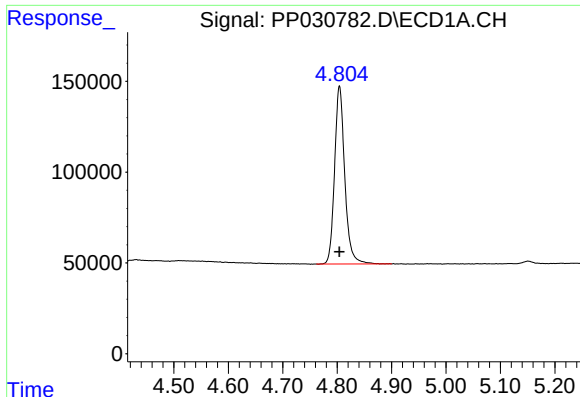

#1 Tetrachloro-m-xylene


R.T.: 4.804 min  
Delta R.T.: 0.000 min  
Response: 1274089  
Conc: 19.20 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-PCB-BL-W-10

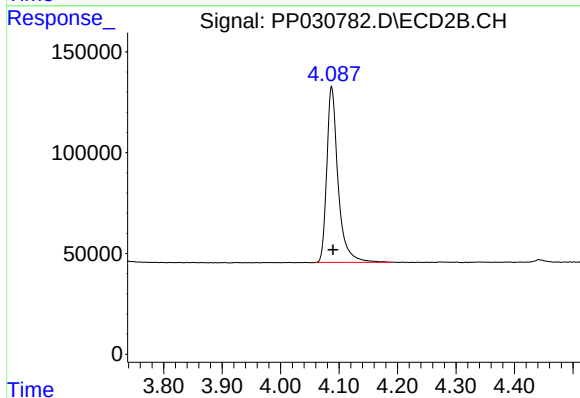


#1 Tetrachloro-m-xylene

R.T.: 4.087 min  
Delta R.T.: -0.003 min  
Response: 1169566  
Conc: 18.85 ng/ml

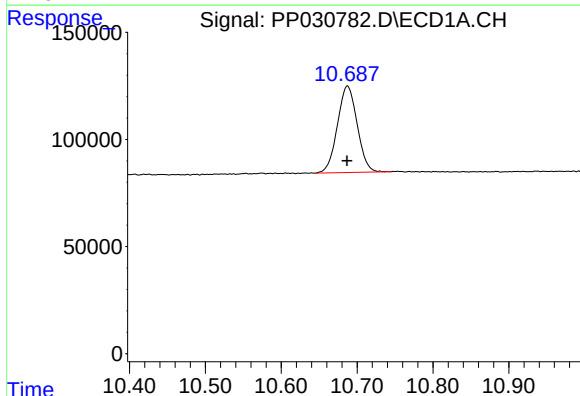

#2 Decachlorobiphenyl

R.T.: 10.687 min  
Delta R.T.: 0.000 min  
Response: 730282  
Conc: 20.06 ng/ml

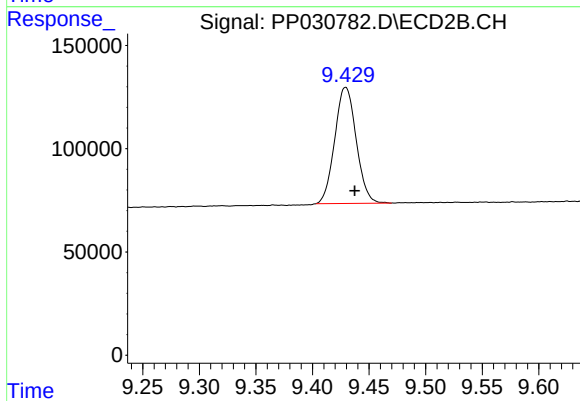

#2 Decachlorobiphenyl

R.T.: 9.429 min  
Delta R.T.: -0.008 min  
Response: 743542  
Conc: 19.91 ng/ml