

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102221\
 Data File : PP040388.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2021 20:12
 Operator : AJ\MA
 Sample : M4315-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 23:39:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.888	3.976	604364	345809	19.901	20.455
2) SA Decachlor...	10.903	9.298	366466	291317	14.827	13.727
Target Compounds						
8) L2 AR-1221-1	5.141	0.000	46567	0	133.714	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102221\
Data File : PP040388.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2021 20:12
Operator : AJ\MA
Sample : M4315-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 23:39:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

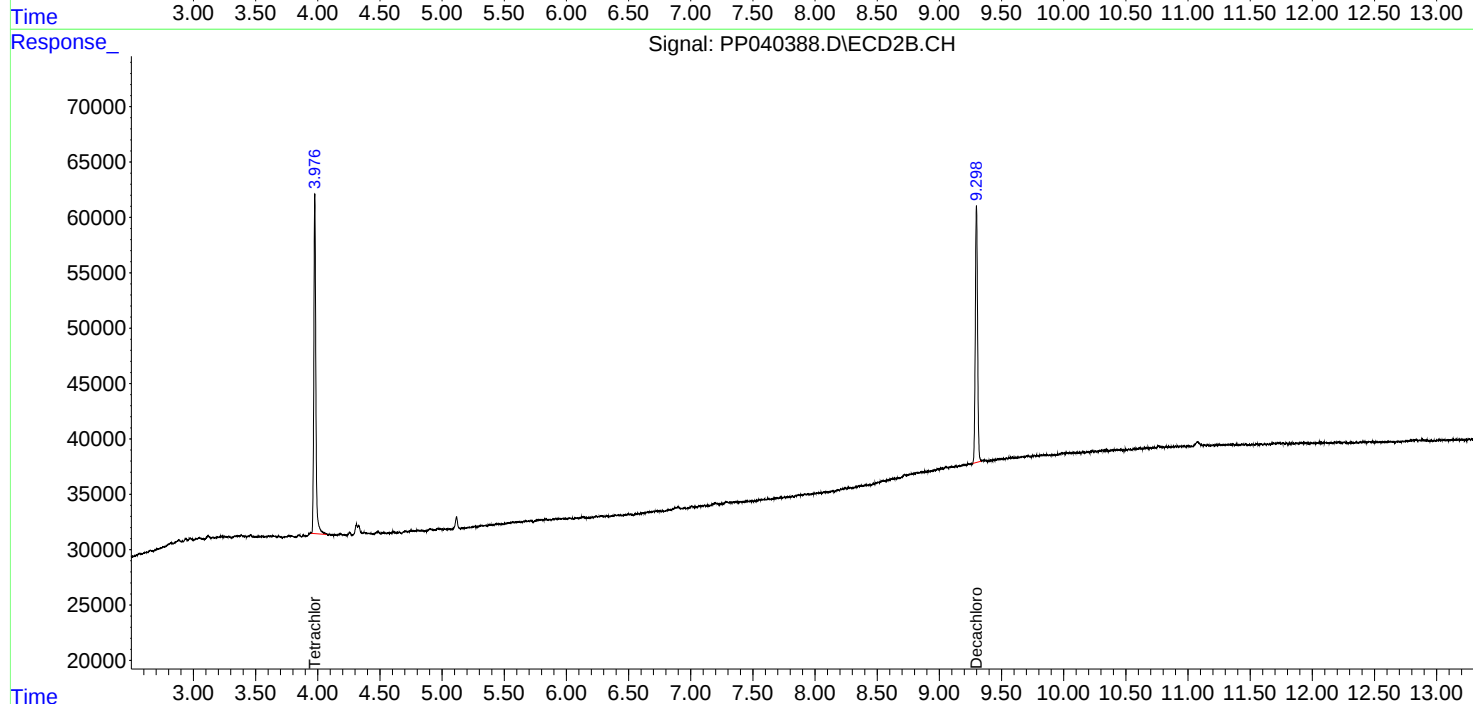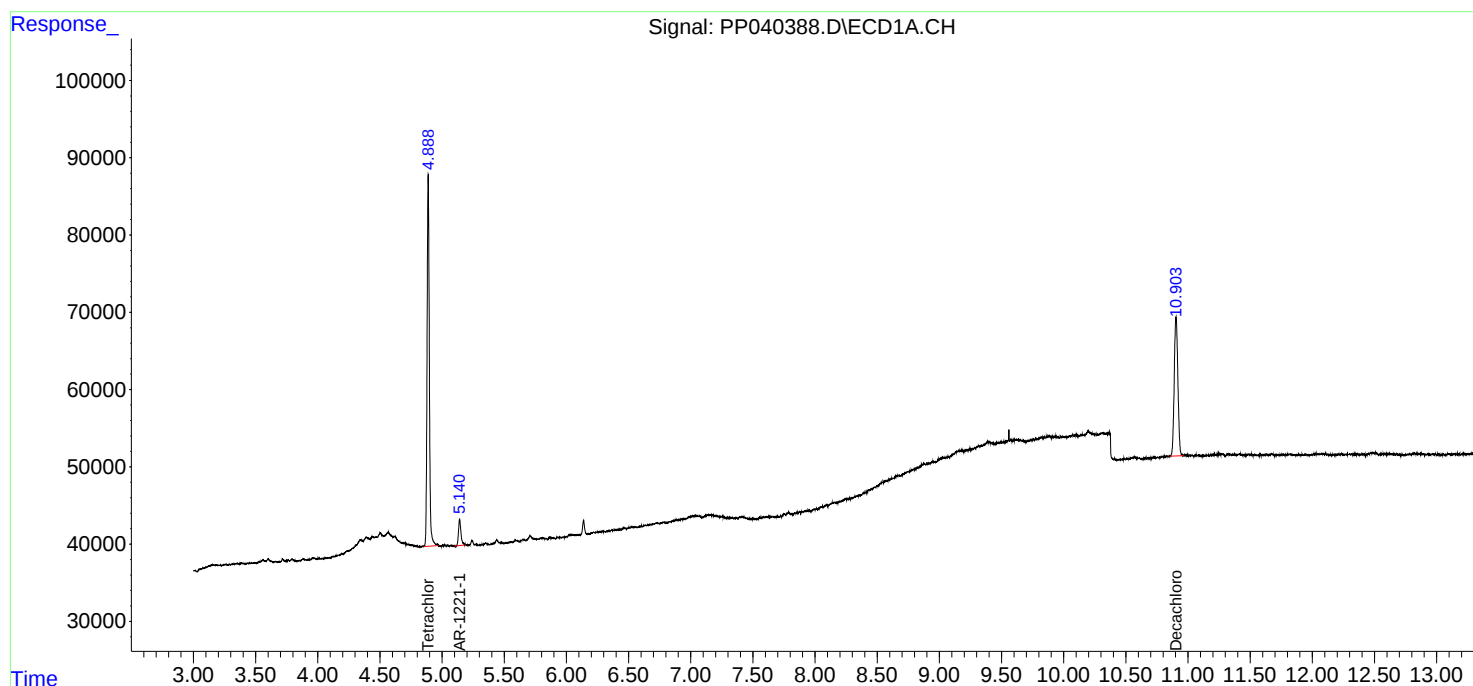


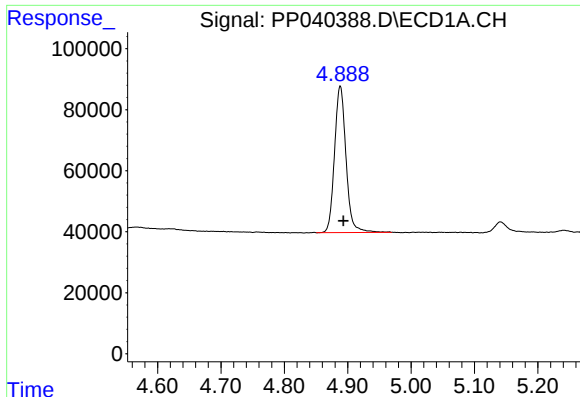

#1 Tetrachloro-m-xylene


R.T.: 4.888 min
Delta R.T.: -0.005 min
Response: 604364
Conc: 19.90 ng/ml

Instrument :
ECD_P
ClientSampleId :

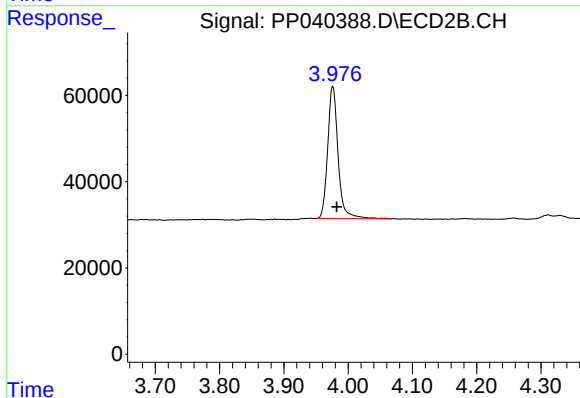


#1 Tetrachloro-m-xylene

R.T.: 3.976 min
Delta R.T.: -0.006 min
Response: 345809
Conc: 20.45 ng/ml

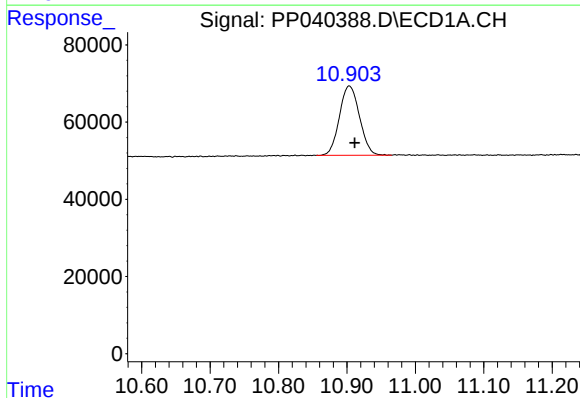


#2 Decachlorobiphenyl

R.T.: 10.903 min
Delta R.T.: -0.008 min
Response: 366466
Conc: 14.83 ng/ml

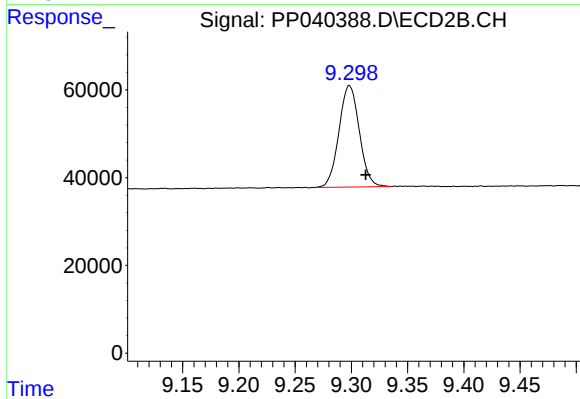

#2 Decachlorobiphenyl


R.T.: 9.298 min
Delta R.T.: -0.015 min
Response: 291317
Conc: 13.73 ng/ml

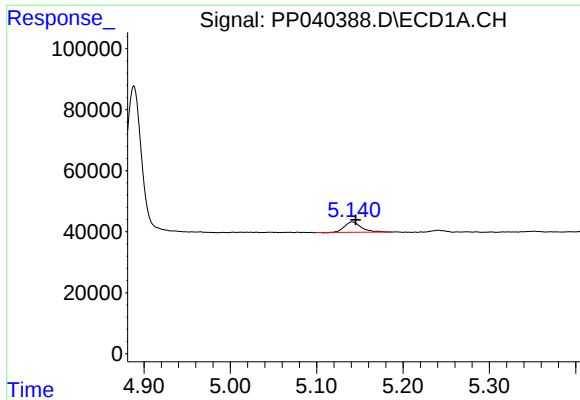

#8 AR-1221-1

R.T.: 5.141 min
Delta R.T.: -0.004 min
Response: 46567
Conc: 133.71 ng/ml

Instrument :
ECD_P
ClientSampleId :

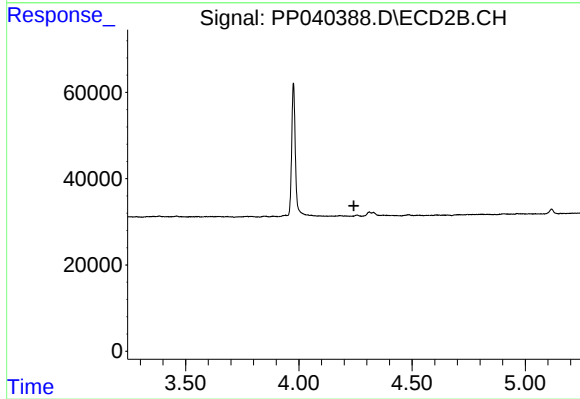

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.243 min
Response: 0
Conc: N.D.