

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102221\  
 Data File : PP040387.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 22 Oct 2021 19:56  
 Operator : AJ\MA  
 Sample : M4315-01  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 MH-D-S

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 22 23:38:51 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP101221.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Oct 13 08:03:59 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|--------|--------|--------|--------|
| -----                       |        |       |        |        |        |        |
| System Monitoring Compounds |        |       |        |        |        |        |
| 1) SA Tetrachlo...          | 4.889  | 3.976 | 700814 | 406469 | 23.077 | 24.043 |
| 2) SA Decachlor...          | 10.906 | 9.299 | 501336 | 358220 | 20.283 | 16.879 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102221\  
Data File : PP040387.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 22 Oct 2021 19:56  
Operator : AJ\MA  
Sample : M4315-01  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
MH-D-S

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 22 23:38:51 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP101221.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Oct 13 08:03:59 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

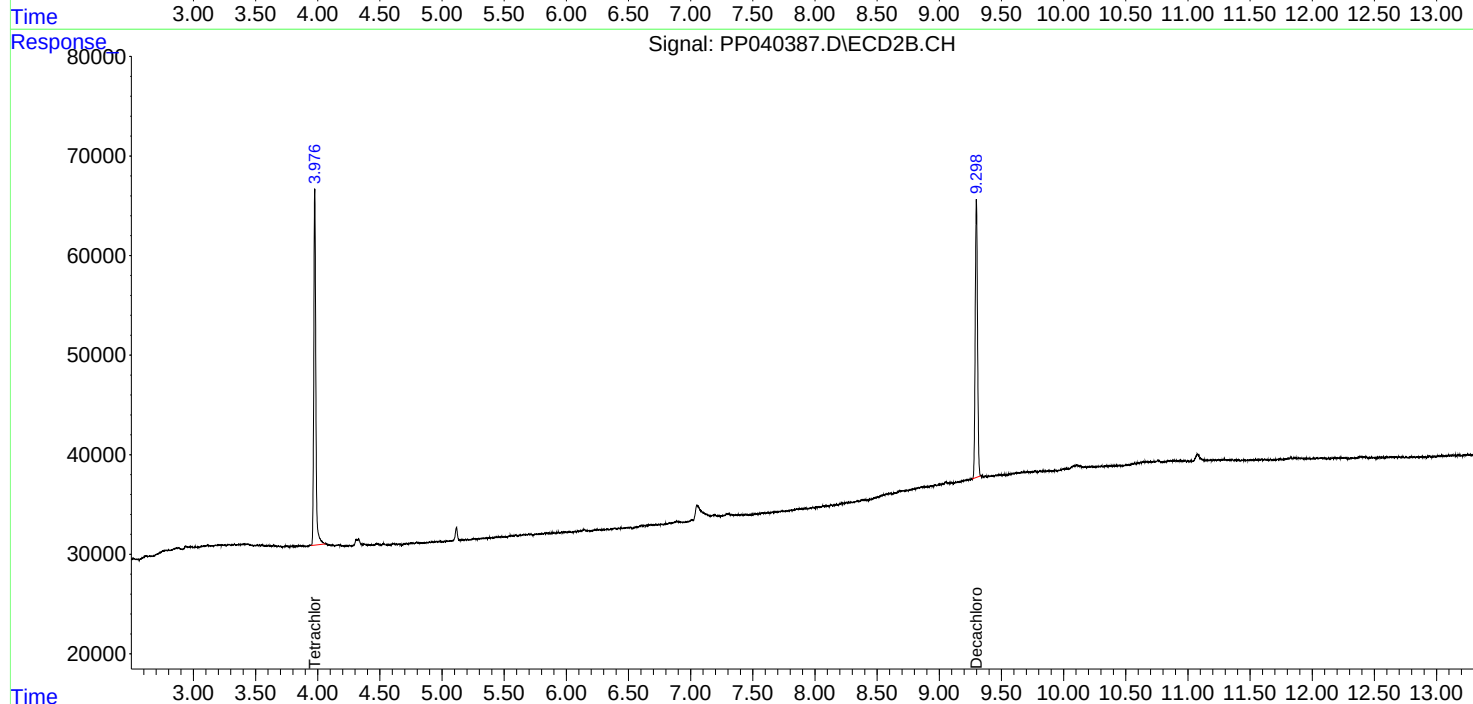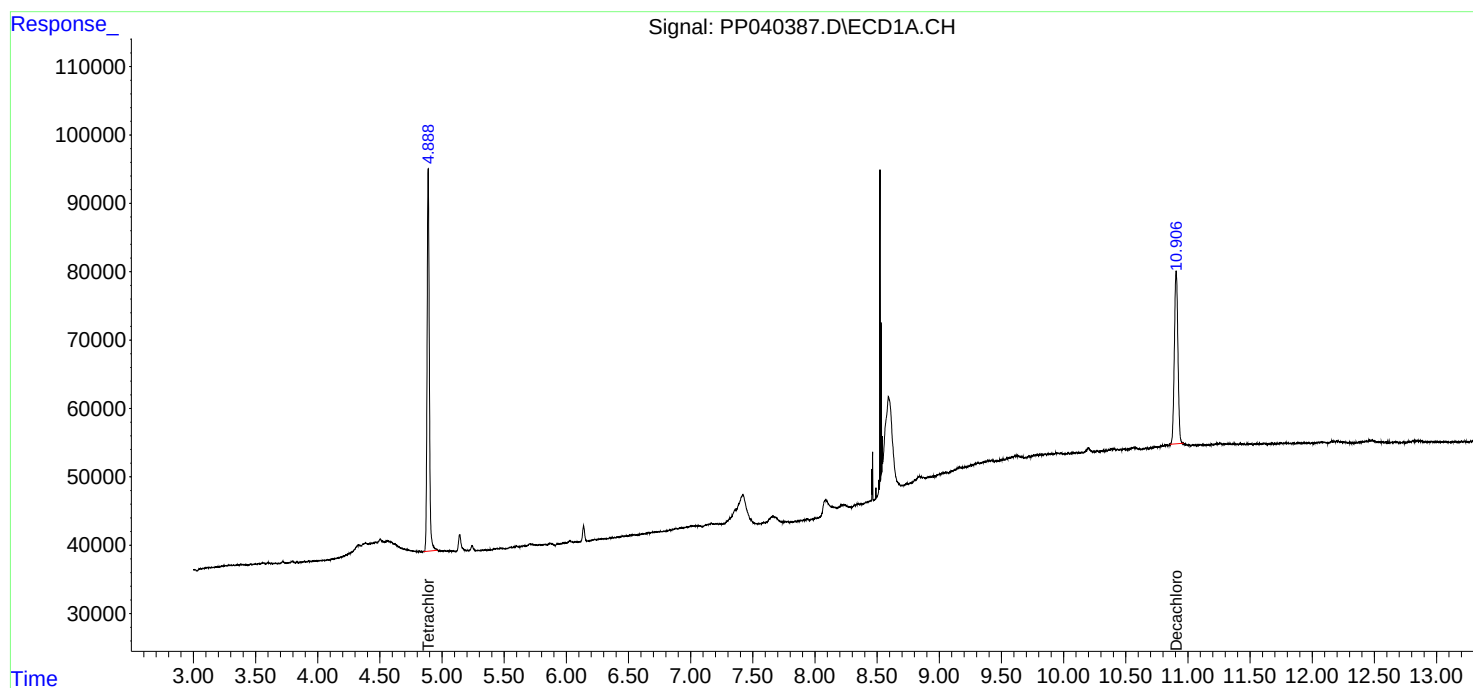


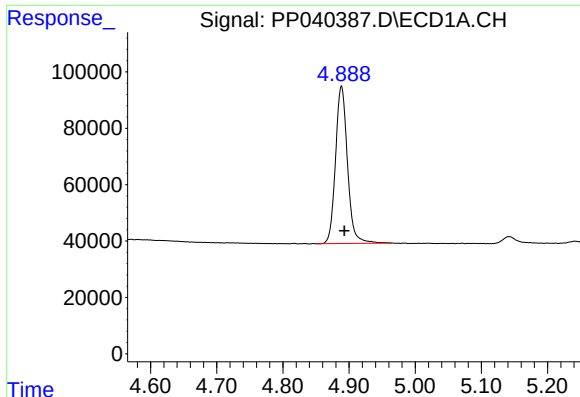

#1 Tetrachloro-m-xylene


R.T.: 4.889 min  
Delta R.T.: -0.004 min  
Response: 700814  
Conc: 23.08 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MH-D-S

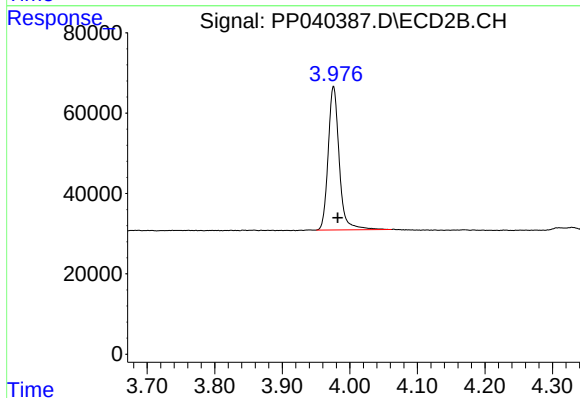


#1 Tetrachloro-m-xylene

R.T.: 3.976 min  
Delta R.T.: -0.006 min  
Response: 406469  
Conc: 24.04 ng/ml

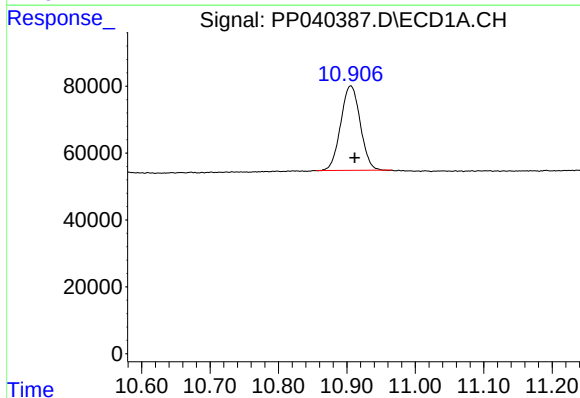

#2 Decachlorobiphenyl

R.T.: 10.906 min  
Delta R.T.: -0.006 min  
Response: 501336  
Conc: 20.28 ng/ml

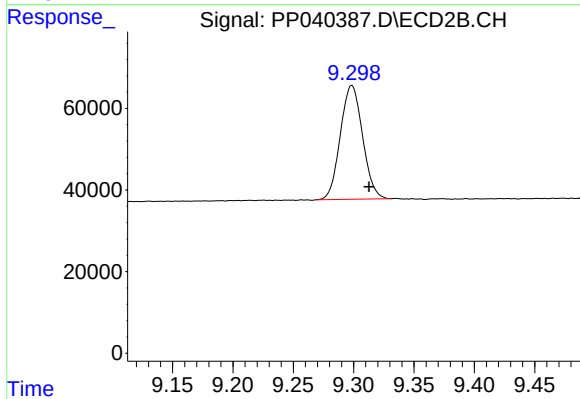

#2 Decachlorobiphenyl

R.T.: 9.299 min  
Delta R.T.: -0.014 min  
Response: 358220  
Conc: 16.88 ng/ml