

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102221\
 Data File : PP040398.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2021 23:27
 Operator : AJ\MA
 Sample : M4312-02 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 5255

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 22 23:41:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.886	3.975	90049	55768	2.965	3.299
2) SA Decachlor...	10.905	9.300	121338	71208	4.909	3.355 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102221\
Data File : PP040398.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2021 23:27
Operator : AJ\MA
Sample : M4312-02 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
5255

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 22 23:41:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

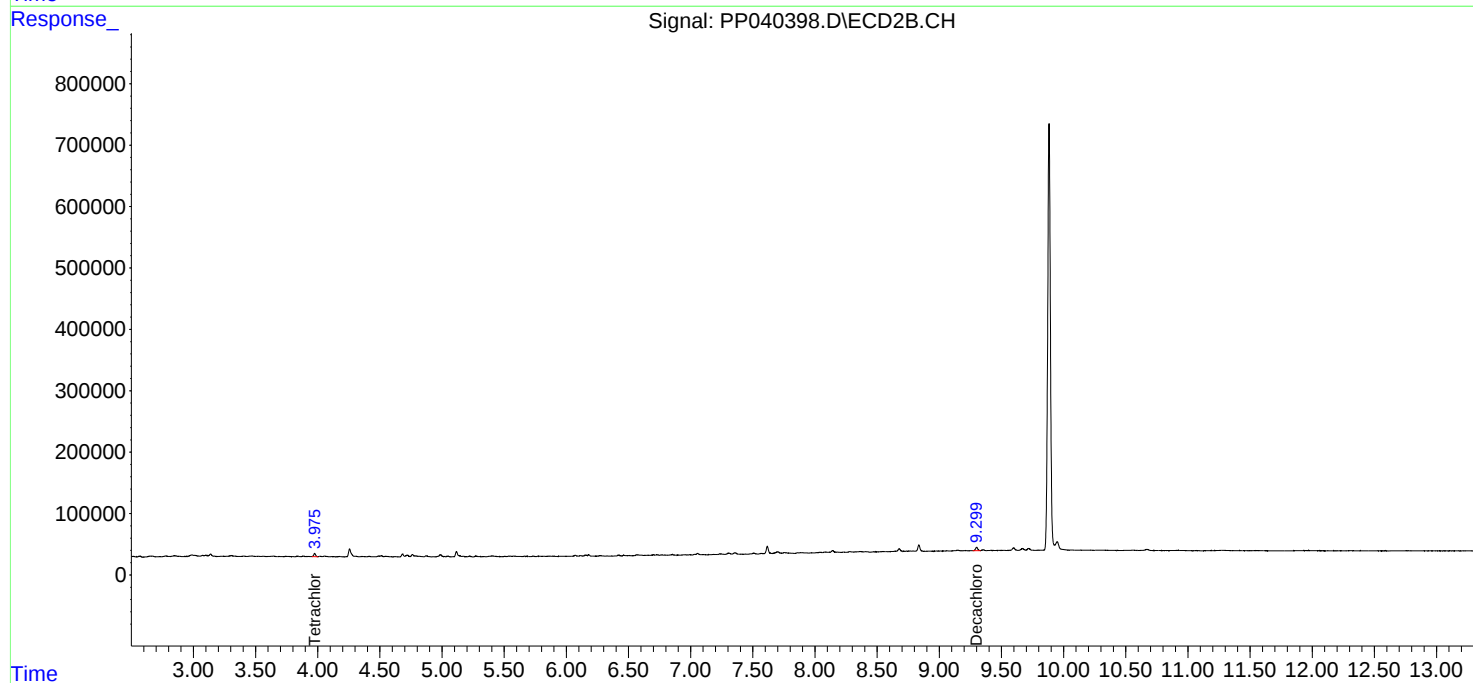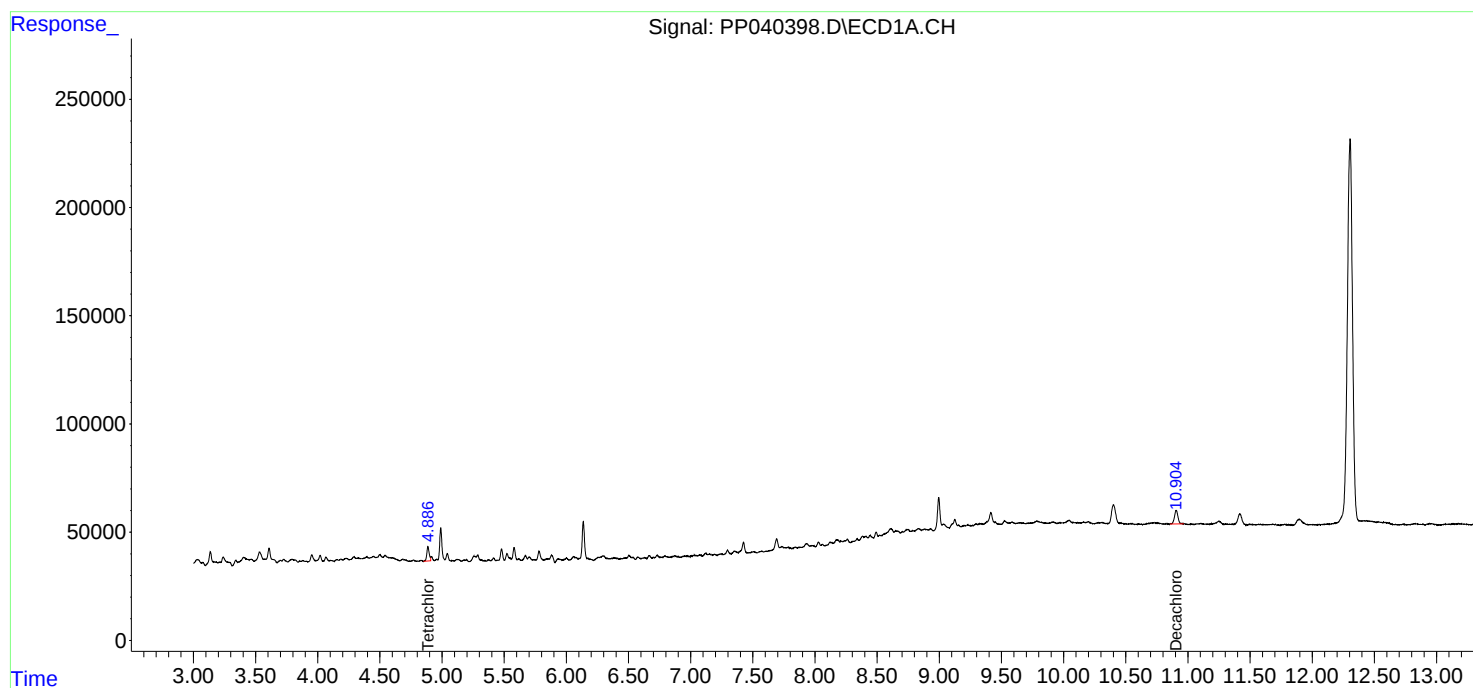


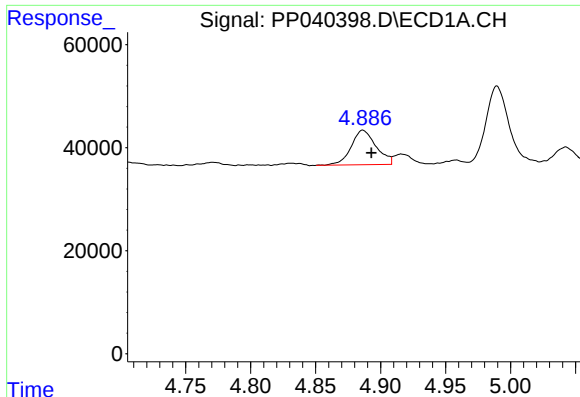

#1 Tetrachloro-m-xylene


R.T.: 4.886 min
Delta R.T.: -0.007 min
Response: 90049
Conc: 2.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
5255

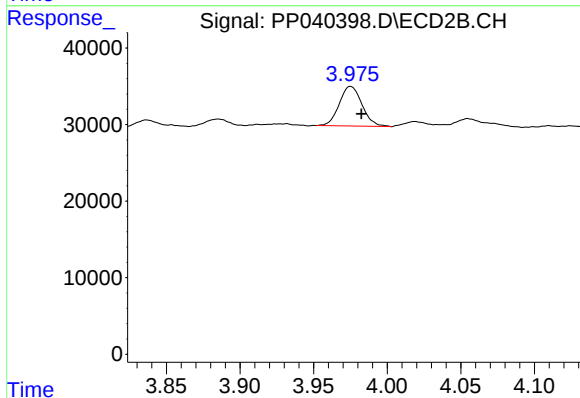


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.007 min
Response: 55768
Conc: 3.30 ng/ml

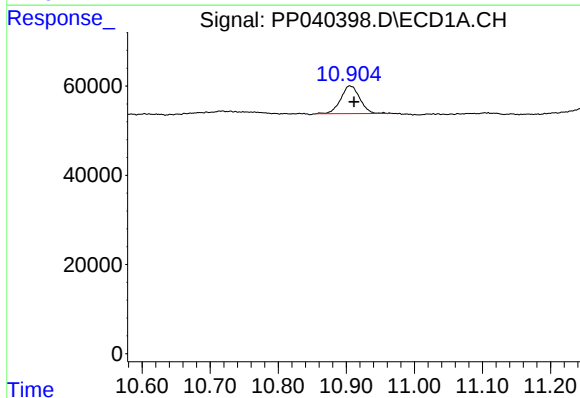

#2 Decachlorobiphenyl

R.T.: 10.905 min
Delta R.T.: -0.006 min
Response: 121338
Conc: 4.91 ng/ml

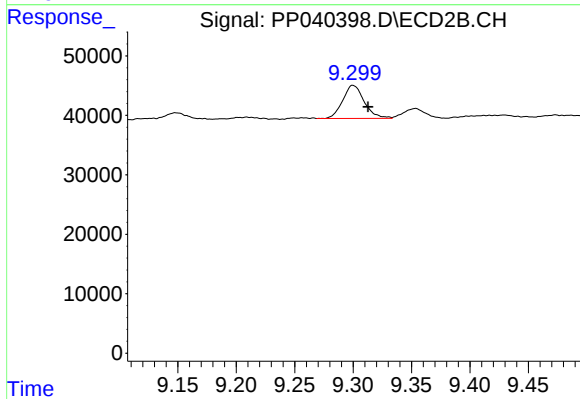

#2 Decachlorobiphenyl

R.T.: 9.300 min
Delta R.T.: -0.013 min
Response: 71208
Conc: 3.36 ng/ml