

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102221\
 Data File : PP040399.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 22 Oct 2021 23:58
 Operator : AJ\MA
 Sample : M4316-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WC-2-IS

Manual Integrations
 APPROVED

mohammad
 10/25/2021 1:42:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 01:58:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 13 08:03:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.885	3.975	534761	291777	17.609	17.259m
2) SA Decachlor...	10.900	9.297f	323190	215513	13.076	10.155

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102221\
Data File : PP040399.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 22 Oct 2021 23:58
Operator : AJ\MA
Sample : M4316-01
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
WC-2-IS


Manual Integrations
APPROVED

mohammad
10/25/2021 1:42:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 01:58:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101221.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 13 08:03:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

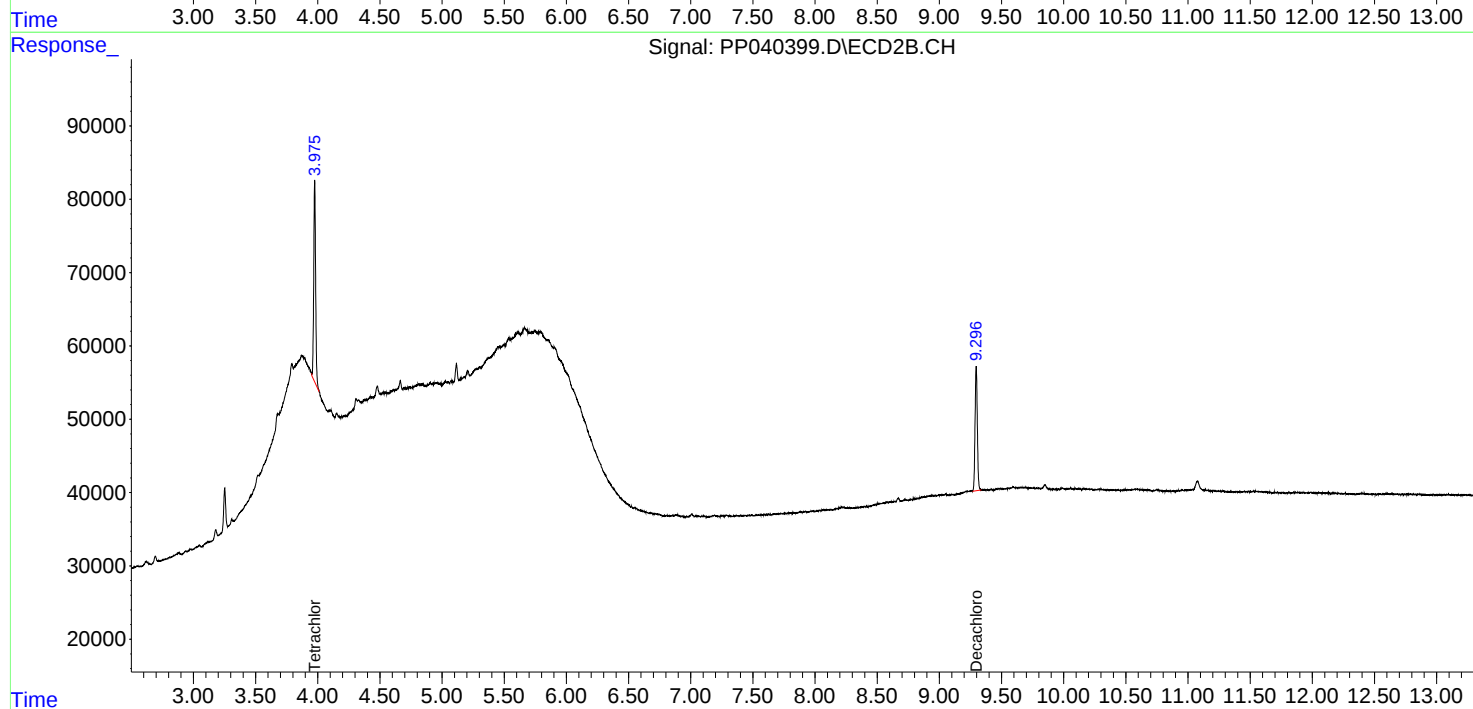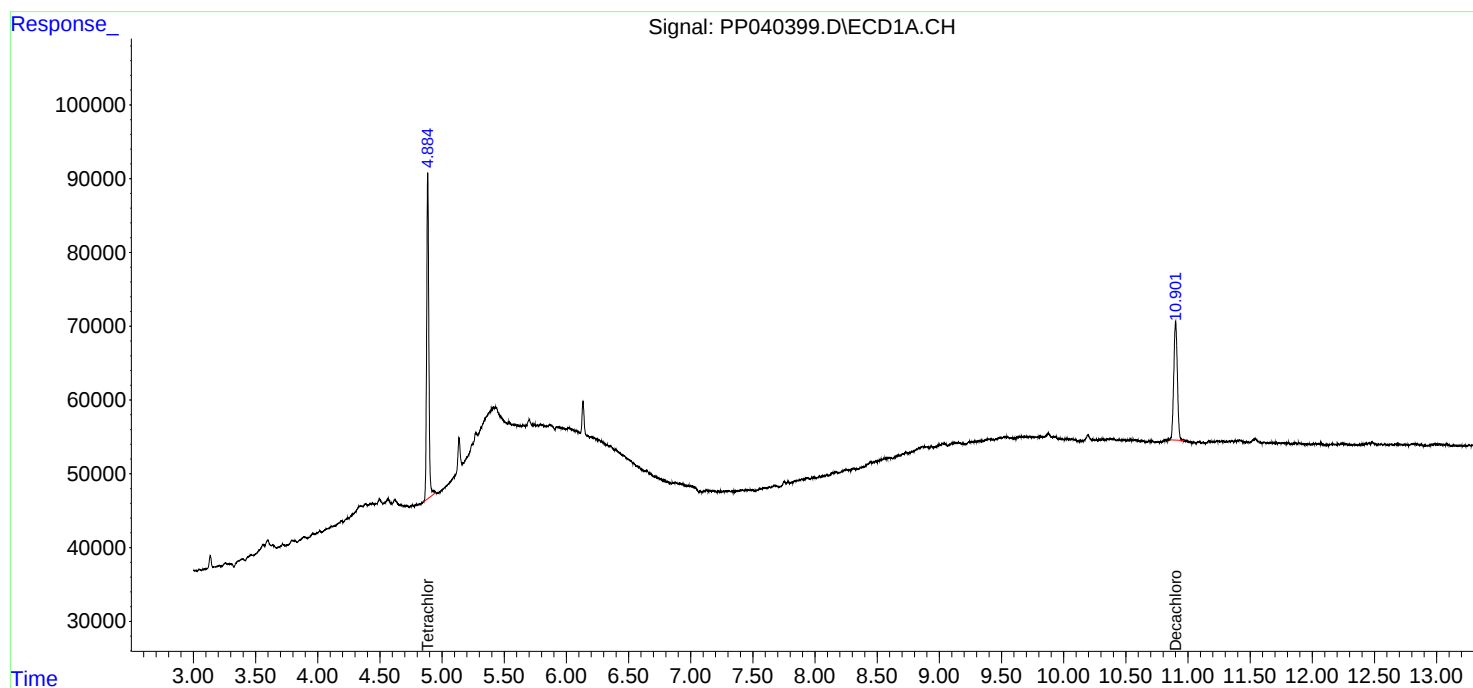

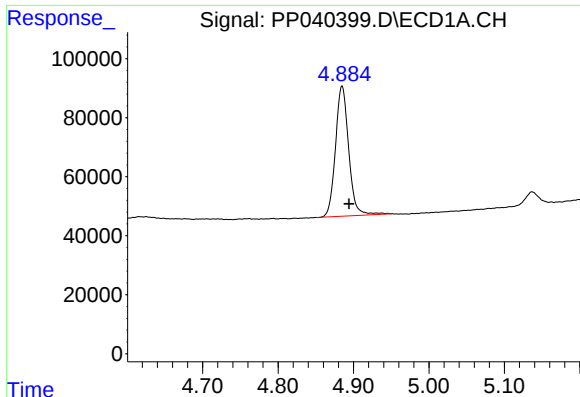


#1 Tetrachloro-m-xylene

R.T.: 4.885 min
Delta R.T.: -0.009 min
Response: 534761
Conc: 17.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
WC-2-IS


Manual Integrations
APPROVED

mohammad
10/25/2021 1:42:21 PM

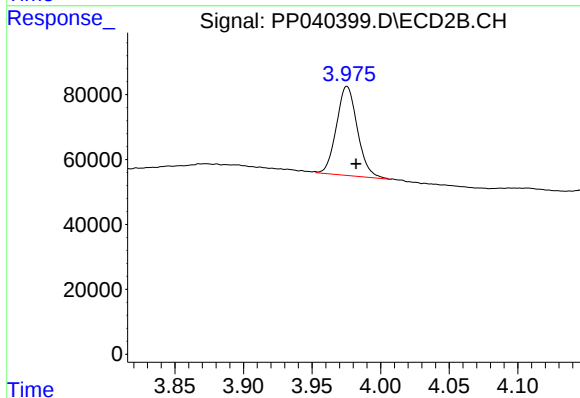


#1 Tetrachloro-m-xylene

R.T.: 3.975 min
Delta R.T.: -0.007 min
Response: 291777
Conc: 17.26 ng/ml m

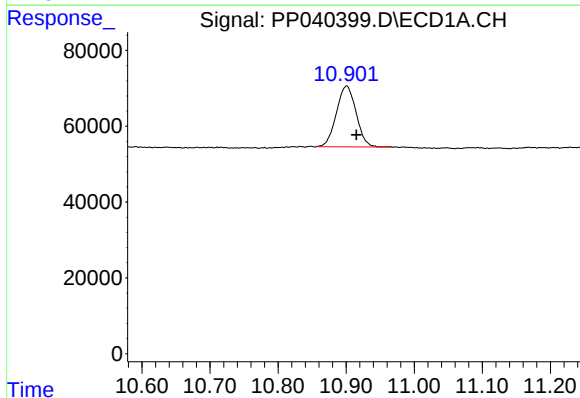

#2 Decachlorobiphenyl

R.T.: 10.900 min
Delta R.T.: -0.015 min
Response: 323190
Conc: 13.08 ng/ml

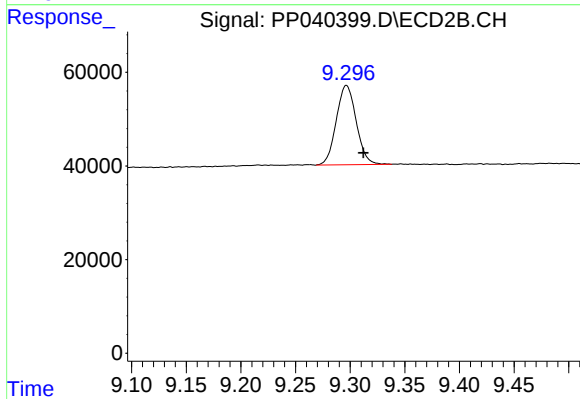

#2 Decachlorobiphenyl

R.T.: 9.297 min
Delta R.T.: -0.015 min
Response: 215513
Conc: 10.15 ng/ml