

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102224\
 Data File : PP068131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2024 15:31
 Operator : YP\AJ
 Sample : P4470-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CL-01-102124

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2024
 Supervised By :Ankita Jodhani 10/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 01:47:33 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	4.048	12701494	13858426	13.722	13.716m
2) SA Decachlor...	10.664	9.207	14078349	13462674	12.228	12.005

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102224\
Data File : PP068131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2024 15:31
Operator : YP\AJ
Sample : P4470-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

CL-01-102124

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 10/23/2024

Supervised By :Ankita Jodhani 10/23/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 01:47:33 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

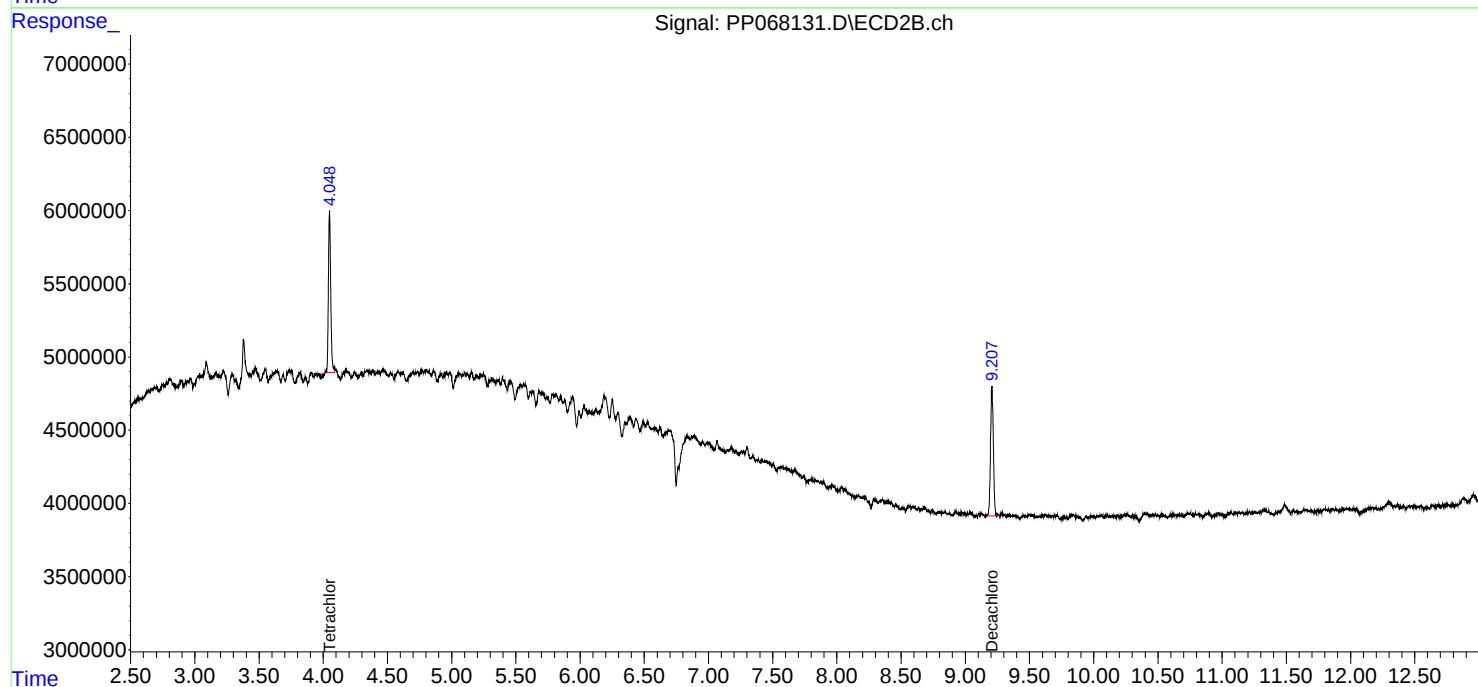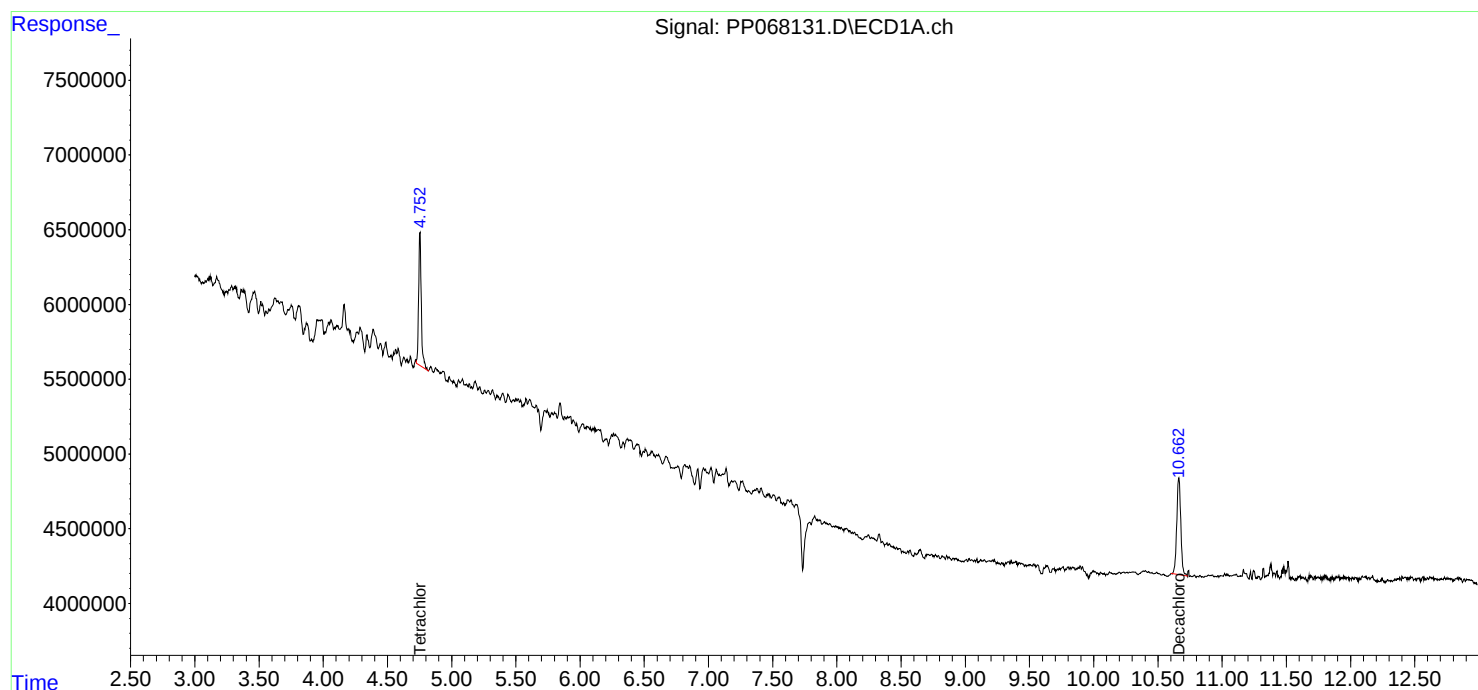

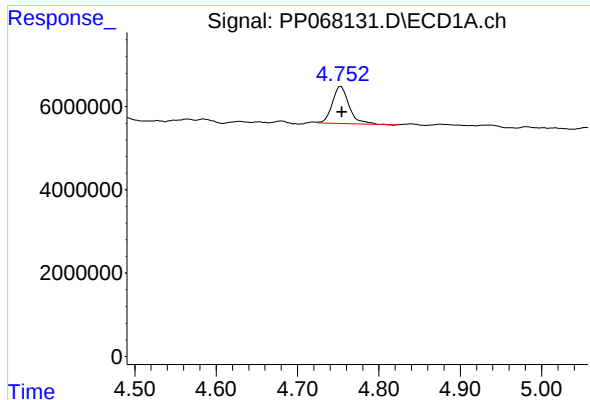


#1 Tetrachloro-m-xylene

R.T.: 4.754 min
Delta R.T.: -0.001 min
Response: 12701494
Conc: 13.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
CL-01-102124


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :Ankita Jodhani 10/23/2024

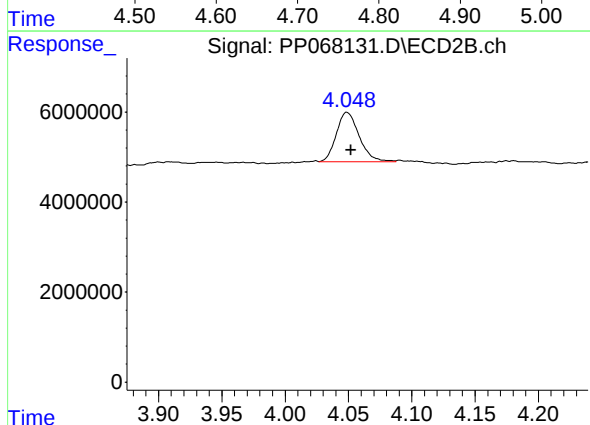


#1 Tetrachloro-m-xylene

R.T.: 4.048 min
Delta R.T.: -0.004 min
Response: 13858426
Conc: 13.72 ng/ml

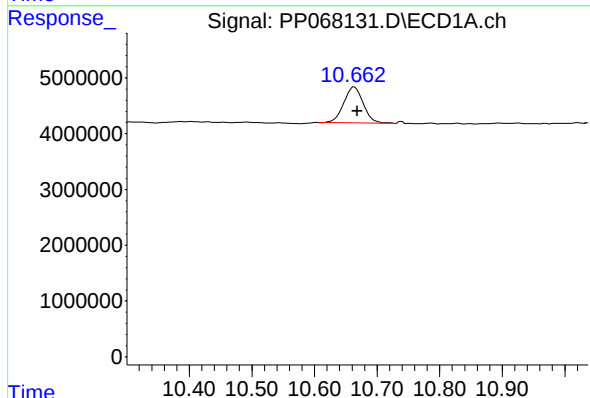

#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.005 min
Response: 14078349
Conc: 12.23 ng/ml

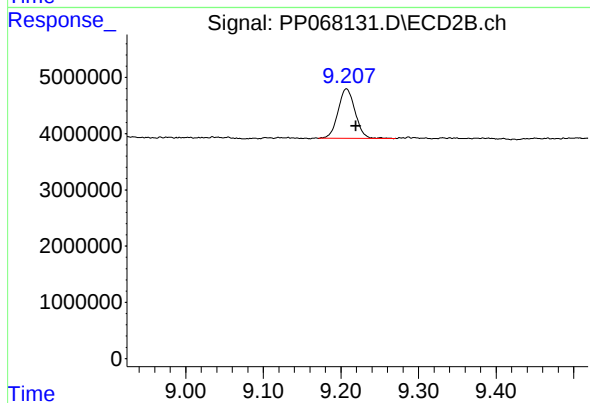

#2 Decachlorobiphenyl

R.T.: 9.207 min
Delta R.T.: -0.012 min
Response: 13462674
Conc: 12.00 ng/ml