

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102225\
 Data File : PP075931.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Oct 2025 12:45
 Operator : YP\AJ
 Sample : Q3407-16 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 L42-B

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/23/2025
 Supervised By :mohammad ahmed 10/27/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 13:30:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 21 18:24:24 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.644	3.786	3323603	11569138	2.326m	1.748
2) SA Decachlor...	10.425	8.779	2523228	13544236	2.344	1.647m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102225\
Data File : PP075931.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Oct 2025 12:45
Operator : YP\AJ
Sample : Q3407-16 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
L42-B


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/23/2025
Supervised By :mohammad ahmed 10/27/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 13:30:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 21 18:24:24 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

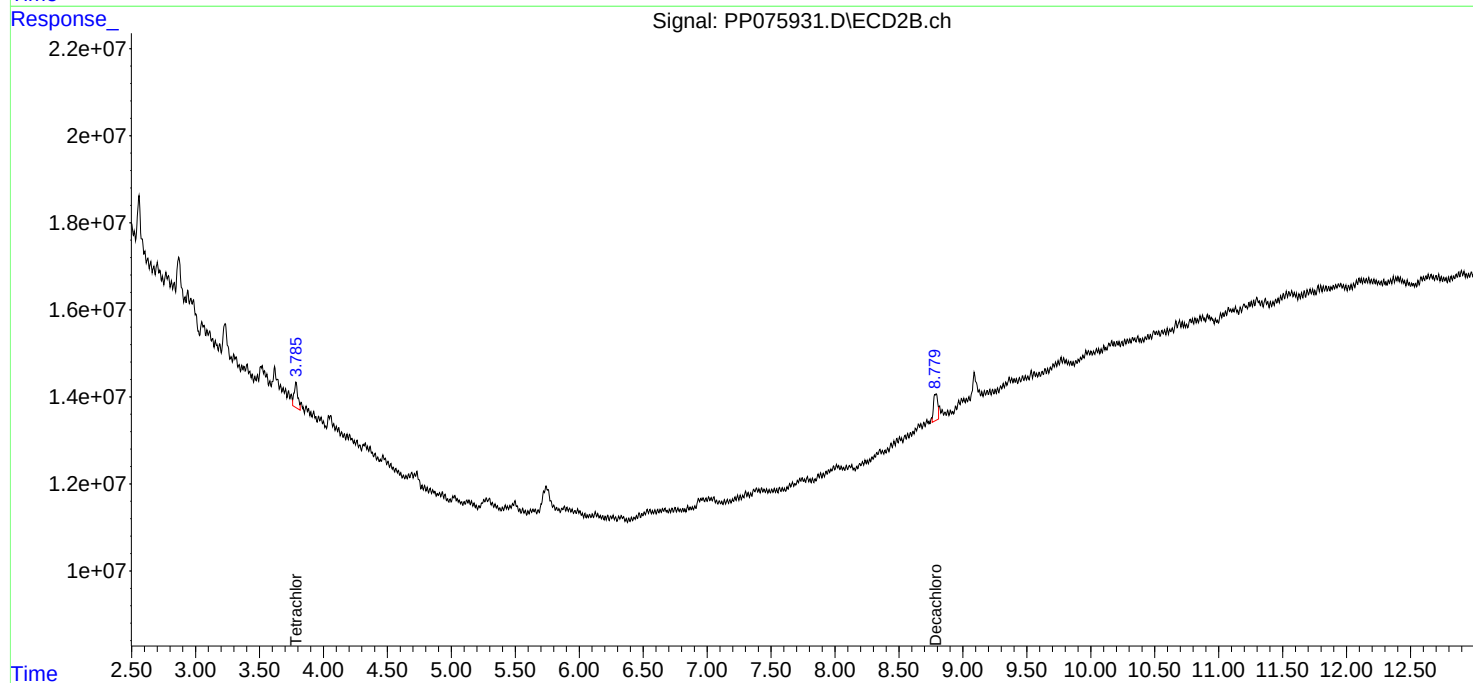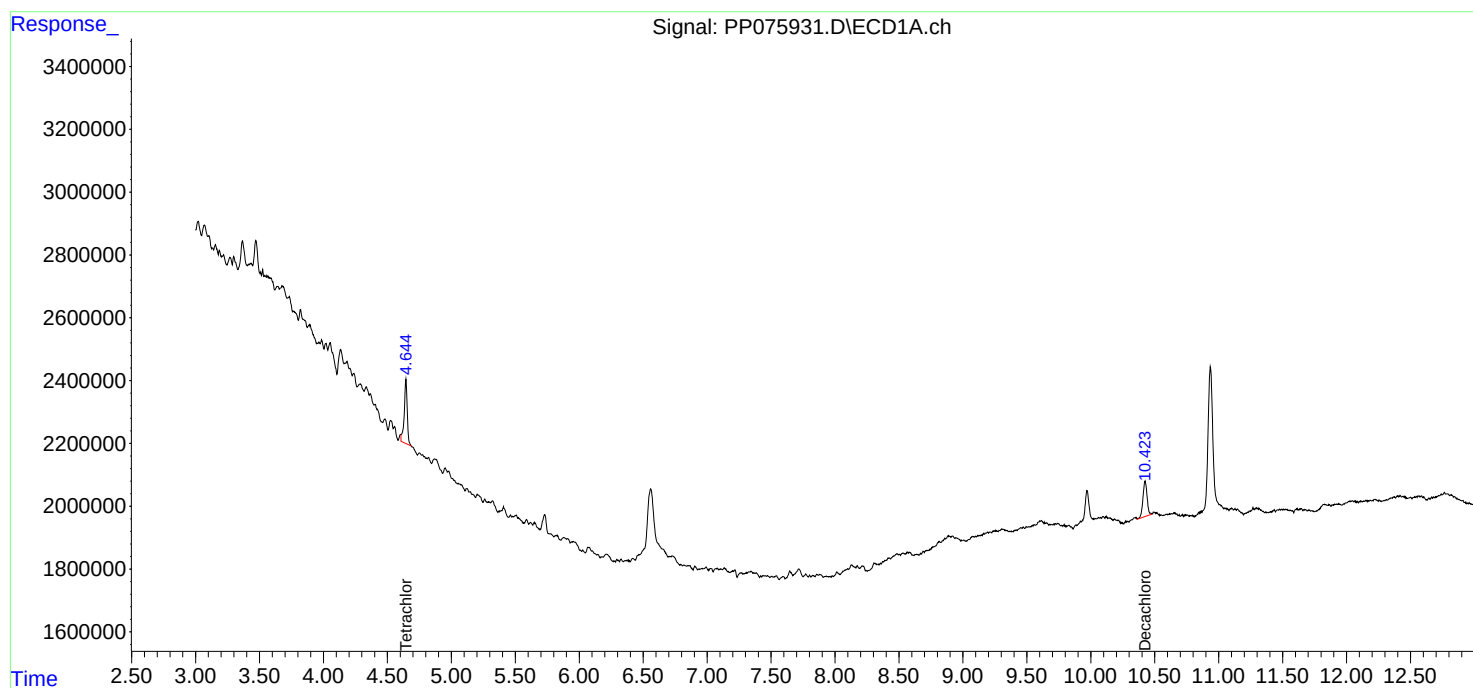

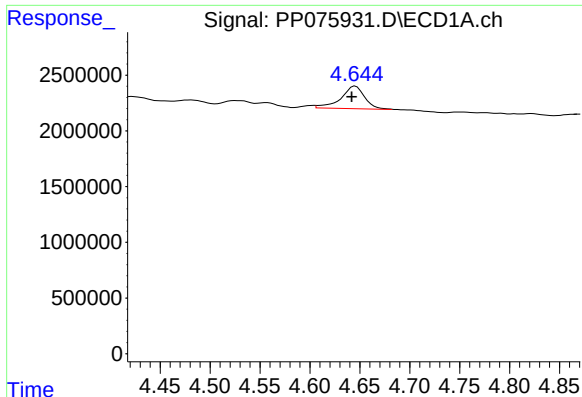

#1 Tetrachloro-m-xylene

R.T.: 4.644 min
Delta R.T.: 0.002 min
Response: 3323603
Conc: 2.33 ng/ml

Instrument :

ECD_P


ClientSampleId :

L42-B

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/23/2025
Supervised By :mohammad ahmed 10/27/2025

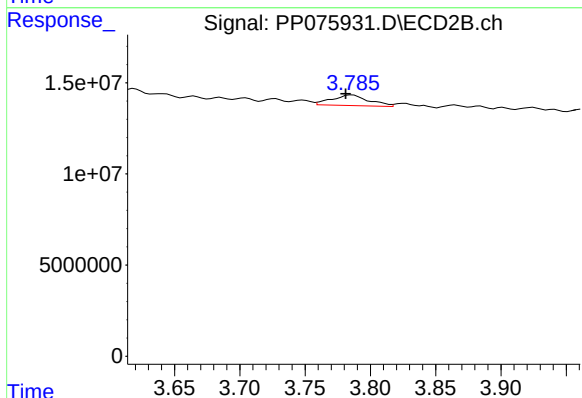


#1 Tetrachloro-m-xylene

R.T.: 3.786 min
Delta R.T.: 0.005 min
Response: 11569138
Conc: 1.75 ng/ml

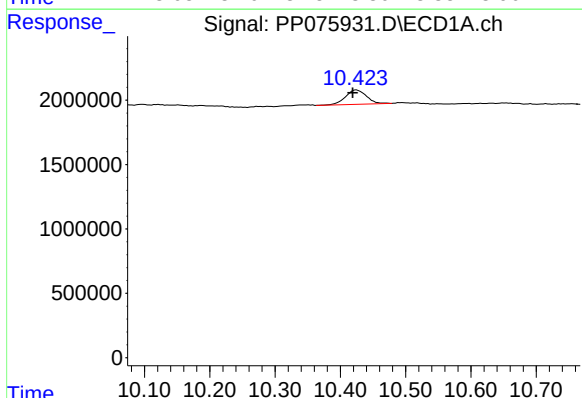

#2 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: 0.006 min
Response: 2523228
Conc: 2.34 ng/ml

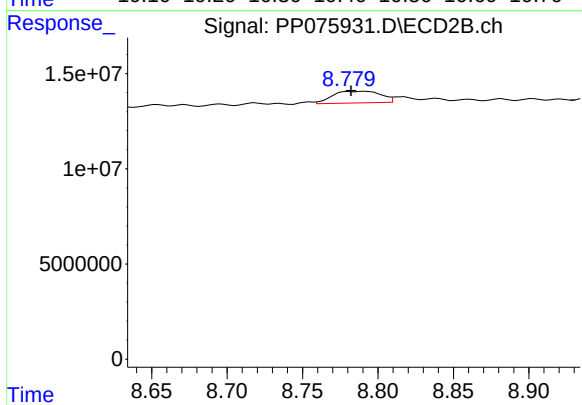

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: -0.003 min
Response: 13544236
Conc: 1.65 ng/ml m