

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102320\
 Data File : PP030796.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 23 Oct 2020 14:43
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-4
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 01:51:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 22 12:07:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.810	4.085	1316941	1185980	19.845	19.111
2) SA Decachlor...	10.695	9.429	767030	768377	21.072	20.576
Target Compounds						
9) L2 AR-1221-2	5.157	0.000	17077	0	36.752	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102320\
Data File : PP030796.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 23 Oct 2020 14:43
Operator : DD\AJ
Sample : MDL-PCB-BL-S-4
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 01:51:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PP102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 22 12:07:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

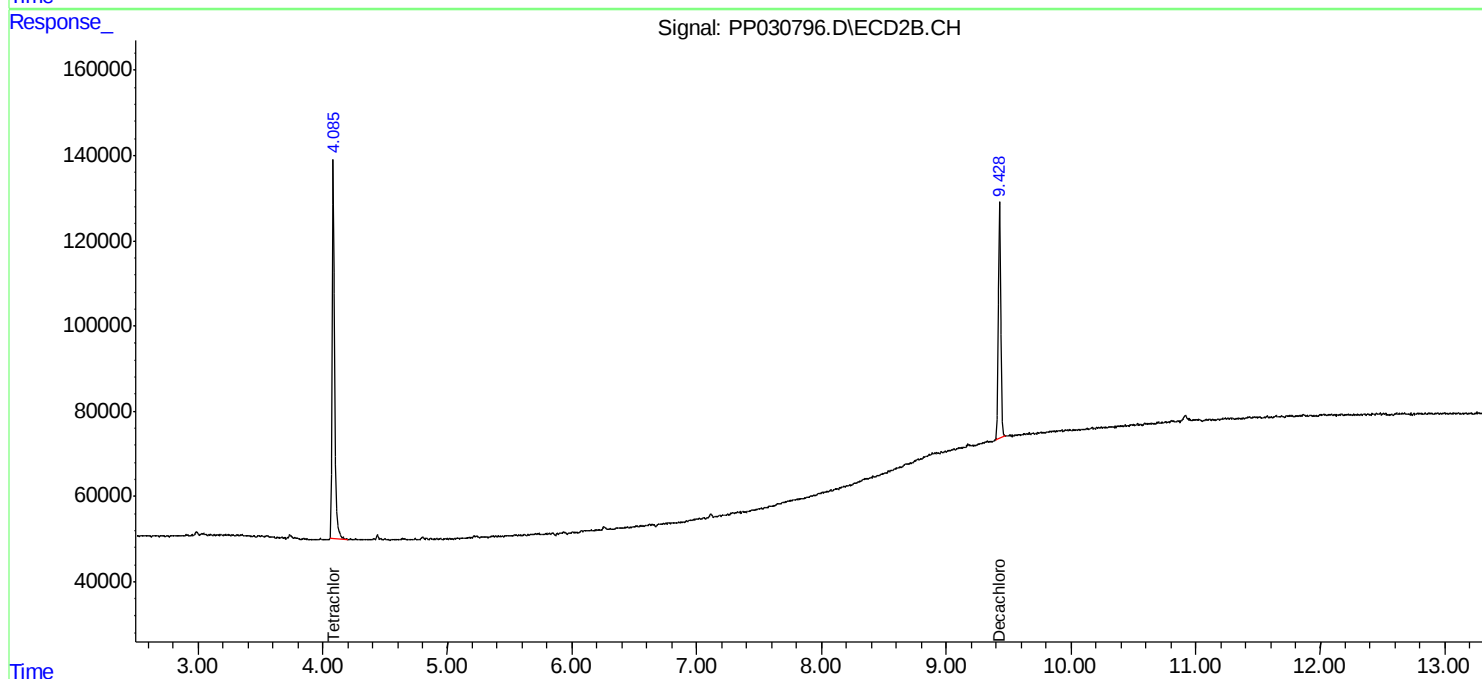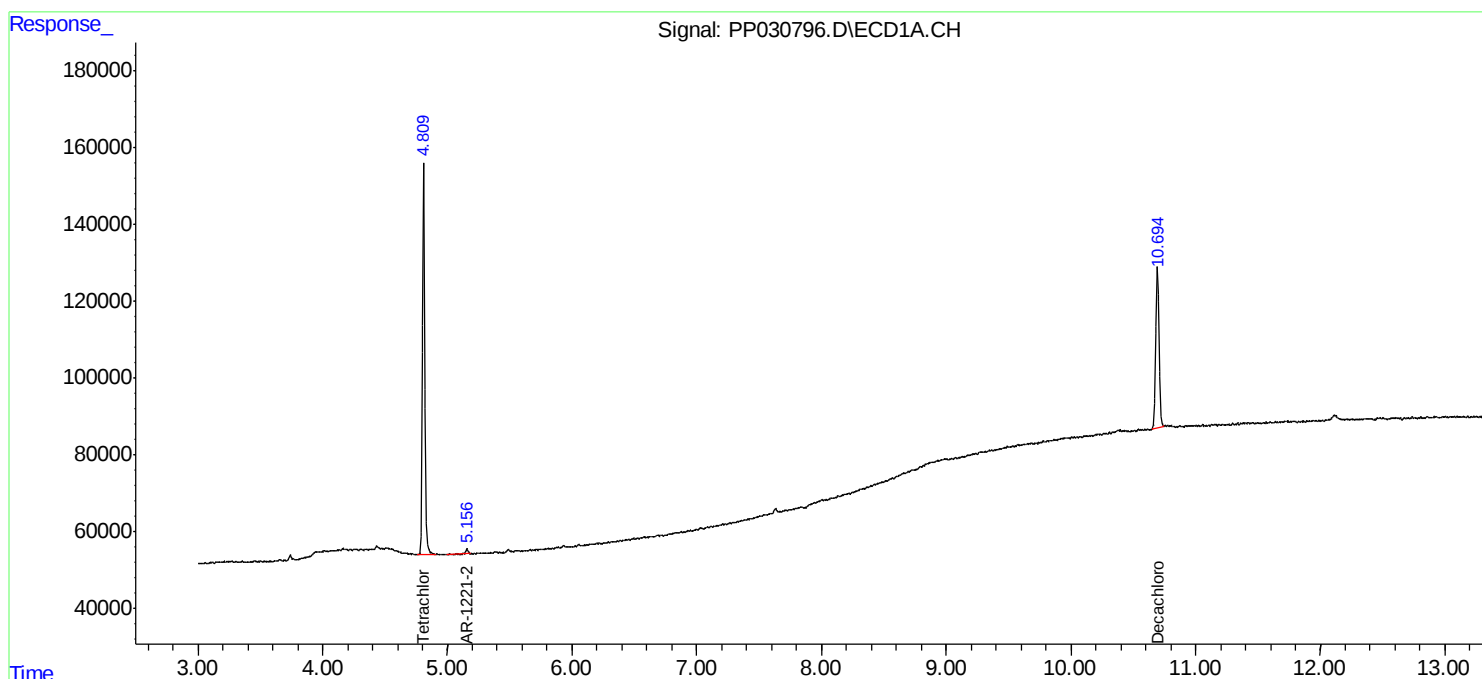


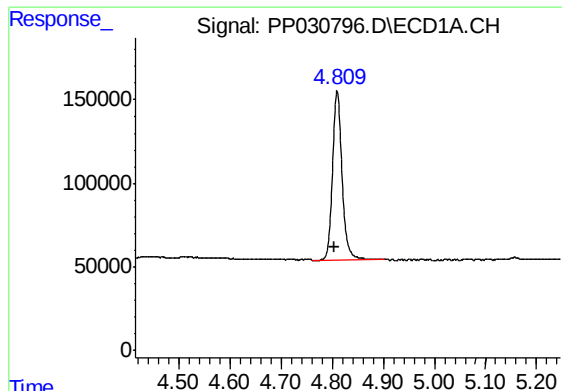

#1 Tetrachloro-m-xylene


R.T.: 4.810 min
Delta R.T.: 0.006 min
Response: 1316941
Conc: 19.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-4

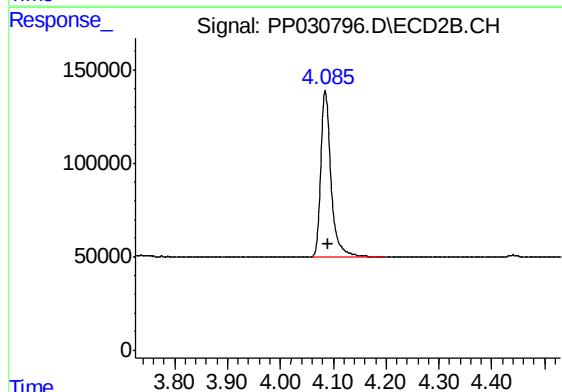


#1 Tetrachloro-m-xylene

R.T.: 4.085 min
Delta R.T.: -0.005 min
Response: 1185980
Conc: 19.11 ng/ml

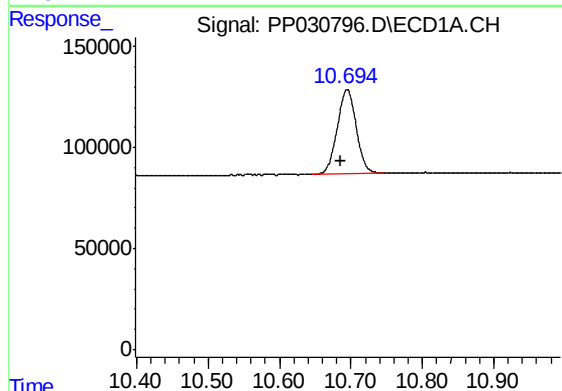


#2 Decachlorobiphenyl

R.T.: 10.695 min
Delta R.T.: 0.008 min
Response: 767030
Conc: 21.07 ng/ml

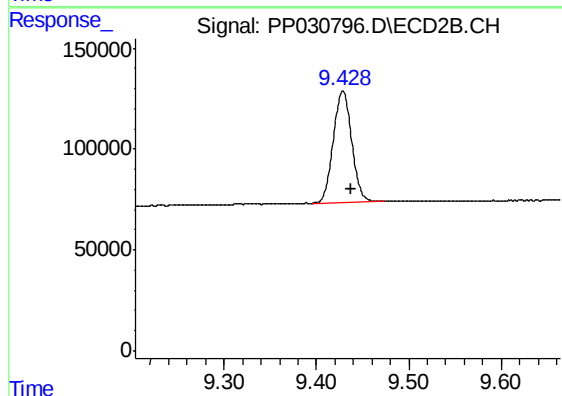

#2 Decachlorobiphenyl


R.T.: 9.429 min
Delta R.T.: -0.009 min
Response: 768377
Conc: 20.58 ng/ml

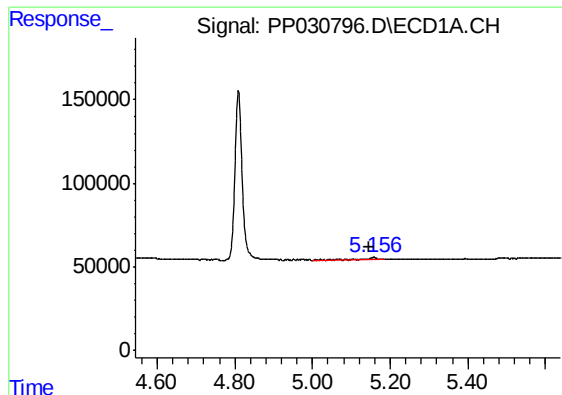

#9 AR-1221-2

R.T.: 5.157 min
Delta R.T.: 0.009 min
Response: 17077
Conc: 36.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-4

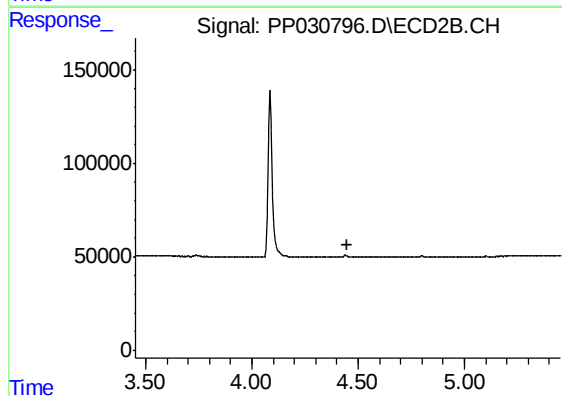

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.452 min
Response: 0
Conc: N.D.