

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102323\
 Data File : PP061189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Oct 2023 20:07
 Operator : YP\AJ
 Sample : 04909-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LCOL-12

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/24/2023
 Supervised By :Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 23 21:38:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.566	3.698	107.4E6	21970878	48.857m	16.251 #
2) SA Decachlor...	10.504	8.765	24494916	8194252	15.642	5.450m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102323\
Data File : PP061189.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Oct 2023 20:07
Operator : YP\AJ
Sample : 04909-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LCOL-12


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2023
Supervised By :Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 23 21:38:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

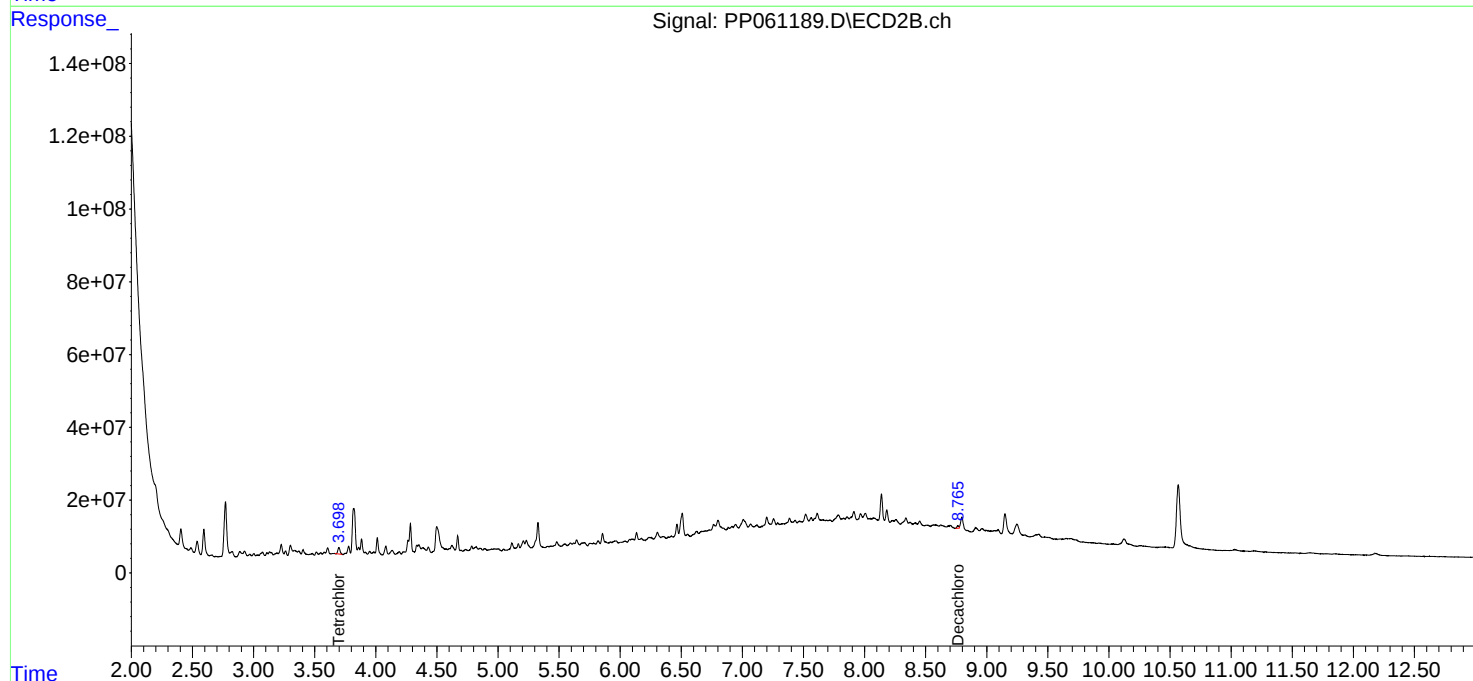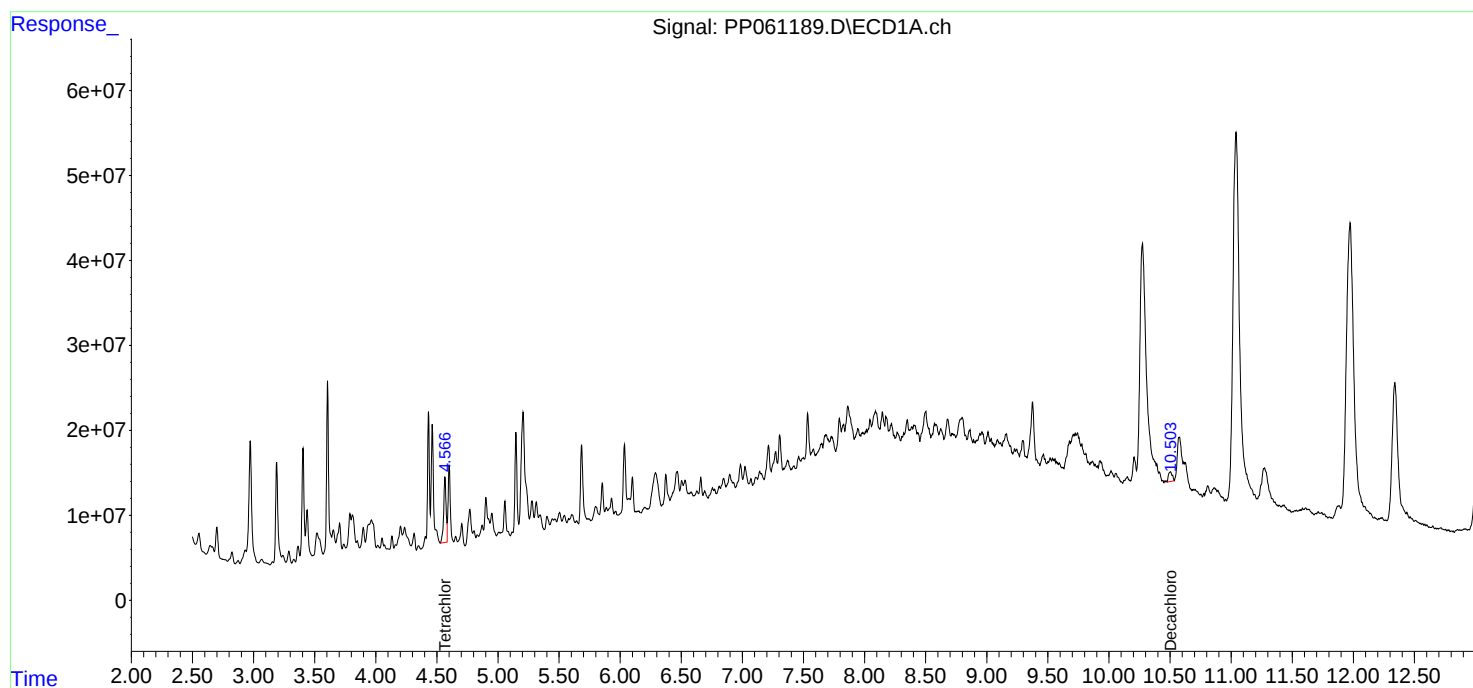

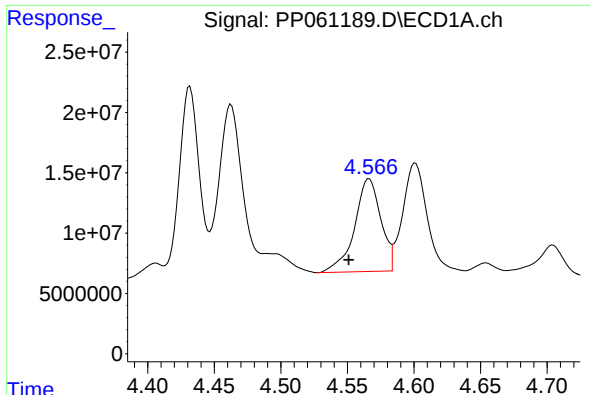


#1 Tetrachloro-m-xylene

R.T.: 4.566 min
Delta R.T.: 0.015 min
Response: 107403042
Conc: 48.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LCOL-12


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2023
Supervised By :Ankita Jodhani 10/24/2023

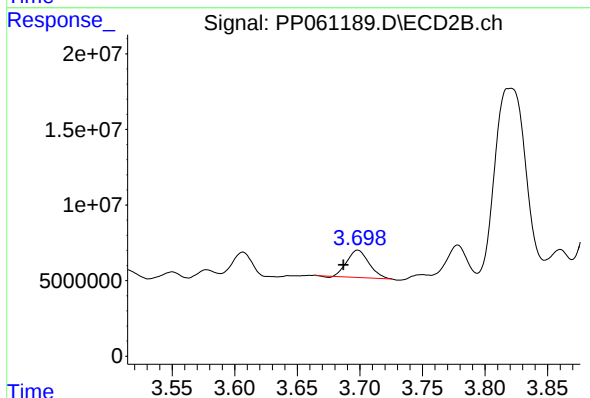


#1 Tetrachloro-m-xylene

R.T.: 3.698 min
Delta R.T.: 0.011 min
Response: 21970878
Conc: 16.25 ng/ml

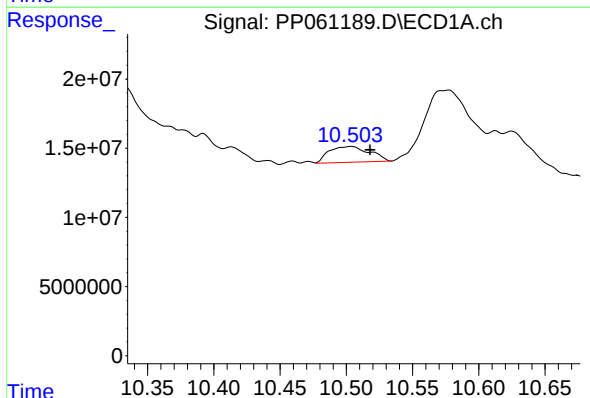

#2 Decachlorobiphenyl

R.T.: 10.504 min
Delta R.T.: -0.014 min
Response: 24494916
Conc: 15.64 ng/ml

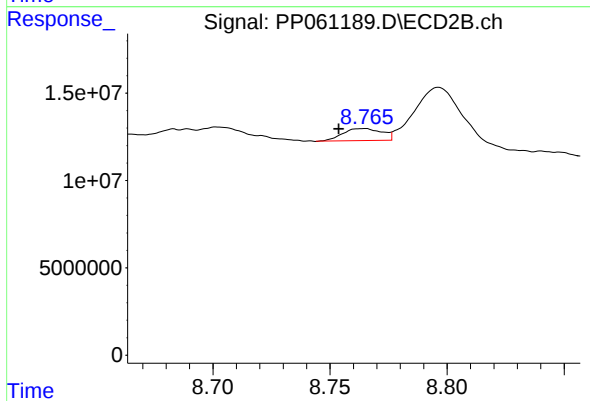

#2 Decachlorobiphenyl

R.T.: 8.765 min
Delta R.T.: 0.011 min
Response: 8194252
Conc: 5.45 ng/ml m