

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102323\
 Data File : PP061203.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 00:37
 Operator : YP\AJ
 Sample : 05005-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 N-4(0-5)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/24/2023
 Supervised By :Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 03:57:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.557	3.693	40156948	28245731	18.267m	20.892
2) SA Decachlor...	10.523	8.762	45612095	21845880	29.127m	14.530m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102323\
Data File : PP061203.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 00:37
Operator : YP\AJ
Sample : 05005-02
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
N-4(0-5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2023
Supervised By :Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 03:57:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

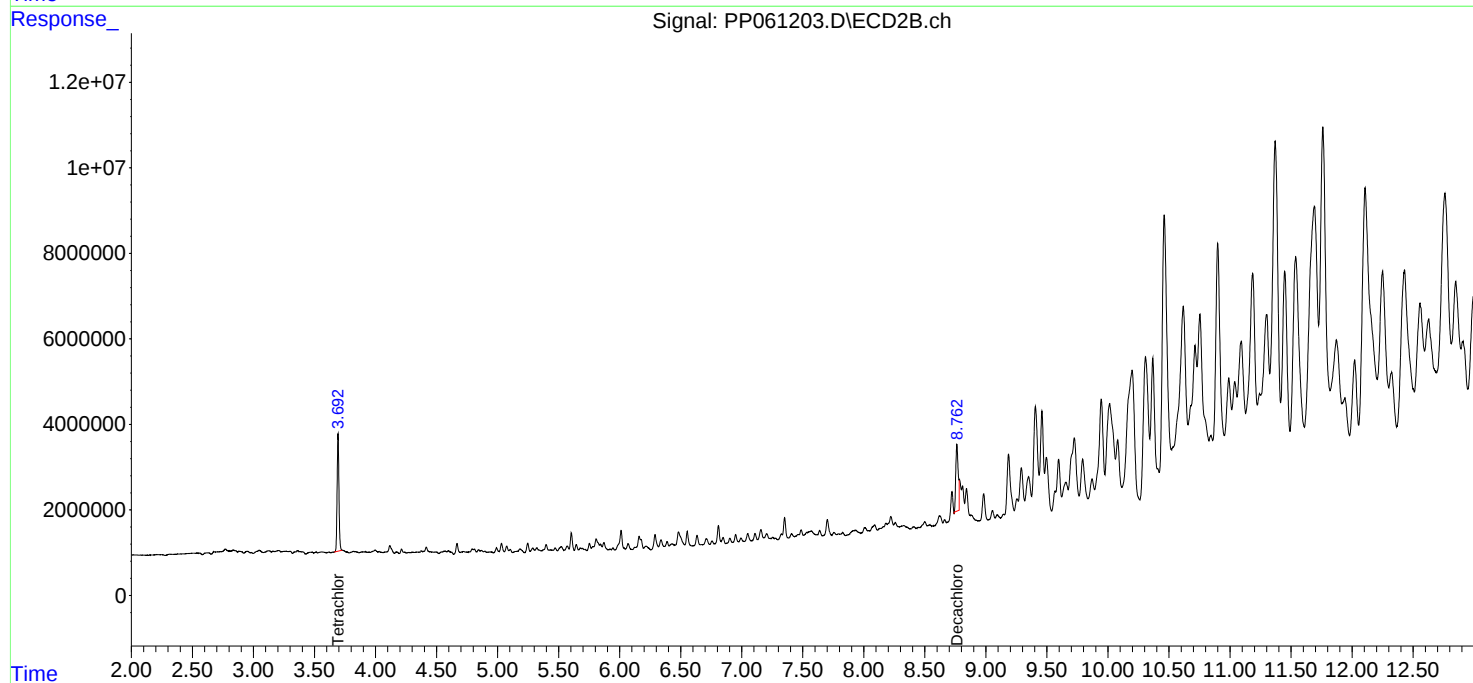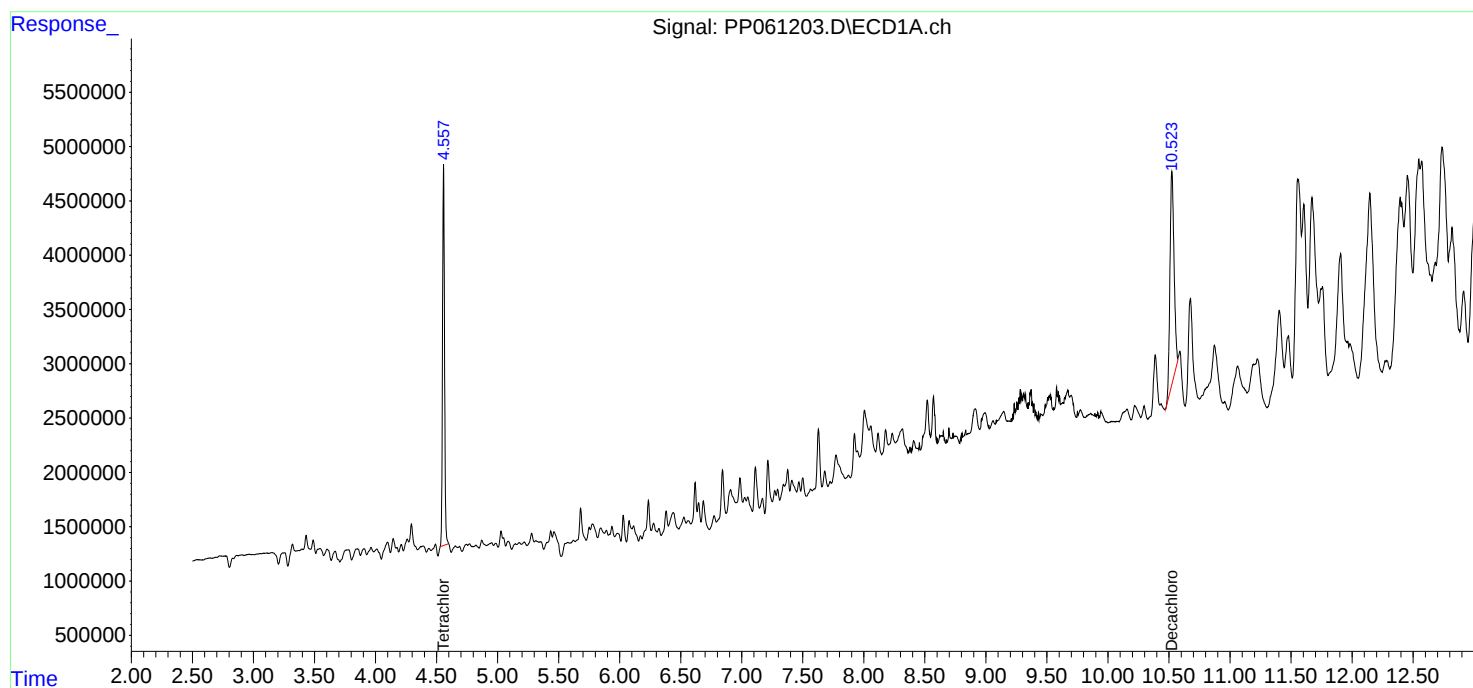

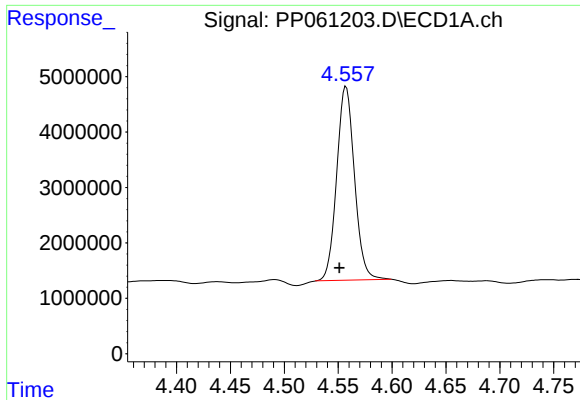


#1 Tetrachloro-m-xylene

R.T.: 4.557 min
Delta R.T.: 0.006 min
Response: 40156948
Conc: 18.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
N-4(0-5)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2023
Supervised By :Ankita Jodhani 10/24/2023

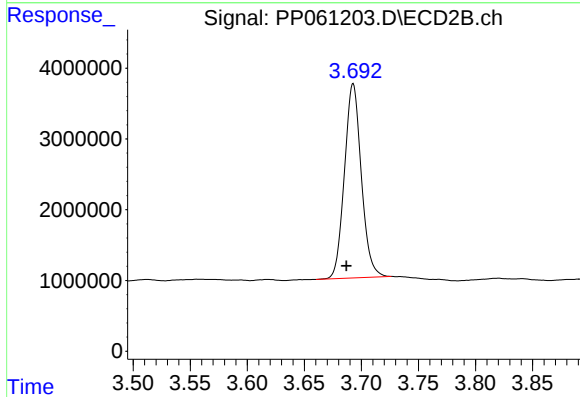


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.006 min
Response: 28245731
Conc: 20.89 ng/ml

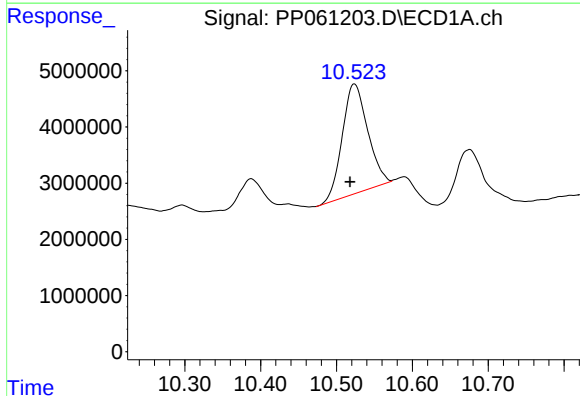

#2 Decachlorobiphenyl

R.T.: 10.523 min
Delta R.T.: 0.005 min
Response: 45612095
Conc: 29.13 ng/ml m

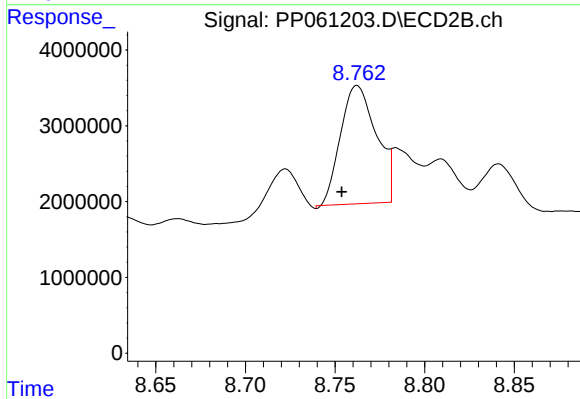

#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.008 min
Response: 21845880
Conc: 14.53 ng/ml m