

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102323\
 Data File : PP061204.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 00:54
 Operator : YP\AJ
 Sample : 05005-03
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 N-2(5-10)

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/24/2023
 Supervised By :Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 03:58:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.558	3.693	36308539	23082131	16.516	17.073
2) SA Decachlor...	10.515	8.762	79848123	15138957	50.989	10.069m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102323\
Data File : PP061204.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 00:54
Operator : YP\AJ
Sample : 05005-03
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
N-2(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2023
Supervised By :Ankita Jodhani 10/24/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 03:58:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

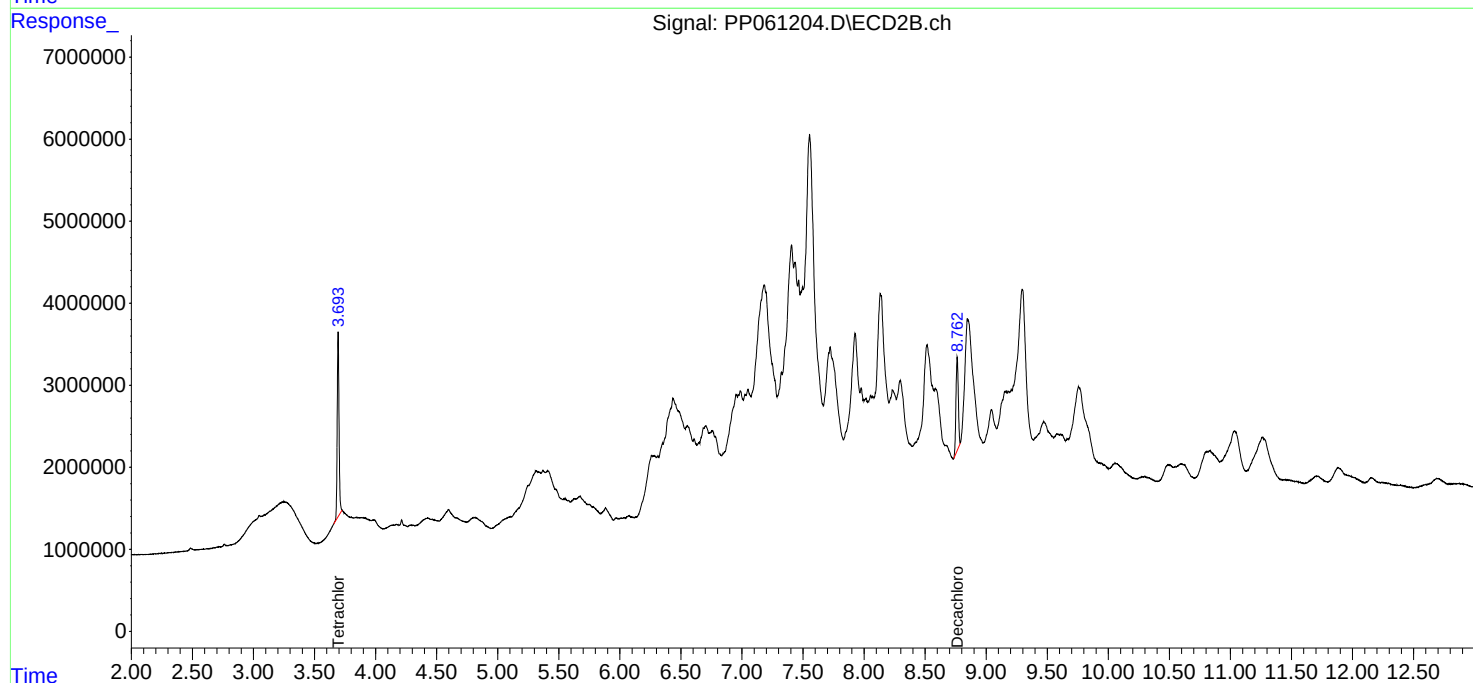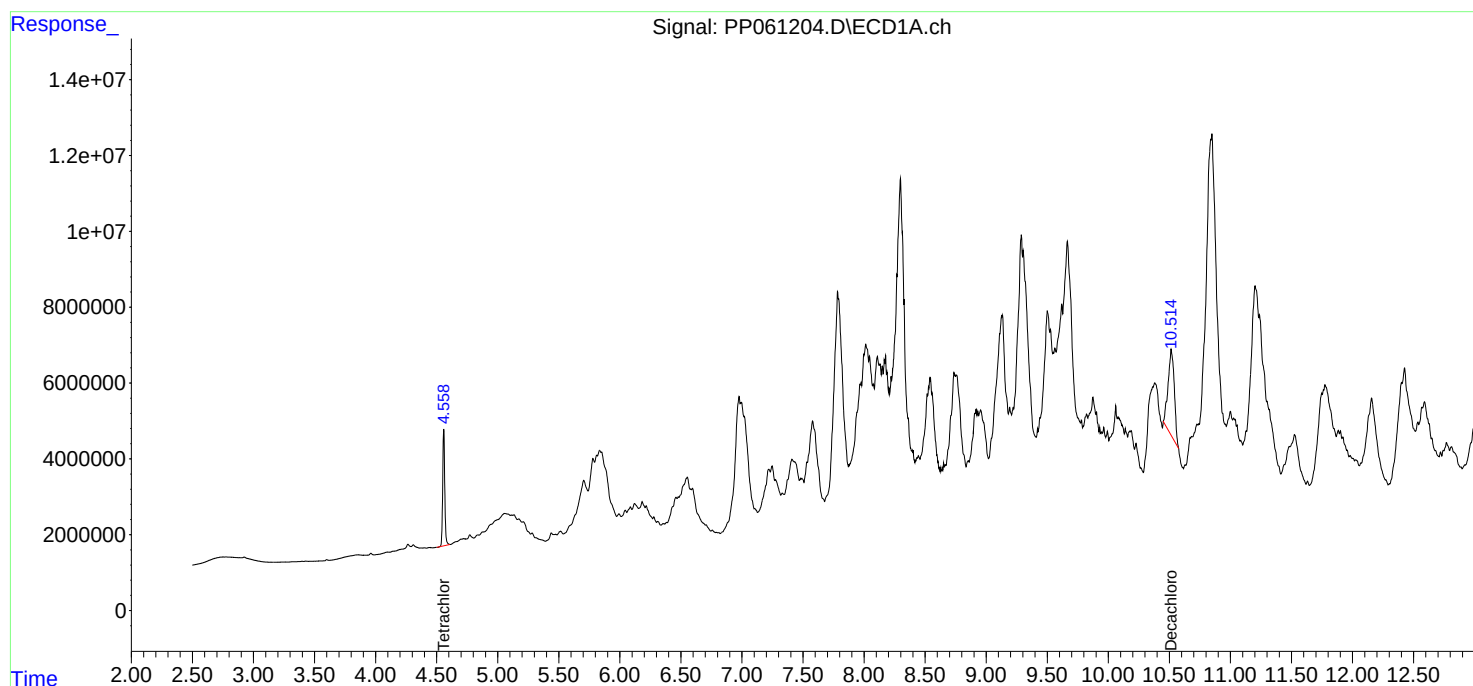

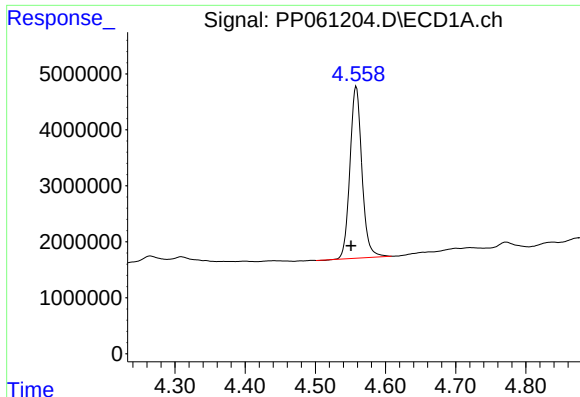


#1 Tetrachloro-m-xylene

R.T.: 4.558 min
Delta R.T.: 0.007 min
Response: 36308539
Conc: 16.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
N-2(5-10)


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/24/2023
Supervised By :Ankita Jodhani 10/24/2023

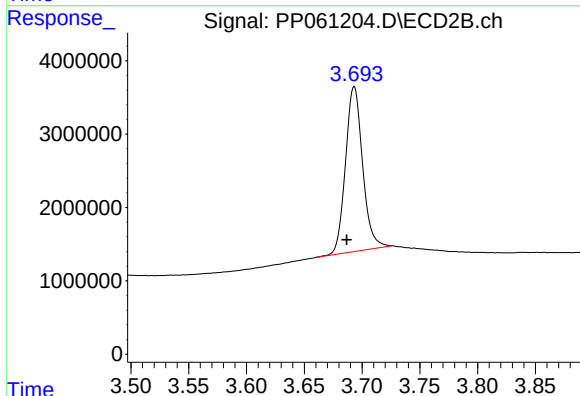


#1 Tetrachloro-m-xylene

R.T.: 3.693 min
Delta R.T.: 0.006 min
Response: 23082131
Conc: 17.07 ng/ml

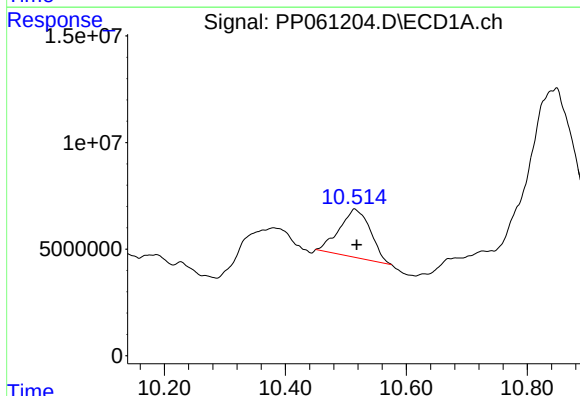

#2 Decachlorobiphenyl

R.T.: 10.515 min
Delta R.T.: -0.003 min
Response: 79848123
Conc: 50.99 ng/ml

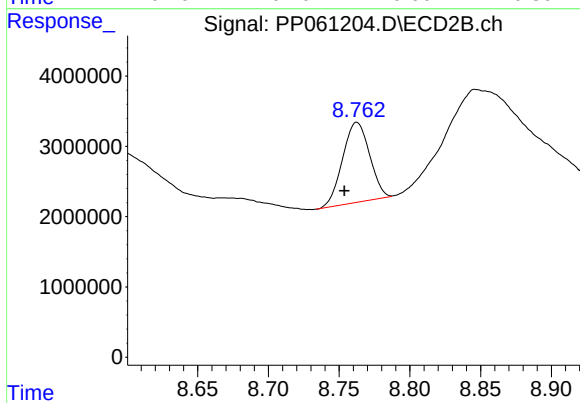

#2 Decachlorobiphenyl

R.T.: 8.762 min
Delta R.T.: 0.008 min
Response: 15138957
Conc: 10.07 ng/ml m