

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102420\
 Data File : PP030815.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2020 9:09
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-6
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 06:19:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 22 12:07:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.805	4.087	1249071	1155663	18.823	18.623
2)	SA Decachlor...	10.693	9.427	755112	785820	20.745	21.043
Target Compounds							
9)	L2 AR-1221-2	5.151	4.443	16914	16676	36.402	40.002
32)	L7 AR-1260-2	8.062	0.000	87402	0	42.163	N.D. #
33)	L7 AR-1260-3	0.000	7.298	0	2832	N.D.	1.351 #
34)	L7 AR-1260-4	8.675f	7.812f	147416	41894	74.198	24.971 #
35)	L7 AR-1260-5	8.960	0.000	111320	0	28.910	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102420\
Data File : PP030815.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2020 9:09
Operator : DD\AJ
Sample : MDL-PCB-BL-S-6
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:19:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 22 12:07:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

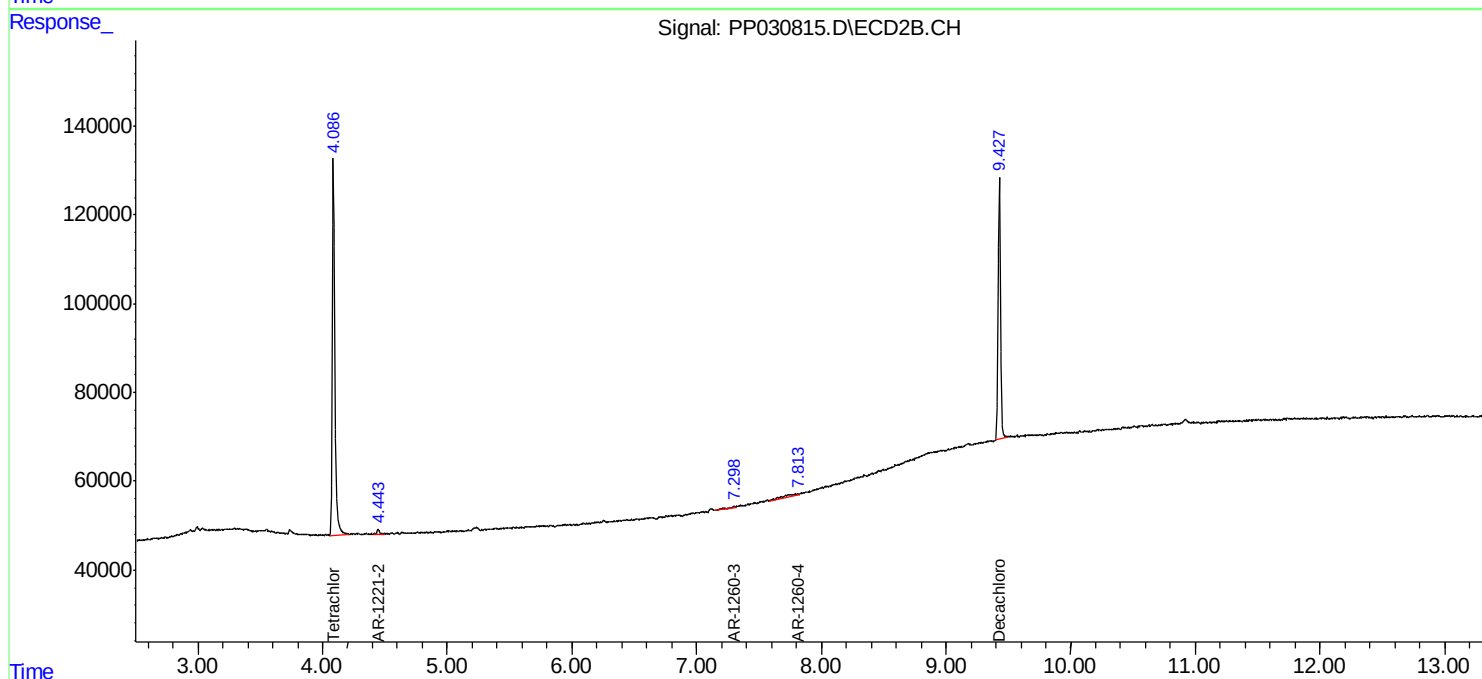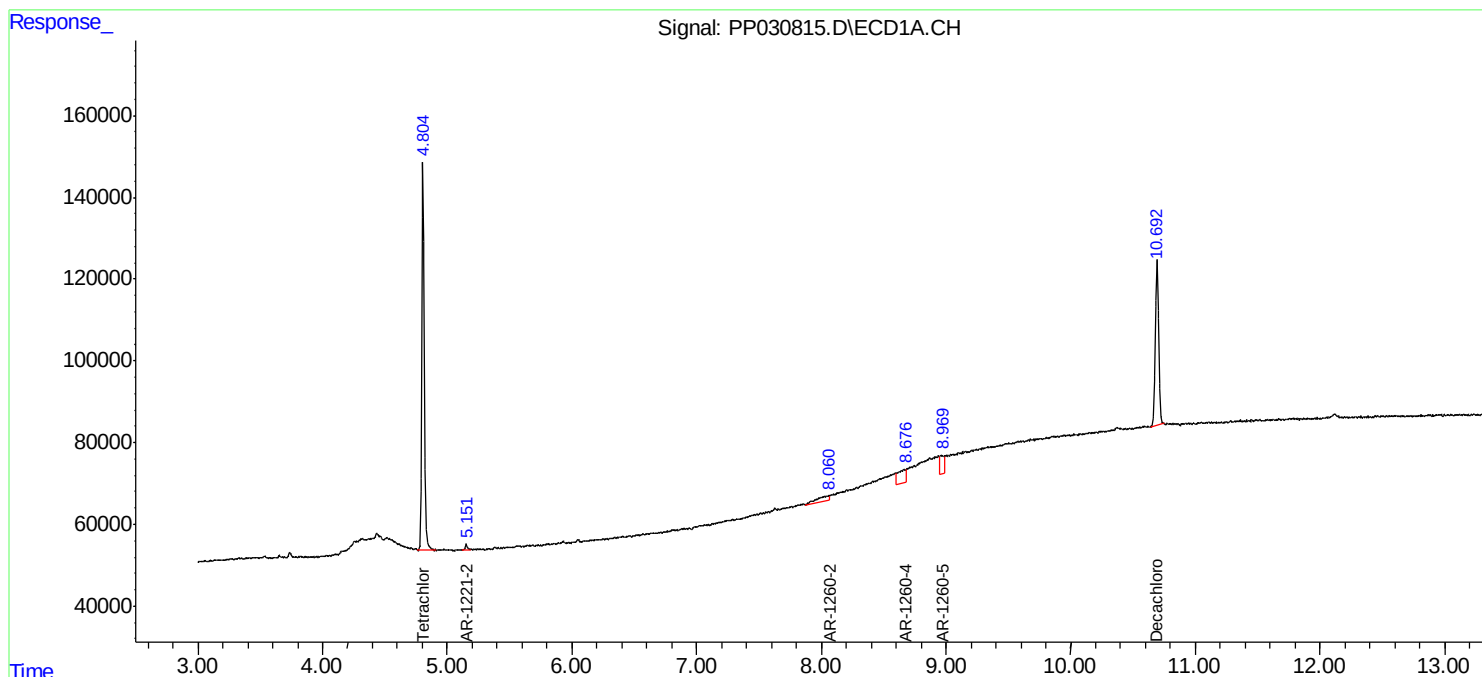


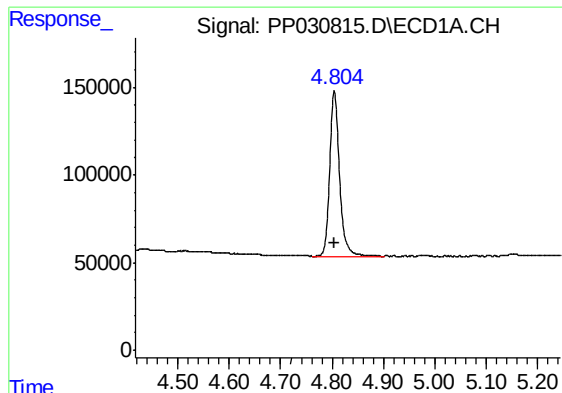

#1 Tetrachloro-m-xylene


R.T.: 4.805 min
Delta R.T.: 0.000 min
Response: 1249071
Conc: 18.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-6

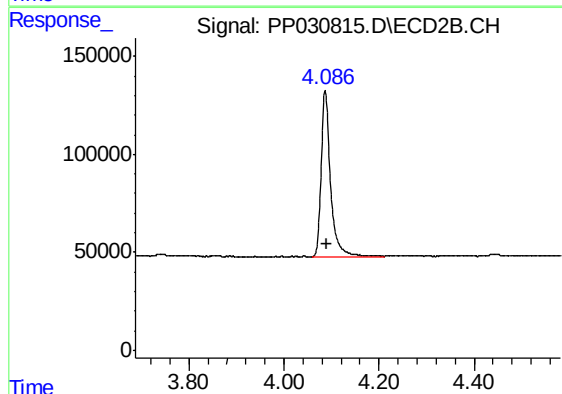


#1 Tetrachloro-m-xylene

R.T.: 4.087 min
Delta R.T.: -0.003 min
Response: 1155663
Conc: 18.62 ng/ml

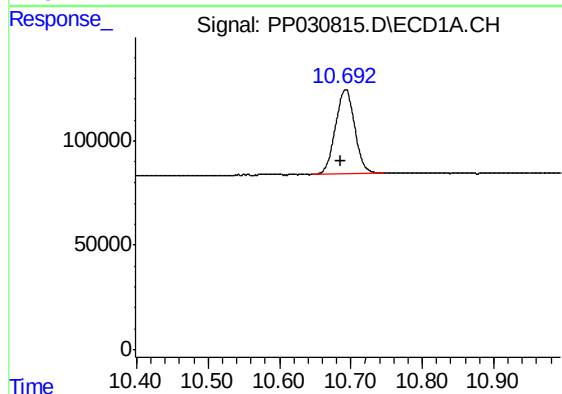


#2 Decachlorobiphenyl

R.T.: 10.693 min
Delta R.T.: 0.006 min
Response: 755112
Conc: 20.74 ng/ml

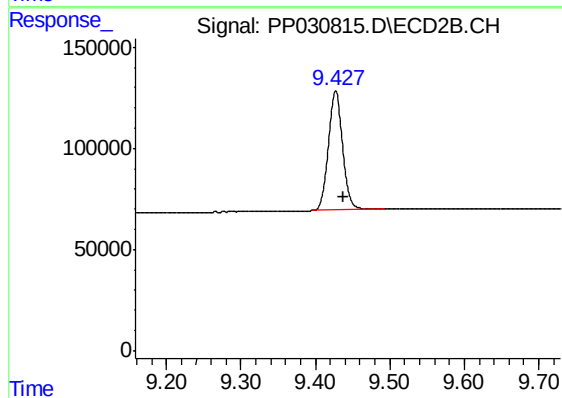

#2 Decachlorobiphenyl


R.T.: 9.427 min
Delta R.T.: -0.010 min
Response: 785820
Conc: 21.04 ng/ml

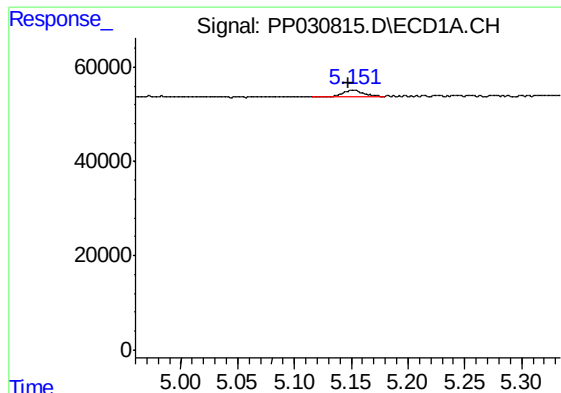

#9 AR-1221-2


R.T.: 5.151 min
Delta R.T.: 0.004 min
Response: 16914
Conc: 36.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-6

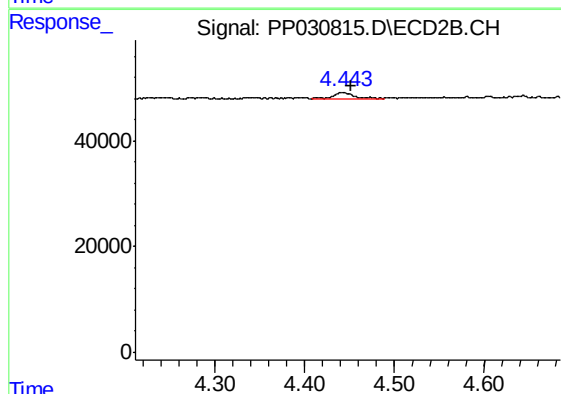


#9 AR-1221-2

R.T.: 4.443 min
Delta R.T.: -0.009 min
Response: 16676
Conc: 40.00 ng/ml

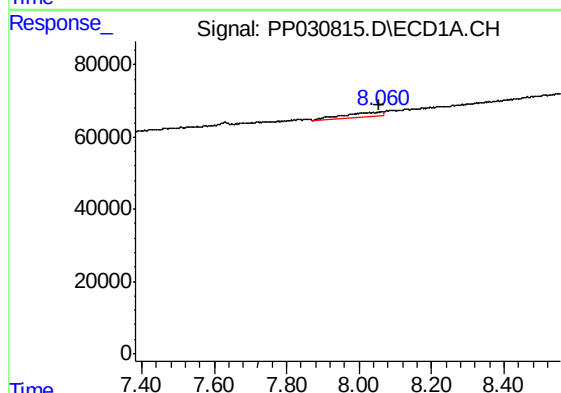


#32 AR-1260-2

R.T.: 8.062 min
Delta R.T.: 0.007 min
Response: 87402
Conc: 42.16 ng/ml

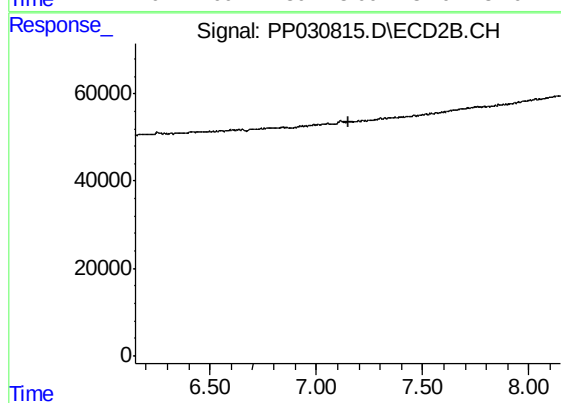

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

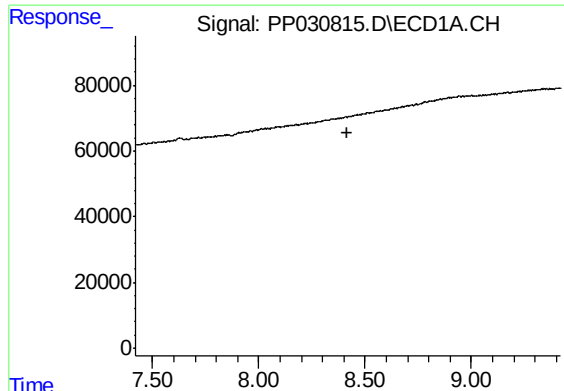

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T. : 8.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-6

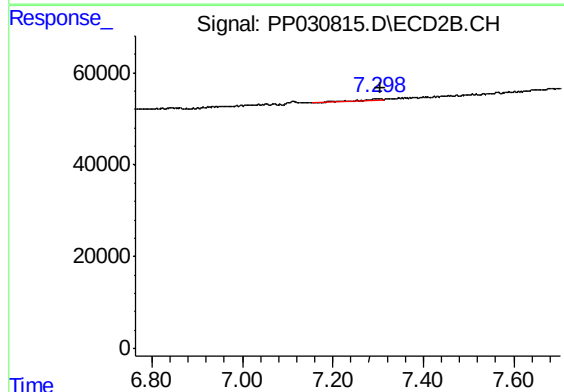


#33 AR-1260-3

R.T.: 7.298 min
Delta R.T.: -0.008 min
Response: 2832
Conc: 1.35 ng/ml

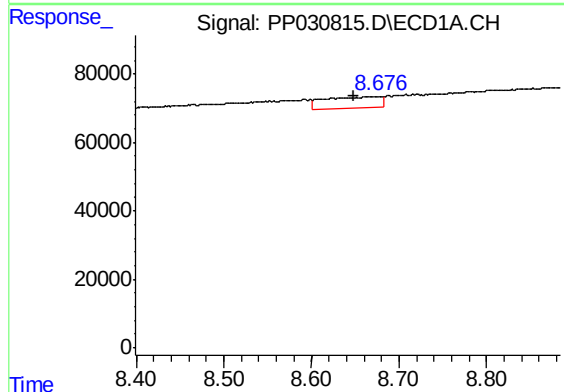


#34 AR-1260-4

R.T.: 8.675 min
Delta R.T.: 0.027 min
Response: 147416
Conc: 74.20 ng/ml

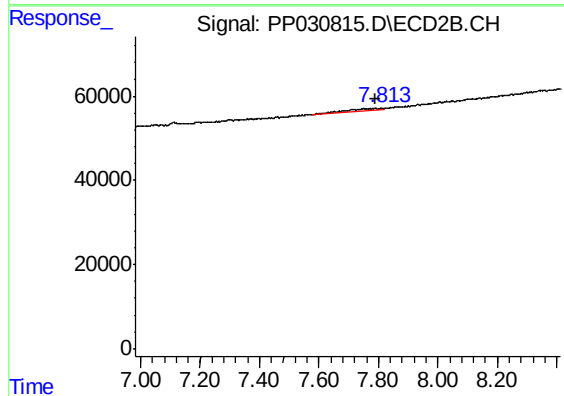

#34 AR-1260-4


R.T.: 7.812 min
Delta R.T.: 0.020 min
Response: 41894
Conc: 24.97 ng/ml

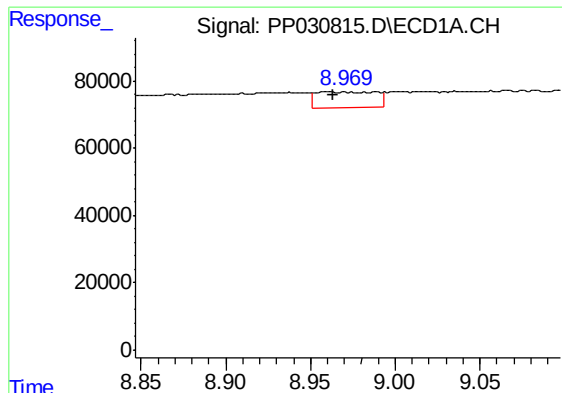

#35 AR-1260-5

R.T.: 8.960 min
Delta R.T.: -0.003 min
Response: 111320
Conc: 28.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-6

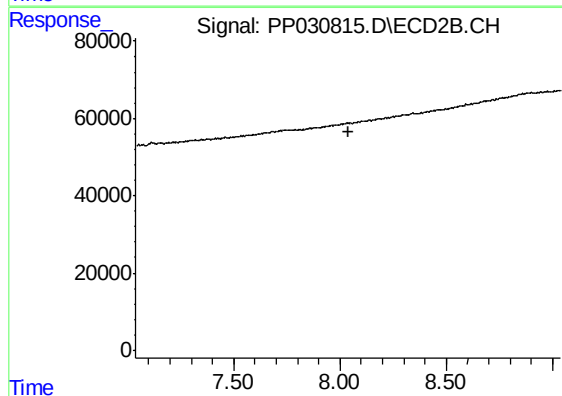

#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 8.037 min
Response: 0
Conc: N.D.