

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102420\
 Data File : PP030816.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Oct 2020 9:26
 Operator : DD\AJ
 Sample : MDL-PCB-BL-S-7
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-PCB-BL-S-7

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 06:19:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Oct 22 12:07:08 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.804	4.086	1225812	1120760	18.472	18.060
2)	SA Decachlor...	10.689	9.426	724985	744630	19.917	19.940
Target Compounds							
9)	L2 AR-1221-2	5.150	4.442	17138	13806	36.885	33.116
32)	L7 AR-1260-2	8.082f	0.000	24285	0	11.715	N.D. #
33)	L7 AR-1260-3	0.000	7.297	0	30627	N.D.	14.611 #
34)	L7 AR-1260-4	8.658	7.786	135773	2426	68.338	1.446 #
35)	L7 AR-1260-5	8.951	8.034	33795	9228	8.777	2.273 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102420\
Data File : PP030816.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Oct 2020 9:26
Operator : DD\AJ
Sample : MDL-PCB-BL-S-7
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:19:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102120.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Oct 22 12:07:08 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

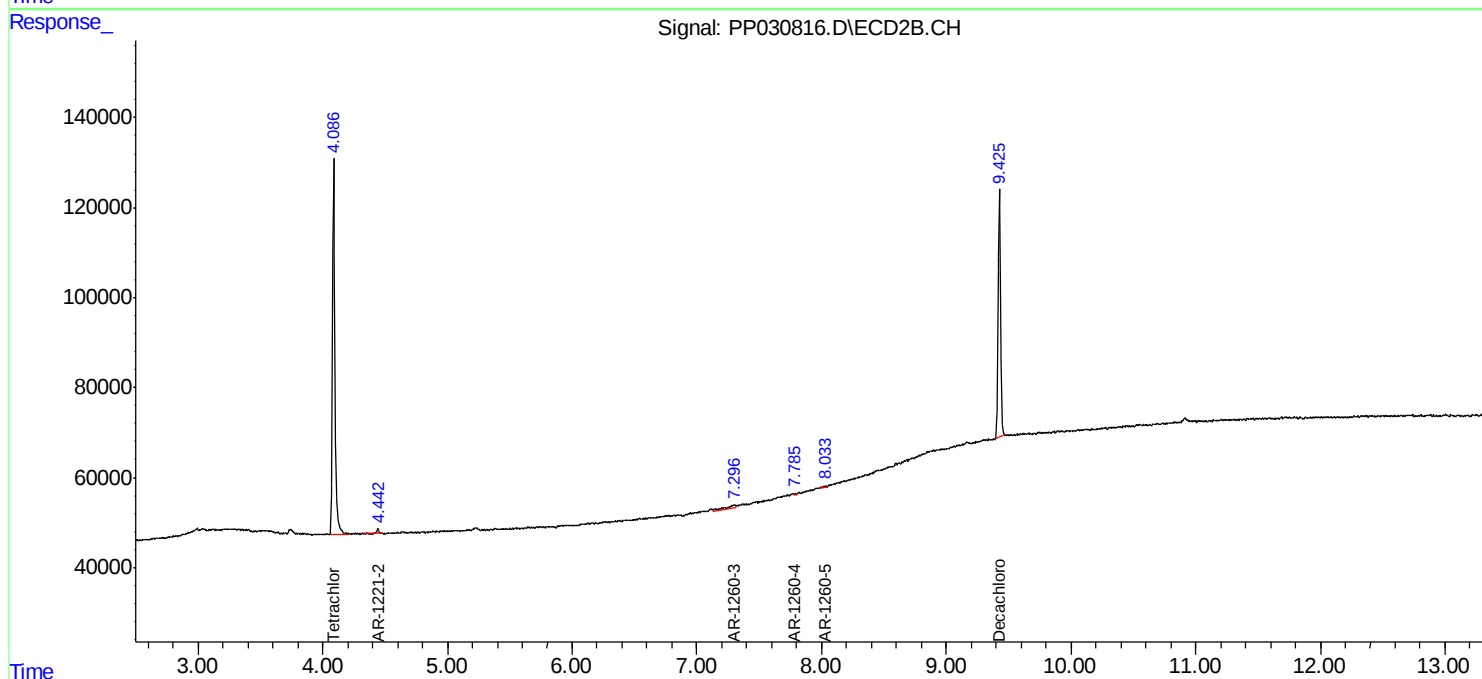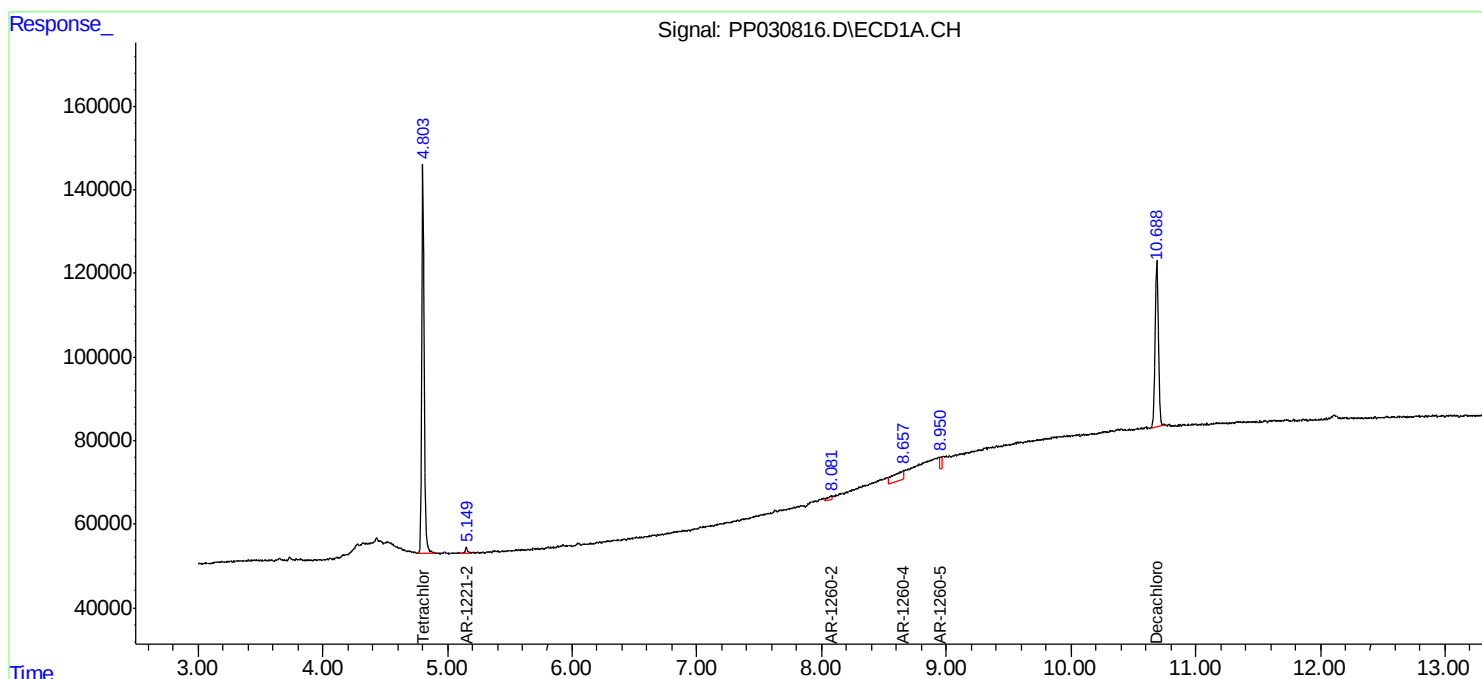


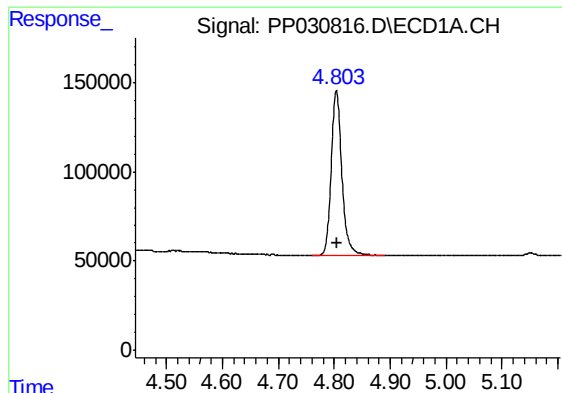

#1 Tetrachloro-m-xylene


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1225812
Conc: 18.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

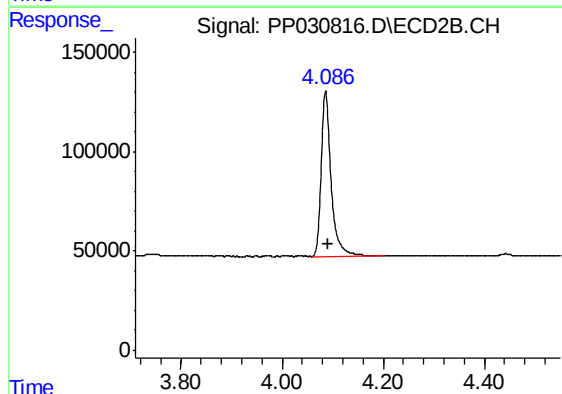


#1 Tetrachloro-m-xylene

R.T.: 4.086 min
Delta R.T.: -0.004 min
Response: 1120760
Conc: 18.06 ng/ml

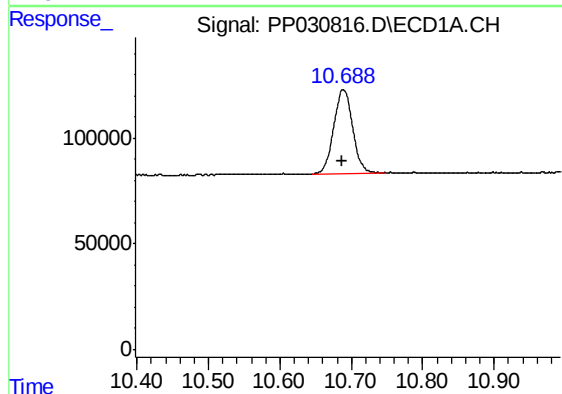


#2 Decachlorobiphenyl

R.T.: 10.689 min
Delta R.T.: 0.002 min
Response: 724985
Conc: 19.92 ng/ml

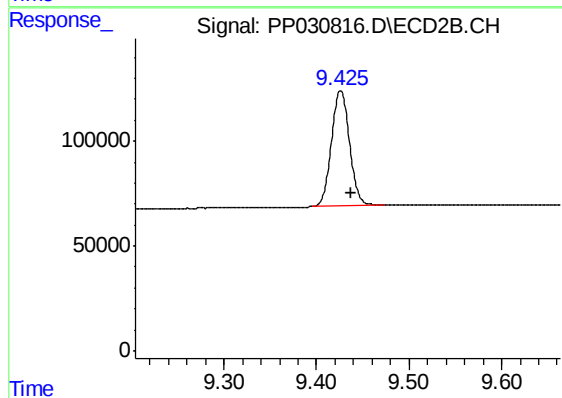

#2 Decachlorobiphenyl


R.T.: 9.426 min
Delta R.T.: -0.011 min
Response: 744630
Conc: 19.94 ng/ml

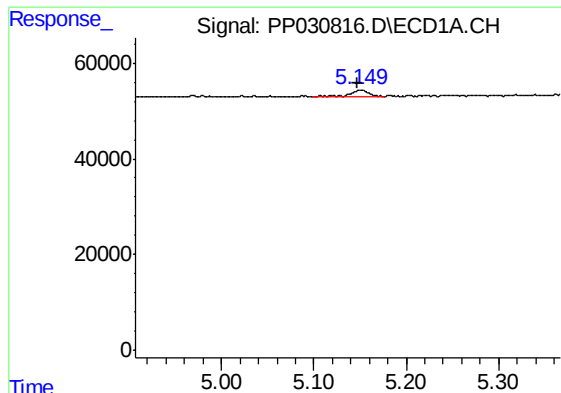

#9 AR-1221-2


R.T.: 5.150 min
Delta R.T.: 0.003 min
Response: 17138
Conc: 36.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

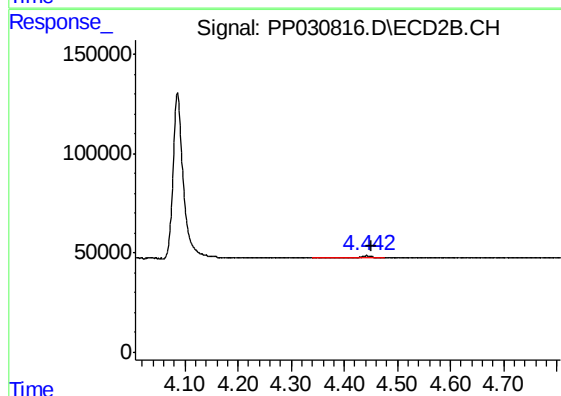


#9 AR-1221-2

R.T.: 4.442 min
Delta R.T.: -0.010 min
Response: 13806
Conc: 33.12 ng/ml

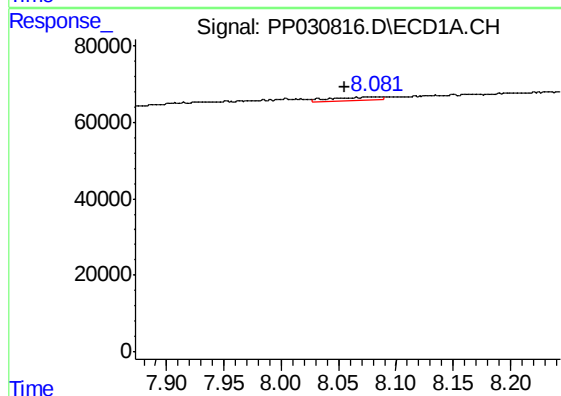


#32 AR-1260-2

R.T.: 8.082 min
Delta R.T.: 0.027 min
Response: 24285
Conc: 11.72 ng/ml

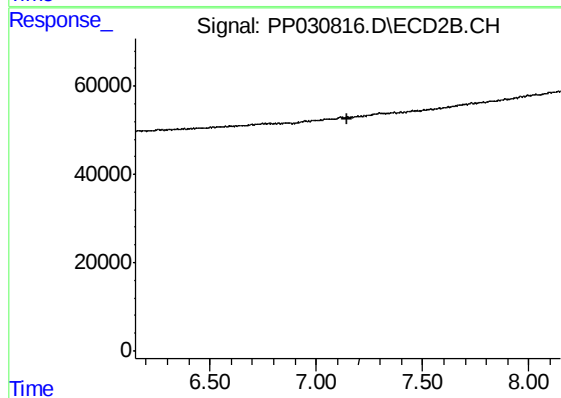

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.149 min
Response: 0
Conc: N.D.

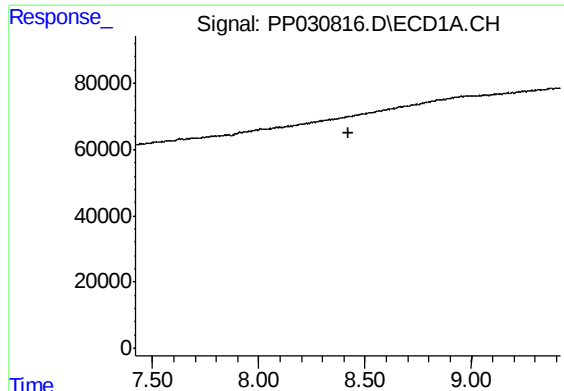

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

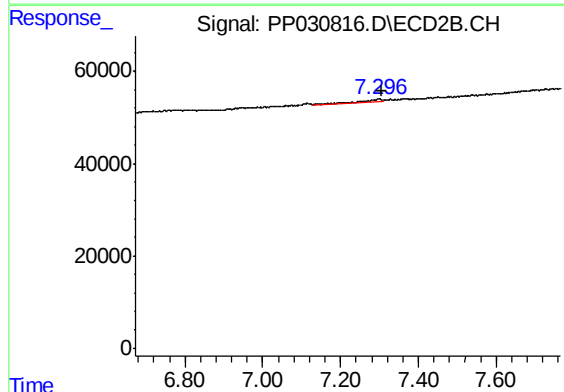


#33 AR-1260-3

R.T.: 7.297 min
Delta R.T.: -0.008 min
Response: 30627
Conc: 14.61 ng/ml

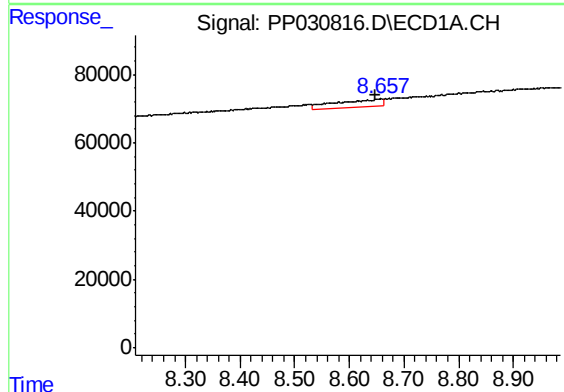


#34 AR-1260-4

R.T.: 8.658 min
Delta R.T.: 0.010 min
Response: 135773
Conc: 68.34 ng/ml

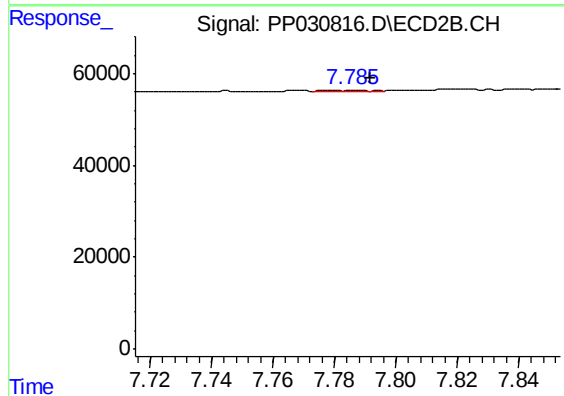

#34 AR-1260-4


R.T.: 7.786 min
Delta R.T.: -0.006 min
Response: 2426
Conc: 1.45 ng/ml

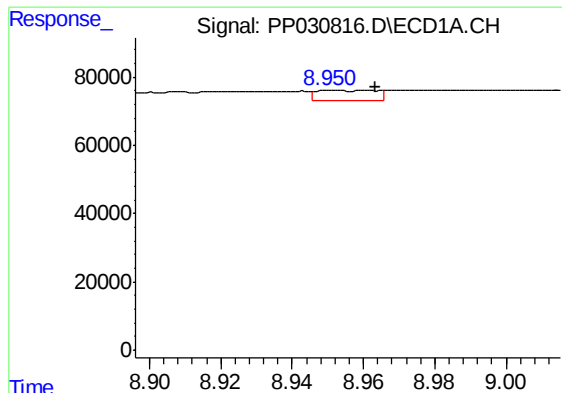

#35 AR-1260-5

R.T.: 8.951 min
Delta R.T.: -0.012 min
Response: 33795
Conc: 8.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-PCB-BL-S-7

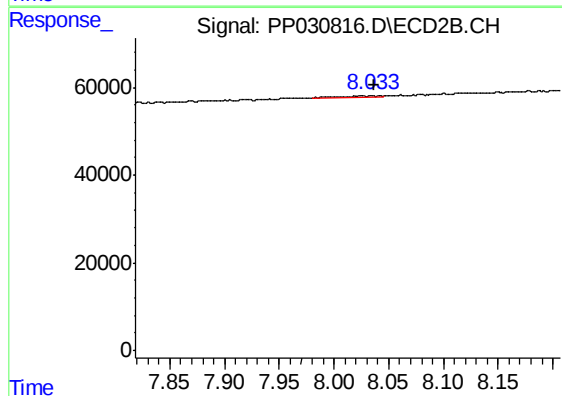

#35 AR-1260-5

R.T.: 8.034 min
Delta R.T.: -0.003 min
Response: 9228
Conc: 2.27 ng/ml