

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102420\  
 Data File : PP030816.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 24 Oct 2020 9:26  
 Operator : DD\AJ  
 Sample : MDL-PCB-BL-S-7  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 MDL-PCB-BL-S-7

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 26 06:19:45 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP102120.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Oct 22 12:07:08 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|---------|--------|--------|
| -----                       |        |       |         |         |        |        |
| System Monitoring Compounds |        |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.804  | 4.086 | 1225812 | 1120760 | 18.472 | 18.060 |
| 2) SA Decachlor...          | 10.689 | 9.426 | 724985  | 744630  | 19.917 | 19.940 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP102420\  
Data File : PP030816.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 24 Oct 2020 9:26  
Operator : DD\AJ  
Sample : MDL-PCB-BL-S-7  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-PCB-BL-S-7

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 26 06:19:45 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP102120.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Oct 22 12:07:08 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

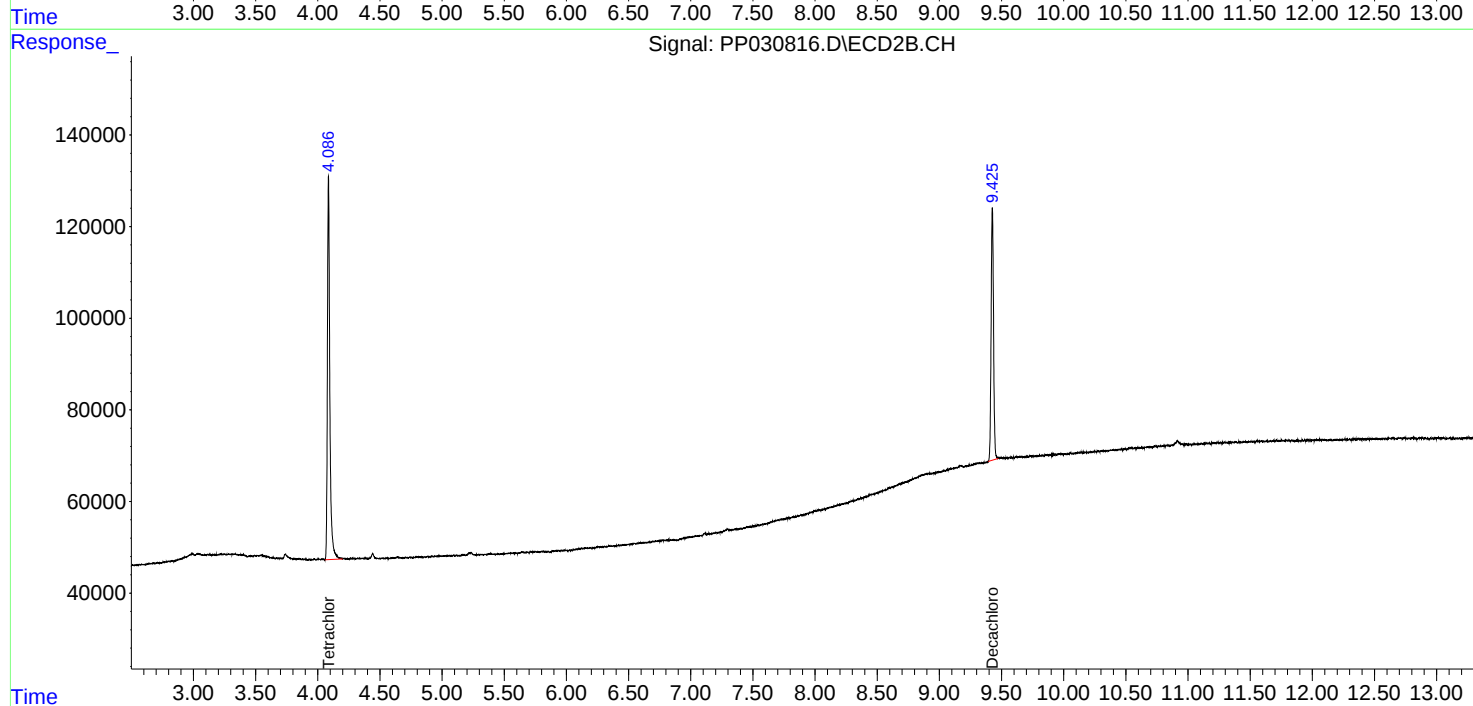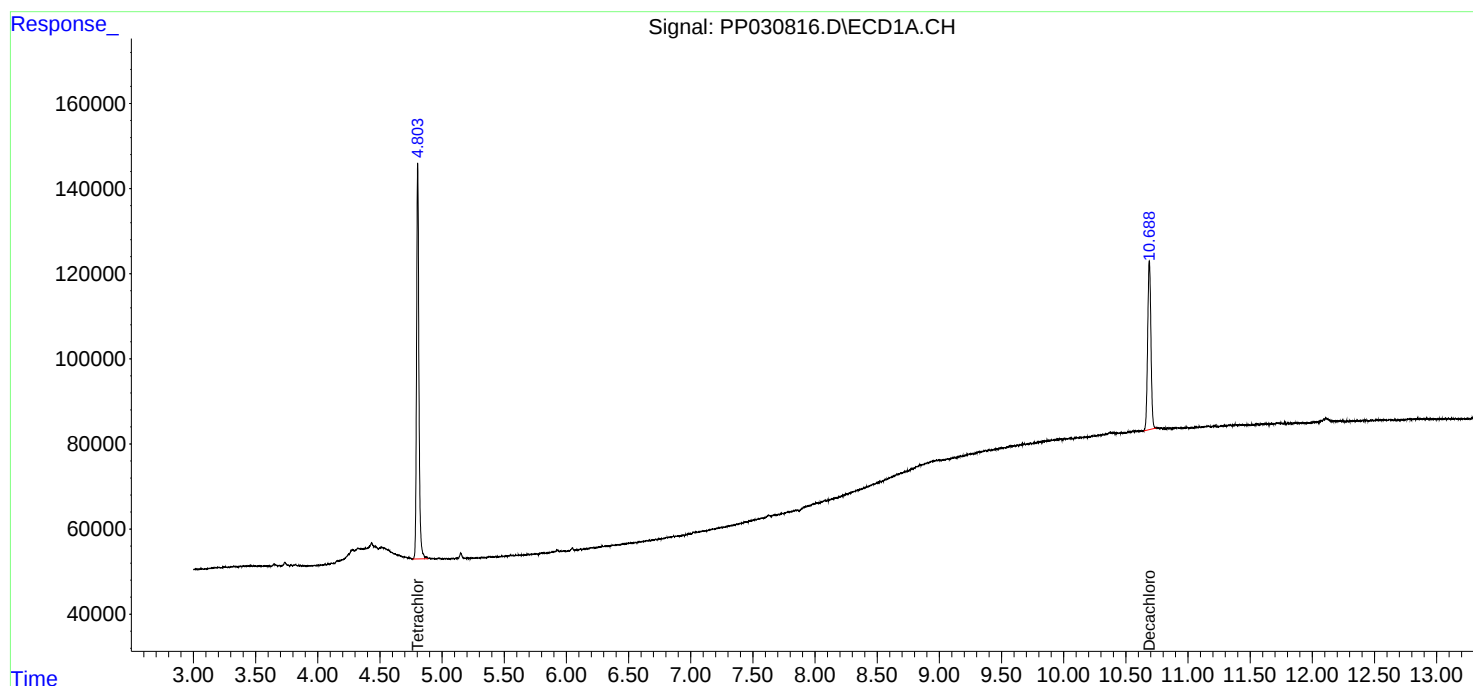


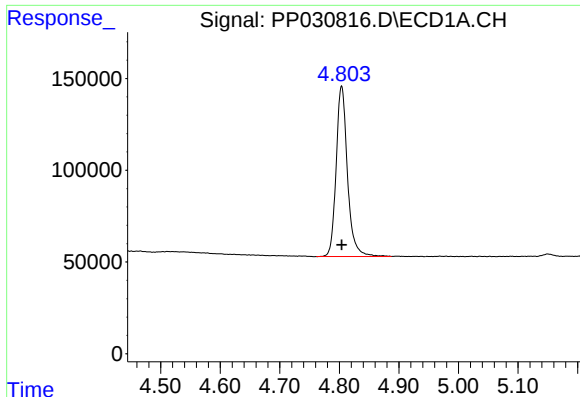

#1 Tetrachloro-m-xylene


R.T.: 4.804 min  
Delta R.T.: 0.000 min  
Response: 1225812  
Conc: 18.47 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
MDL-PCB-BL-S-7

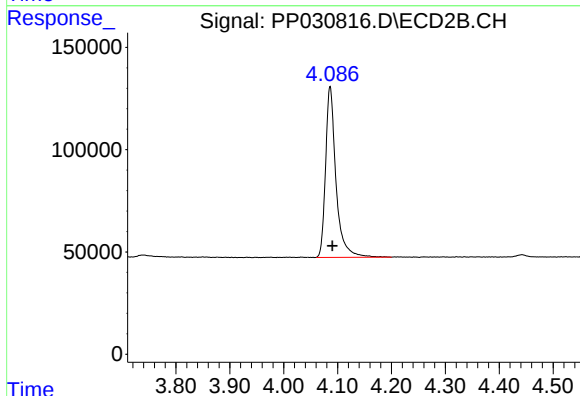


#1 Tetrachloro-m-xylene

R.T.: 4.086 min  
Delta R.T.: -0.004 min  
Response: 1120760  
Conc: 18.06 ng/ml

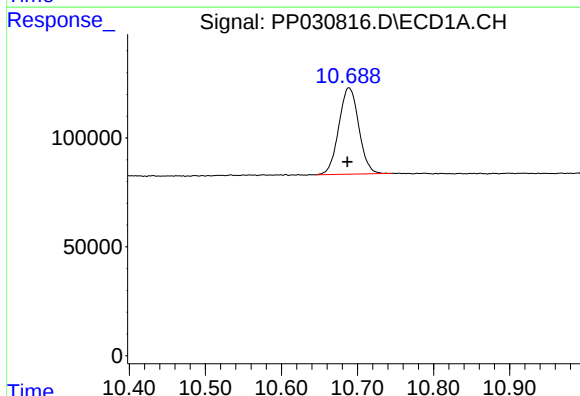

#2 Decachlorobiphenyl

R.T.: 10.689 min  
Delta R.T.: 0.002 min  
Response: 724985  
Conc: 19.92 ng/ml

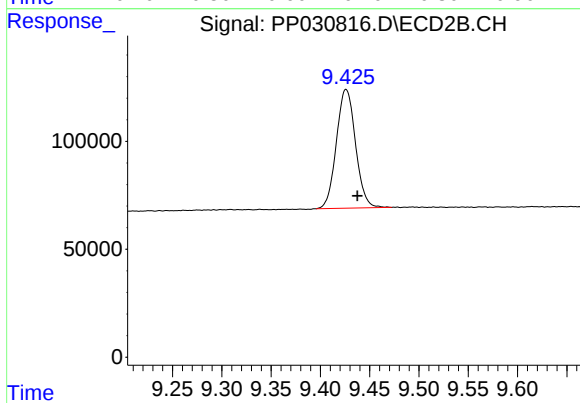

#2 Decachlorobiphenyl

R.T.: 9.426 min  
Delta R.T.: -0.011 min  
Response: 744630  
Conc: 19.94 ng/ml