

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 10:35
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:53:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.422	3.672	31547264	29280184	19.068	21.976
2)	SA Decachlor...	10.235	8.760	38392332	29723038	23.958	23.914
Target Compounds							
3)	L1 AR-1016-1	5.596	4.775	905077	953203	20.624	20.723
4)	L1 AR-1016-2	5.618	4.793	1391290	1372889	22.036	21.928
5)	L1 AR-1016-3	5.681	4.972	925911	674156	22.934	19.552
6)	L1 AR-1016-4	5.779	5.014	616399	632926	17.880	21.832
7)	L1 AR-1016-5	6.076	5.232	665473	809442	17.408	21.673
8)	L2 AR-1221-1	4.631	0.000	3272076	0	149.389	N.D. #
9)	L2 AR-1221-2	4.728	3.962	568302	2007955	35.435	150.798 #
10)	L2 AR-1221-3	4.795	4.053	610461	677861	12.512	16.347 #
11)	L3 AR-1232-1	4.795	4.053	610461	677861	16.443	21.379 #
12)	L3 AR-1232-2	5.325	4.793	731315	1372889	36.099	44.751
13)	L3 AR-1232-3	5.618	4.972	1391290	674156	45.781	41.951
14)	L3 AR-1232-4	5.779	5.056	616399	759401	38.618	50.193 #
15)	L3 AR-1232-5	5.871	5.232	566701	809442	41.854	47.381
16)	L4 AR-1242-1	5.596	4.775	905077	953203	25.891	24.737
17)	L4 AR-1242-2	5.618	4.793	1391290	1372889	26.001	26.198
18)	L4 AR-1242-3	5.681	4.972	925911	674156	26.916	23.321
19)	L4 AR-1242-4	5.779	5.056	616399	759401	21.544	25.047
20)	L4 AR-1242-5	6.525	5.589	227174	759054	6.295	21.753 #
21)	L5 AR-1248-1	5.596	4.775	905077	953203	31.194	33.590
22)	L5 AR-1248-2	5.871	5.014	566701	632926	13.371	15.442
23)	L5 AR-1248-3	6.076	5.056	665473	759401	12.875	18.061 #
24)	L5 AR-1248-4	6.478	5.232	189068	809442	3.431	16.505 #
25)	L5 AR-1248-5	6.525	5.631	227174	169773	3.997	4.087
26)	L6 AR-1254-1	6.456	5.589	634791	759054	10.171	10.479
27)	L6 AR-1254-2	6.674	5.738	595549	578508	6.201	9.008 #
28)	L6 AR-1254-3	7.047	6.162	772647	1005993	8.264	10.161
29)	L6 AR-1254-4	7.331	6.406f	232035	358080	3.757	6.951 #
30)	L6 AR-1254-5	7.748	6.800	2056623	1599492	27.124	19.189 #
31)	L7 AR-1260-1	7.207	6.278	1569163	1604414	20.602	22.832
32)	L7 AR-1260-2	7.465	6.468	1804876	2094607	21.561	26.141
33)	L7 AR-1260-3	7.826	6.624	1457719	1679078	22.619	22.059
34)	L7 AR-1260-4	8.052	7.100	1912735	1370690	25.322	23.452
35)	L7 AR-1260-5	8.376	7.344	3519574	2740226	26.432	21.882
36)	L8 AR-1262-1	7.826	6.892	1457719	644990	14.894	17.436
37)	L8 AR-1262-2	8.376	7.100	3519574	1370690	23.102	17.066 #
38)	L8 AR-1262-3	8.704	7.630	1962665	696071	17.794	11.263 #
39)	L8 AR-1262-4	8.771	7.693	1639260	1908227	26.158	17.178 #
40)	L8 AR-1262-5	9.458	8.195	1427209	760864	22.263	15.505 #
41)	L9 AR-1268-1	8.704	7.630	1962665	696071	9.553	3.859 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 10:35
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1660 LOD 25 PPB
 ALS Vial : 5 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:53:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.771f	7.693	1639260	1908227	8.383	11.661 #
43) L9	AR-1268-3	9.013	7.905	305716	193644	1.701	1.330
44) L9	AR-1268-4	9.458	8.195	1427209	760864	18.263	13.625 #
45) L9	AR-1268-5	9.887	8.496	463072	379056	0.800	0.857


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

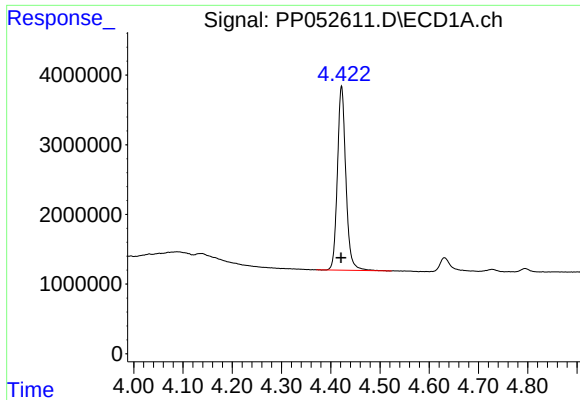

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 31547264
Conc: 19.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

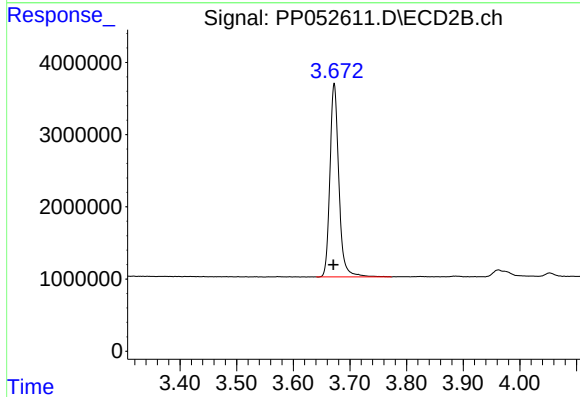


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.001 min
Response: 29280184
Conc: 21.98 ng/ml

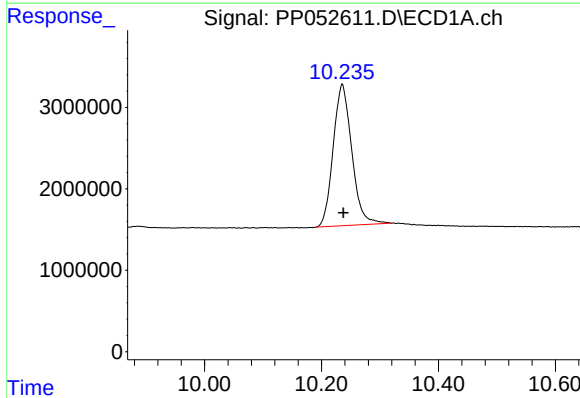


#2 Decachlorobiphenyl

R.T.: 10.235 min
Delta R.T.: -0.002 min
Response: 38392332
Conc: 23.96 ng/ml

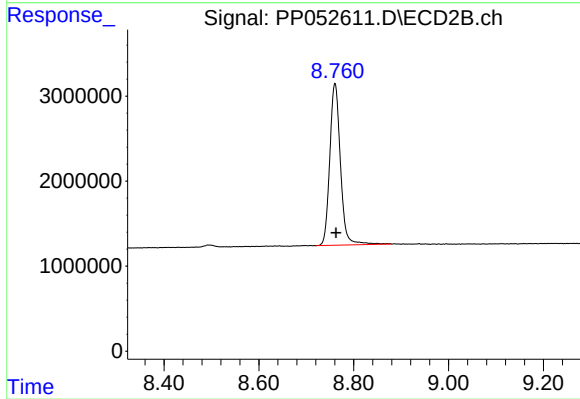

#2 Decachlorobiphenyl


R.T.: 8.760 min
Delta R.T.: -0.002 min
Response: 29723038
Conc: 23.91 ng/ml

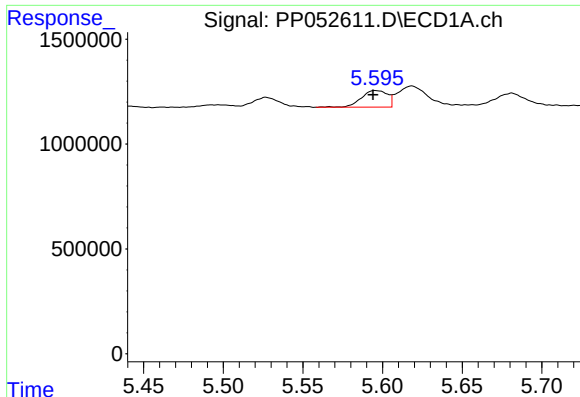

#3 AR-1016-1


R.T.: 5.596 min
Delta R.T.: 0.002 min
Response: 905077
Conc: 20.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

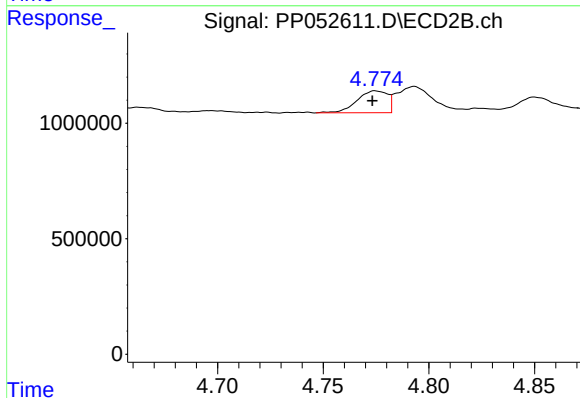


#3 AR-1016-1

R.T.: 4.775 min
Delta R.T.: 0.002 min
Response: 953203
Conc: 20.72 ng/ml

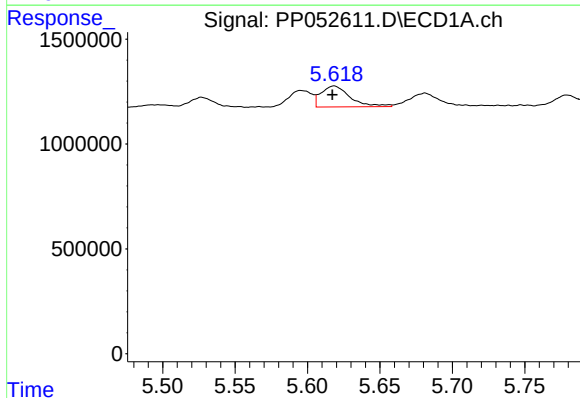


#4 AR-1016-2

R.T.: 5.618 min
Delta R.T.: 0.001 min
Response: 1391290
Conc: 22.04 ng/ml

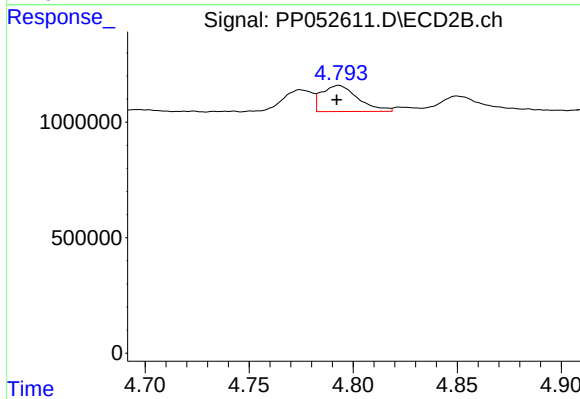

#4 AR-1016-2


R.T.: 4.793 min
Delta R.T.: 0.001 min
Response: 1372889
Conc: 21.93 ng/ml

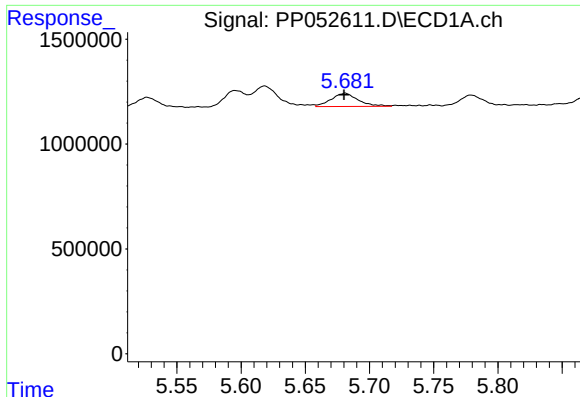

#5 AR-1016-3


R.T.: 5.681 min
Delta R.T.: 0.000 min
Response: 925911
Conc: 22.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

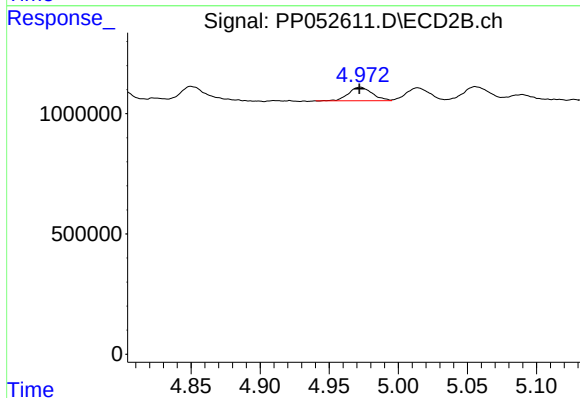


#5 AR-1016-3

R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 674156
Conc: 19.55 ng/ml

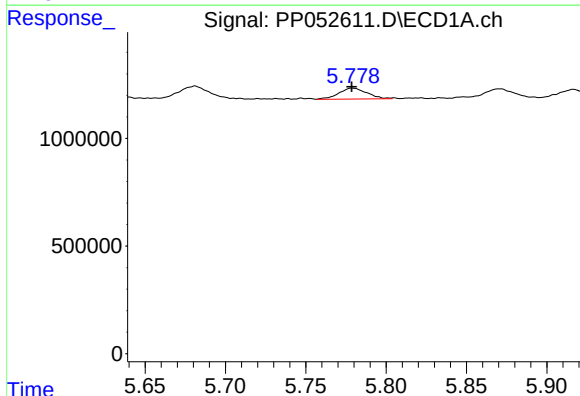


#6 AR-1016-4

R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 616399
Conc: 17.88 ng/ml

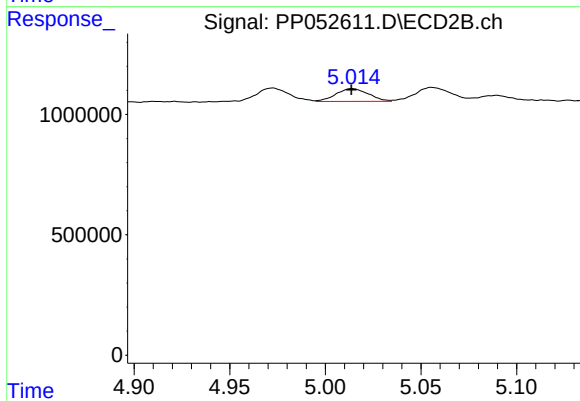

#6 AR-1016-4


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 632926
Conc: 21.83 ng/ml

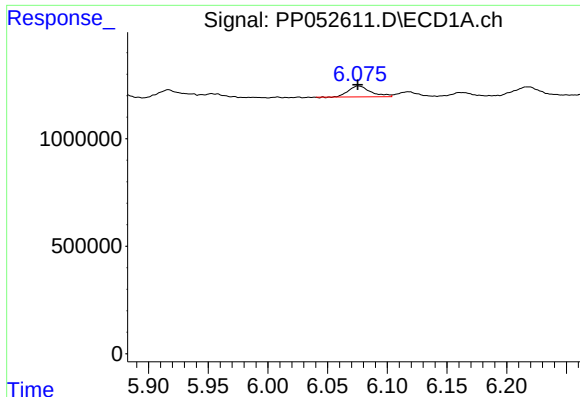

#7 AR-1016-5


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 665473
Conc: 17.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

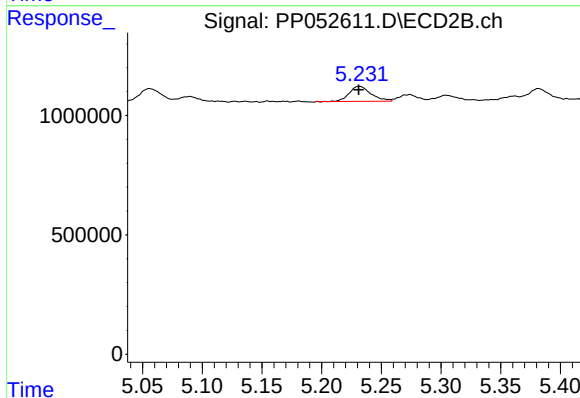


#7 AR-1016-5

R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 809442
Conc: 21.67 ng/ml

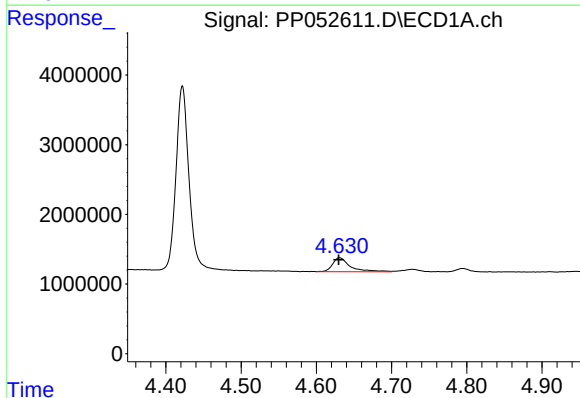


#8 AR-1221-1

R.T.: 4.631 min
Delta R.T.: 0.001 min
Response: 3272076
Conc: 149.39 ng/ml

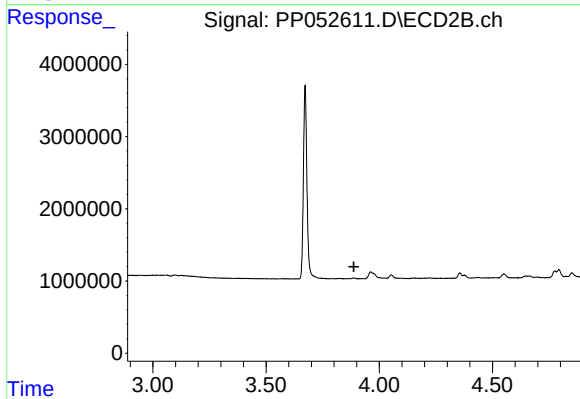

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

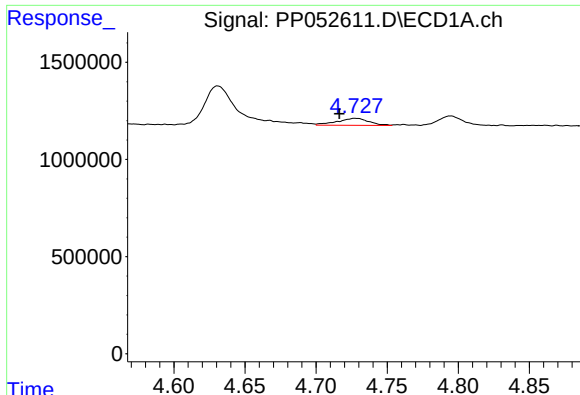

#9 AR-1221-2


R.T.: 4.728 min
Delta R.T.: 0.011 min
Response: 568302
Conc: 35.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

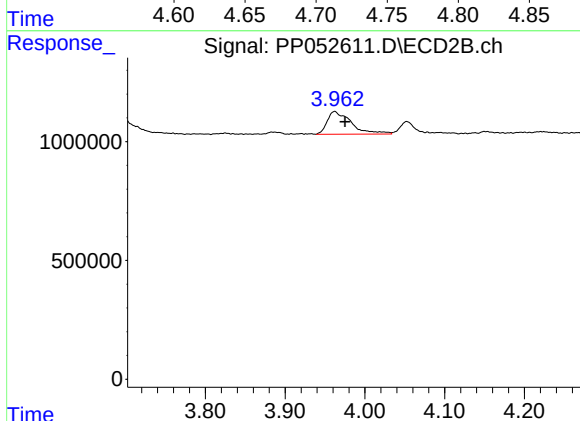


#9 AR-1221-2

R.T.: 3.962 min
Delta R.T.: -0.013 min
Response: 2007955
Conc: 150.80 ng/ml

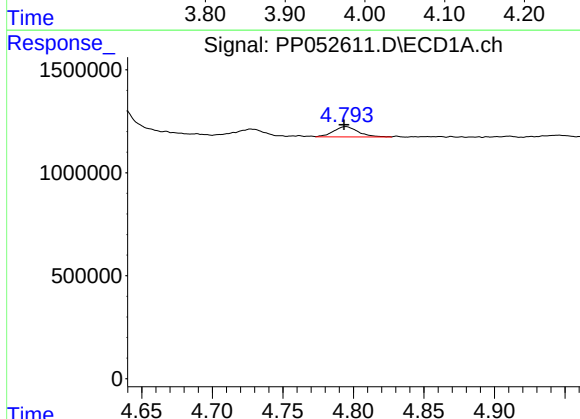


#10 AR-1221-3

R.T.: 4.795 min
Delta R.T.: 0.001 min
Response: 610461
Conc: 12.51 ng/ml

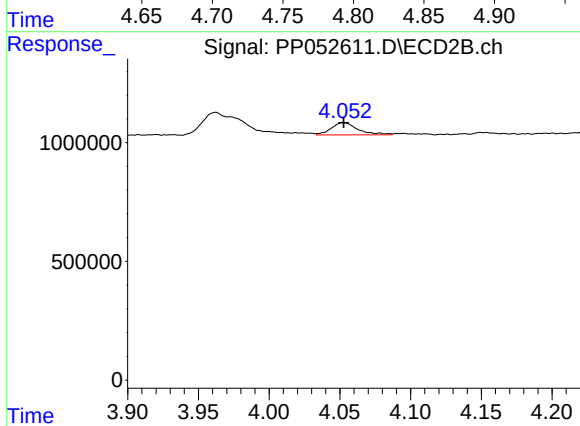

#10 AR-1221-3


R.T.: 4.053 min
Delta R.T.: 0.000 min
Response: 677861
Conc: 16.35 ng/ml

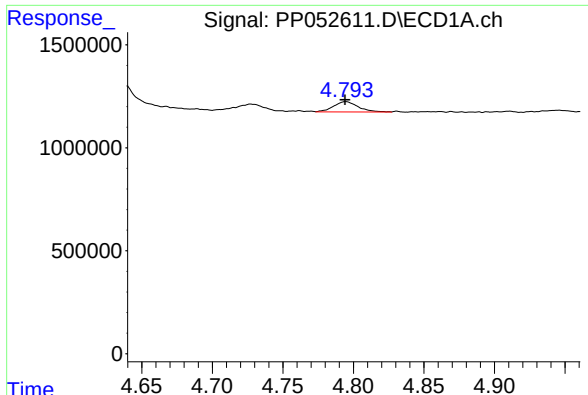

#11 AR-1232-1


R.T.: 4.795 min
Delta R.T.: 0.000 min
Response: 610461
Conc: 16.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

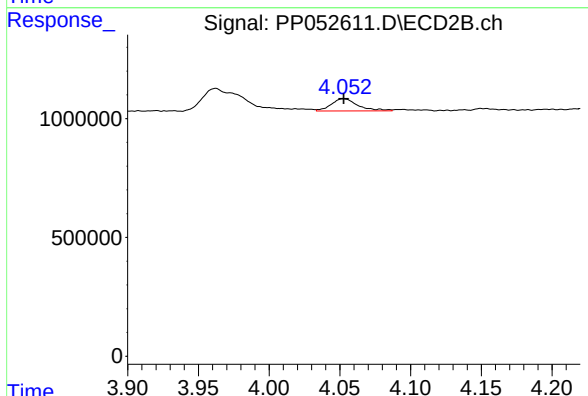


#11 AR-1232-1

R.T.: 4.053 min
Delta R.T.: 0.000 min
Response: 677861
Conc: 21.38 ng/ml

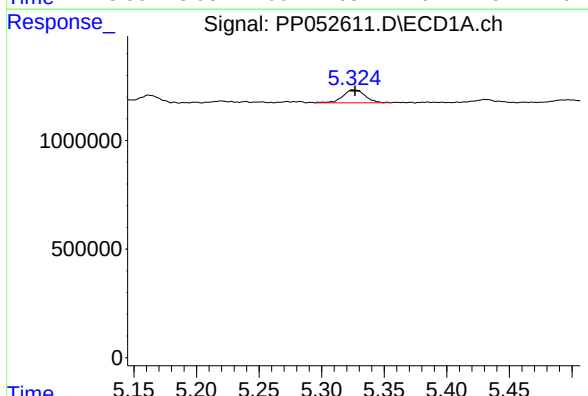


#12 AR-1232-2

R.T.: 5.325 min
Delta R.T.: -0.001 min
Response: 731315
Conc: 36.10 ng/ml

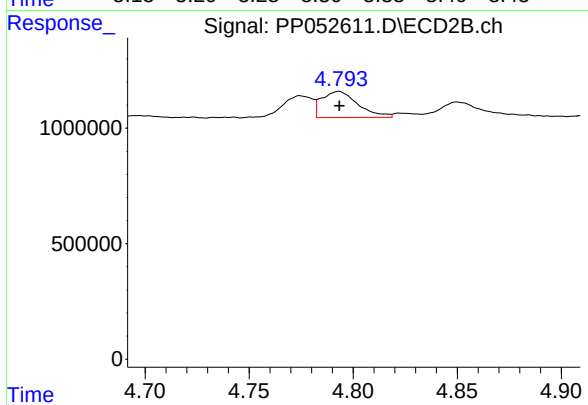

#12 AR-1232-2


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 1372889
Conc: 44.75 ng/ml

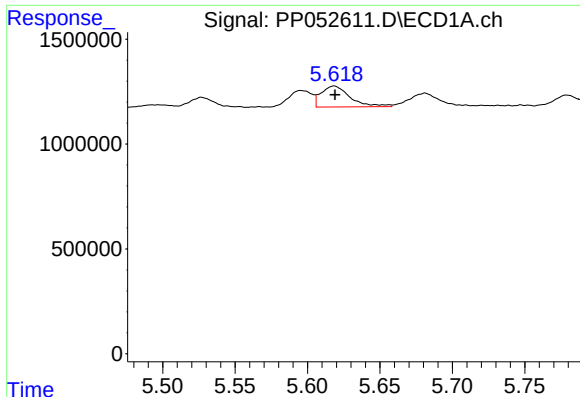

#13 AR-1232-3


R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 1391290
Conc: 45.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

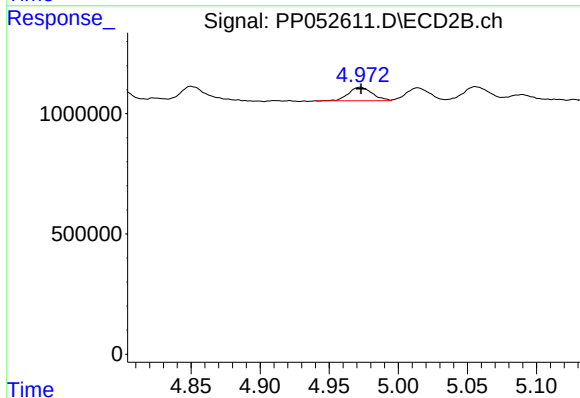


#13 AR-1232-3

R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 674156
Conc: 41.95 ng/ml

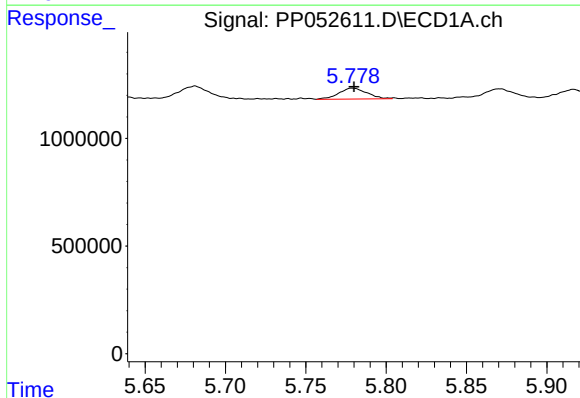


#14 AR-1232-4

R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 616399
Conc: 38.62 ng/ml

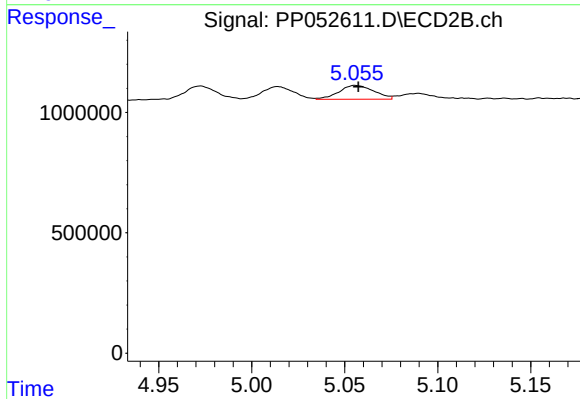

#14 AR-1232-4


R.T.: 5.056 min
Delta R.T.: -0.002 min
Response: 759401
Conc: 50.19 ng/ml

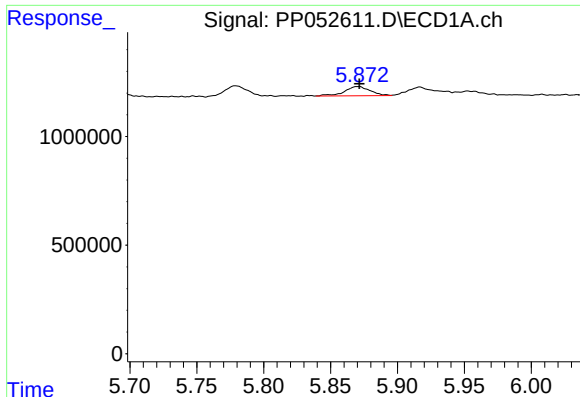

#15 AR-1232-5


R.T.: 5.871 min
Delta R.T.: 0.000 min
Response: 566701
Conc: 41.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

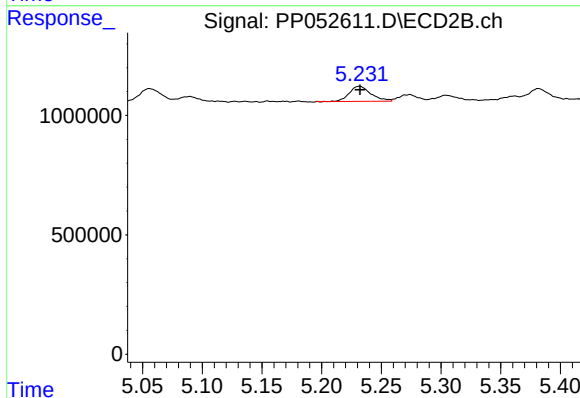


#15 AR-1232-5

R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 809442
Conc: 47.38 ng/ml

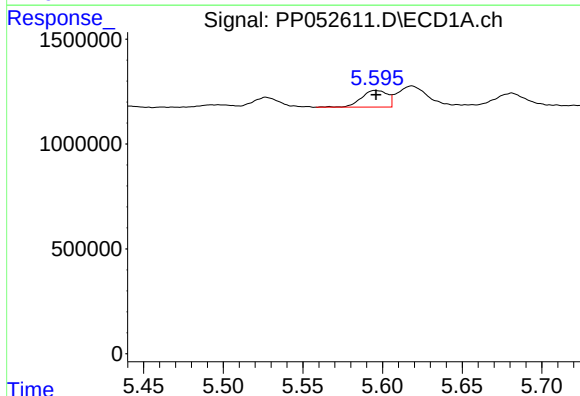


#16 AR-1242-1

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 905077
Conc: 25.89 ng/ml

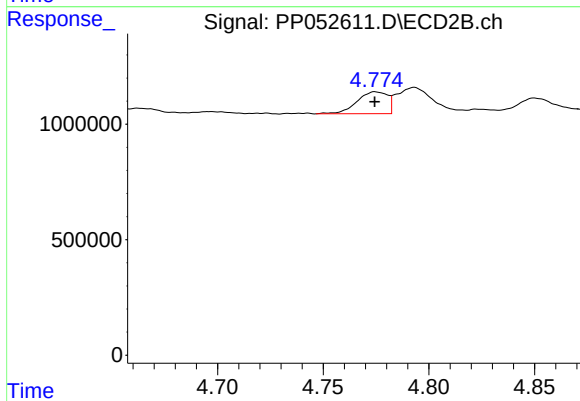

#16 AR-1242-1


R.T.: 4.775 min
Delta R.T.: 0.000 min
Response: 953203
Conc: 24.74 ng/ml

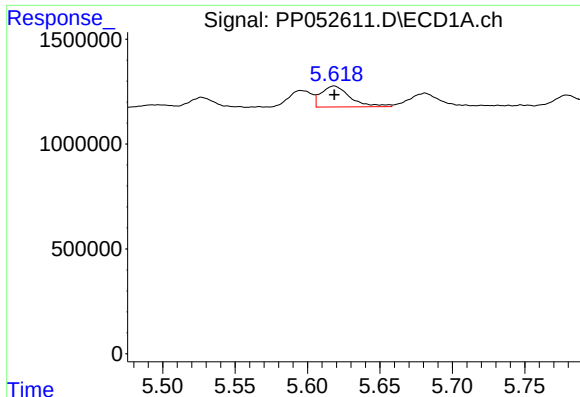

#17 AR-1242-2


R.T.: 5.618 min
Delta R.T.: 0.000 min
Response: 1391290
Conc: 26.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

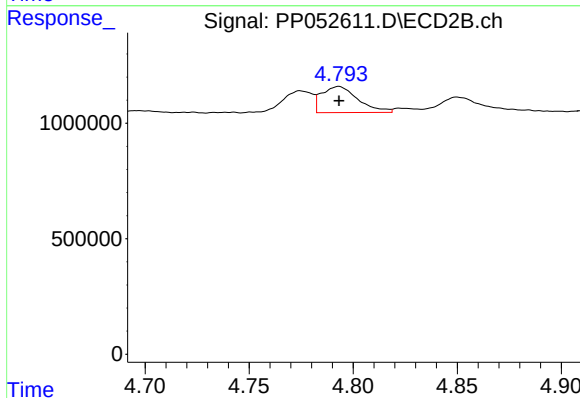


#17 AR-1242-2

R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 1372889
Conc: 26.20 ng/ml

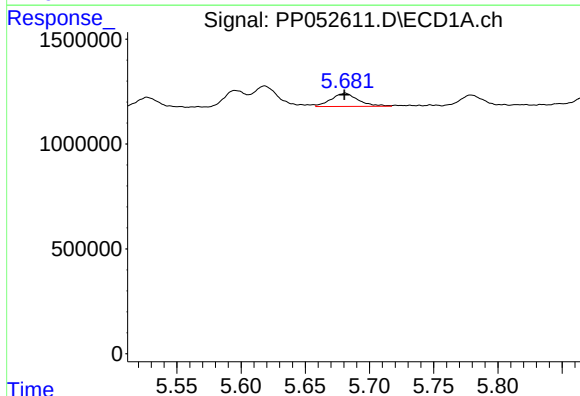


#18 AR-1242-3

R.T.: 5.681 min
Delta R.T.: 0.000 min
Response: 925911
Conc: 26.92 ng/ml

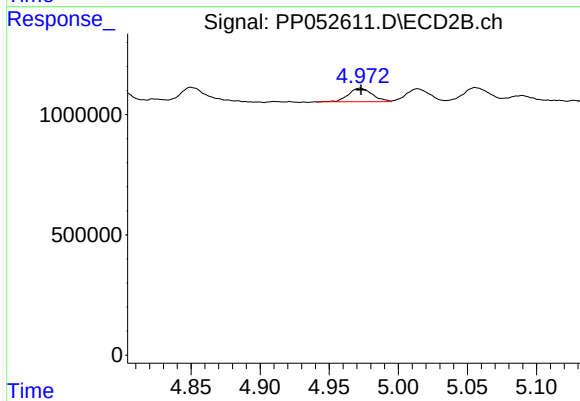

#18 AR-1242-3


R.T.: 4.972 min
Delta R.T.: 0.000 min
Response: 674156
Conc: 23.32 ng/ml

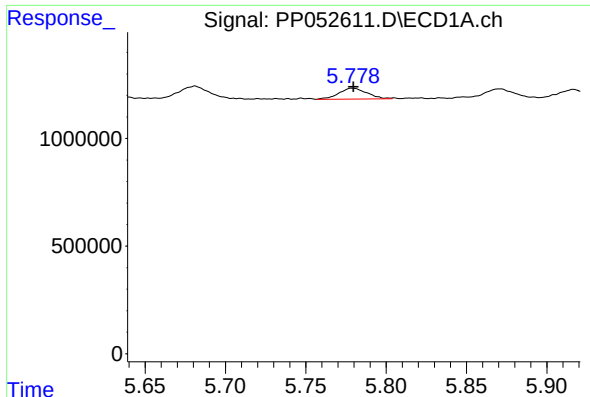

#19 AR-1242-4


R.T.: 5.779 min
Delta R.T.: 0.000 min
Response: 616399
Conc: 21.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

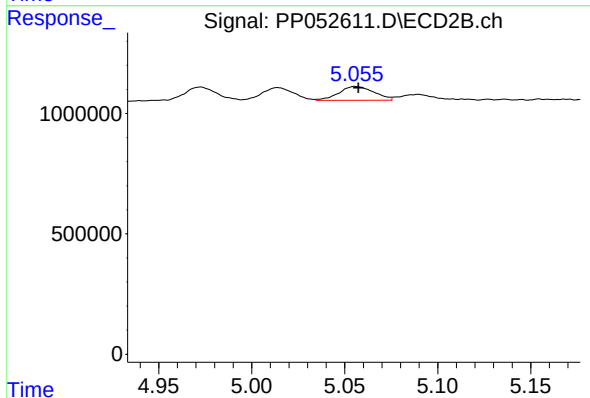


#19 AR-1242-4

R.T.: 5.056 min
Delta R.T.: -0.002 min
Response: 759401
Conc: 25.05 ng/ml

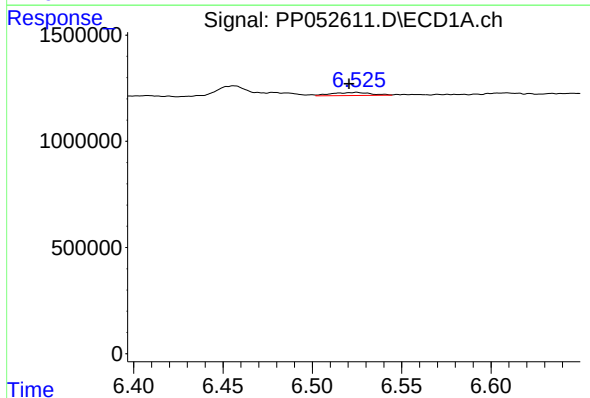


#20 AR-1242-5

R.T.: 6.525 min
Delta R.T.: 0.004 min
Response: 227174
Conc: 6.30 ng/ml

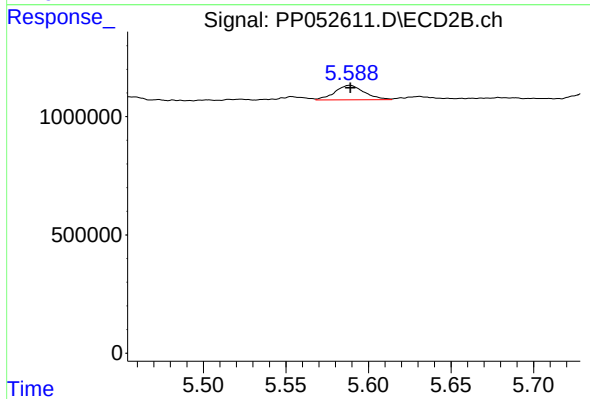

#20 AR-1242-5


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 759054
Conc: 21.75 ng/ml

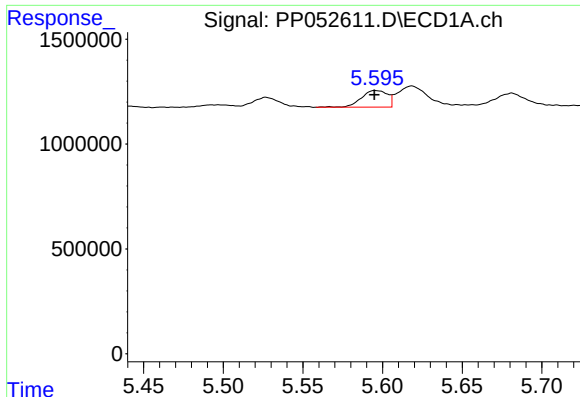

#21 AR-1248-1


R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 905077
Conc: 31.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

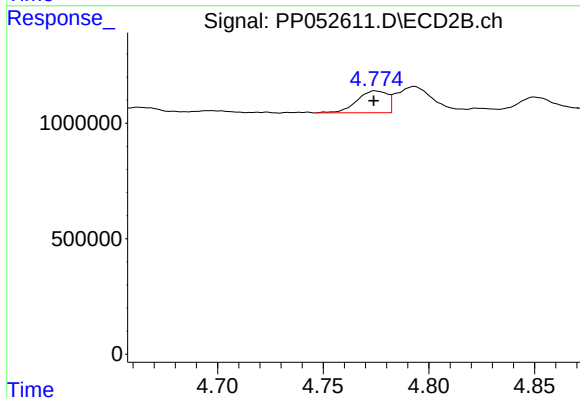


#21 AR-1248-1

R.T.: 4.775 min
Delta R.T.: 0.001 min
Response: 953203
Conc: 33.59 ng/ml

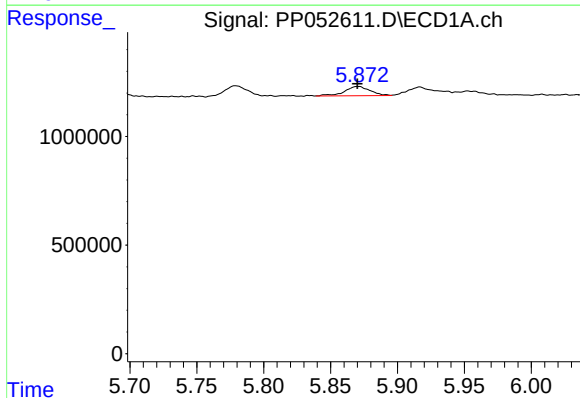


#22 AR-1248-2

R.T.: 5.871 min
Delta R.T.: 0.000 min
Response: 566701
Conc: 13.37 ng/ml

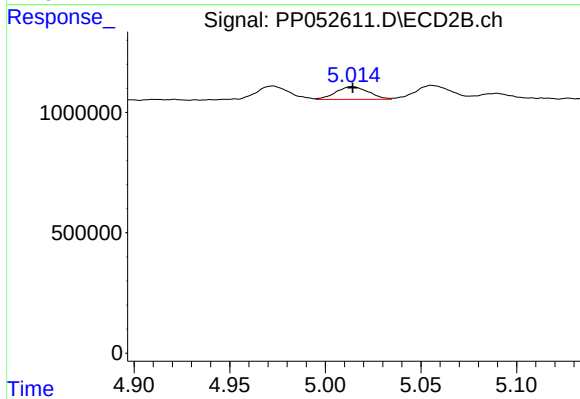

#22 AR-1248-2


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 632926
Conc: 15.44 ng/ml

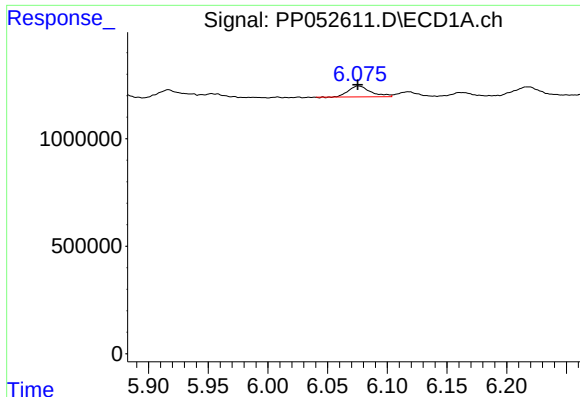

#23 AR-1248-3


R.T.: 6.076 min
Delta R.T.: 0.000 min
Response: 665473
Conc: 12.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

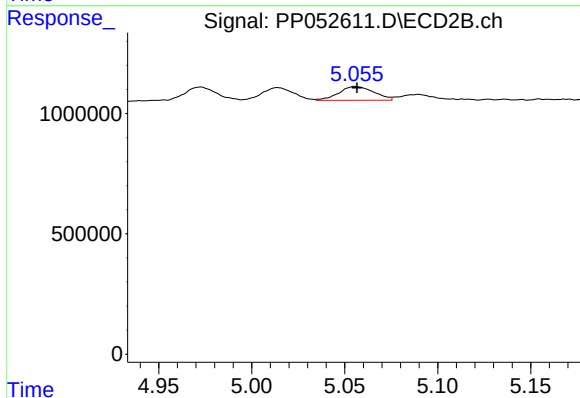


#23 AR-1248-3

R.T.: 5.056 min
Delta R.T.: 0.000 min
Response: 759401
Conc: 18.06 ng/ml

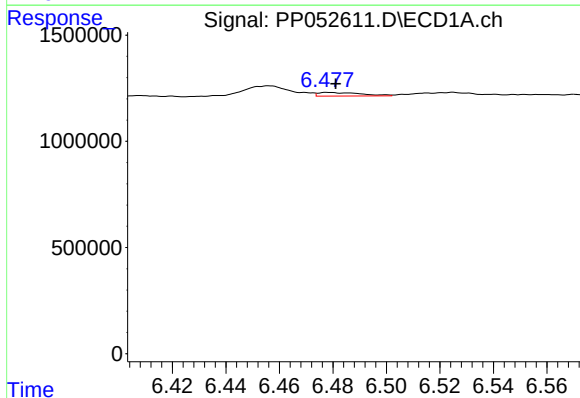


#24 AR-1248-4

R.T.: 6.478 min
Delta R.T.: -0.003 min
Response: 189068
Conc: 3.43 ng/ml

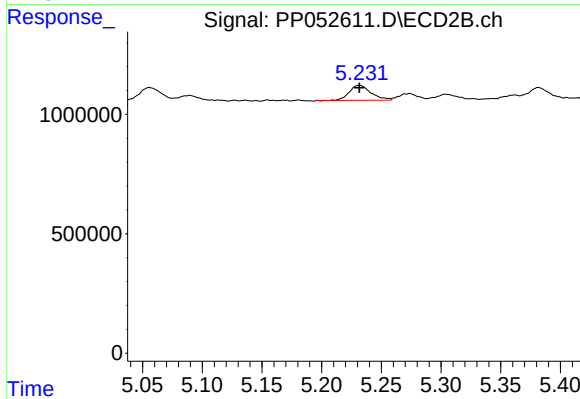

#24 AR-1248-4


R.T.: 5.232 min
Delta R.T.: 0.000 min
Response: 809442
Conc: 16.50 ng/ml

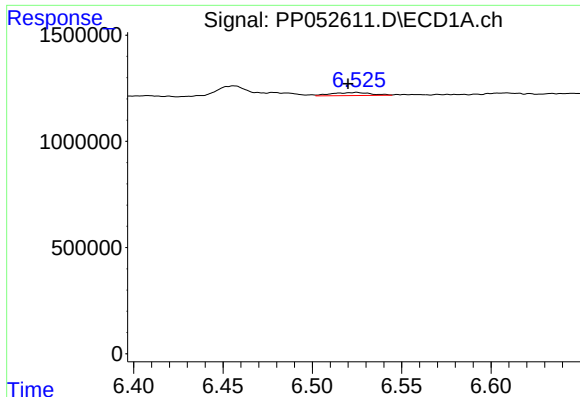

#25 AR-1248-5


R.T.: 6.525 min
Delta R.T.: 0.005 min
Response: 227174
Conc: 4.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

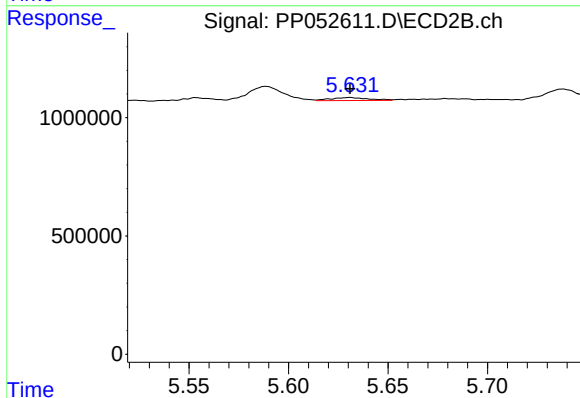


#25 AR-1248-5

R.T.: 5.631 min
Delta R.T.: 0.000 min
Response: 169773
Conc: 4.09 ng/ml

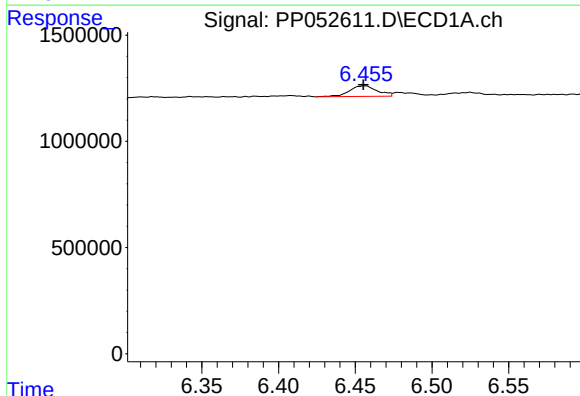


#26 AR-1254-1

R.T.: 6.456 min
Delta R.T.: 0.000 min
Response: 634791
Conc: 10.17 ng/ml

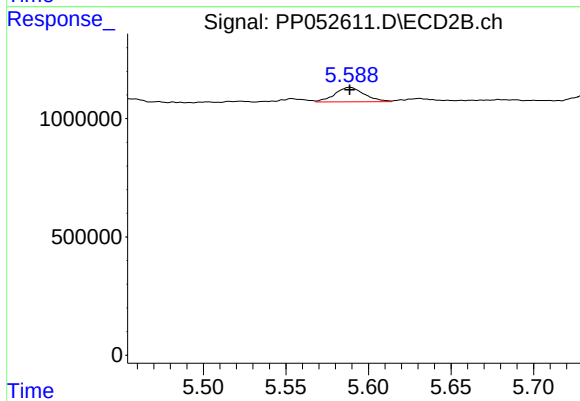

#26 AR-1254-1


R.T.: 5.589 min
Delta R.T.: 0.000 min
Response: 759054
Conc: 10.48 ng/ml

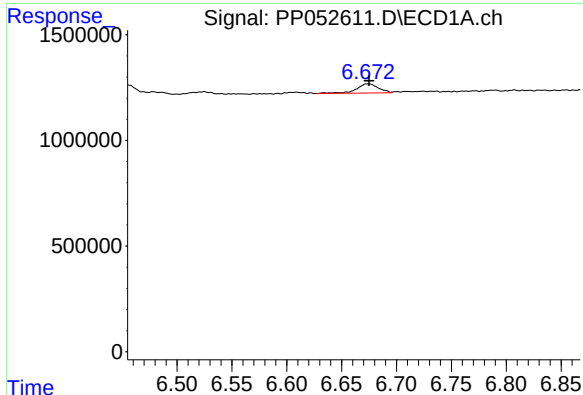

#27 AR-1254-2


R.T.: 6.674 min
Delta R.T.: -0.001 min
Response: 595549
Conc: 6.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

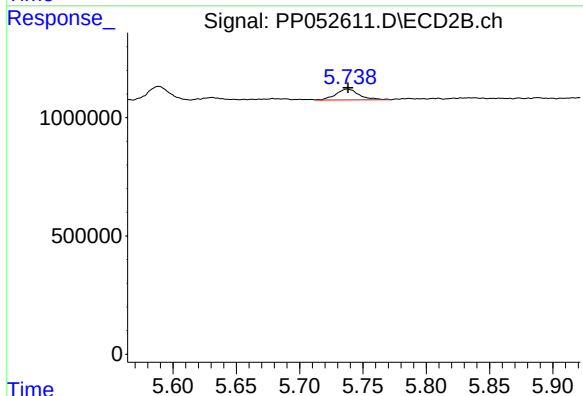


#27 AR-1254-2

R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 578508
Conc: 9.01 ng/ml

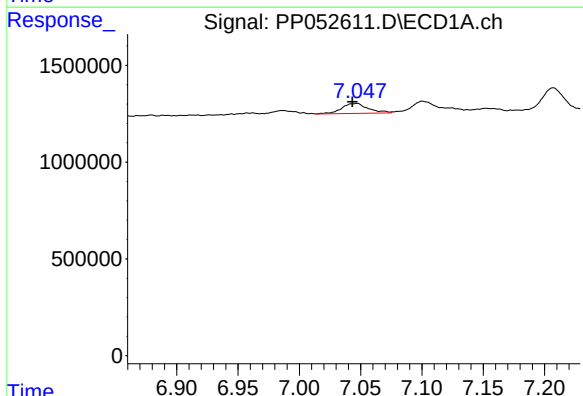


#28 AR-1254-3

R.T.: 7.047 min
Delta R.T.: 0.003 min
Response: 772647
Conc: 8.26 ng/ml

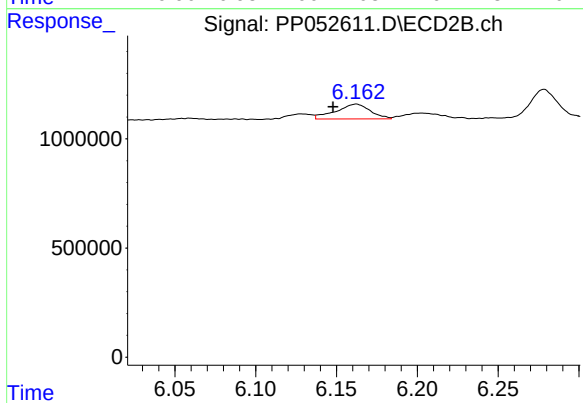

#28 AR-1254-3


R.T.: 6.162 min
Delta R.T.: 0.014 min
Response: 1005993
Conc: 10.16 ng/ml

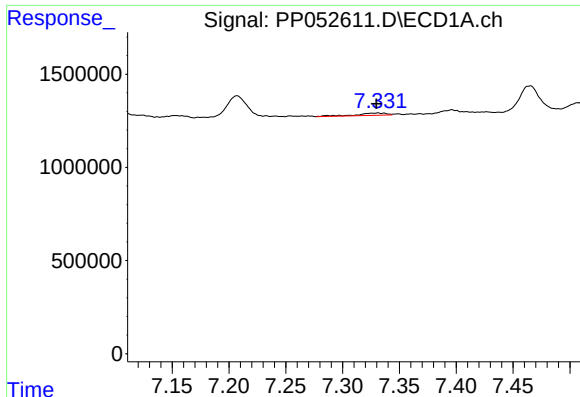

#29 AR-1254-4


R.T.: 7.331 min
Delta R.T.: 0.001 min
Response: 232035
Conc: 3.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

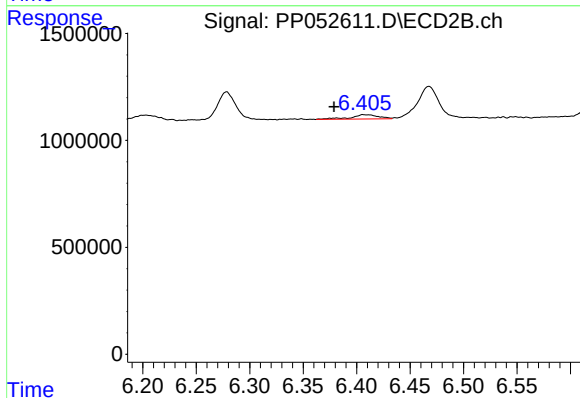


#29 AR-1254-4

R.T.: 6.406 min
Delta R.T.: 0.028 min
Response: 358080
Conc: 6.95 ng/ml

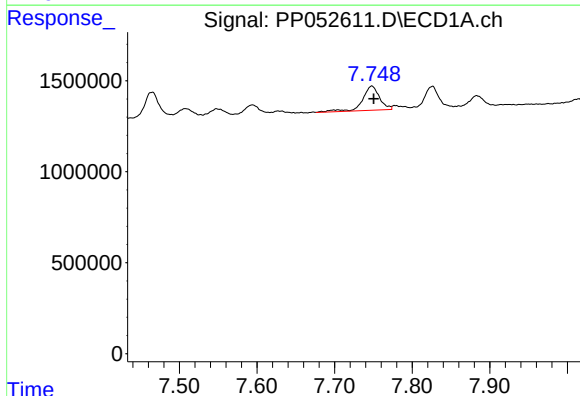


#30 AR-1254-5

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 2056623
Conc: 27.12 ng/ml

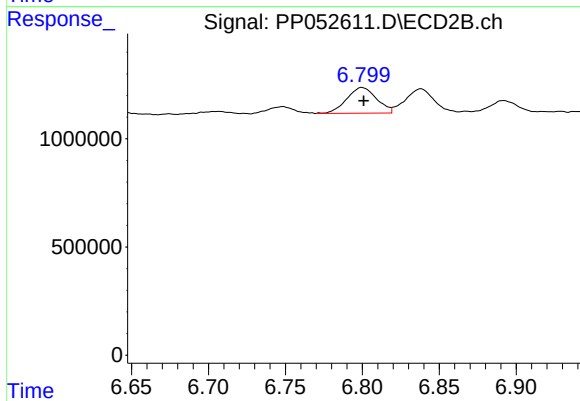

#30 AR-1254-5


R.T.: 6.800 min
Delta R.T.: -0.001 min
Response: 1599492
Conc: 19.19 ng/ml

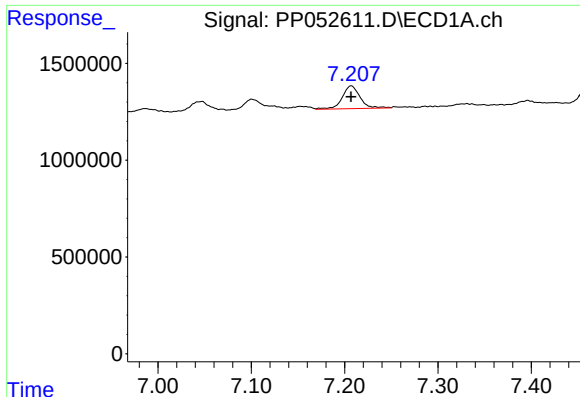

#31 AR-1260-1

R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 1569163
Conc: 20.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

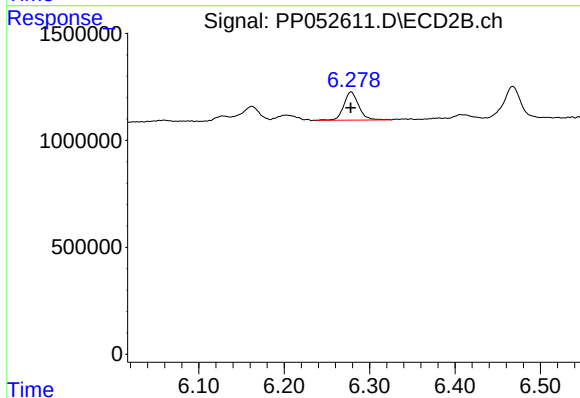

#31 AR-1260-1


R.T.: 6.278 min
Delta R.T.: 0.000 min
Response: 1604414
Conc: 22.83 ng/ml

#32 AR-1260-2

R.T.: 7.465 min
Delta R.T.: 0.000 min
Response: 1804876
Conc: 21.56 ng/ml

#32 AR-1260-2


R.T.: 6.468 min
Delta R.T.: 0.000 min
Response: 2094607
Conc: 26.14 ng/ml

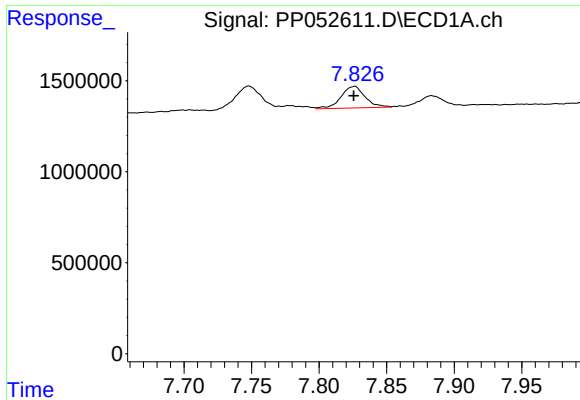

#33 AR-1260-3


R.T.: 7.826 min
Delta R.T.: 0.000 min
Response: 1457719
Conc: 22.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

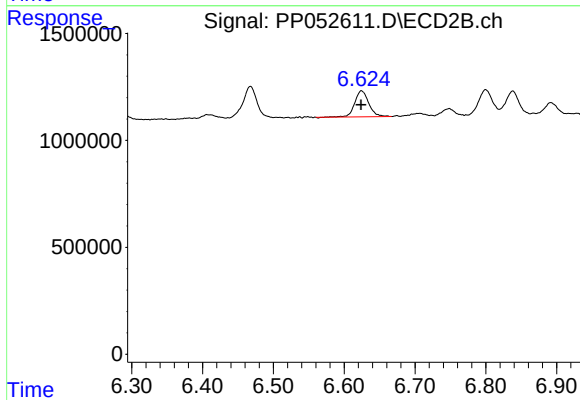


#33 AR-1260-3

R.T.: 6.624 min
Delta R.T.: 0.000 min
Response: 1679078
Conc: 22.06 ng/ml

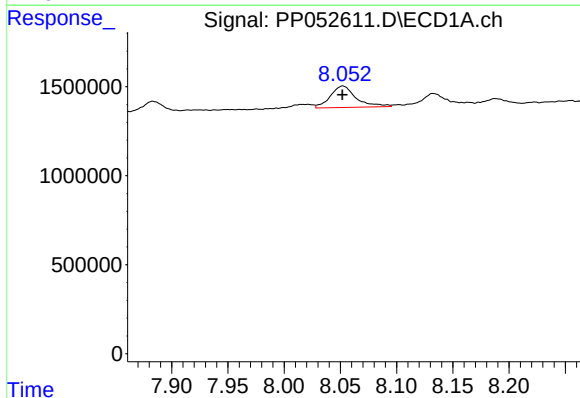


#34 AR-1260-4

R.T.: 8.052 min
Delta R.T.: 0.000 min
Response: 1912735
Conc: 25.32 ng/ml

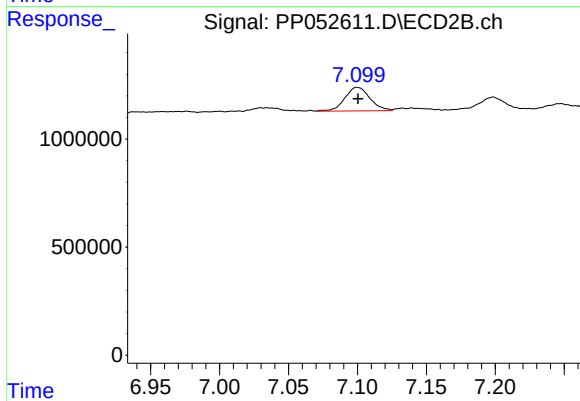

#34 AR-1260-4


R.T.: 7.100 min
Delta R.T.: 0.000 min
Response: 1370690
Conc: 23.45 ng/ml

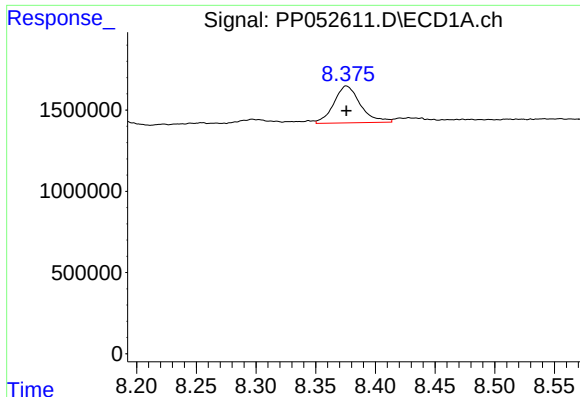

#35 AR-1260-5


R.T.: 8.376 min
Delta R.T.: 0.000 min
Response: 3519574
Conc: 26.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

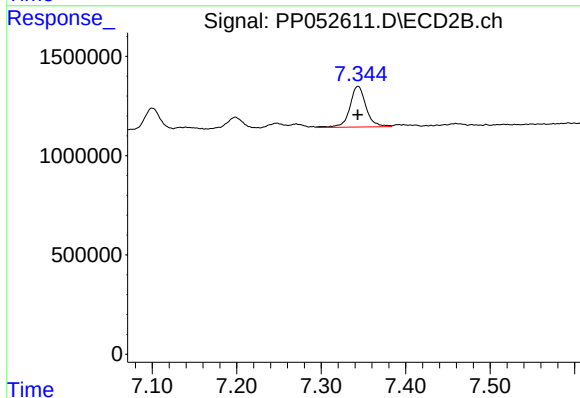


#35 AR-1260-5

R.T.: 7.344 min
Delta R.T.: 0.000 min
Response: 2740226
Conc: 21.88 ng/ml

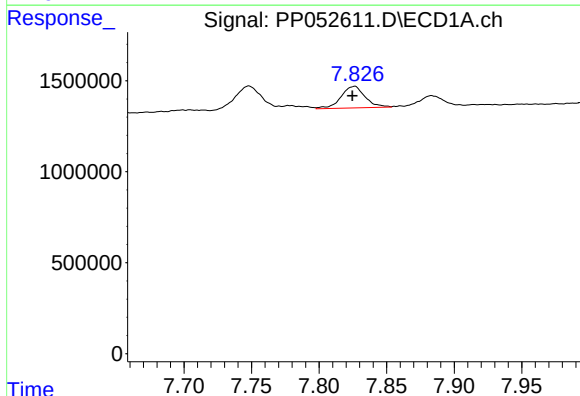


#36 AR-1262-1

R.T.: 7.826 min
Delta R.T.: 0.001 min
Response: 1457719
Conc: 14.89 ng/ml

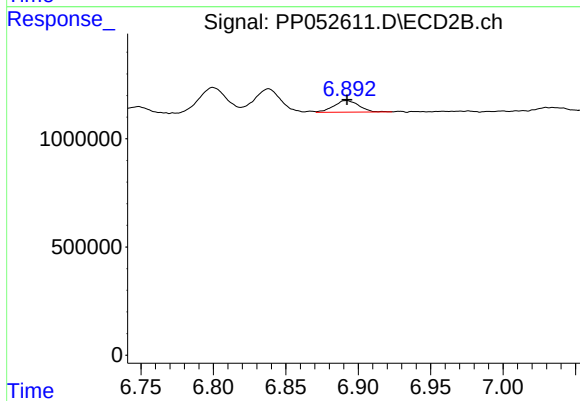

#36 AR-1262-1


R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 644990
Conc: 17.44 ng/ml

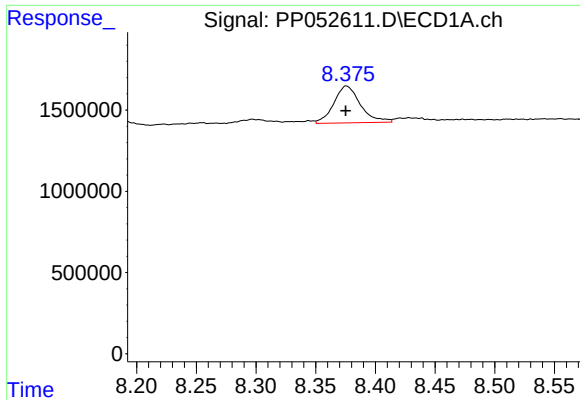

#37 AR-1262-2


R.T.: 8.376 min
Delta R.T.: 0.000 min
Response: 3519574
Conc: 23.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

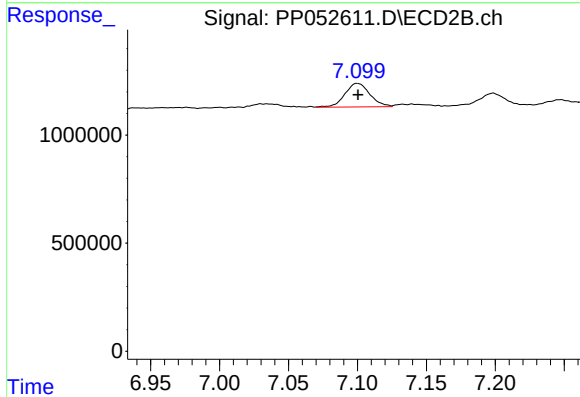


#37 AR-1262-2

R.T.: 7.100 min
Delta R.T.: 0.000 min
Response: 1370690
Conc: 17.07 ng/ml

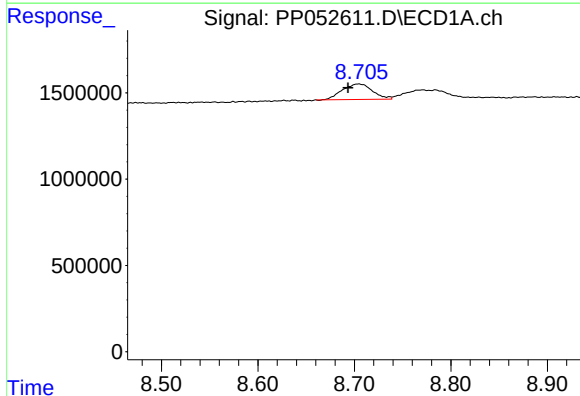


#38 AR-1262-3

R.T.: 8.704 min
Delta R.T.: 0.011 min
Response: 1962665
Conc: 17.79 ng/ml

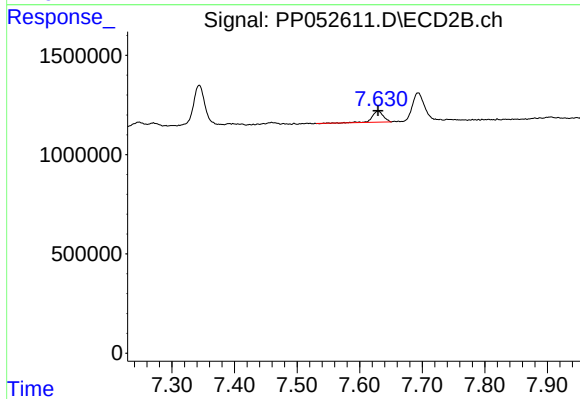

#38 AR-1262-3


R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 696071
Conc: 11.26 ng/ml

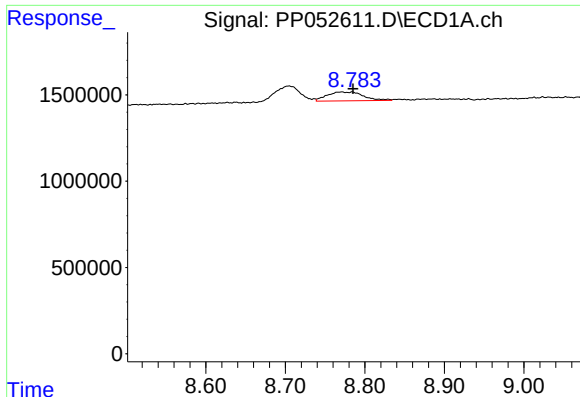

#39 AR-1262-4


R.T.: 8.771 min
Delta R.T.: -0.014 min
Response: 1639260
Conc: 26.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

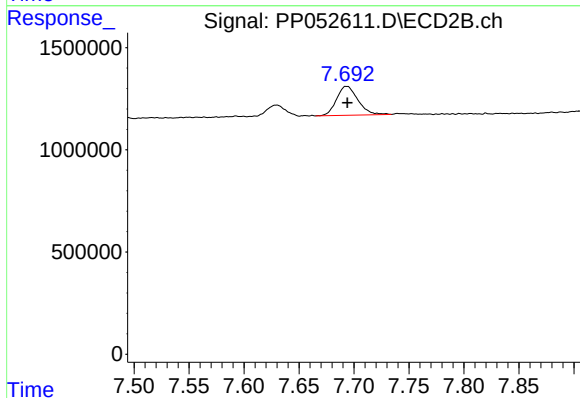


#39 AR-1262-4

R.T.: 7.693 min
Delta R.T.: 0.000 min
Response: 1908227
Conc: 17.18 ng/ml

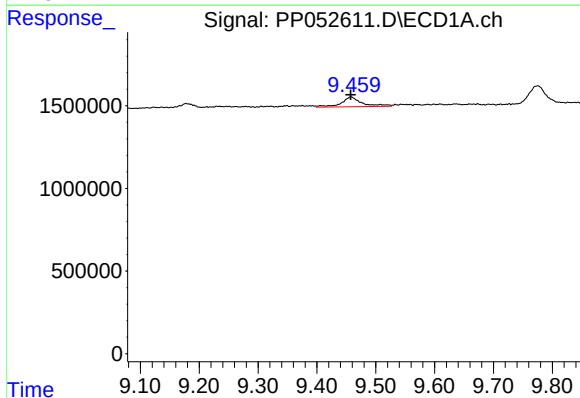


#40 AR-1262-5

R.T.: 9.458 min
Delta R.T.: 0.000 min
Response: 1427209
Conc: 22.26 ng/ml

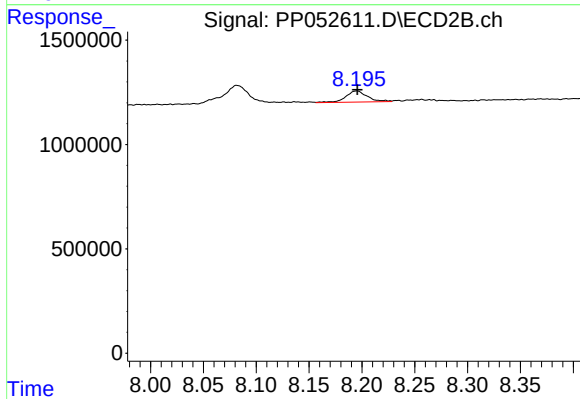

#40 AR-1262-5


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 760864
Conc: 15.50 ng/ml

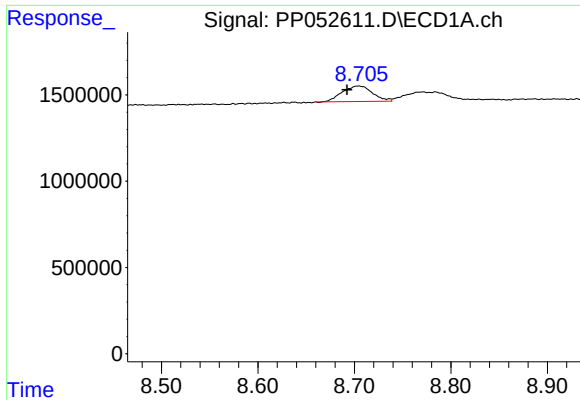

#41 AR-1268-1


R.T.: 8.704 min
Delta R.T.: 0.012 min
Response: 1962665
Conc: 9.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

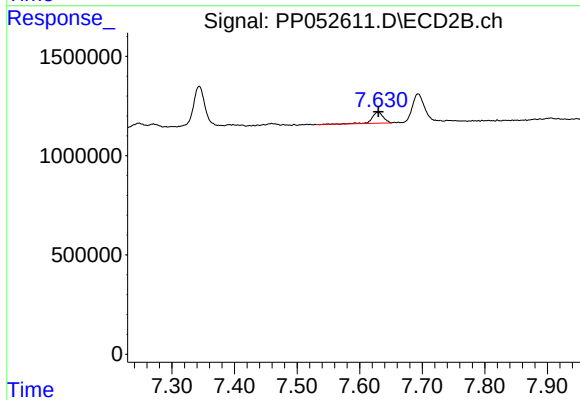


#41 AR-1268-1

R.T.: 7.630 min
Delta R.T.: 0.000 min
Response: 696071
Conc: 3.86 ng/ml

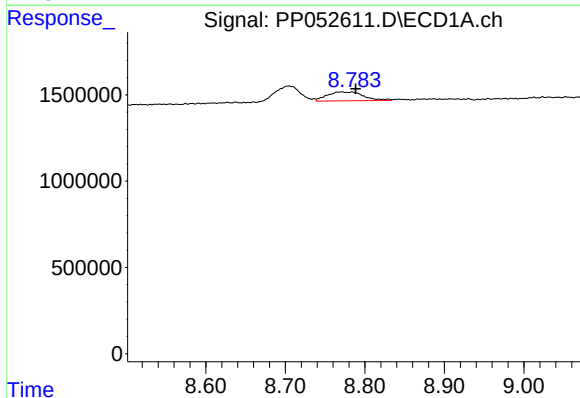


#42 AR-1268-2

R.T.: 8.771 min
Delta R.T.: -0.017 min
Response: 1639260
Conc: 8.38 ng/ml

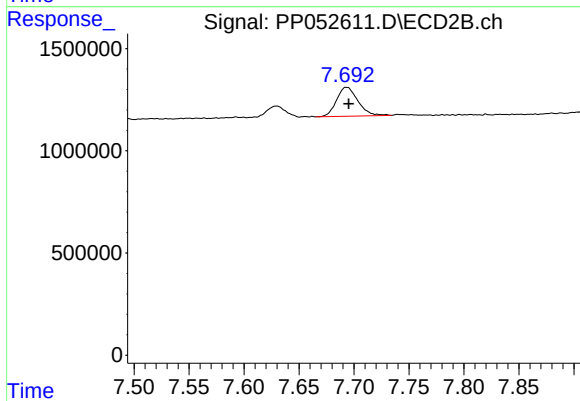

#42 AR-1268-2


R.T.: 7.693 min
Delta R.T.: -0.002 min
Response: 1908227
Conc: 11.66 ng/ml

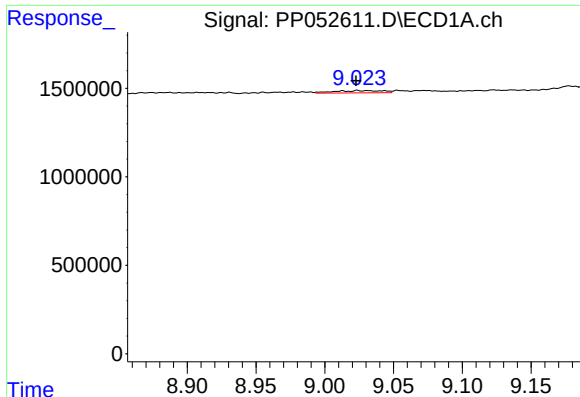

#43 AR-1268-3


R.T.: 9.013 min
Delta R.T.: -0.010 min
Response: 305716
Conc: 1.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

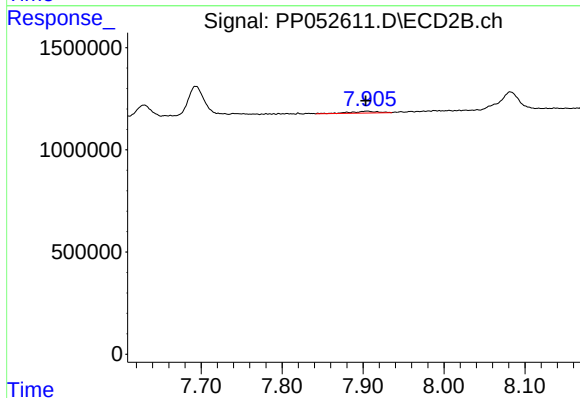


#43 AR-1268-3

R.T.: 7.905 min
Delta R.T.: 0.002 min
Response: 193644
Conc: 1.33 ng/ml

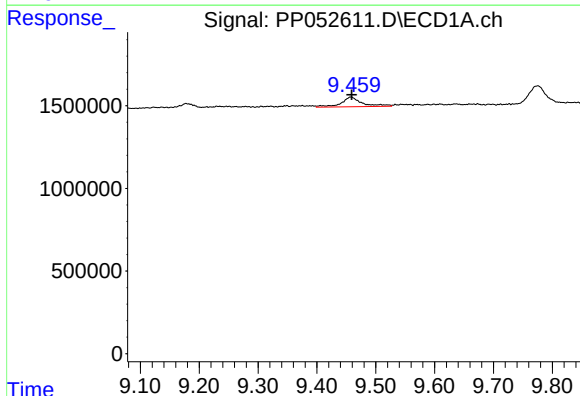


#44 AR-1268-4

R.T.: 9.458 min
Delta R.T.: -0.001 min
Response: 1427209
Conc: 18.26 ng/ml

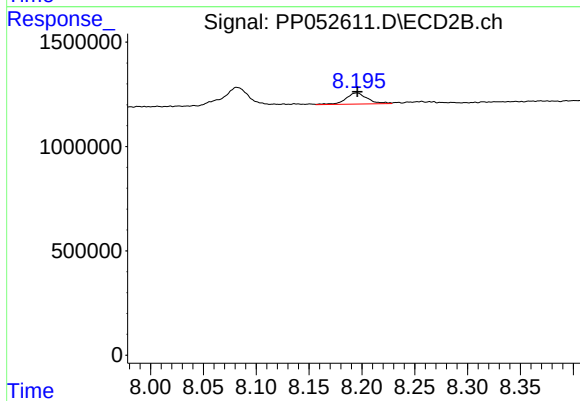

#44 AR-1268-4


R.T.: 8.195 min
Delta R.T.: 0.000 min
Response: 760864
Conc: 13.63 ng/ml

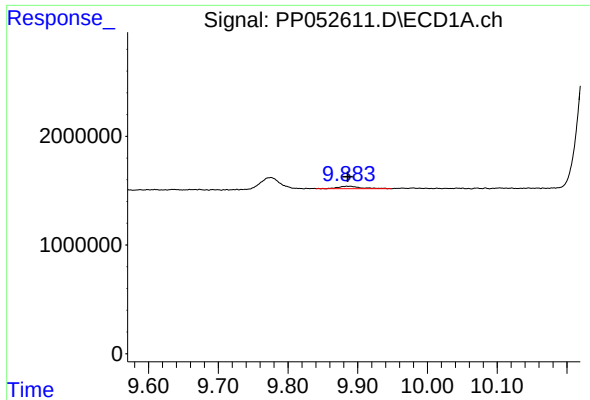

#45 AR-1268-5

R.T.: 9.887 min
Delta R.T.: 0.002 min
Response: 463072
Conc: 0.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

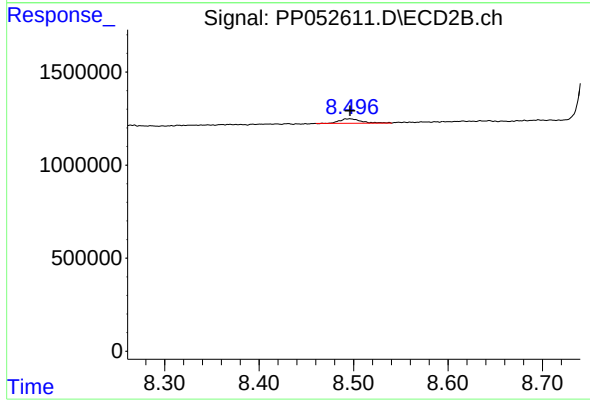

#45 AR-1268-5

R.T.: 8.496 min
Delta R.T.: 0.000 min
Response: 379056
Conc: 0.86 ng/ml