

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 11:57
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:55:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.422	3.672	29608696	28914952	17.896	21.702
2)	SA Decachlor...	10.234	8.761	37320580	29333541	23.289	23.601
Target Compounds							
3)	L1 AR-1016-1	5.589	0.000	57494	0	1.310	N.D. #
4)	L1 AR-1016-2	5.626	0.000	84986	0	1.346	N.D. #
5)	L1 AR-1016-3	5.672	0.000	112316	0	2.782	N.D. #
6)	L1 AR-1016-4	0.000	5.014	0	604061	N.D.	20.836 #
7)	L1 AR-1016-5	6.075	5.231	276368	468588	7.229	12.547 #
8)	L2 AR-1221-1	4.632	0.000	12765331	0	582.811	N.D. #
9)	L2 AR-1221-2	4.729	3.962	1474187	5719664	91.919	429.549 #
10)	L2 AR-1221-3	0.000	4.054	0	95951	N.D.	2.314 #
11)	L3 AR-1232-1	0.000	4.054	0	95951	N.D.	3.026 #
12)	L3 AR-1232-2	5.310f	0.000	92050	0	4.544	N.D. #
13)	L3 AR-1232-3	5.626	0.000	84986	0	2.797	N.D. #
14)	L3 AR-1232-4	0.000	5.056	0	154721	N.D.	10.226 #
15)	L3 AR-1232-5	5.870	5.231	533724	468588	39.418	27.429 #
16)	L4 AR-1242-1	5.589	0.000	57494	0	1.645	N.D. #
17)	L4 AR-1242-2	5.626	0.000	84986	0	1.588	N.D. #
18)	L4 AR-1242-3	5.672	0.000	112316	0	3.265	N.D. #
19)	L4 AR-1242-4	0.000	5.056	0	154721	N.D.	5.103 #
20)	L4 AR-1242-5	6.525	5.588	418605	1444384	11.600	41.394 #
21)	L5 AR-1248-1	5.589	0.000	57494	0	1.982	N.D. #
22)	L5 AR-1248-2	5.870	5.014	533724	604061	12.593	14.737
23)	L5 AR-1248-3	6.075	5.056	276368	154721	5.347	3.680 #
24)	L5 AR-1248-4	6.480	5.231	422659	468588	7.670	9.555
25)	L5 AR-1248-5	6.525	0.000	418605	0	7.365	N.D. #
26)	L6 AR-1254-1	6.455	5.588	993315	1444384	15.916	19.941 #
27)	L6 AR-1254-2	6.674	5.738	1554104	1199626	16.181	18.680
28)	L6 AR-1254-3	7.042	6.147	1602827	1860163	17.144	18.789
29)	L6 AR-1254-4	7.328	6.378	881653	887458	14.276	17.227
30)	L6 AR-1254-5	7.749	6.800	1163040	1343377	15.339	16.116
31)	L7 AR-1260-1	7.207	6.279	580381	943394	7.620	13.425 #
32)	L7 AR-1260-2	7.463	6.467	664392	862228	7.937	10.761 #
33)	L7 AR-1260-3	7.816	6.623	193483	764325	3.002	10.041 #
34)	L7 AR-1260-4	8.040	0.000	572164	0	7.575	N.D. #
35)	L7 AR-1260-5	8.374	7.345	341755	149910	2.567	1.197 #
36)	L8 AR-1262-1	7.816	0.000	193483	0	1.977	N.D. #
37)	L8 AR-1262-2	8.374	0.000	341755	0	2.243	N.D. #
38)	L8 AR-1262-3	8.706	0.000	71186	0	0.645	N.D. #
39)	L8 AR-1262-4	8.762f	7.692	248766	200706	3.970	1.807 #
40)	L8 AR-1262-5	9.462	0.000	243008	0	3.791	N.D. #
41)	L9 AR-1268-1	8.706	0.000	71186	0	0.346	N.D. #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 11:57
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1254 LOD 25 PPB
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:55:24 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.762f	7.692	248766	200706	1.272	1.226
43) L9	AR-1268-3	9.022	0.000	372610	0	2.073	N.D. #
44) L9	AR-1268-4	9.462	0.000	243008	0	3.110	N.D. #
45) L9	AR-1268-5	9.882	8.496	320028	142680	0.553	0.322 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
Data File : PP052616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 11:57
Operator : YP\AJ
Sample : N4955-07
Misc : AR1254 LOD 25 PPB
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:55:24 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Oct 23 15:44:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

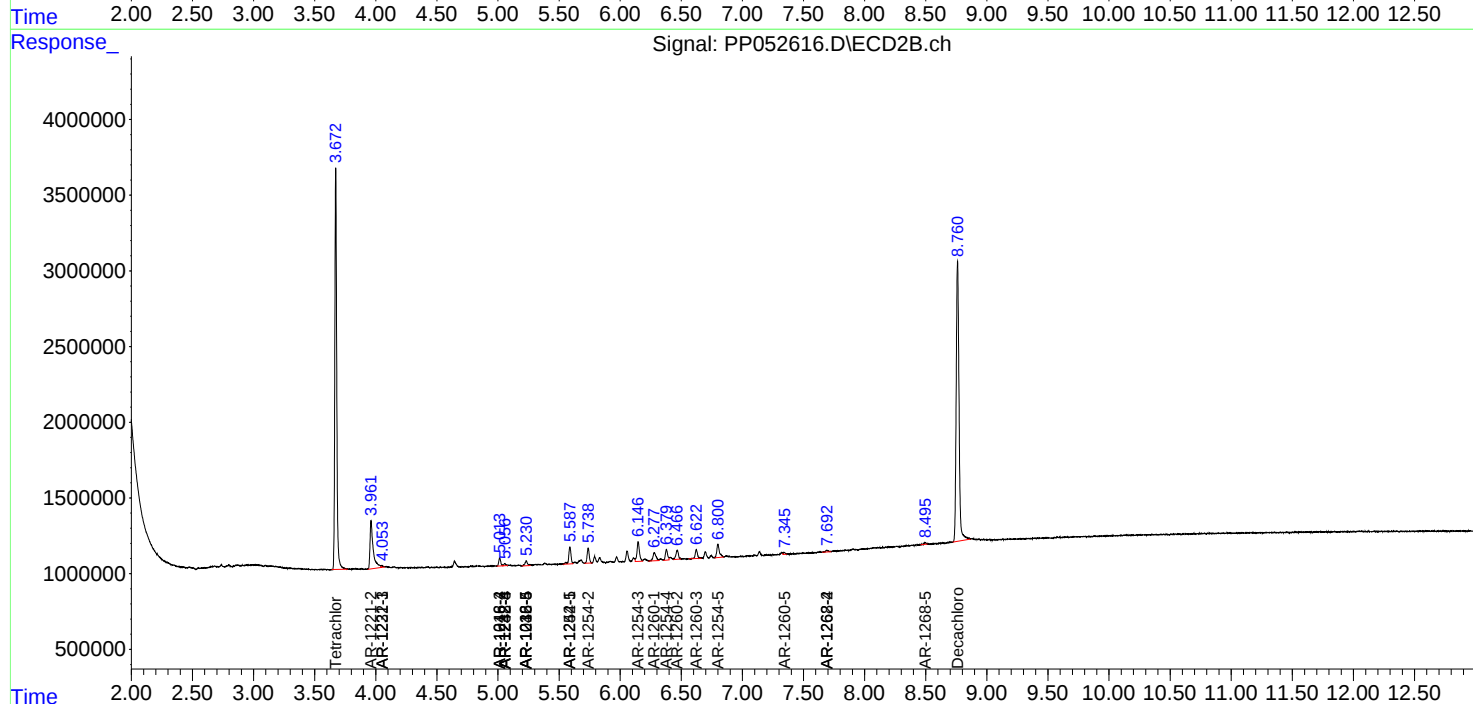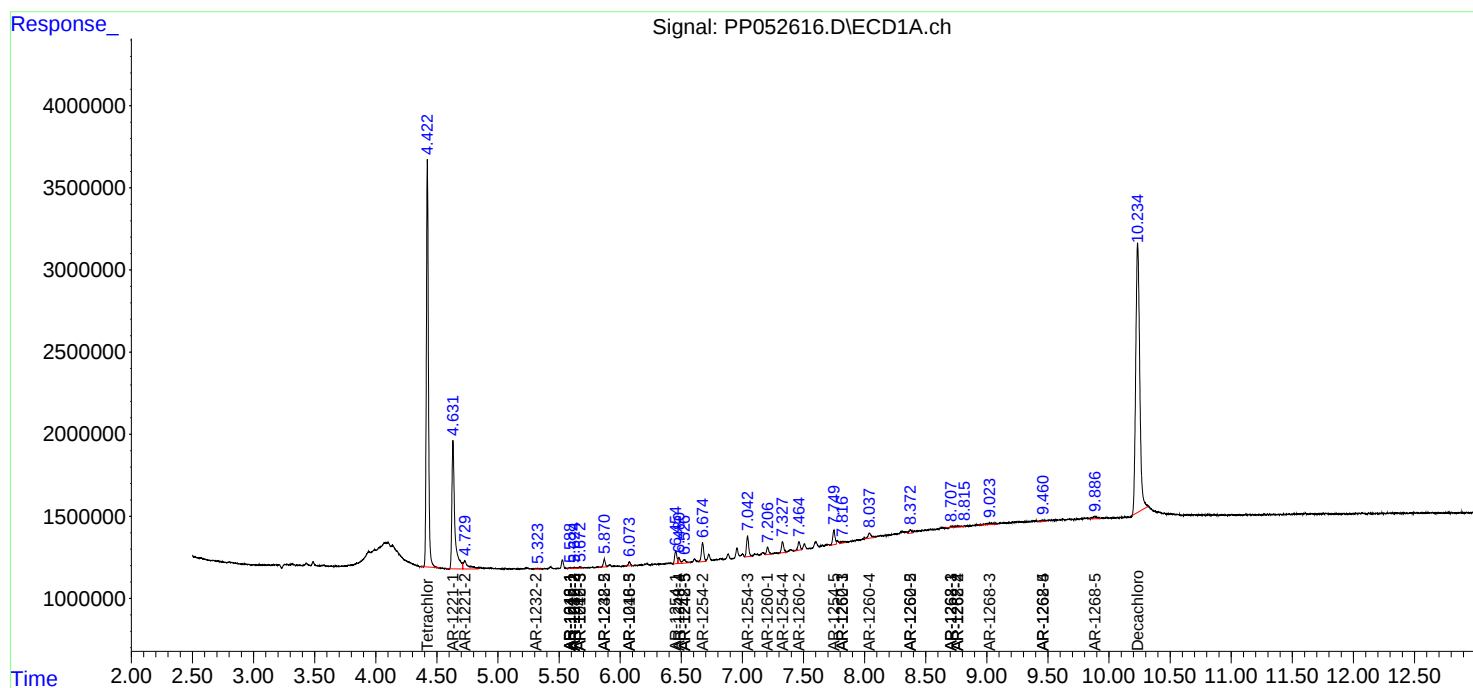


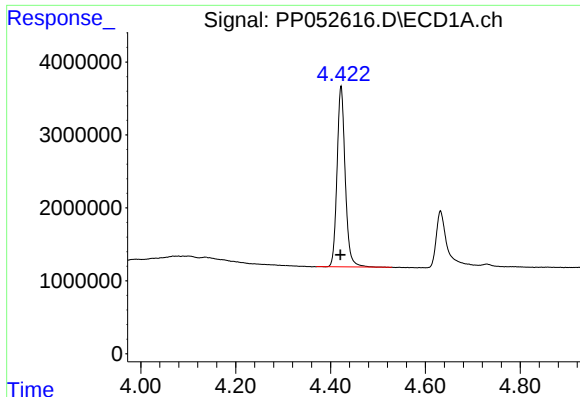

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: 0.001 min
Response: 29608696
Conc: 17.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

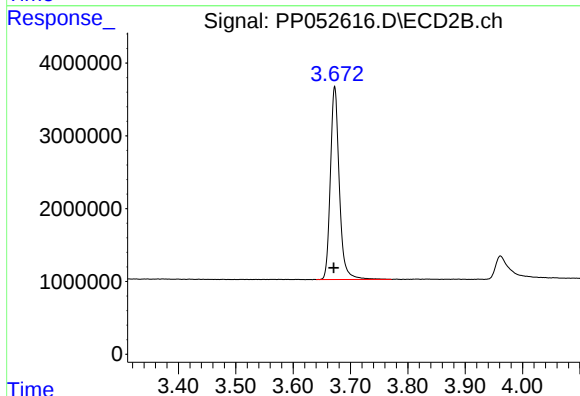


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.001 min
Response: 28914952
Conc: 21.70 ng/ml

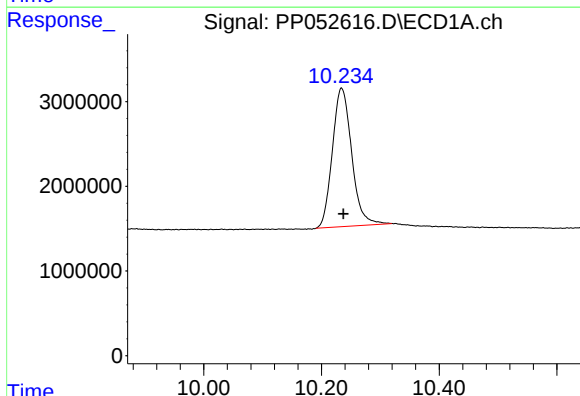


#2 Decachlorobiphenyl

R.T.: 10.234 min
Delta R.T.: -0.003 min
Response: 37320580
Conc: 23.29 ng/ml

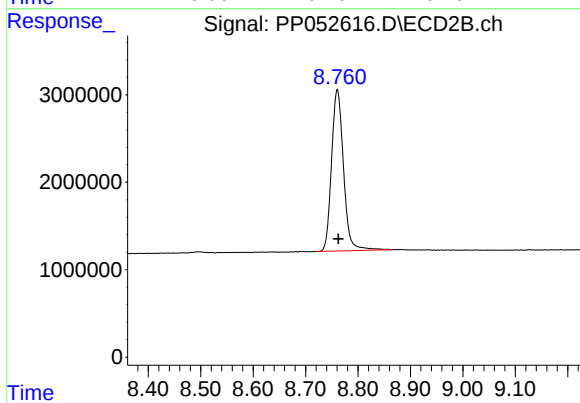

#2 Decachlorobiphenyl


R.T.: 8.761 min
Delta R.T.: -0.002 min
Response: 29333541
Conc: 23.60 ng/ml

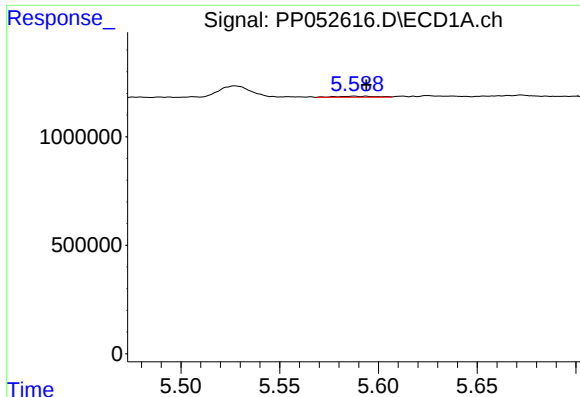

#3 AR-1016-1


R.T.: 5.589 min
Delta R.T.: -0.005 min
Response: 57494
Conc: 1.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

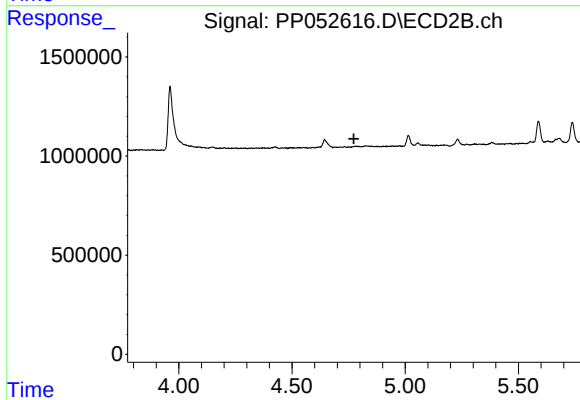


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.773 min
Response: 0
Conc: N.D.

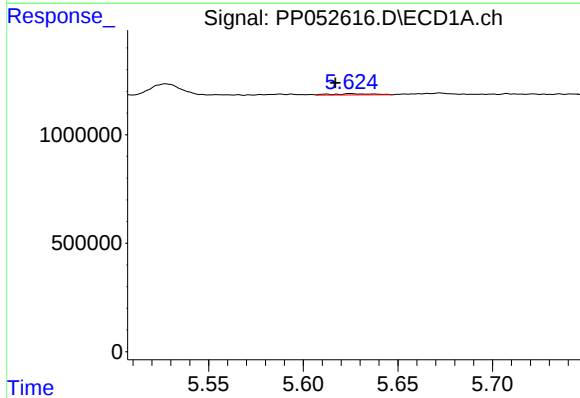


#4 AR-1016-2

R.T.: 5.626 min
Delta R.T.: 0.009 min
Response: 84986
Conc: 1.35 ng/ml

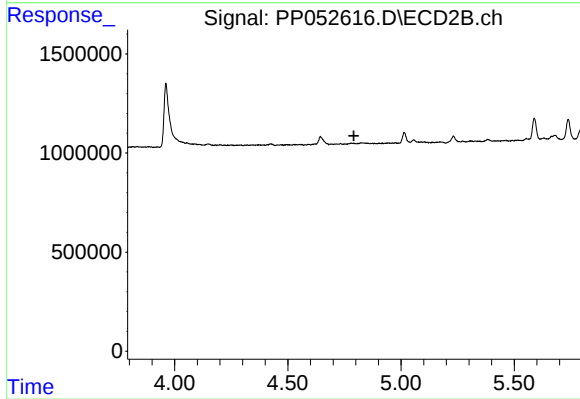

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.792 min
Response: 0
Conc: N.D.

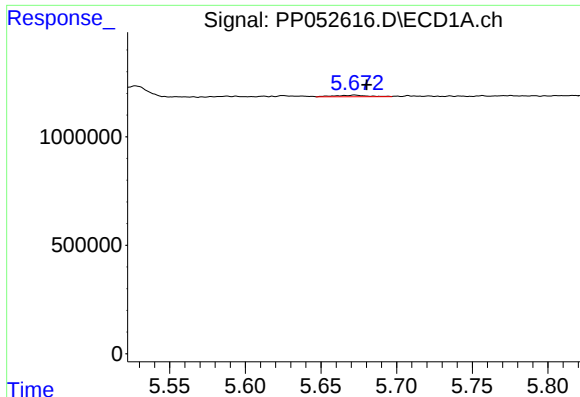

#5 AR-1016-3


R.T.: 5.672 min
Delta R.T.: -0.008 min
Response: 112316
Conc: 2.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

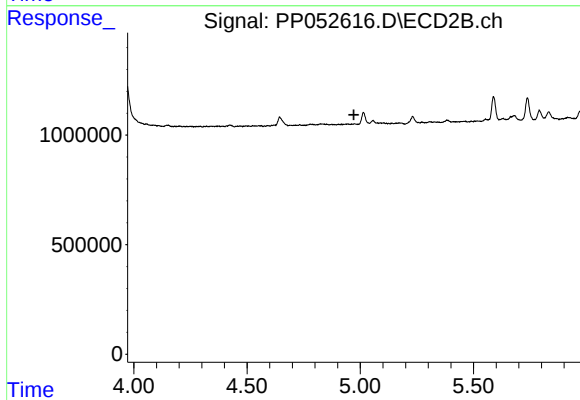


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

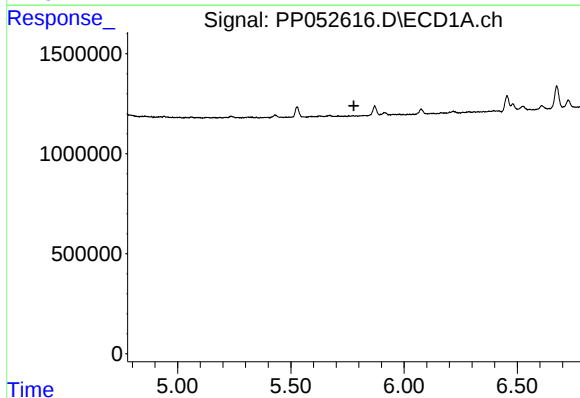


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

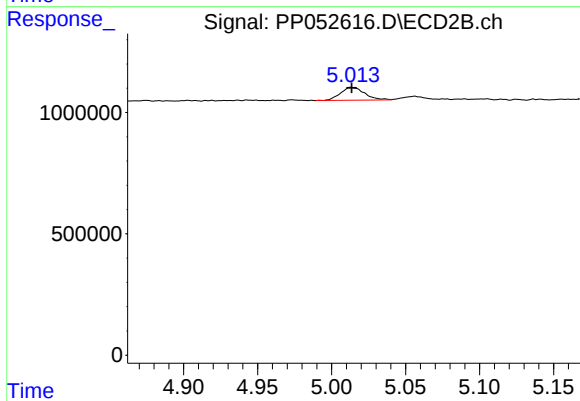

#6 AR-1016-4


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 604061
Conc: 20.84 ng/ml

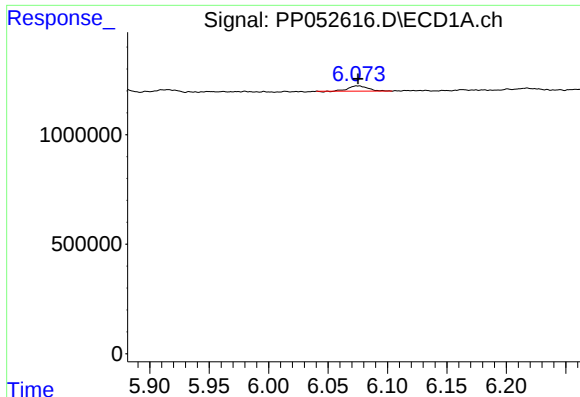

#7 AR-1016-5


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 276368
Conc: 7.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

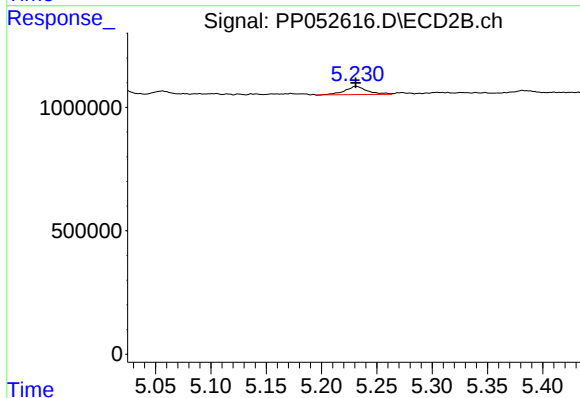


#7 AR-1016-5

R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 468588
Conc: 12.55 ng/ml

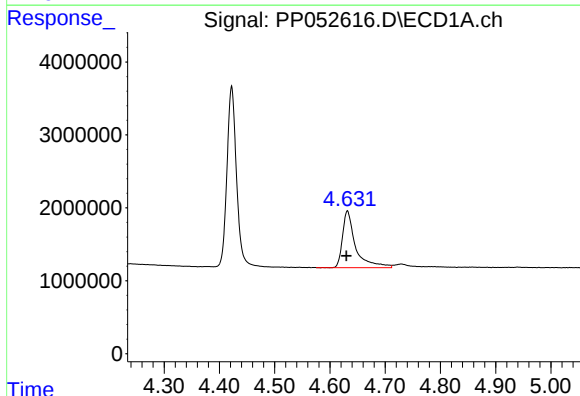


#8 AR-1221-1

R.T.: 4.632 min
Delta R.T.: 0.002 min
Response: 12765331
Conc: 582.81 ng/ml

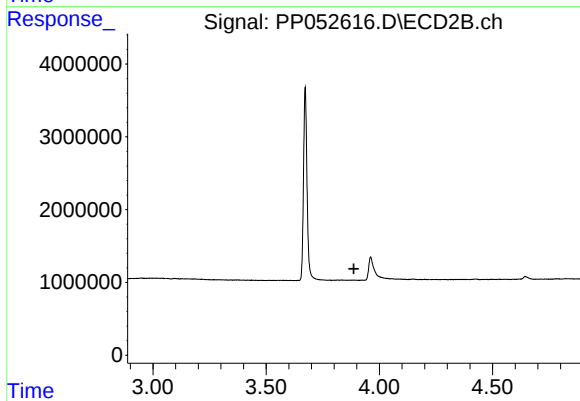

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

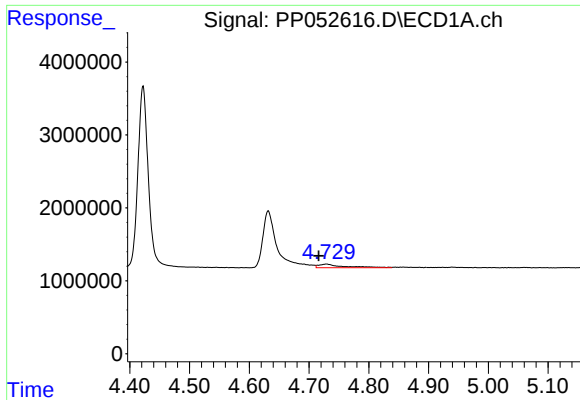

#9 AR-1221-2


R.T.: 4.729 min
Delta R.T.: 0.013 min
Response: 1474187
Conc: 91.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

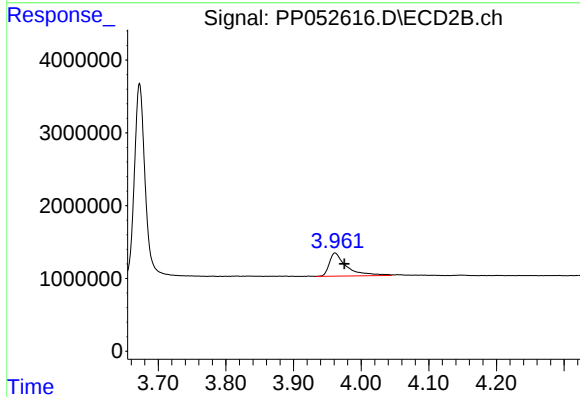


#9 AR-1221-2

R.T.: 3.962 min
Delta R.T.: -0.014 min
Response: 5719664
Conc: 429.55 ng/ml

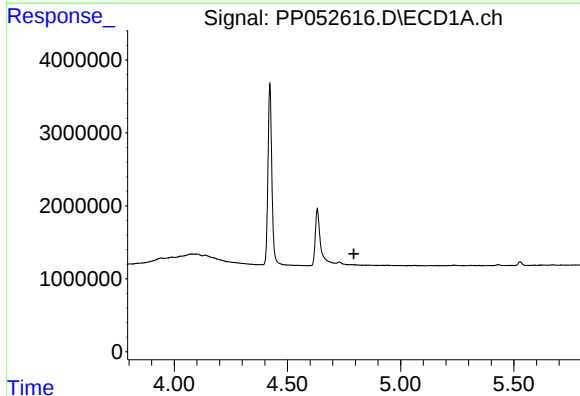


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

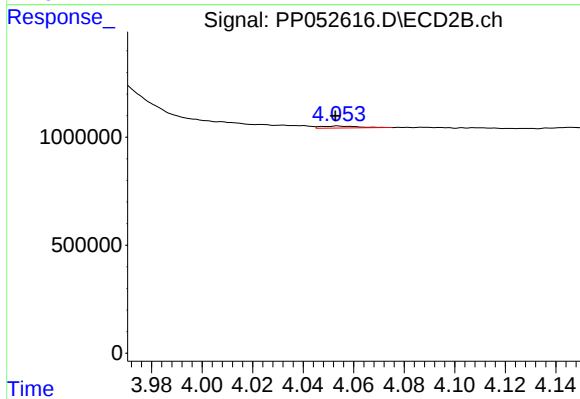

#10 AR-1221-3


R.T.: 4.054 min
Delta R.T.: 0.000 min
Response: 95951
Conc: 2.31 ng/ml

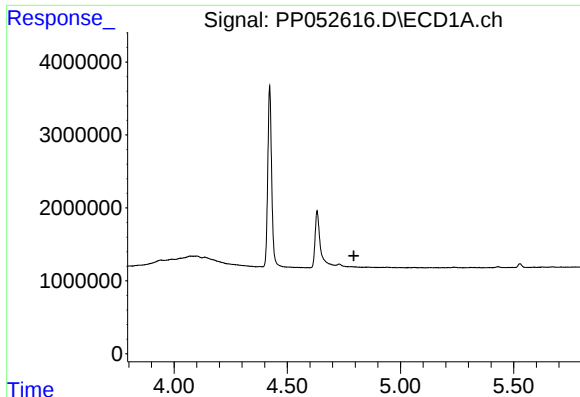

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.794 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

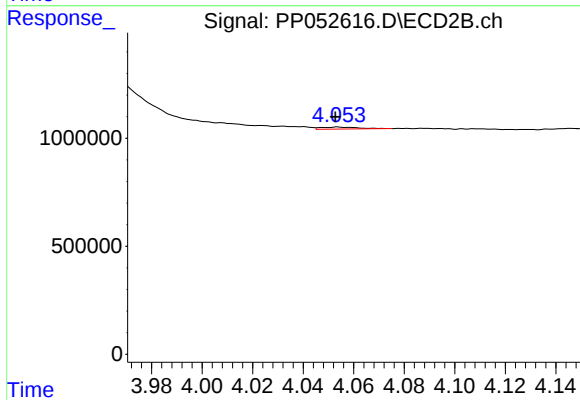


#11 AR-1232-1

R.T.: 4.054 min
Delta R.T.: 0.000 min
Response: 95951
Conc: 3.03 ng/ml

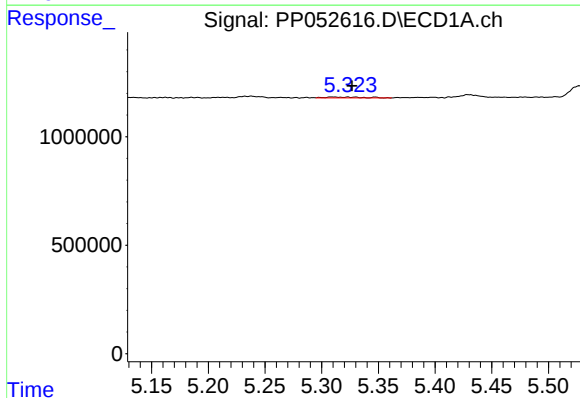


#12 AR-1232-2

R.T.: 5.310 min
Delta R.T.: -0.016 min
Response: 92050
Conc: 4.54 ng/ml

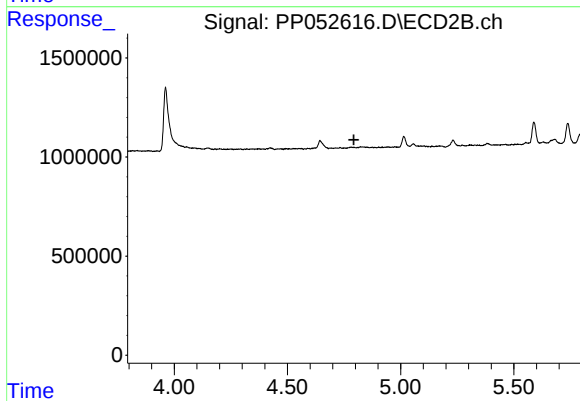

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T.: 4.793 min
Response: 0
Conc: N.D.

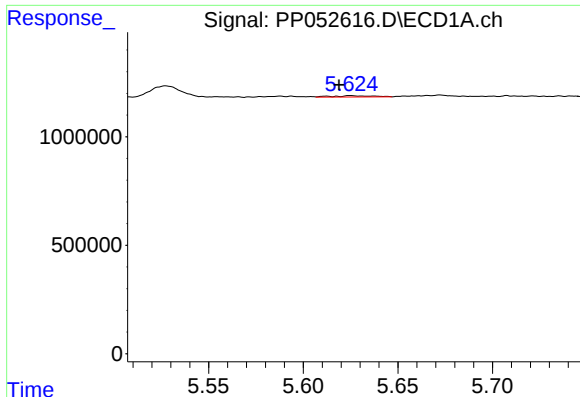

#13 AR-1232-3


R.T.: 5.626 min
Delta R.T.: 0.007 min
Response: 84986
Conc: 2.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

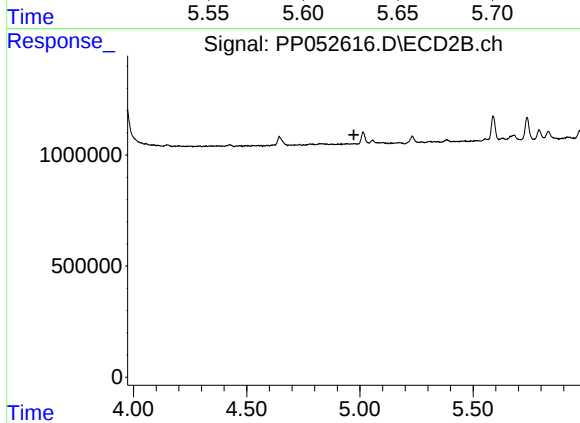


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

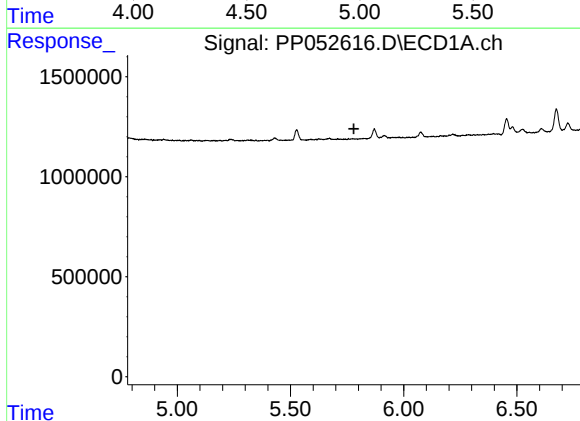


#14 AR-1232-4

R.T.: 0.000 min
Exp R.T. : 5.780 min
Response: 0
Conc: N.D.

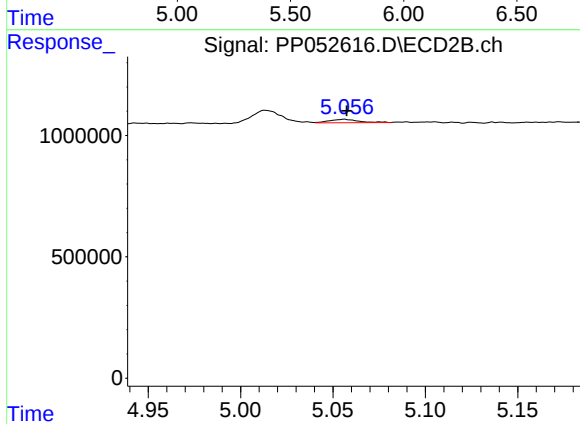

#14 AR-1232-4


R.T.: 5.056 min
Delta R.T.: -0.001 min
Response: 154721
Conc: 10.23 ng/ml

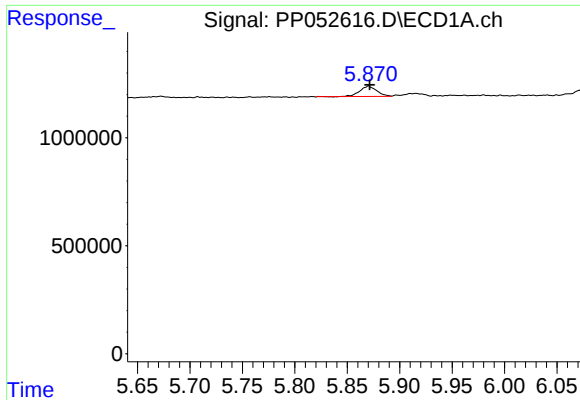

#15 AR-1232-5


R.T.: 5.870 min
Delta R.T.: -0.001 min
Response: 533724
Conc: 39.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

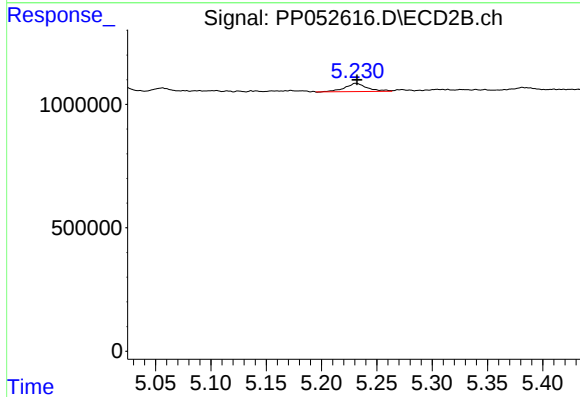


#15 AR-1232-5

R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 468588
Conc: 27.43 ng/ml

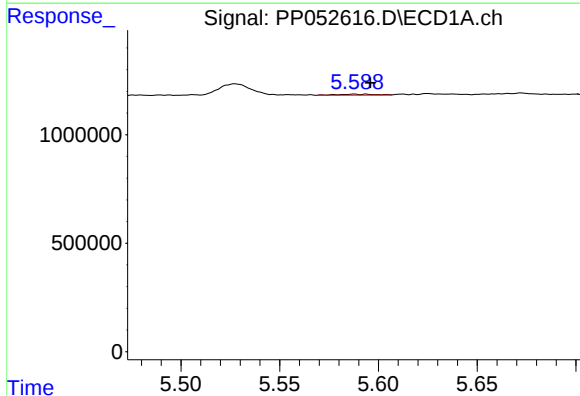


#16 AR-1242-1

R.T.: 5.589 min
Delta R.T.: -0.007 min
Response: 57494
Conc: 1.64 ng/ml

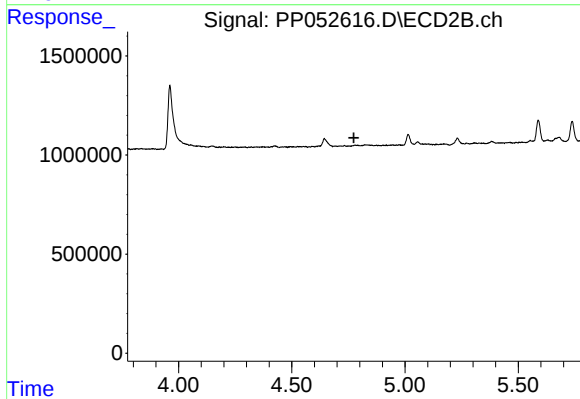

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.774 min
Response: 0
Conc: N.D.

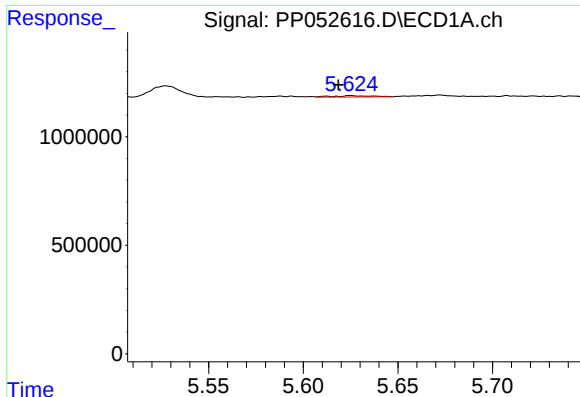

#17 AR-1242-2


R.T.: 5.626 min
Delta R.T.: 0.008 min
Response: 84986
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

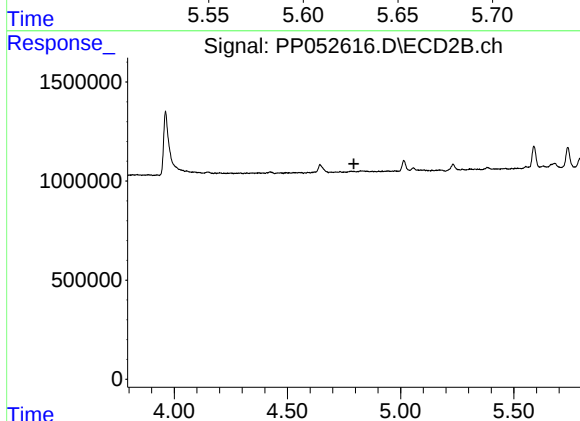


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

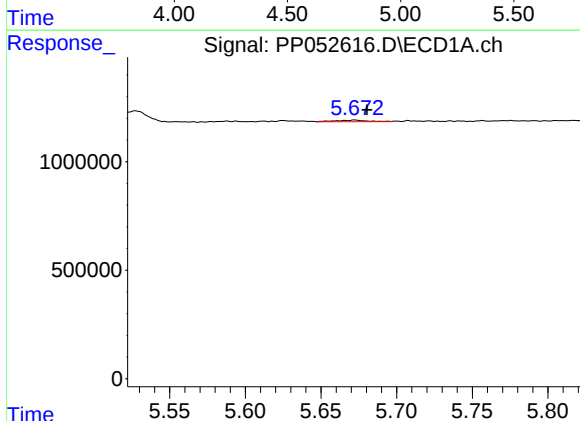


#18 AR-1242-3

R.T.: 5.672 min
Delta R.T.: -0.009 min
Response: 112316
Conc: 3.27 ng/ml

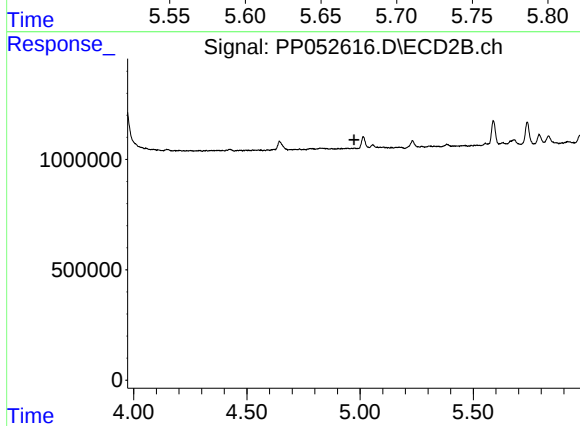

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

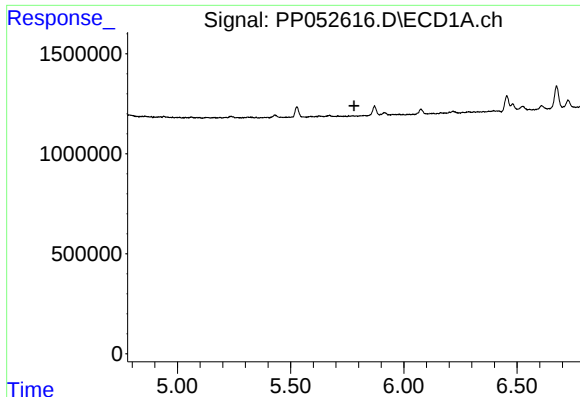

#19 AR-1242-4


R.T.: 0.000 min
Exp R.T.: 5.780 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

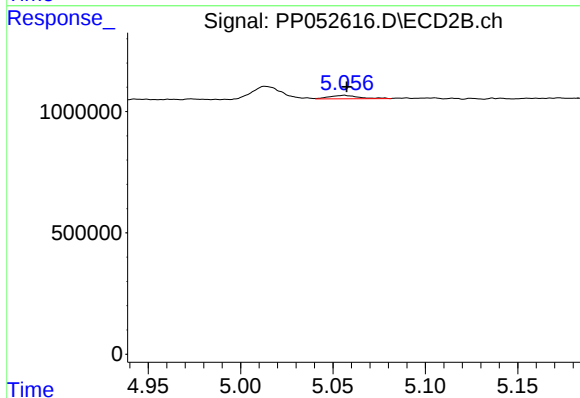


#19 AR-1242-4

R.T.: 5.056 min
Delta R.T.: -0.001 min
Response: 154721
Conc: 5.10 ng/ml

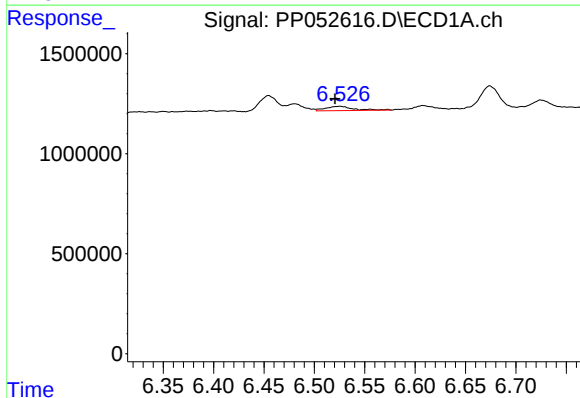


#20 AR-1242-5

R.T.: 6.525 min
Delta R.T.: 0.004 min
Response: 418605
Conc: 11.60 ng/ml

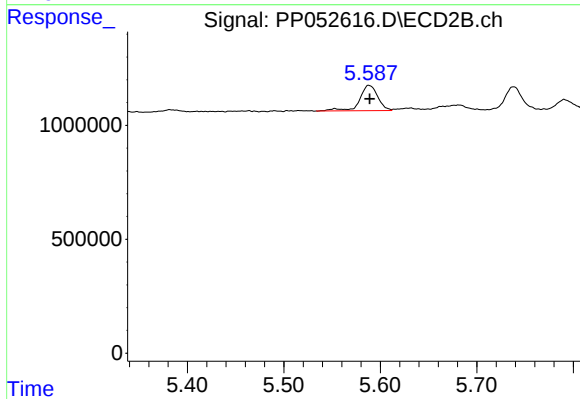

#20 AR-1242-5


R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 1444384
Conc: 41.39 ng/ml

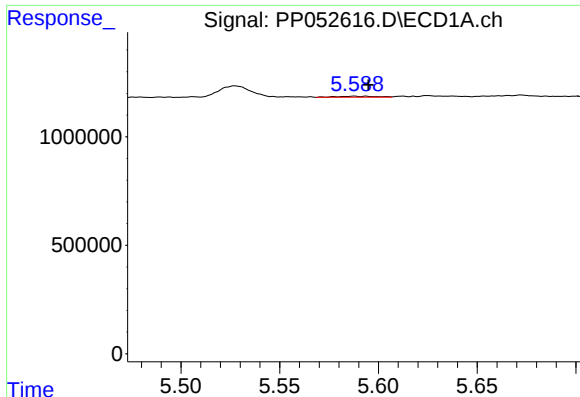

#21 AR-1248-1


R.T.: 5.589 min
Delta R.T.: -0.006 min
Response: 57494
Conc: 1.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

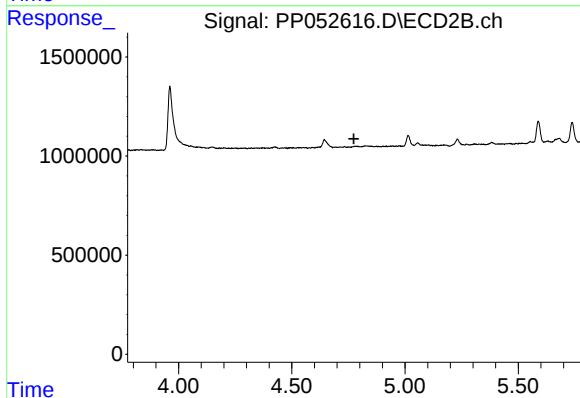


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.774 min
Response: 0
Conc: N.D.

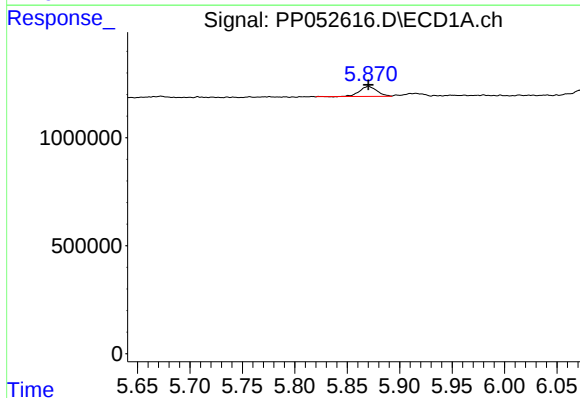


#22 AR-1248-2

R.T.: 5.870 min
Delta R.T.: 0.000 min
Response: 533724
Conc: 12.59 ng/ml

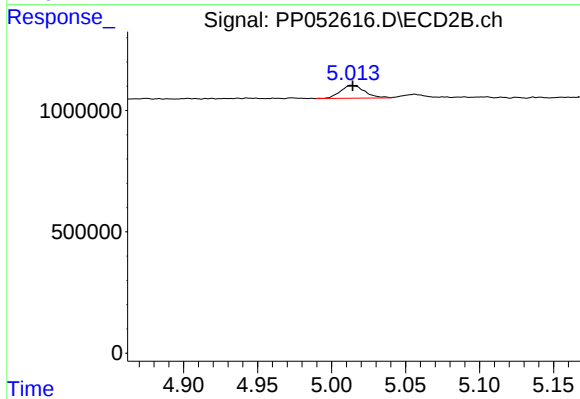

#22 AR-1248-2


R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 604061
Conc: 14.74 ng/ml

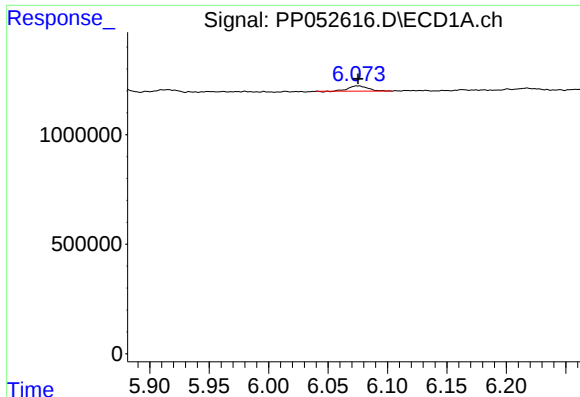

#23 AR-1248-3


R.T.: 6.075 min
Delta R.T.: 0.000 min
Response: 276368
Conc: 5.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

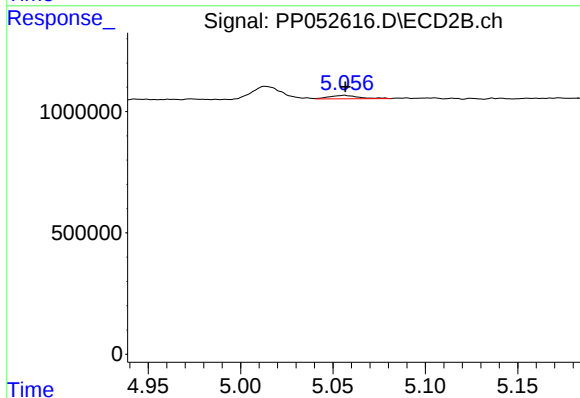


#23 AR-1248-3

R.T.: 5.056 min
Delta R.T.: 0.000 min
Response: 154721
Conc: 3.68 ng/ml

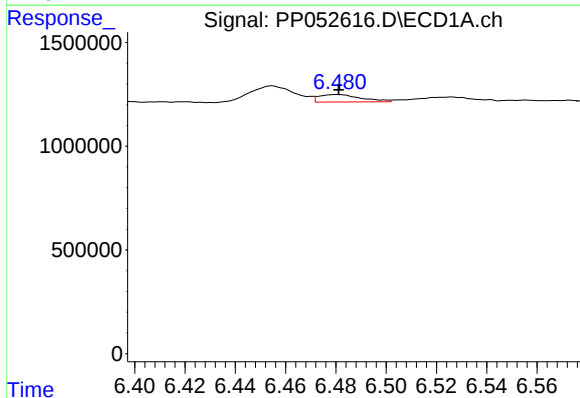


#24 AR-1248-4

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 422659
Conc: 7.67 ng/ml

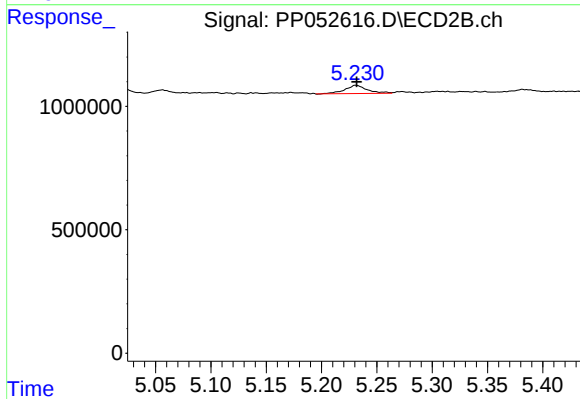

#24 AR-1248-4


R.T.: 5.231 min
Delta R.T.: 0.000 min
Response: 468588
Conc: 9.55 ng/ml

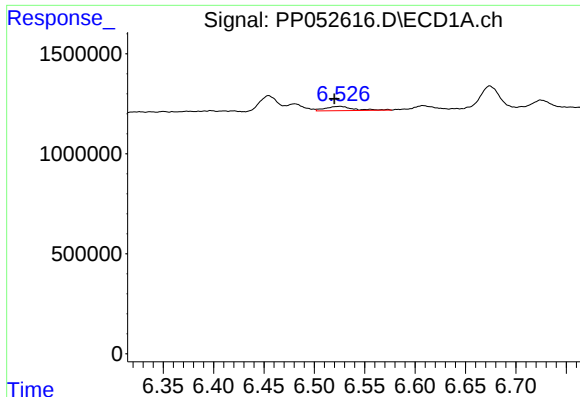

#25 AR-1248-5


R.T.: 6.525 min
Delta R.T.: 0.005 min
Response: 418605
Conc: 7.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

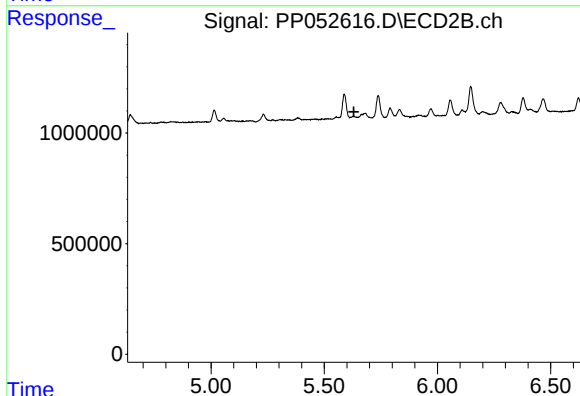


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.631 min
Response: 0
Conc: N.D.

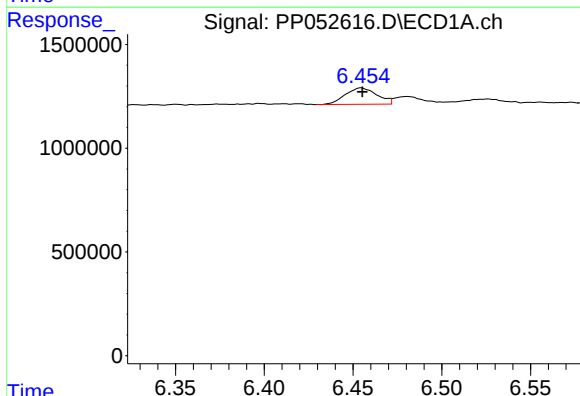


#26 AR-1254-1

R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 993315
Conc: 15.92 ng/ml

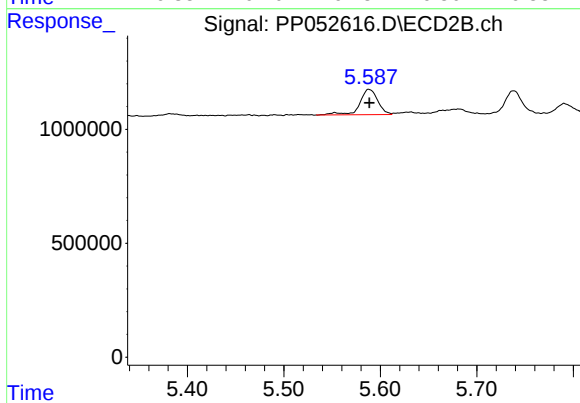

#26 AR-1254-1


R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 1444384
Conc: 19.94 ng/ml

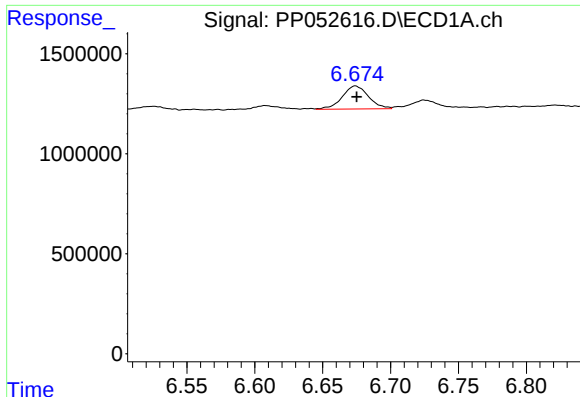

#27 AR-1254-2


R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 1554104
Conc: 16.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

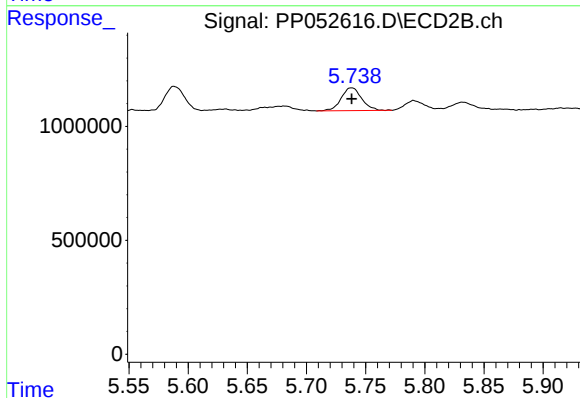


#27 AR-1254-2

R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 1199626
Conc: 18.68 ng/ml

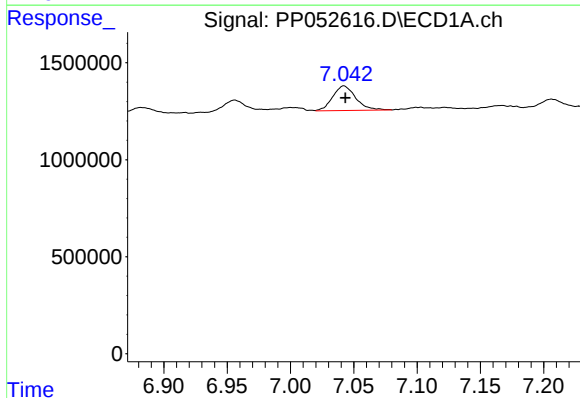


#28 AR-1254-3

R.T.: 7.042 min
Delta R.T.: -0.001 min
Response: 1602827
Conc: 17.14 ng/ml

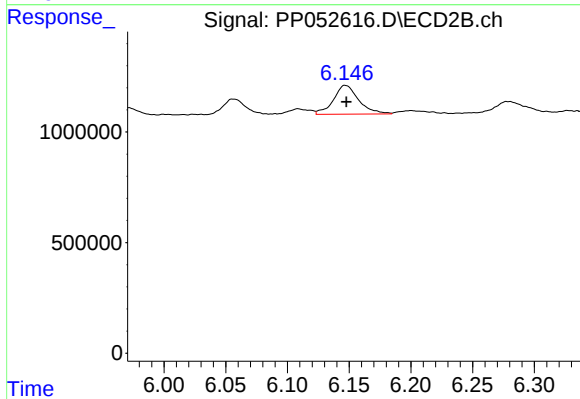

#28 AR-1254-3


R.T.: 6.147 min
Delta R.T.: 0.000 min
Response: 1860163
Conc: 18.79 ng/ml

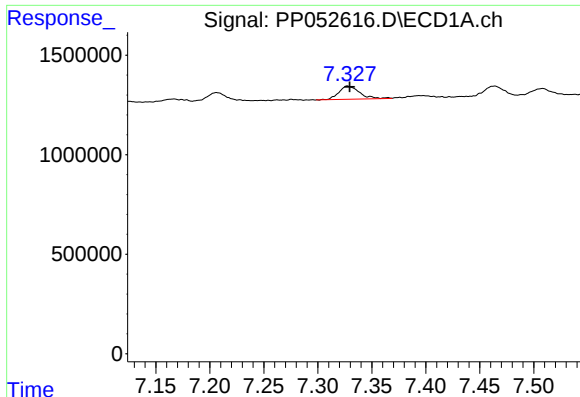

#29 AR-1254-4


R.T.: 7.328 min
Delta R.T.: -0.001 min
Response: 881653
Conc: 14.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

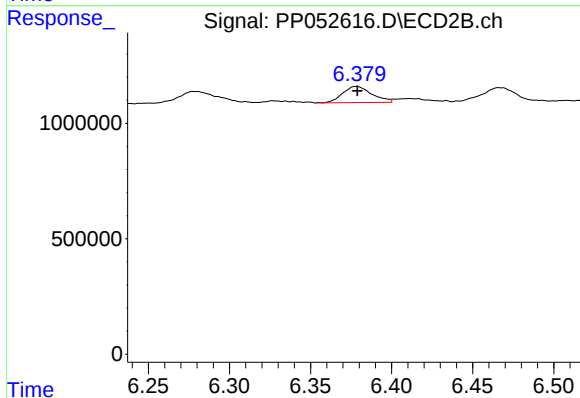


#29 AR-1254-4

R.T.: 6.378 min
Delta R.T.: 0.000 min
Response: 887458
Conc: 17.23 ng/ml

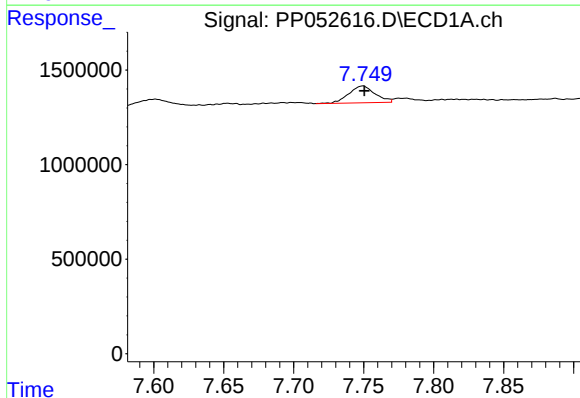


#30 AR-1254-5

R.T.: 7.749 min
Delta R.T.: -0.001 min
Response: 1163040
Conc: 15.34 ng/ml

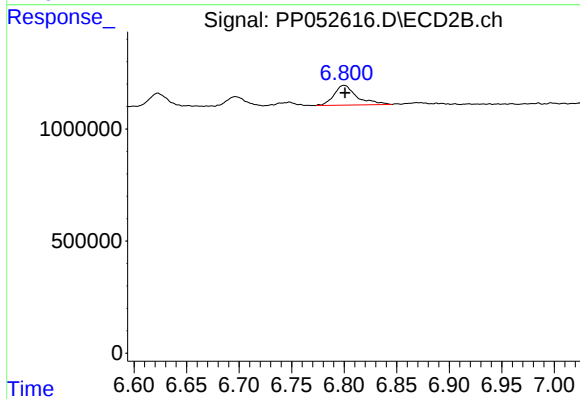

#30 AR-1254-5


R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 1343377
Conc: 16.12 ng/ml

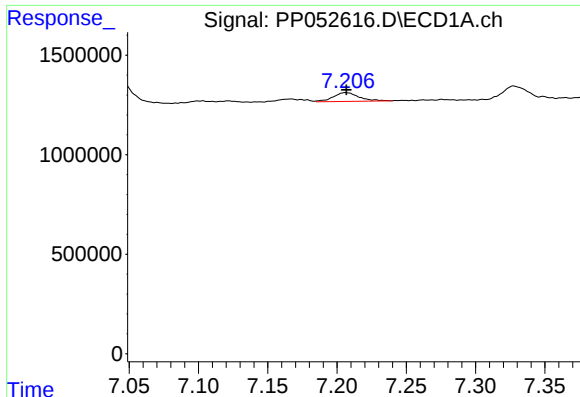

#31 AR-1260-1


R.T.: 7.207 min
Delta R.T.: 0.000 min
Response: 580381
Conc: 7.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

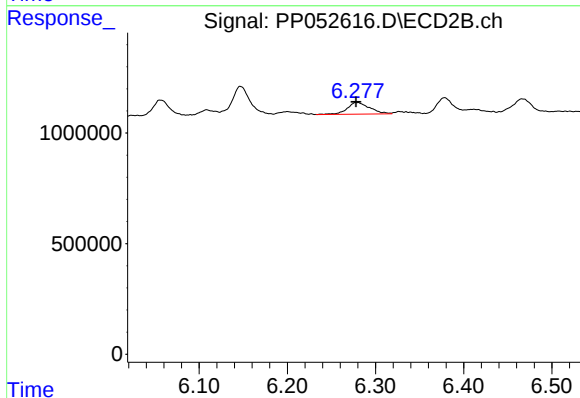


#31 AR-1260-1

R.T.: 6.279 min
Delta R.T.: 0.001 min
Response: 943394
Conc: 13.43 ng/ml

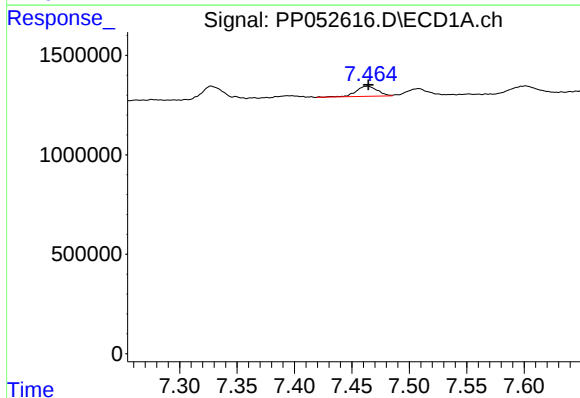


#32 AR-1260-2

R.T.: 7.463 min
Delta R.T.: -0.001 min
Response: 664392
Conc: 7.94 ng/ml

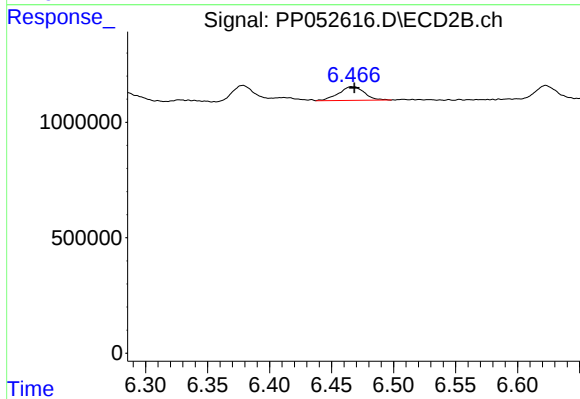

#32 AR-1260-2


R.T.: 6.467 min
Delta R.T.: -0.002 min
Response: 862228
Conc: 10.76 ng/ml

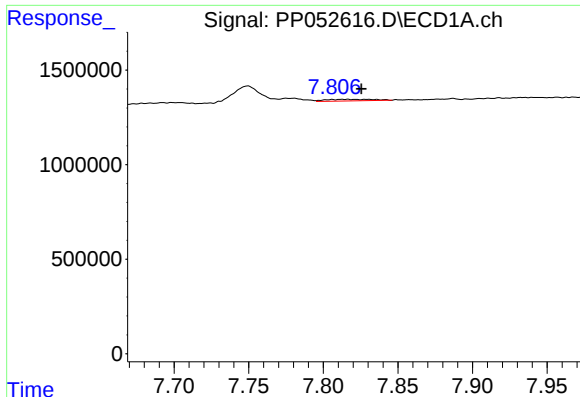

#33 AR-1260-3


R.T.: 7.816 min
Delta R.T.: -0.010 min
Response: 193483
Conc: 3.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

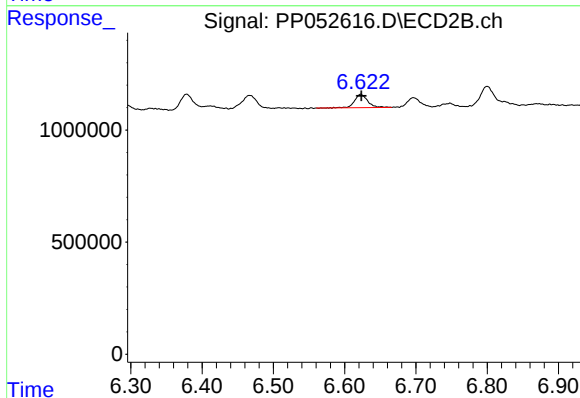


#33 AR-1260-3

R.T.: 6.623 min
Delta R.T.: -0.001 min
Response: 764325
Conc: 10.04 ng/ml

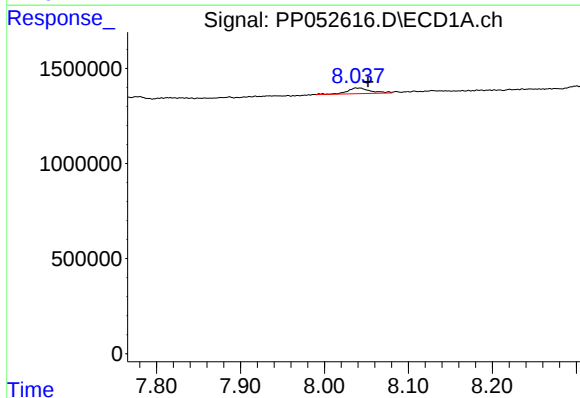


#34 AR-1260-4

R.T.: 8.040 min
Delta R.T.: -0.012 min
Response: 572164
Conc: 7.57 ng/ml

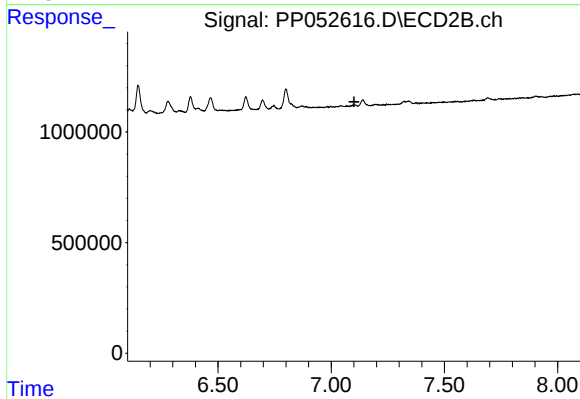

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.100 min
Response: 0
Conc: N.D.

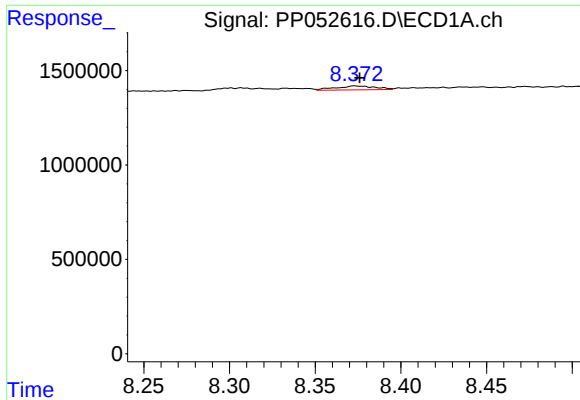

#35 AR-1260-5


R.T.: 8.374 min
Delta R.T.: -0.001 min
Response: 341755
Conc: 2.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

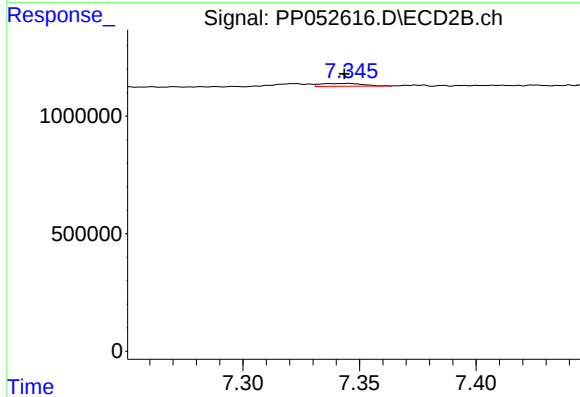


#35 AR-1260-5

R.T.: 7.345 min
Delta R.T.: 0.001 min
Response: 149910
Conc: 1.20 ng/ml

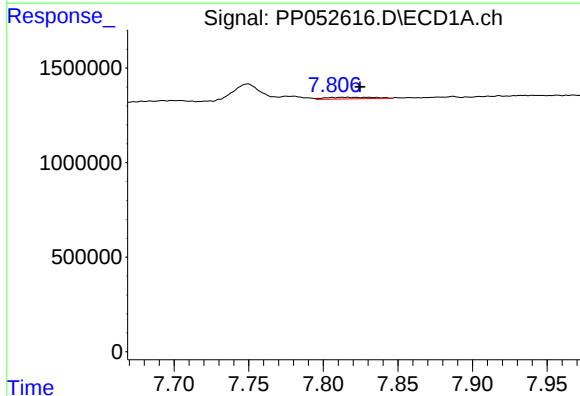


#36 AR-1262-1

R.T.: 7.816 min
Delta R.T.: -0.009 min
Response: 193483
Conc: 1.98 ng/ml

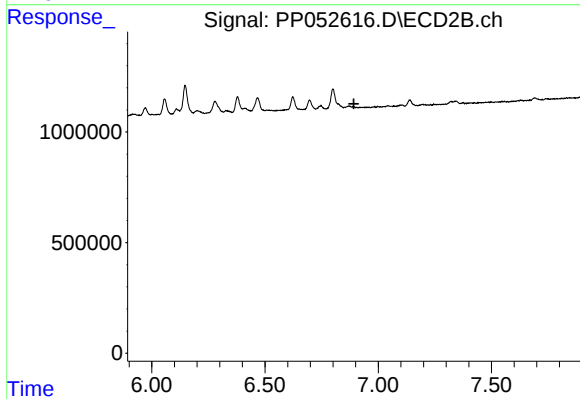

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 6.892 min
Response: 0
Conc: N.D.

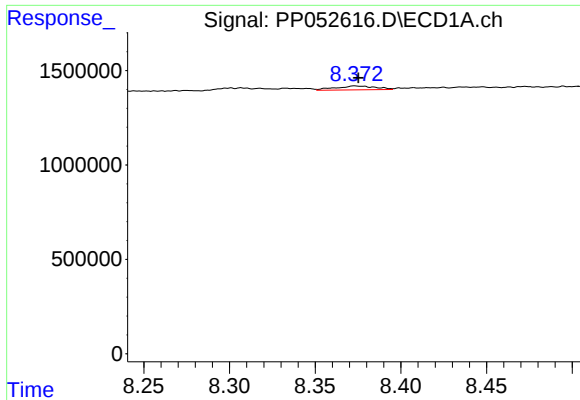

#37 AR-1262-2


R.T.: 8.374 min
Delta R.T.: 0.000 min
Response: 341755
Conc: 2.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

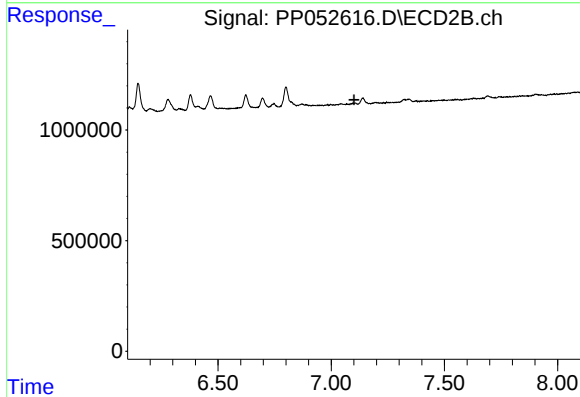


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.100 min
Response: 0
Conc: N.D.

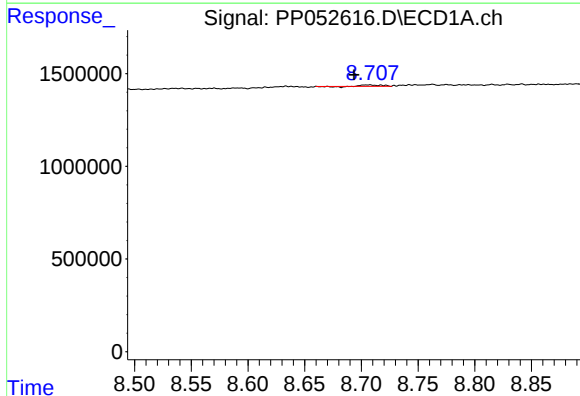


#38 AR-1262-3

R.T.: 8.706 min
Delta R.T.: 0.012 min
Response: 71186
Conc: 0.65 ng/ml

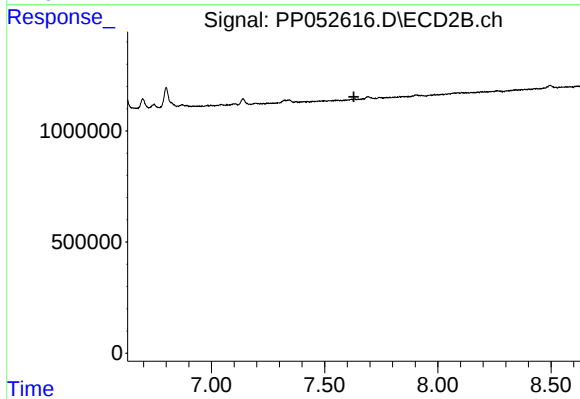

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 7.629 min
Response: 0
Conc: N.D.

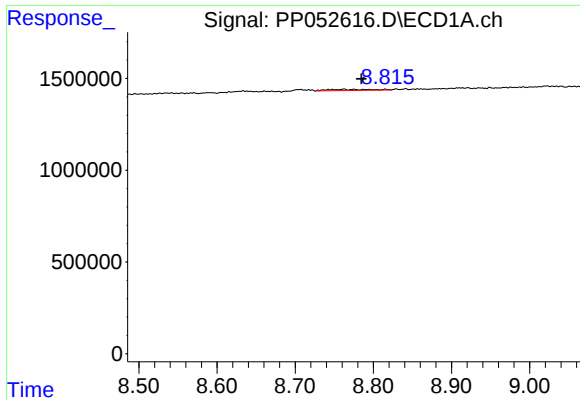

#39 AR-1262-4


R.T.: 8.762 min
Delta R.T.: -0.023 min
Response: 248766
Conc: 3.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

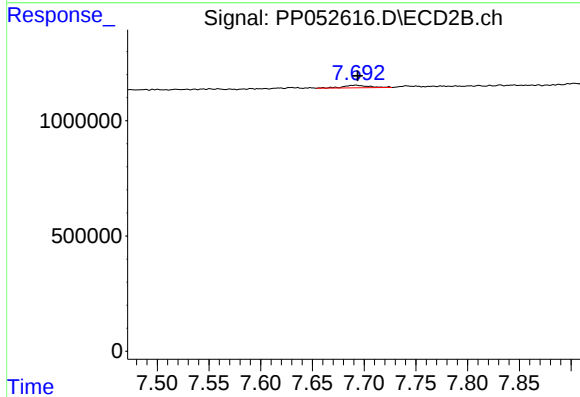


#39 AR-1262-4

R.T.: 7.692 min
Delta R.T.: -0.002 min
Response: 200706
Conc: 1.81 ng/ml

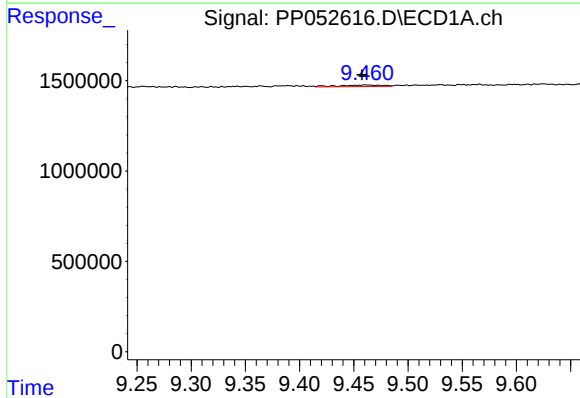


#40 AR-1262-5

R.T.: 9.462 min
Delta R.T.: 0.004 min
Response: 243008
Conc: 3.79 ng/ml

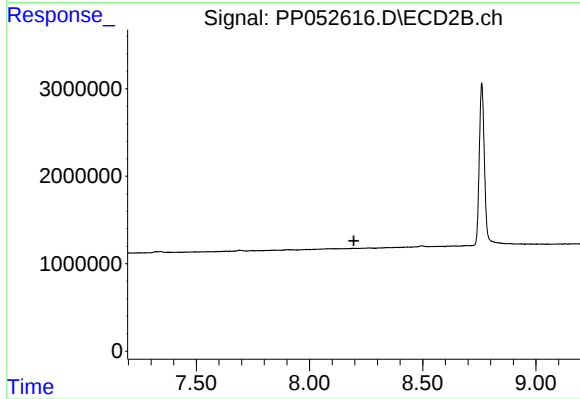

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 8.196 min
Response: 0
Conc: N.D.

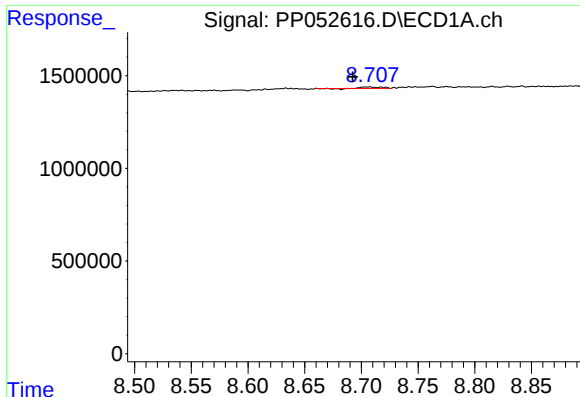

#41 AR-1268-1


R.T.: 8.706 min
Delta R.T.: 0.013 min
Response: 71186
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

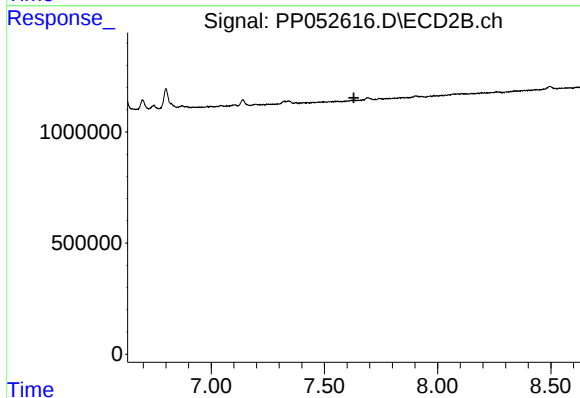


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 7.630 min
Response: 0
Conc: N.D.

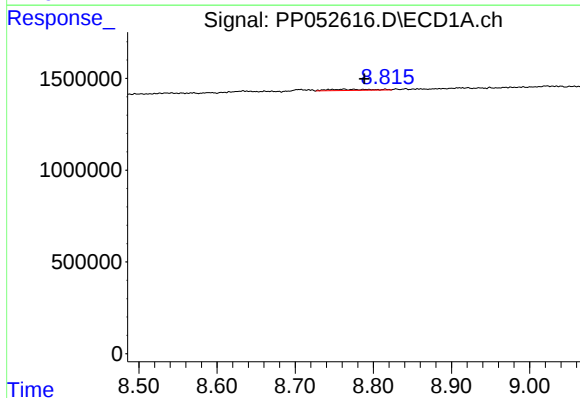


#42 AR-1268-2

R.T.: 8.762 min
Delta R.T.: -0.027 min
Response: 248766
Conc: 1.27 ng/ml

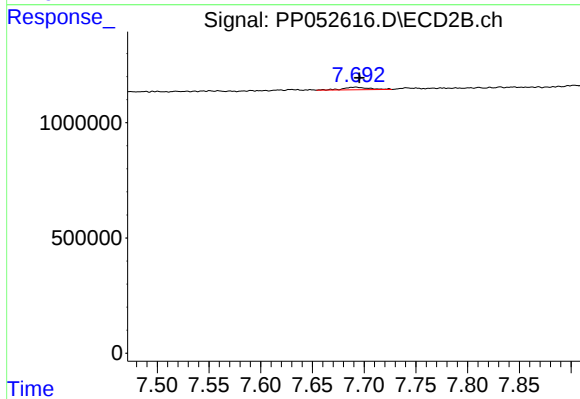

#42 AR-1268-2


R.T.: 7.692 min
Delta R.T.: -0.003 min
Response: 200706
Conc: 1.23 ng/ml

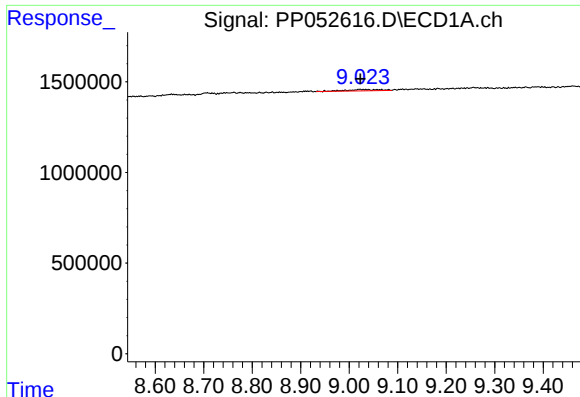

#43 AR-1268-3


R.T.: 9.022 min
Delta R.T.: -0.001 min
Response: 372610
Conc: 2.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

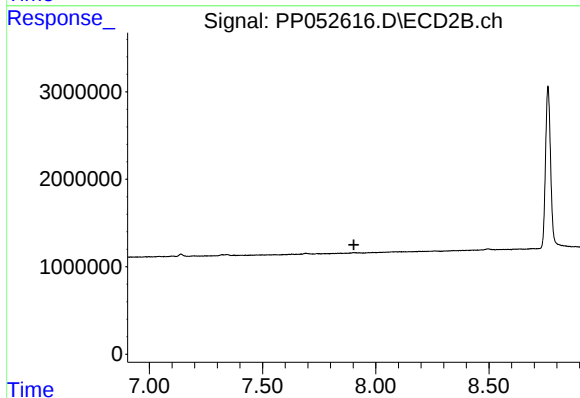


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 7.903 min
Response: 0
Conc: N.D.

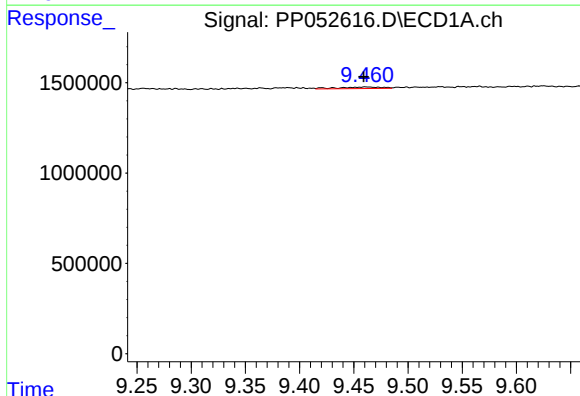


#44 AR-1268-4

R.T.: 9.462 min
Delta R.T.: 0.003 min
Response: 243008
Conc: 3.11 ng/ml

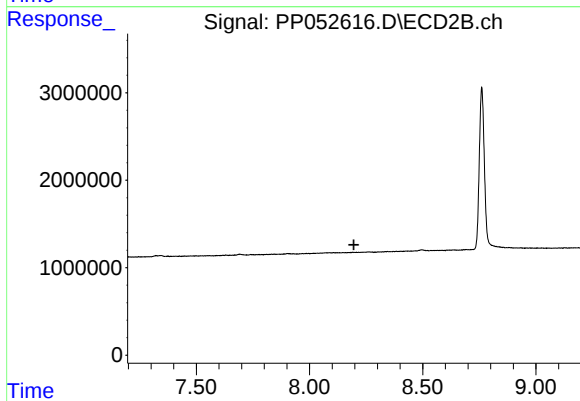

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 8.196 min
Response: 0
Conc: N.D.

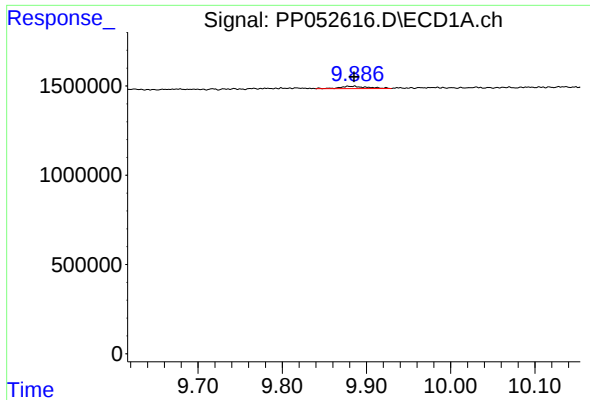

#45 AR-1268-5

R.T.: 9.882 min
Delta R.T.: -0.004 min
Response: 320028
Conc: 0.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

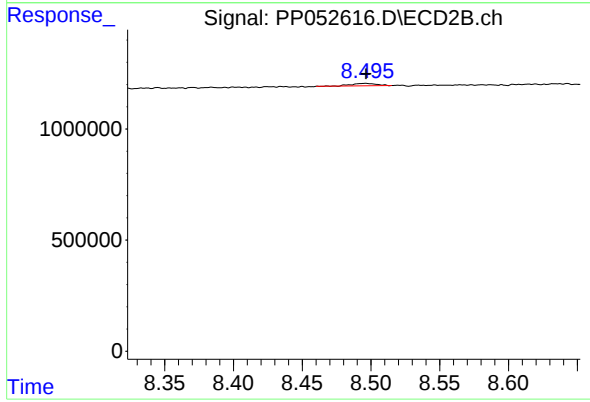

#45 AR-1268-5

R.T.: 8.496 min
Delta R.T.: 0.000 min
Response: 142680
Conc: 0.32 ng/ml