

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 18:01
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 23:07:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.423	3.672	27892576	28989490	16.859	21.758 #
2)	SA Decachlor...	10.236	8.760	32106299	29184024	20.035	23.481
Target Compounds							
3)	L1 AR-1016-1	5.601	0.000	115233	0	2.626	N.D. #
4)	L1 AR-1016-2	5.630	0.000	85274	0	1.351	N.D. #
5)	L1 AR-1016-3	5.674	0.000	194614	0	4.821	N.D. #
6)	L1 AR-1016-4	5.785	0.000	26499	0	0.769	N.D. #
7)	L1 AR-1016-5	6.094f	0.000	108986	0	2.851	N.D. #
8)	L2 AR-1221-1	4.632	0.000	965518	0	44.081	N.D. #
9)	L2 AR-1221-2	4.730	3.977	412357	727666	25.711	54.648 #
10)	L2 AR-1221-3	4.792	0.000	150937	0	3.094	N.D. #
11)	L3 AR-1232-1	4.792	0.000	150937	0	4.066	N.D. #
12)	L3 AR-1232-2	5.323	0.000	138615	0	6.842	N.D. #
13)	L3 AR-1232-3	5.630	0.000	85274	0	2.806	N.D. #
14)	L3 AR-1232-4	5.785	0.000	26499	0	1.660	N.D. #
15)	L3 AR-1232-5	5.873	0.000	82952	0	6.126	N.D. #
16)	L4 AR-1242-1	5.601	0.000	115233	0	3.296	N.D. #
17)	L4 AR-1242-2	5.630	0.000	85274	0	1.594	N.D. #
18)	L4 AR-1242-3	5.674	0.000	194614	0	5.657	N.D. #
19)	L4 AR-1242-4	5.785	0.000	26499	0	0.926	N.D. #
20)	L4 AR-1242-5	6.525	5.590	82165	327936	2.277	9.398 #
21)	L5 AR-1248-1	5.601	0.000	115233	0	3.972	N.D. #
22)	L5 AR-1248-2	5.873	0.000	82952	0	1.957	N.D. #
23)	L5 AR-1248-3	6.094f	0.000	108986	0	2.109	N.D. #
24)	L5 AR-1248-4	6.480	0.000	68799	0	1.248	N.D. #
25)	L5 AR-1248-5	6.525	0.000	82165	0	1.446	N.D. #
26)	L6 AR-1254-1	6.454	5.590	323097	327936	5.177	4.527
27)	L6 AR-1254-2	6.674	5.738	438960	344677	4.570	5.367
28)	L6 AR-1254-3	7.044	6.163	264902	1349035	2.833	13.626 #
29)	L6 AR-1254-4	7.333	6.407f	83122	312484	1.346	6.066 #
30)	L6 AR-1254-5	7.745	6.800	1687424	1336754	22.255	16.037 #
31)	L7 AR-1260-1	7.208	6.279	1886438	2004682	24.768	28.528
32)	L7 AR-1260-2	7.466	6.469	1932690	2151713	23.088	26.853
33)	L7 AR-1260-3	7.827	6.627	3206969	2290050	49.761	30.086 #
34)	L7 AR-1260-4	8.052	7.100	2971038	2786366	39.333	47.674
35)	L7 AR-1260-5	8.376	7.343	4899265	4715893	36.793	37.659
36)	L8 AR-1262-1	7.827	6.892	3206969	1292319	32.767	34.934
37)	L8 AR-1262-2	8.376	7.100	4899265	2786366	32.158	34.693
38)	L8 AR-1262-3	8.695	7.629	3600661	2295594	32.644	37.144
39)	L8 AR-1262-4	8.787	7.694	3142714	3710203	50.148	33.400 #
40)	L8 AR-1262-5	9.457	8.196	2097107	1579672	32.713	32.190
41)	L9 AR-1268-1	8.695	7.629	3600661	2295594	17.526	12.727 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052638.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 18:01
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1262 LOD 40 PPB
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 23:07:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.787	7.694	3142714	3710203	16.071	22.672 #
43) L9	AR-1268-3	9.021	7.903	307323	241603	1.710	1.660
44) L9	AR-1268-4	9.457	8.196	2097107	1579672	26.835	28.288
45) L9	AR-1268-5	9.884	8.495	942111	794099	1.628	1.795



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
Data File : PP052638.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 18:01
Operator : YP\AJ
Sample : N4955-07
Misc : AR1262 LOD 40 PPB
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 23:07:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Oct 23 15:44:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

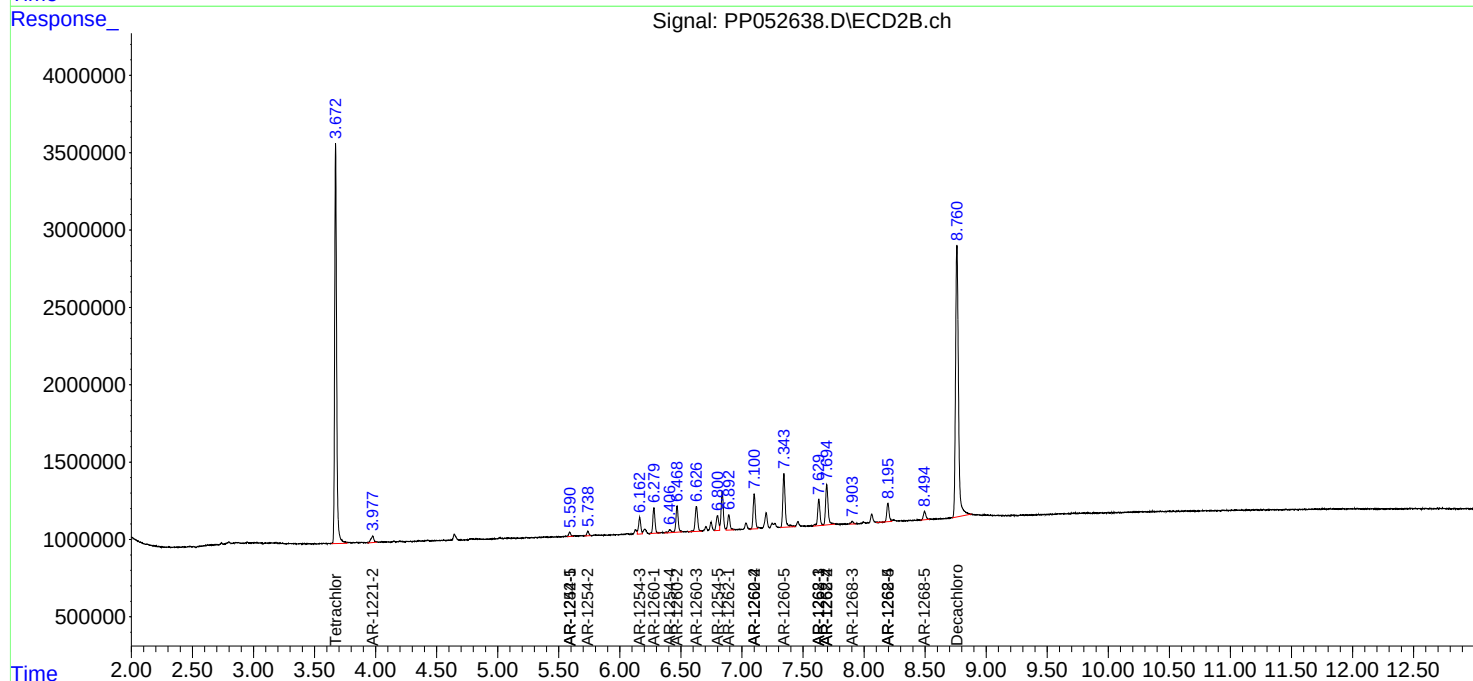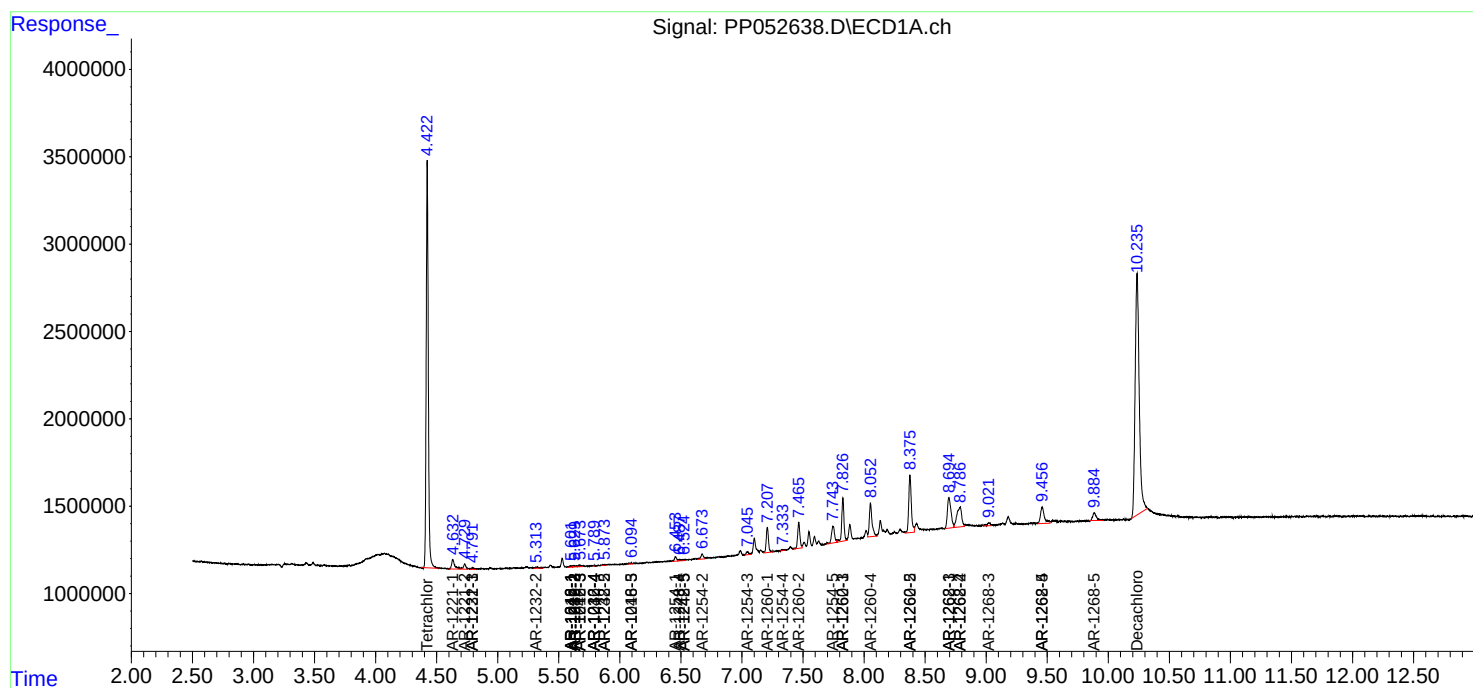


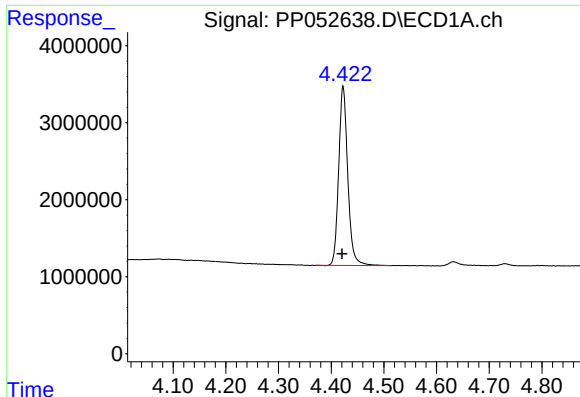

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: 0.002 min
Response: 27892576
Conc: 16.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

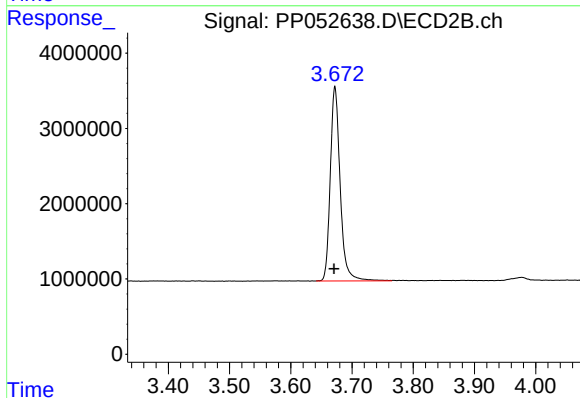


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.001 min
Response: 28989490
Conc: 21.76 ng/ml

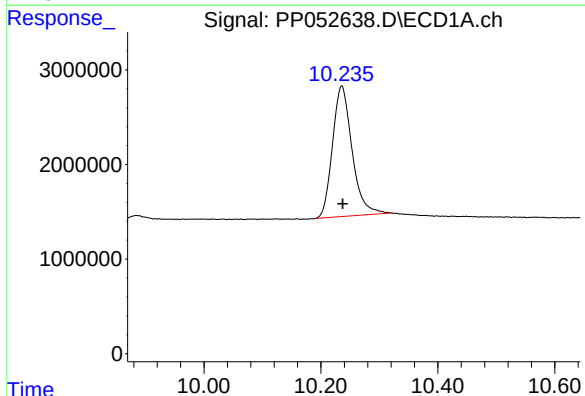


#2 Decachlorobiphenyl

R.T.: 10.236 min
Delta R.T.: -0.002 min
Response: 32106299
Conc: 20.04 ng/ml

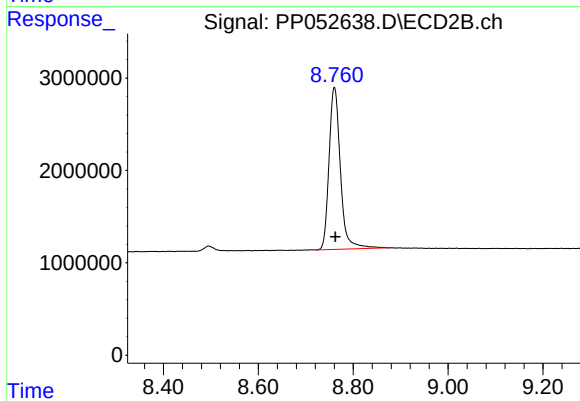

#2 Decachlorobiphenyl


R.T.: 8.760 min
Delta R.T.: -0.002 min
Response: 29184024
Conc: 23.48 ng/ml

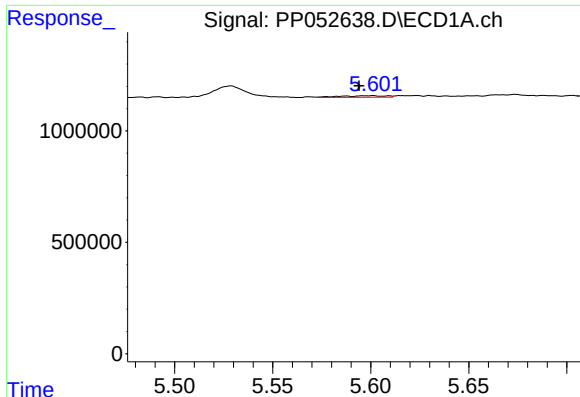

#3 AR-1016-1


R.T.: 5.601 min
Delta R.T.: 0.007 min
Response: 115233
Conc: 2.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

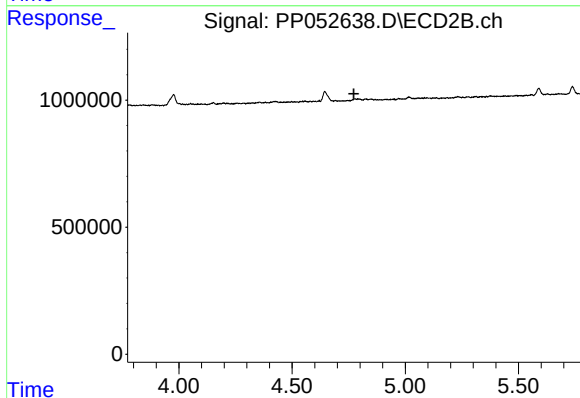


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.773 min
Response: 0
Conc: N.D.

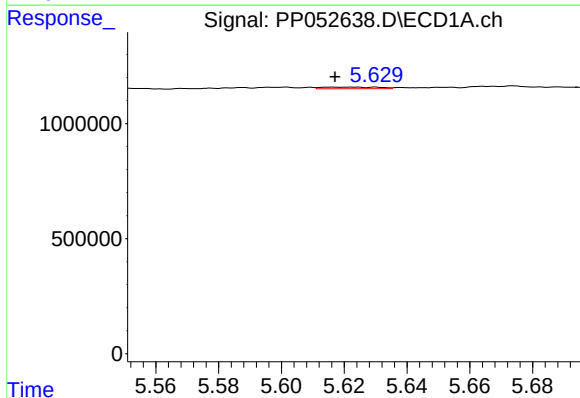


#4 AR-1016-2

R.T.: 5.630 min
Delta R.T.: 0.013 min
Response: 85274
Conc: 1.35 ng/ml

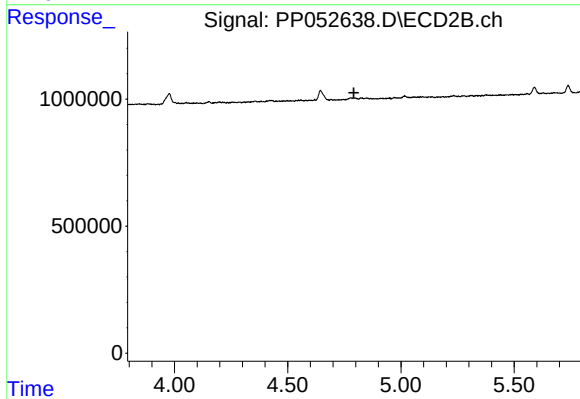

#4 AR-1016-2


R.T.: 0.000 min
Exp R.T. : 4.792 min
Response: 0
Conc: N.D.

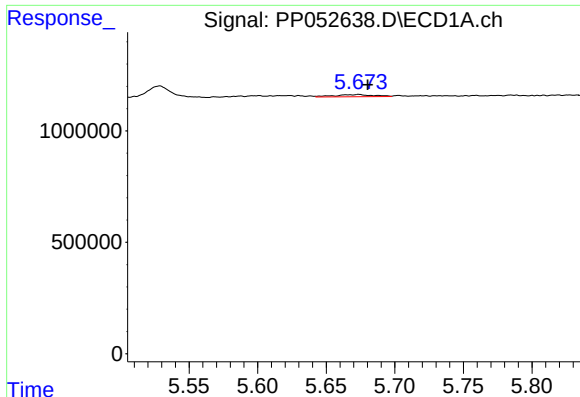

#5 AR-1016-3


R.T.: 5.674 min
Delta R.T.: -0.006 min
Response: 194614
Conc: 4.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

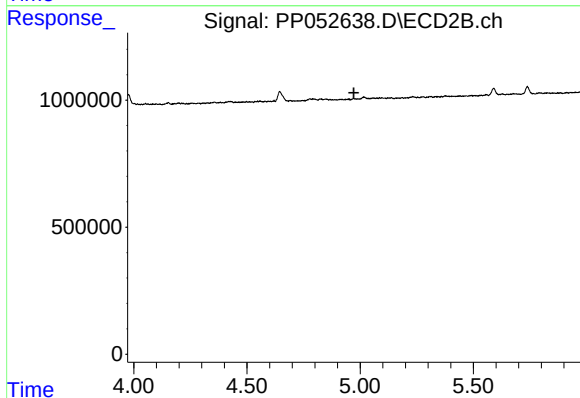


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

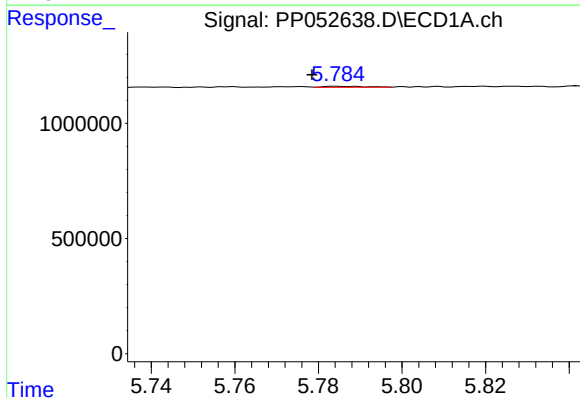


#6 AR-1016-4

R.T.: 5.785 min
Delta R.T.: 0.006 min
Response: 26499
Conc: 0.77 ng/ml

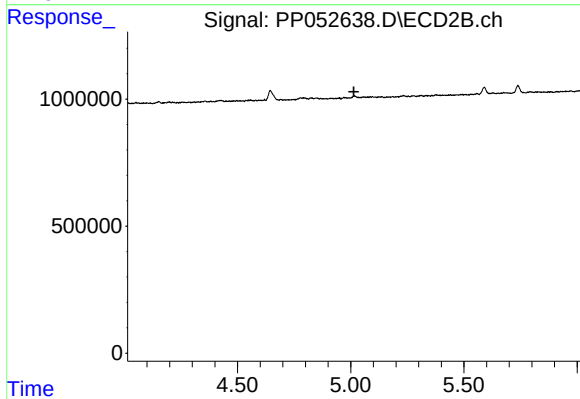

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 5.014 min
Response: 0
Conc: N.D.

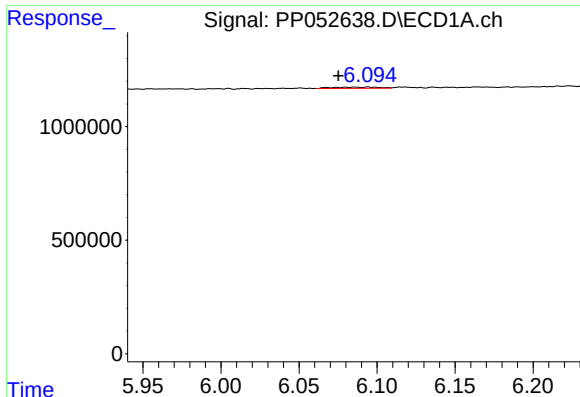

#7 AR-1016-5


R.T.: 6.094 min
Delta R.T.: 0.019 min
Response: 108986
Conc: 2.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

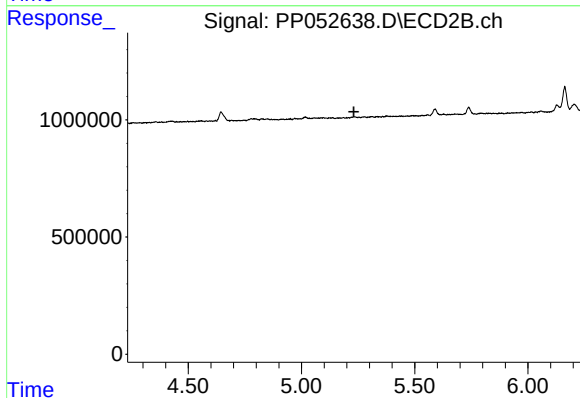


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.231 min
Response: 0
Conc: N.D.

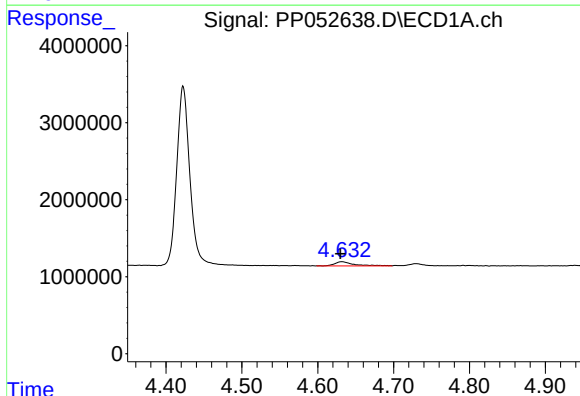


#8 AR-1221-1

R.T.: 4.632 min
Delta R.T.: 0.002 min
Response: 965518
Conc: 44.08 ng/ml

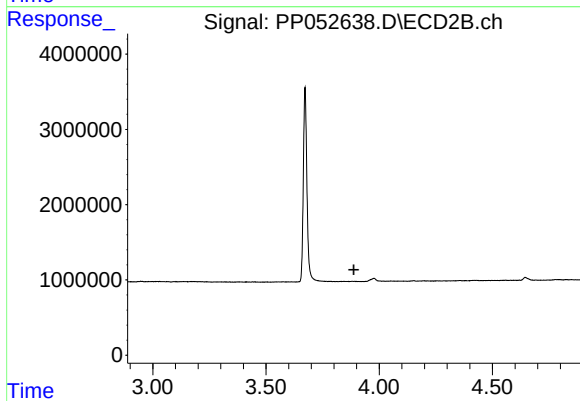

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T. : 3.888 min
Response: 0
Conc: N.D.

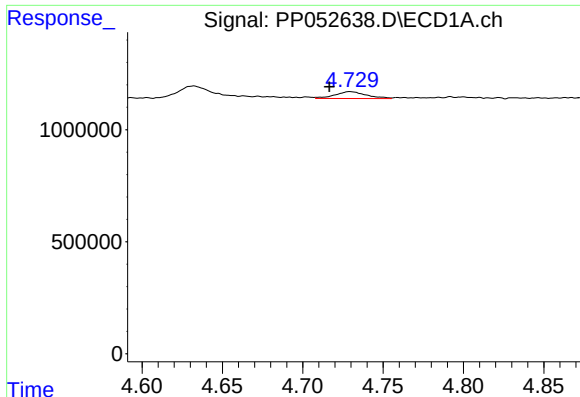

#9 AR-1221-2


R.T.: 4.730 min
Delta R.T.: 0.013 min
Response: 412357
Conc: 25.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

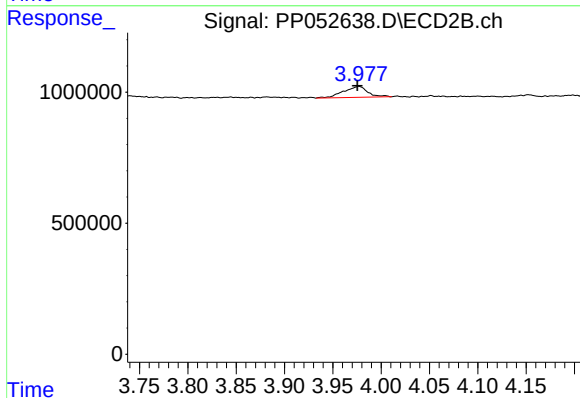


#9 AR-1221-2

R.T.: 3.977 min
Delta R.T.: 0.002 min
Response: 727666
Conc: 54.65 ng/ml

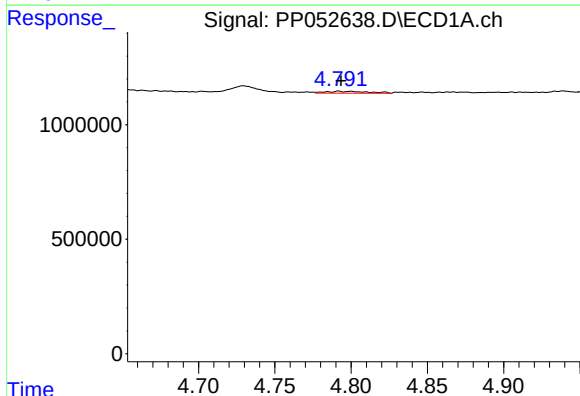


#10 AR-1221-3

R.T.: 4.792 min
Delta R.T.: -0.001 min
Response: 150937
Conc: 3.09 ng/ml

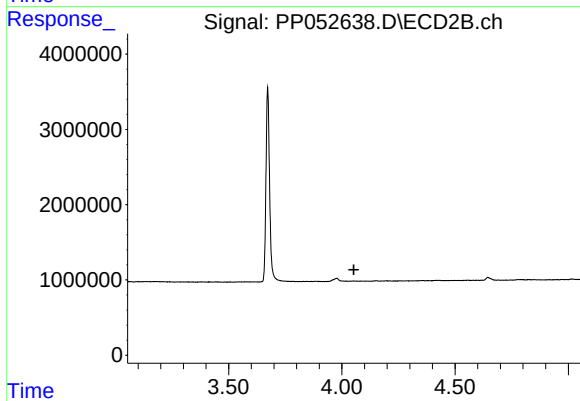

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.053 min
Response: 0
Conc: N.D.

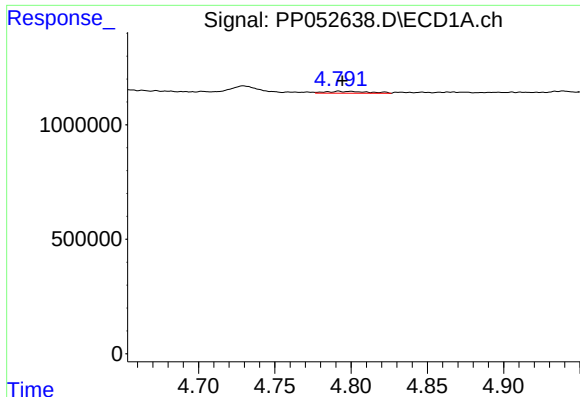

#11 AR-1232-1


R.T.: 4.792 min
Delta R.T.: -0.002 min
Response: 150937
Conc: 4.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

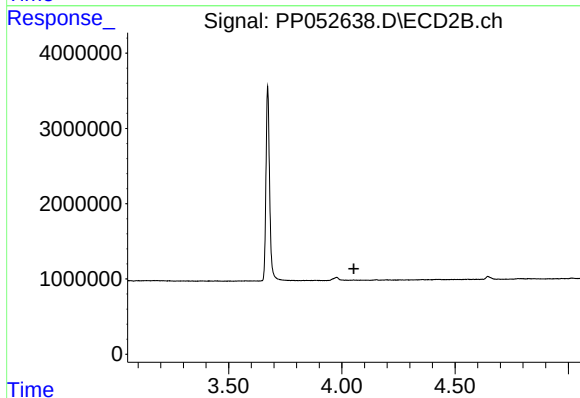


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.053 min
Response: 0
Conc: N.D.

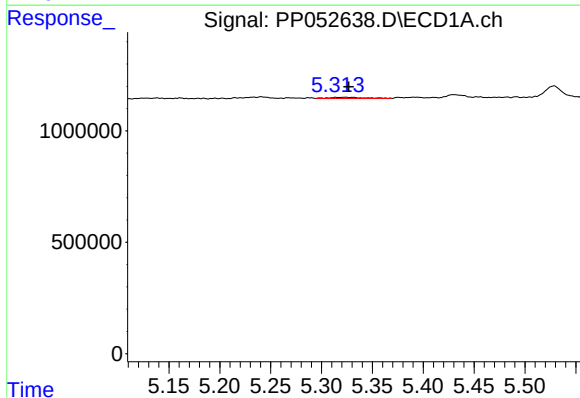


#12 AR-1232-2

R.T.: 5.323 min
Delta R.T.: -0.004 min
Response: 138615
Conc: 6.84 ng/ml

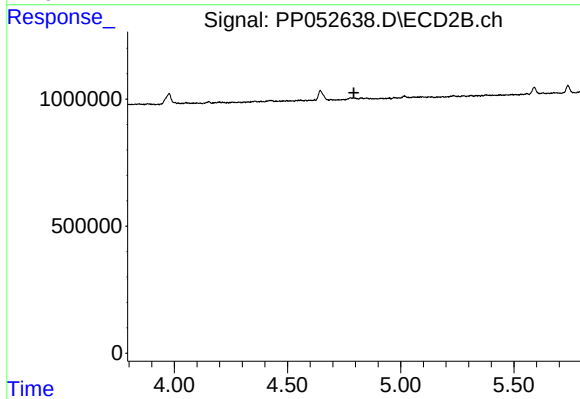

#12 AR-1232-2


R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

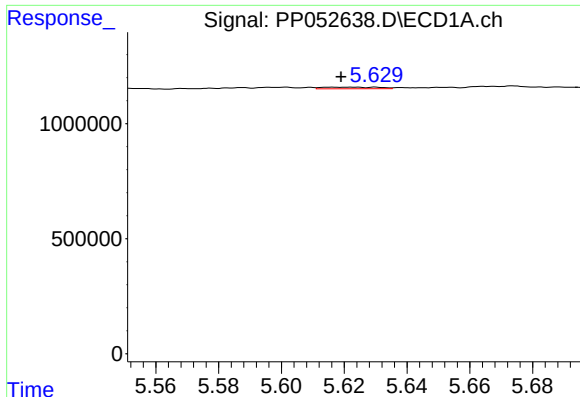

#13 AR-1232-3


R.T.: 5.630 min
Delta R.T.: 0.011 min
Response: 85274
Conc: 2.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

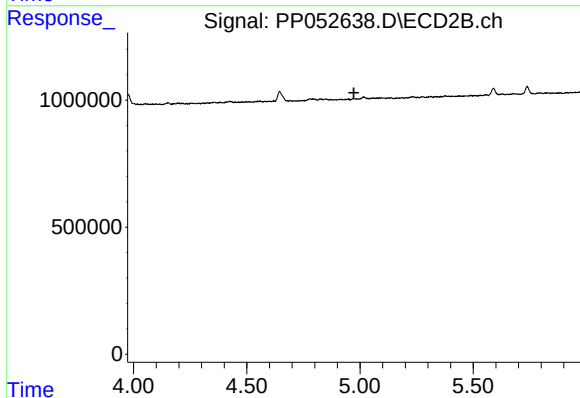


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

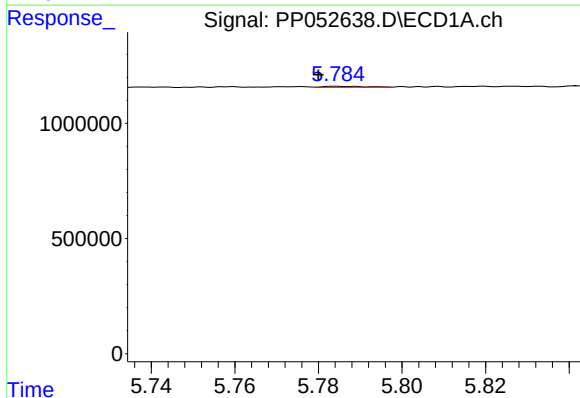


#14 AR-1232-4

R.T.: 5.785 min
Delta R.T.: 0.005 min
Response: 26499
Conc: 1.66 ng/ml

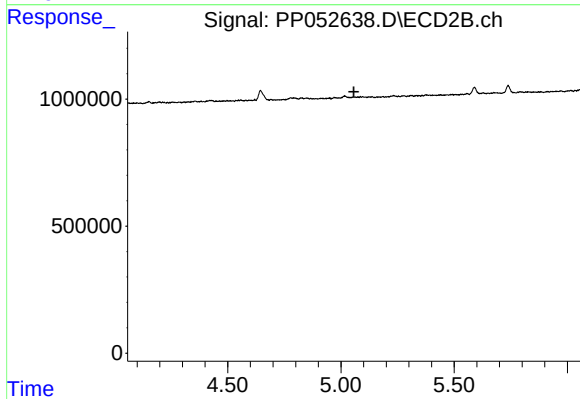

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.057 min
Response: 0
Conc: N.D.

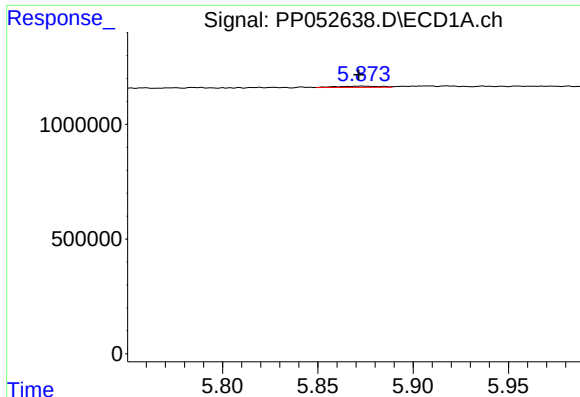

#15 AR-1232-5


R.T.: 5.873 min
Delta R.T.: 0.002 min
Response: 82952
Conc: 6.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

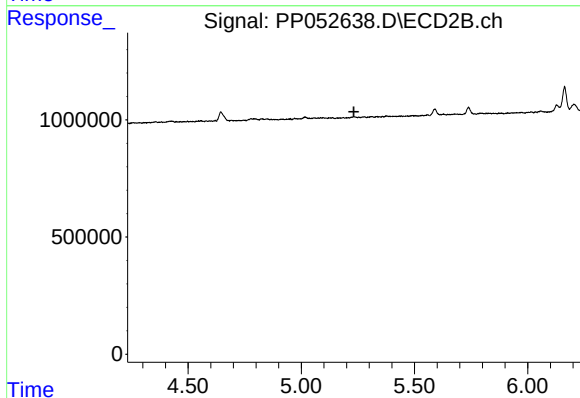


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.232 min
Response: 0
Conc: N.D.

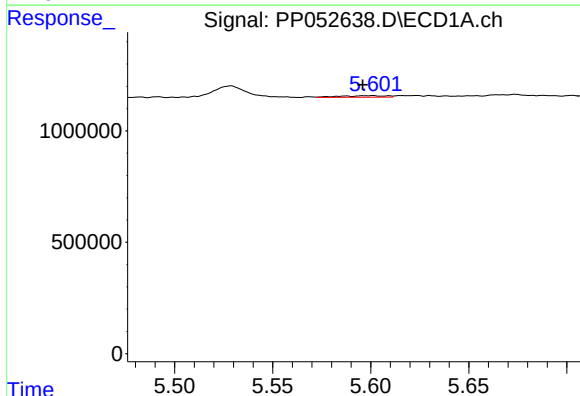


#16 AR-1242-1

R.T.: 5.601 min
Delta R.T.: 0.005 min
Response: 115233
Conc: 3.30 ng/ml

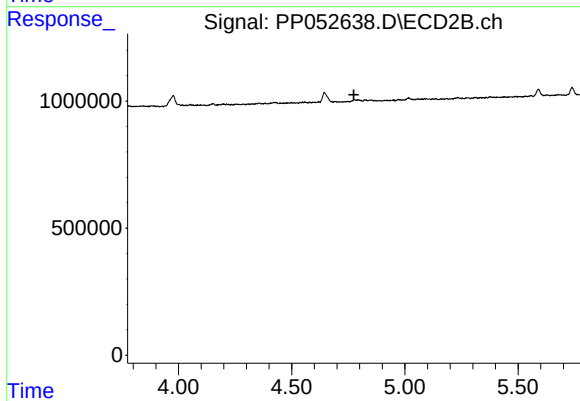

#16 AR-1242-1


R.T.: 0.000 min
Exp R.T. : 4.774 min
Response: 0
Conc: N.D.

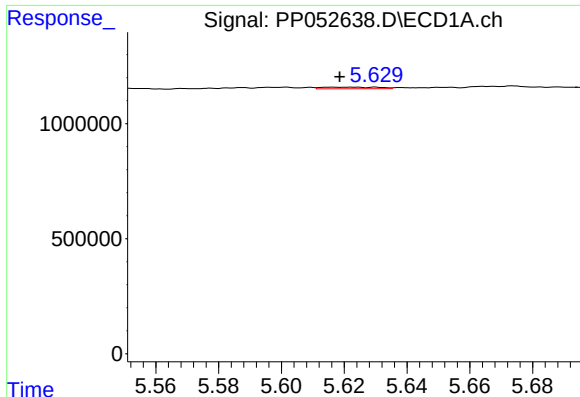

#17 AR-1242-2


R.T.: 5.630 min
Delta R.T.: 0.012 min
Response: 85274
Conc: 1.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

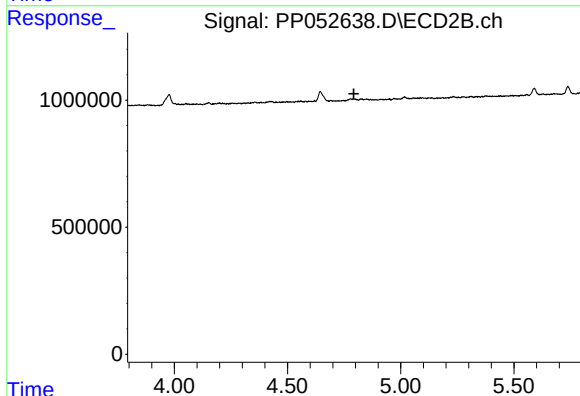


#17 AR-1242-2

R.T.: 0.000 min
Exp R.T. : 4.793 min
Response: 0
Conc: N.D.

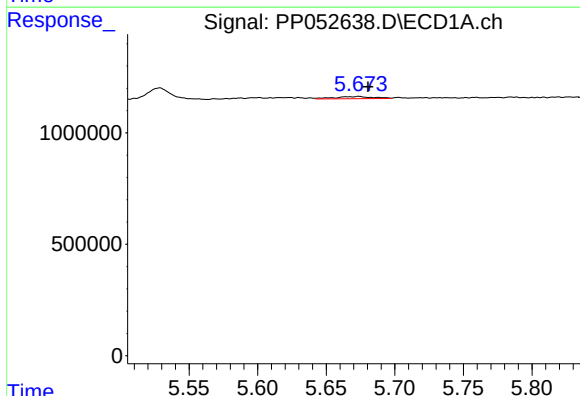


#18 AR-1242-3

R.T.: 5.674 min
Delta R.T.: -0.007 min
Response: 194614
Conc: 5.66 ng/ml

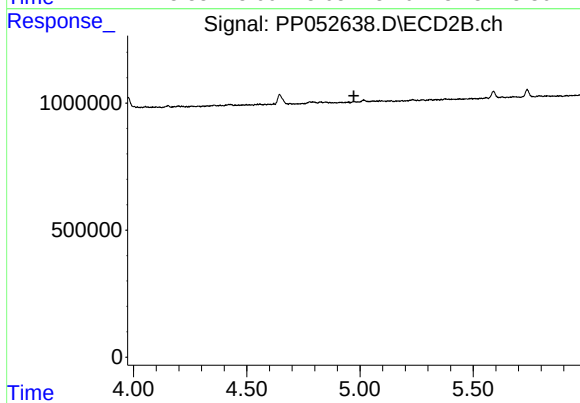

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.973 min
Response: 0
Conc: N.D.

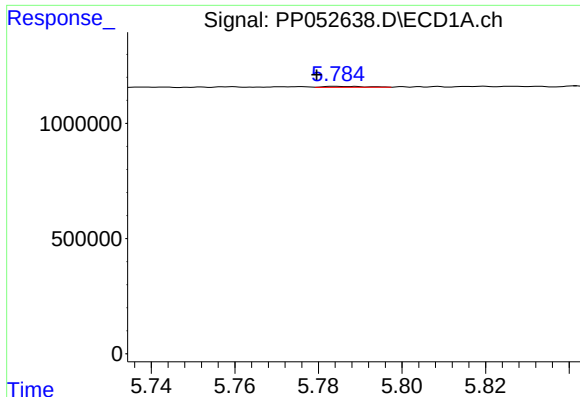

#19 AR-1242-4


R.T.: 5.785 min
Delta R.T.: 0.005 min
Response: 26499
Conc: 0.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

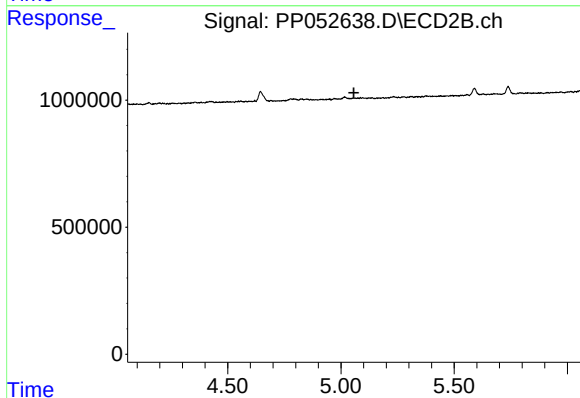


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.057 min
Response: 0
Conc: N.D.

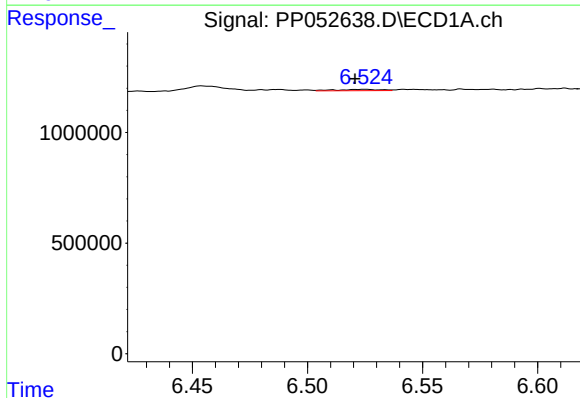


#20 AR-1242-5

R.T.: 6.525 min
Delta R.T.: 0.004 min
Response: 82165
Conc: 2.28 ng/ml

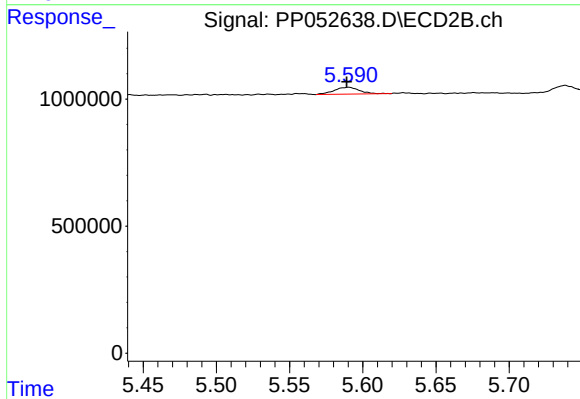

#20 AR-1242-5


R.T.: 5.590 min
Delta R.T.: 0.001 min
Response: 327936
Conc: 9.40 ng/ml

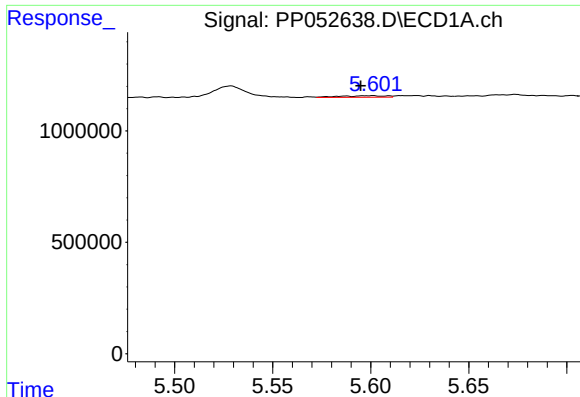

#21 AR-1248-1


R.T.: 5.601 min
Delta R.T.: 0.006 min
Response: 115233
Conc: 3.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

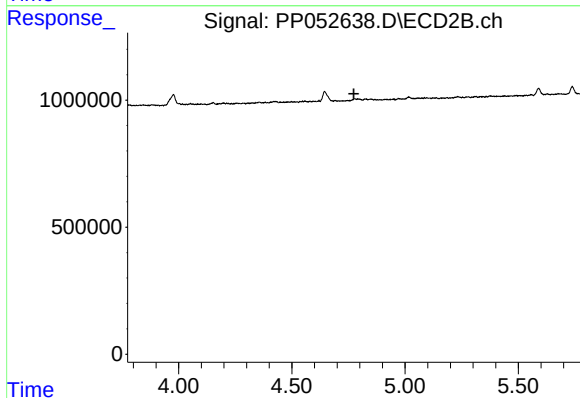


#21 AR-1248-1

R.T.: 0.000 min
Exp R.T. : 4.774 min
Response: 0
Conc: N.D.

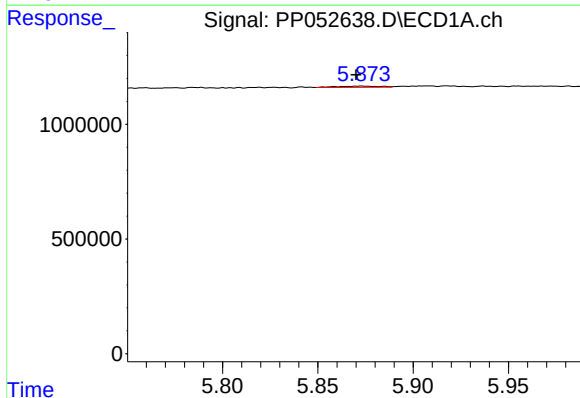


#22 AR-1248-2

R.T.: 5.873 min
Delta R.T.: 0.003 min
Response: 82952
Conc: 1.96 ng/ml

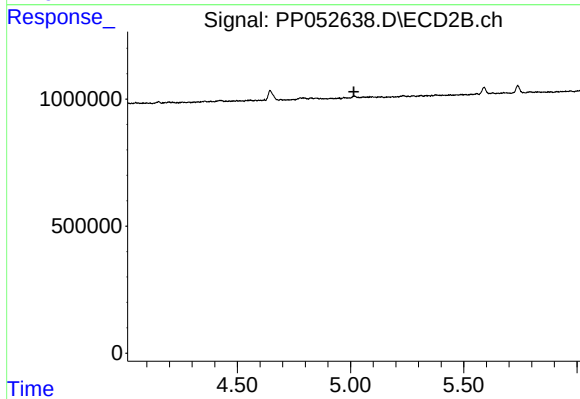

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.014 min
Response: 0
Conc: N.D.

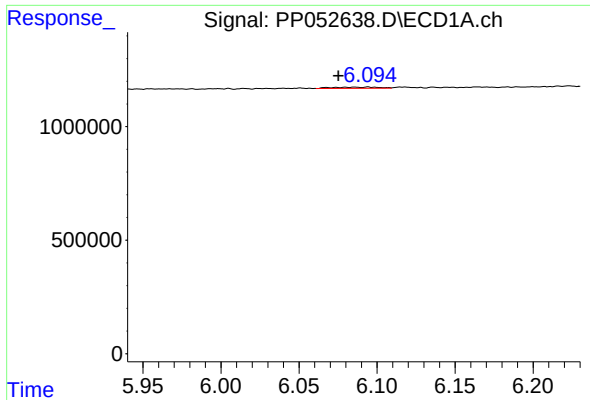

#23 AR-1248-3


R.T.: 6.094 min
Delta R.T.: 0.019 min
Response: 108986
Conc: 2.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

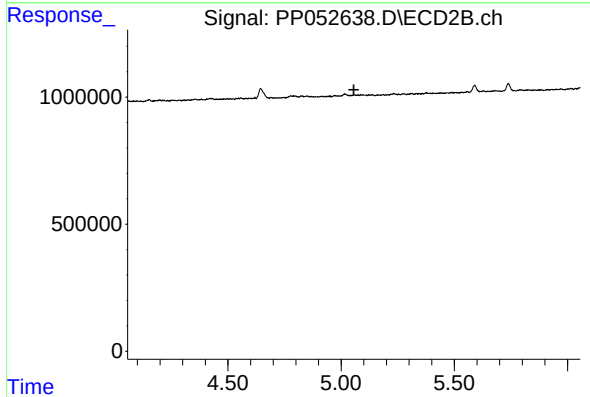


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.057 min
Response: 0
Conc: N.D.

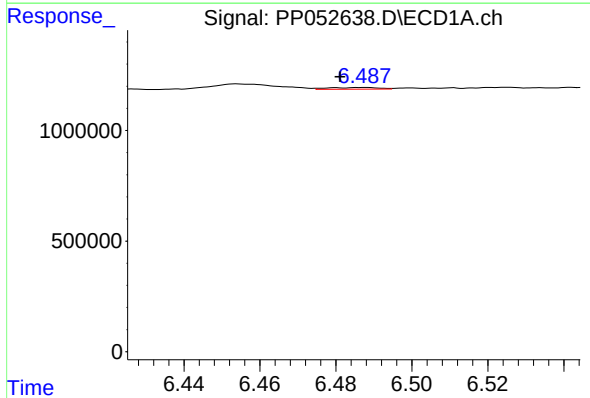


#24 AR-1248-4

R.T.: 6.480 min
Delta R.T.: 0.000 min
Response: 68799
Conc: 1.25 ng/ml

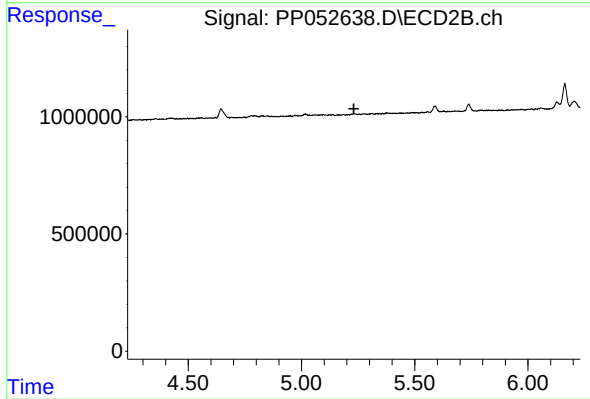

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.232 min
Response: 0
Conc: N.D.

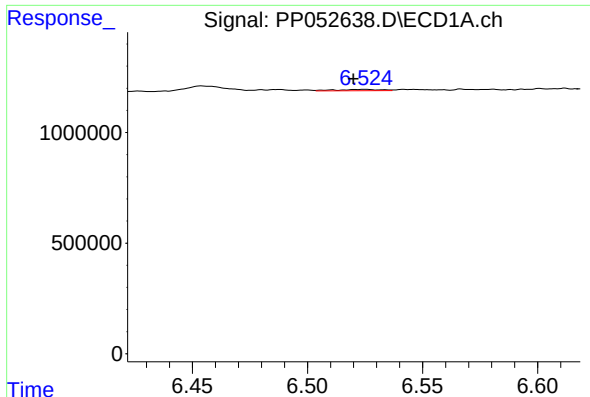

#25 AR-1248-5


R.T.: 6.525 min
Delta R.T.: 0.005 min
Response: 82165
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

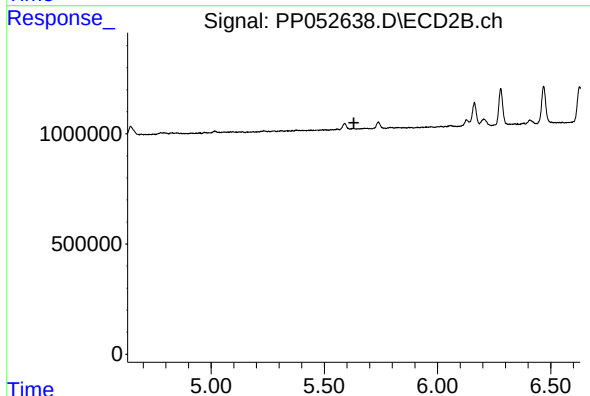


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.631 min
Response: 0
Conc: N.D.

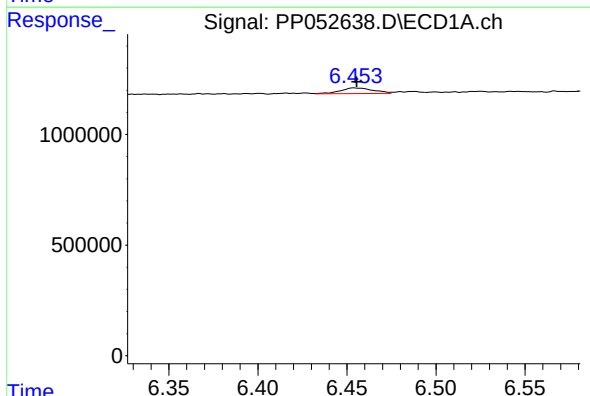


#26 AR-1254-1

R.T.: 6.454 min
Delta R.T.: 0.000 min
Response: 323097
Conc: 5.18 ng/ml

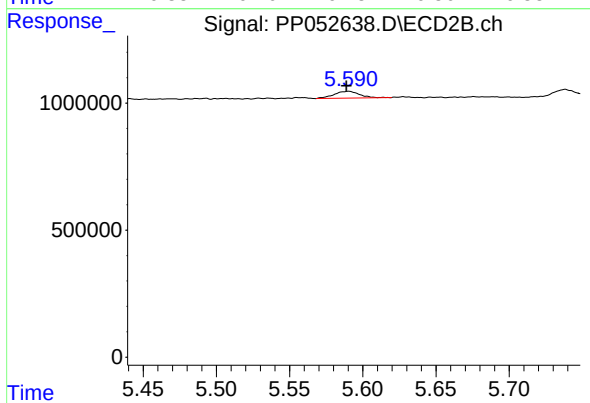

#26 AR-1254-1


R.T.: 5.590 min
Delta R.T.: 0.001 min
Response: 327936
Conc: 4.53 ng/ml

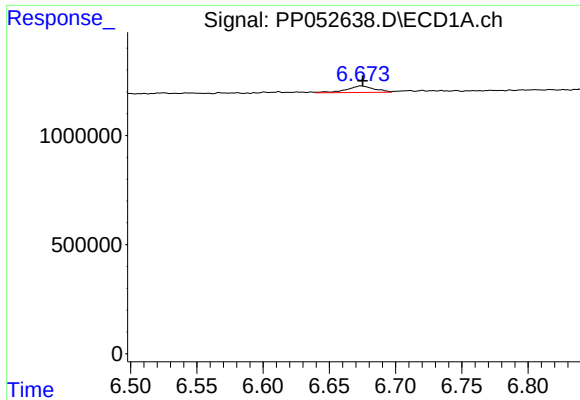

#27 AR-1254-2


R.T.: 6.674 min
Delta R.T.: -0.001 min
Response: 438960
Conc: 4.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

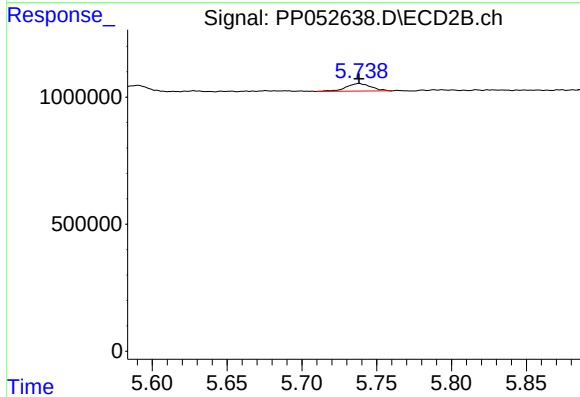


#27 AR-1254-2

R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 344677
Conc: 5.37 ng/ml

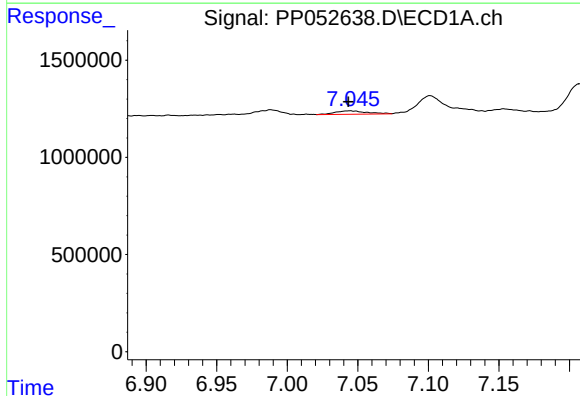


#28 AR-1254-3

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 264902
Conc: 2.83 ng/ml

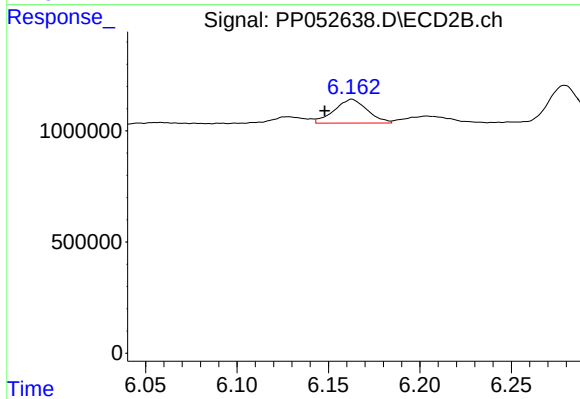

#28 AR-1254-3


R.T.: 6.163 min
Delta R.T.: 0.015 min
Response: 1349035
Conc: 13.63 ng/ml

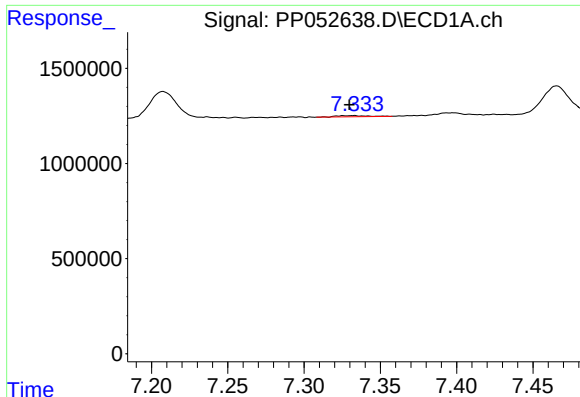

#29 AR-1254-4


R.T.: 7.333 min
Delta R.T.: 0.003 min
Response: 83122
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

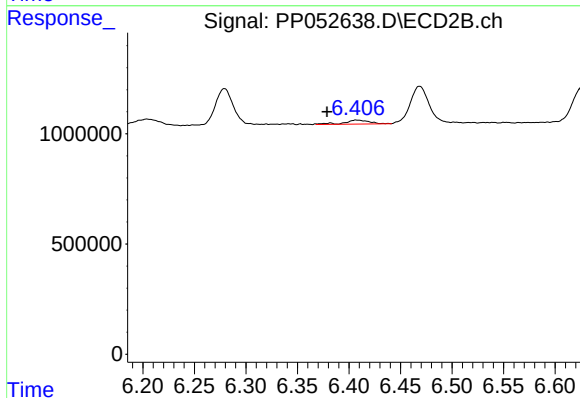


#29 AR-1254-4

R.T.: 6.407 min
Delta R.T.: 0.028 min
Response: 312484
Conc: 6.07 ng/ml

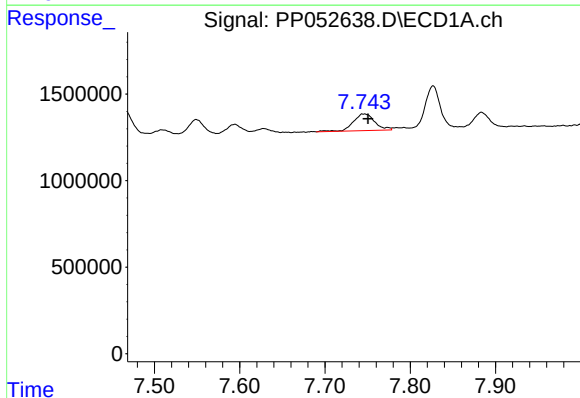


#30 AR-1254-5

R.T.: 7.745 min
Delta R.T.: -0.005 min
Response: 1687424
Conc: 22.25 ng/ml

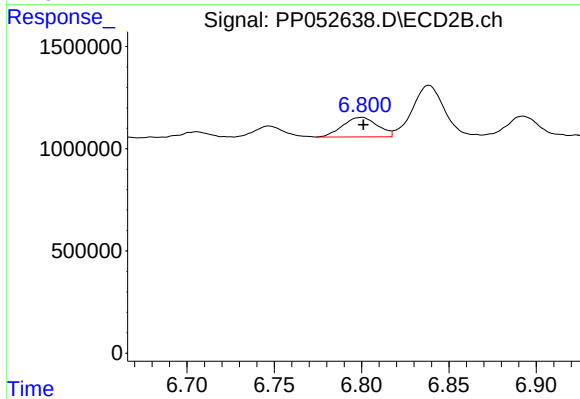

#30 AR-1254-5


R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 1336754
Conc: 16.04 ng/ml

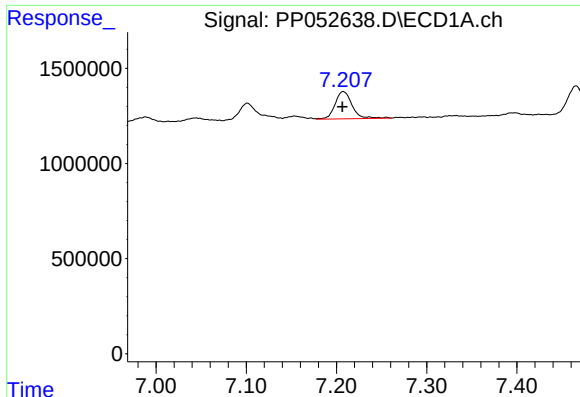

#31 AR-1260-1


R.T.: 7.208 min
Delta R.T.: 0.000 min
Response: 1886438
Conc: 24.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

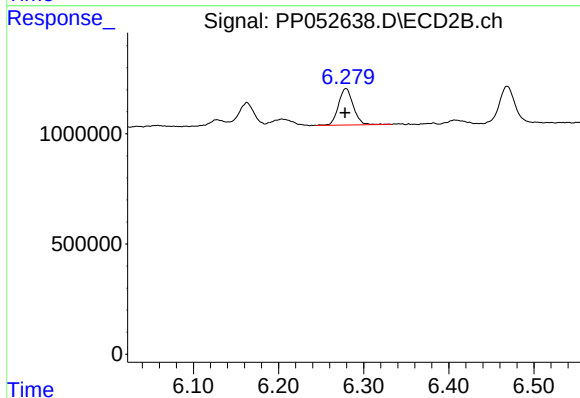


#31 AR-1260-1

R.T.: 6.279 min
Delta R.T.: 0.001 min
Response: 2004682
Conc: 28.53 ng/ml

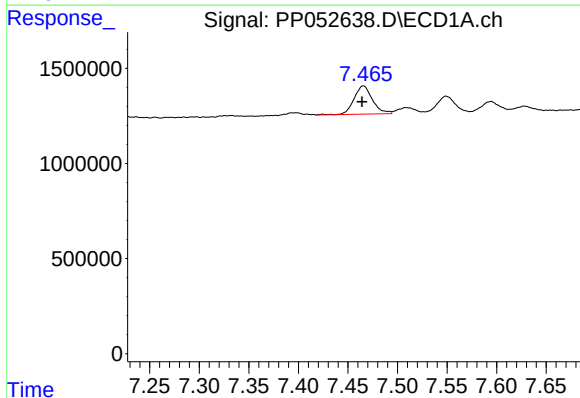


#32 AR-1260-2

R.T.: 7.466 min
Delta R.T.: 0.001 min
Response: 1932690
Conc: 23.09 ng/ml

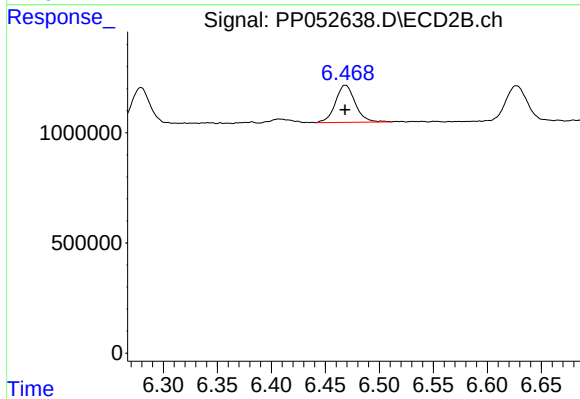

#32 AR-1260-2


R.T.: 6.469 min
Delta R.T.: 0.000 min
Response: 2151713
Conc: 26.85 ng/ml

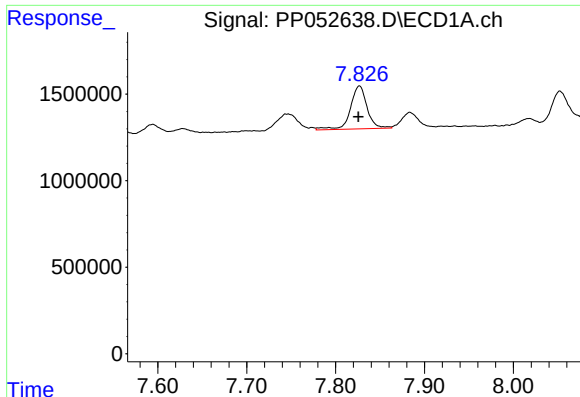

#33 AR-1260-3


R.T.: 7.827 min
Delta R.T.: 0.001 min
Response: 3206969
Conc: 49.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

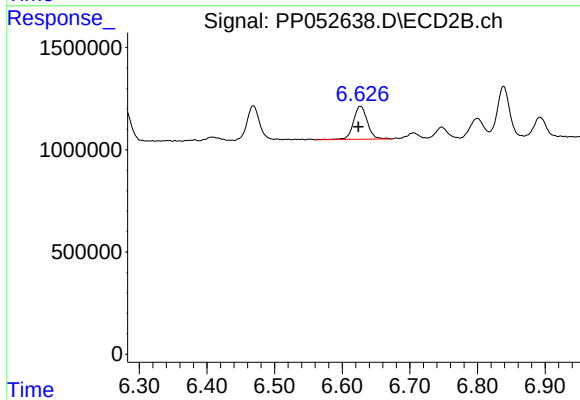


#33 AR-1260-3

R.T.: 6.627 min
Delta R.T.: 0.003 min
Response: 2290050
Conc: 30.09 ng/ml

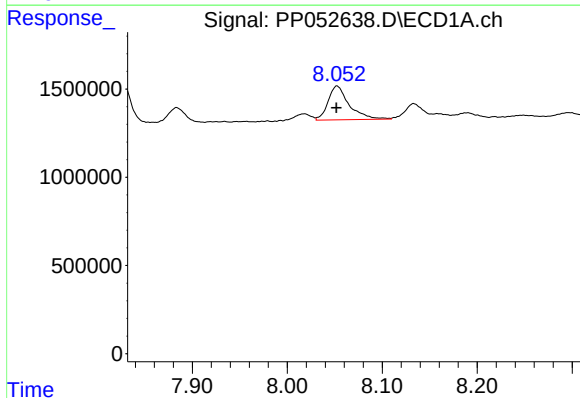


#34 AR-1260-4

R.T.: 8.052 min
Delta R.T.: 0.000 min
Response: 2971038
Conc: 39.33 ng/ml

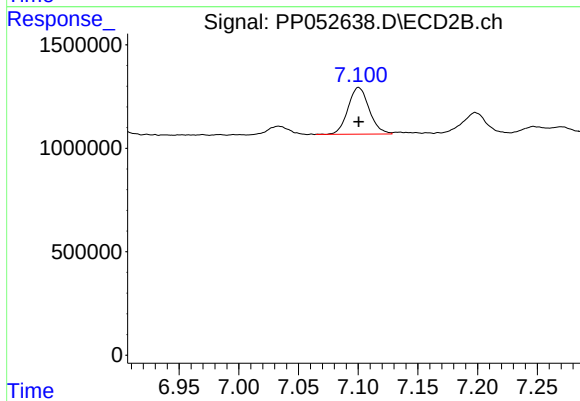

#34 AR-1260-4


R.T.: 7.100 min
Delta R.T.: 0.000 min
Response: 2786366
Conc: 47.67 ng/ml

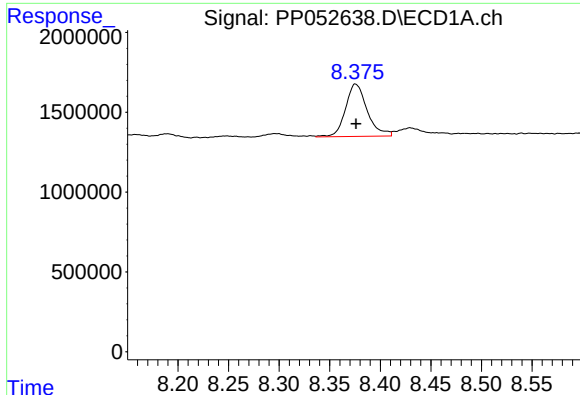

#35 AR-1260-5


R.T.: 8.376 min
Delta R.T.: 0.000 min
Response: 4899265
Conc: 36.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

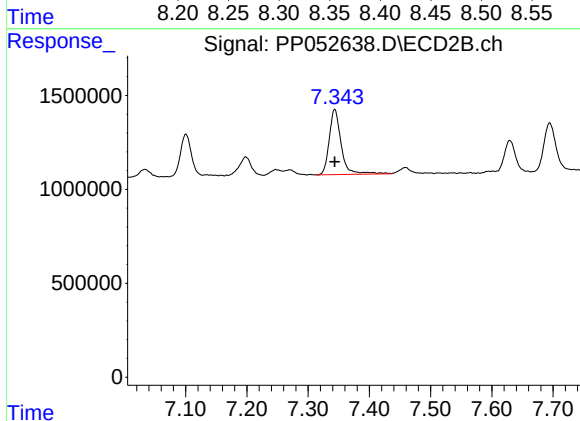


#35 AR-1260-5

R.T.: 7.343 min
Delta R.T.: 0.000 min
Response: 4715893
Conc: 37.66 ng/ml

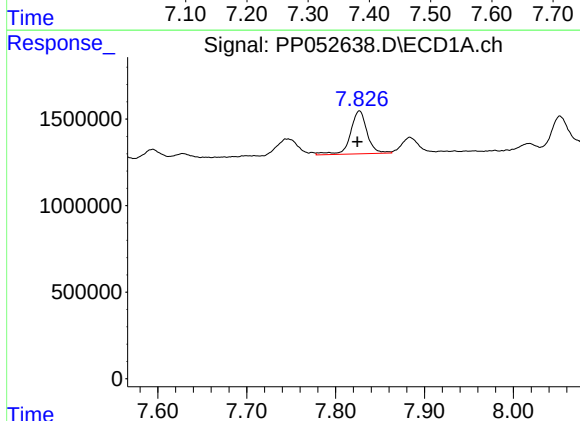


#36 AR-1262-1

R.T.: 7.827 min
Delta R.T.: 0.002 min
Response: 3206969
Conc: 32.77 ng/ml

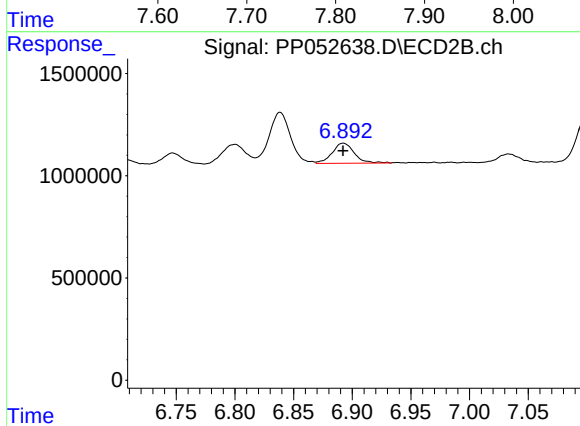

#36 AR-1262-1


R.T.: 6.892 min
Delta R.T.: 0.000 min
Response: 1292319
Conc: 34.93 ng/ml

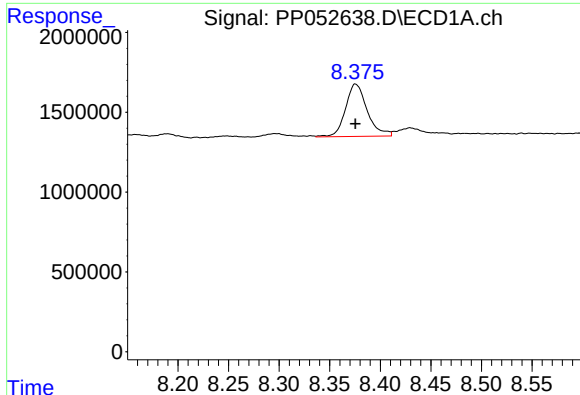

#37 AR-1262-2


R.T.: 8.376 min
Delta R.T.: 0.000 min
Response: 4899265
Conc: 32.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

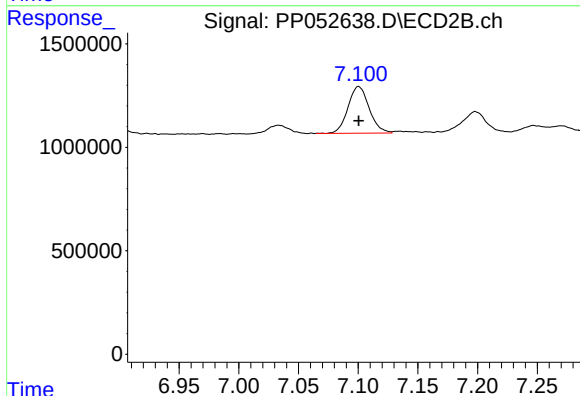


#37 AR-1262-2

R.T.: 7.100 min
Delta R.T.: 0.000 min
Response: 2786366
Conc: 34.69 ng/ml

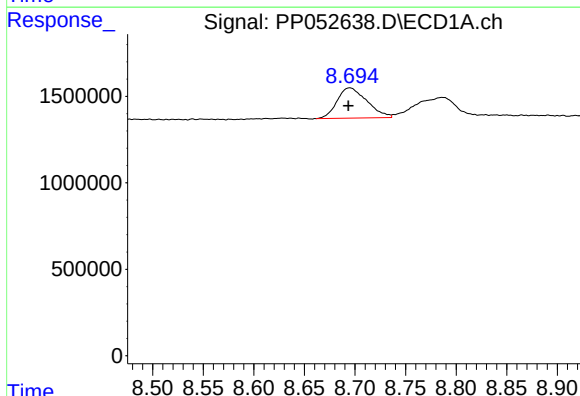


#38 AR-1262-3

R.T.: 8.695 min
Delta R.T.: 0.001 min
Response: 3600661
Conc: 32.64 ng/ml

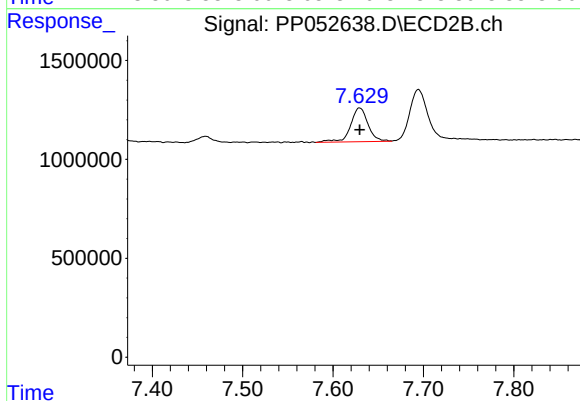

#38 AR-1262-3


R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 2295594
Conc: 37.14 ng/ml

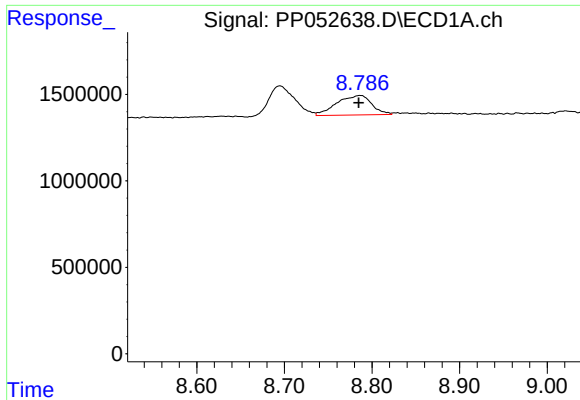

#39 AR-1262-4


R.T.: 8.787 min
Delta R.T.: 0.002 min
Response: 3142714
Conc: 50.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

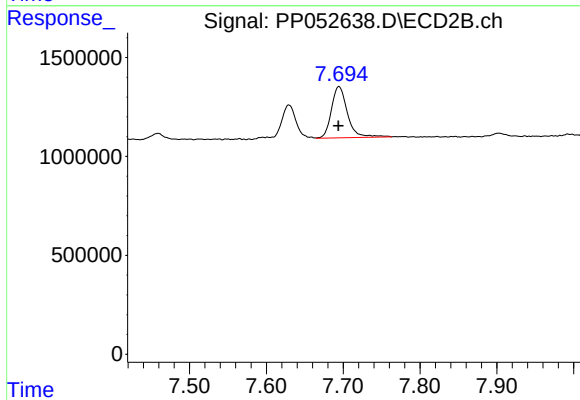


#39 AR-1262-4

R.T.: 7.694 min
Delta R.T.: 0.000 min
Response: 3710203
Conc: 33.40 ng/ml

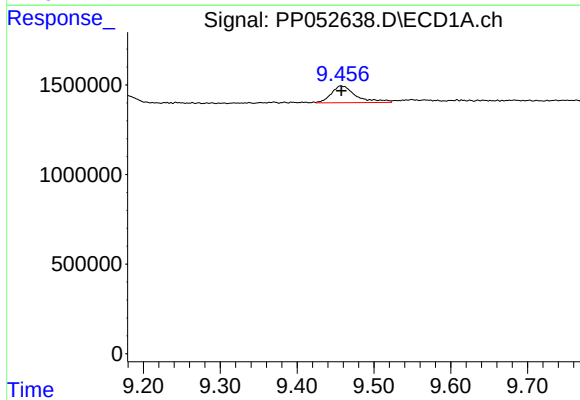


#40 AR-1262-5

R.T.: 9.457 min
Delta R.T.: 0.000 min
Response: 2097107
Conc: 32.71 ng/ml

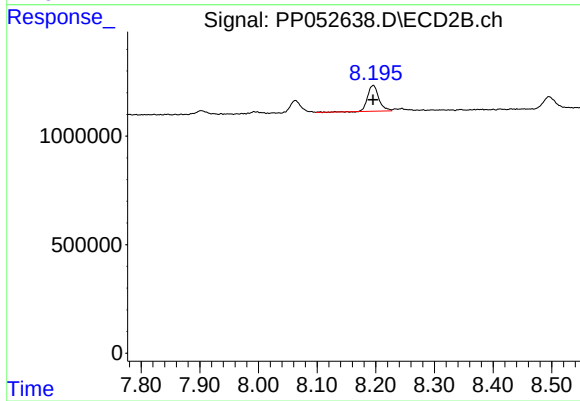

#40 AR-1262-5


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 1579672
Conc: 32.19 ng/ml

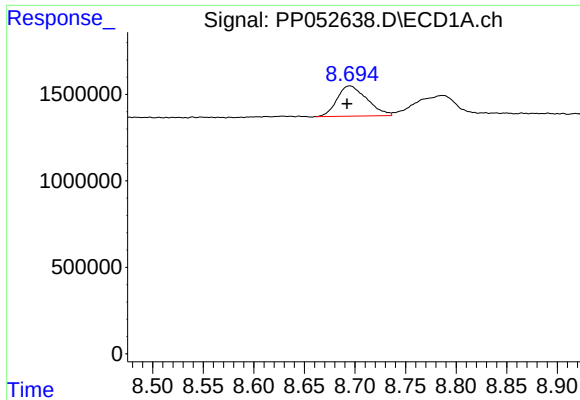

#41 AR-1268-1


R.T.: 8.695 min
Delta R.T.: 0.002 min
Response: 3600661
Conc: 17.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

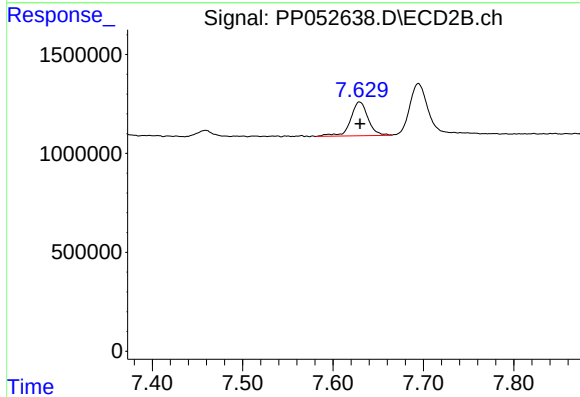


#41 AR-1268-1

R.T.: 7.629 min
Delta R.T.: 0.000 min
Response: 2295594
Conc: 12.73 ng/ml

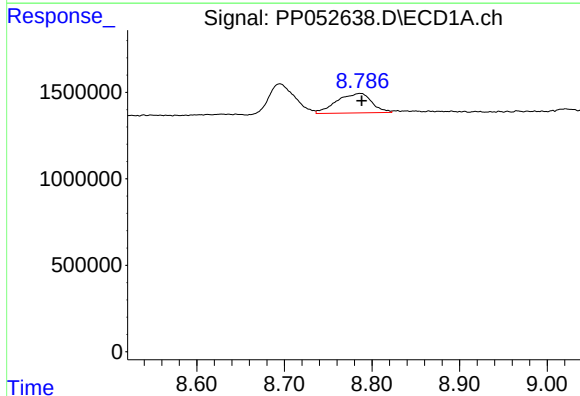


#42 AR-1268-2

R.T.: 8.787 min
Delta R.T.: -0.002 min
Response: 3142714
Conc: 16.07 ng/ml

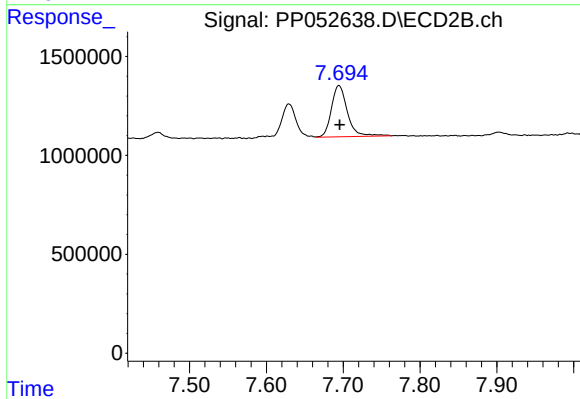

#42 AR-1268-2


R.T.: 7.694 min
Delta R.T.: 0.000 min
Response: 3710203
Conc: 22.67 ng/ml

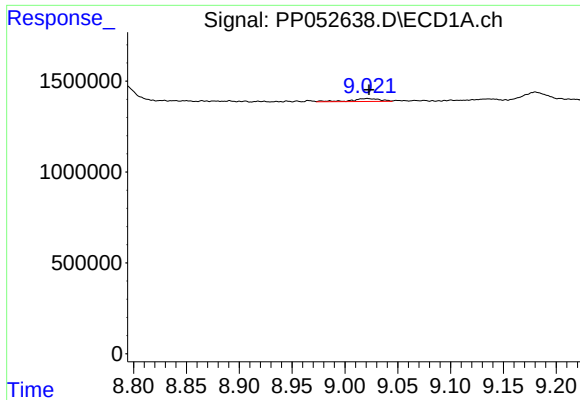

#43 AR-1268-3


R.T.: 9.021 min
Delta R.T.: -0.001 min
Response: 307323
Conc: 1.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

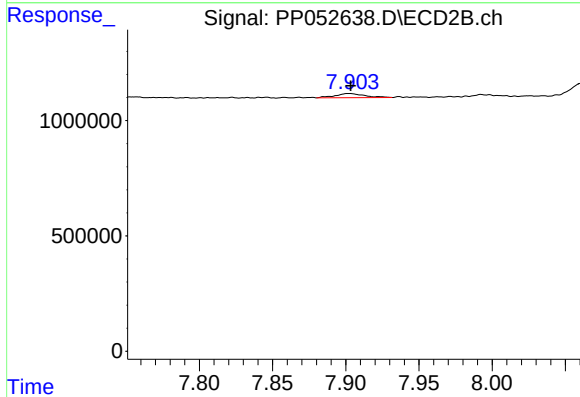


#43 AR-1268-3

R.T.: 7.903 min
Delta R.T.: 0.000 min
Response: 241603
Conc: 1.66 ng/ml

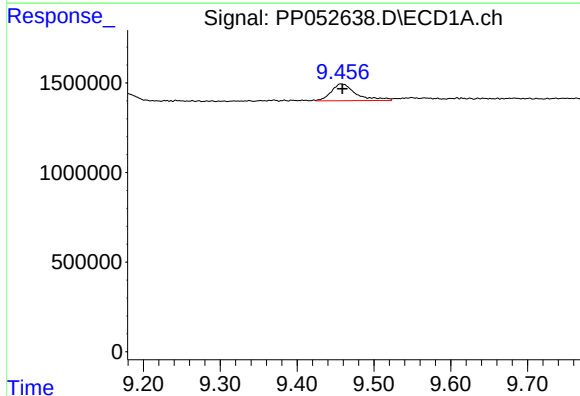


#44 AR-1268-4

R.T.: 9.457 min
Delta R.T.: -0.002 min
Response: 2097107
Conc: 26.84 ng/ml

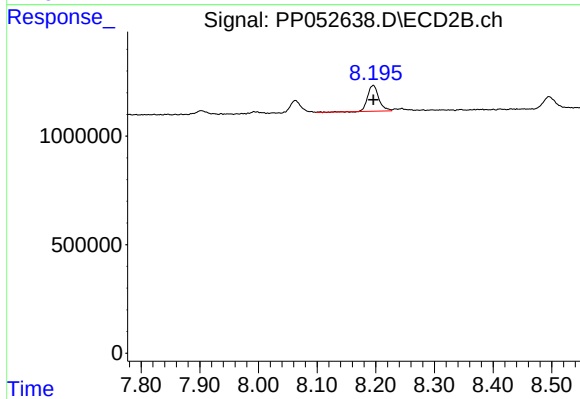

#44 AR-1268-4


R.T.: 8.196 min
Delta R.T.: 0.000 min
Response: 1579672
Conc: 28.29 ng/ml

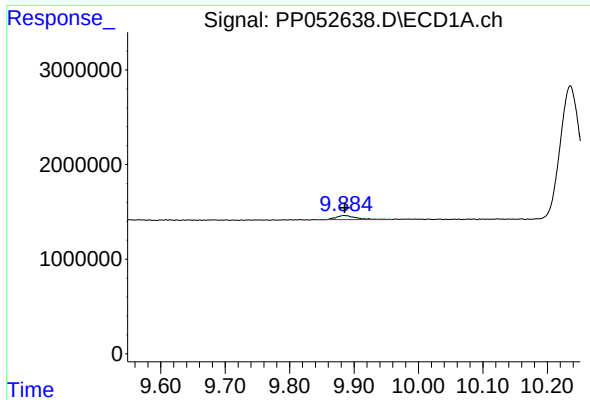

#45 AR-1268-5

R.T.: 9.884 min
Delta R.T.: -0.001 min
Response: 942111
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

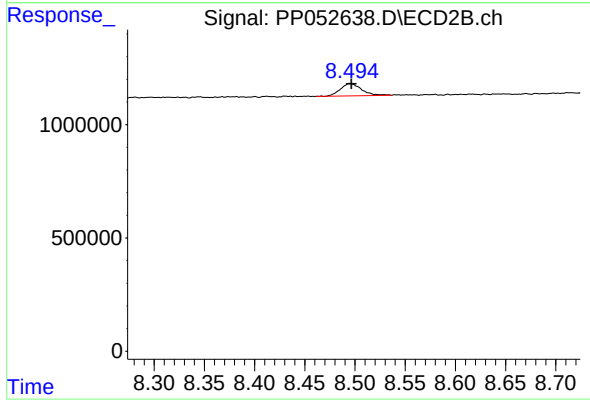

#45 AR-1268-5

R.T.: 8.495 min
Delta R.T.: -0.001 min
Response: 794099
Conc: 1.79 ng/ml