

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052612.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 10:51
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:53:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.422	3.672	29847531	28310112	18.041	21.248
2) SA Decachlor...	10.234	8.761	37008960	29168795	23.095	23.468
Target Compounds						
8) L2 AR-1221-1	4.630	3.888	480302	451305	21.929	25.647
9) L2 AR-1221-2	4.727	3.976	588710	724081	36.707	54.379 #
10) L2 AR-1221-3	4.793	4.054	968173	998868	19.844	24.089



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
Data File : PP052612.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 10:51
Operator : YP\AJ
Sample : N4955-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:53:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Oct 23 15:44:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

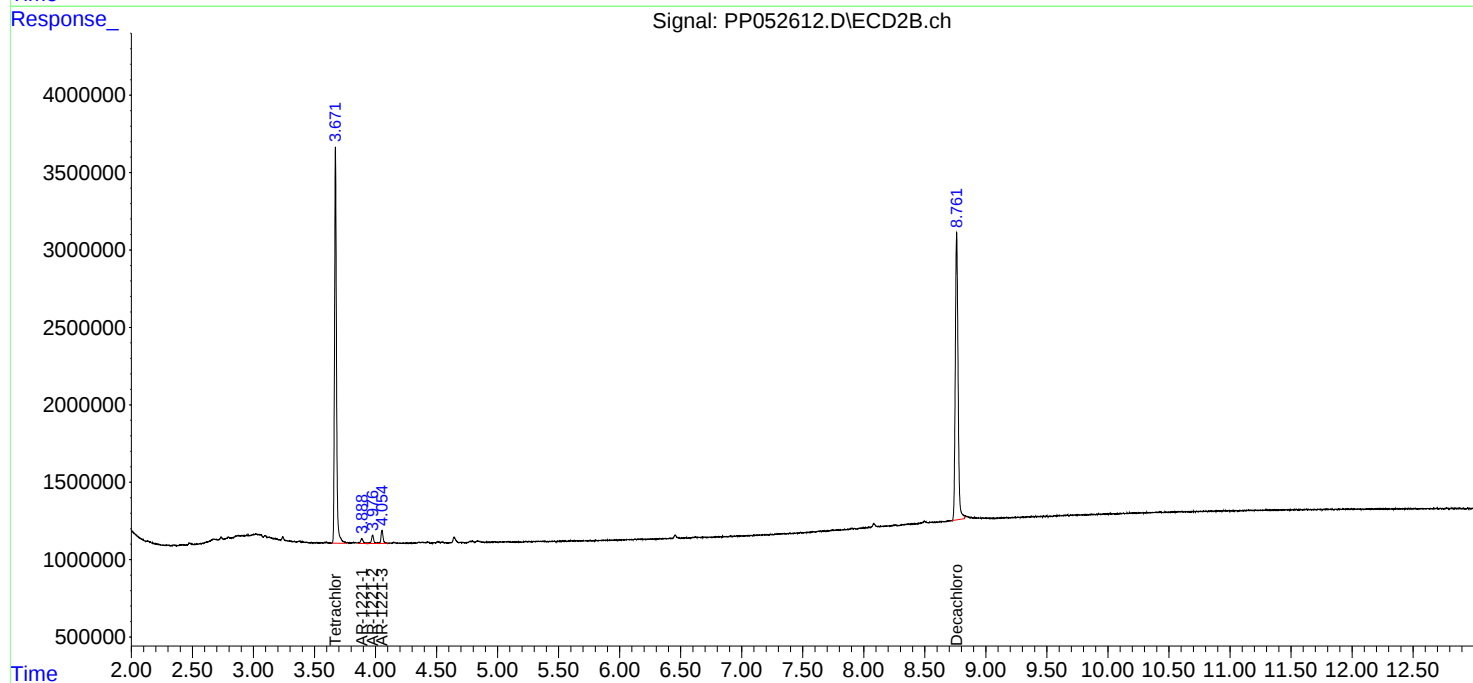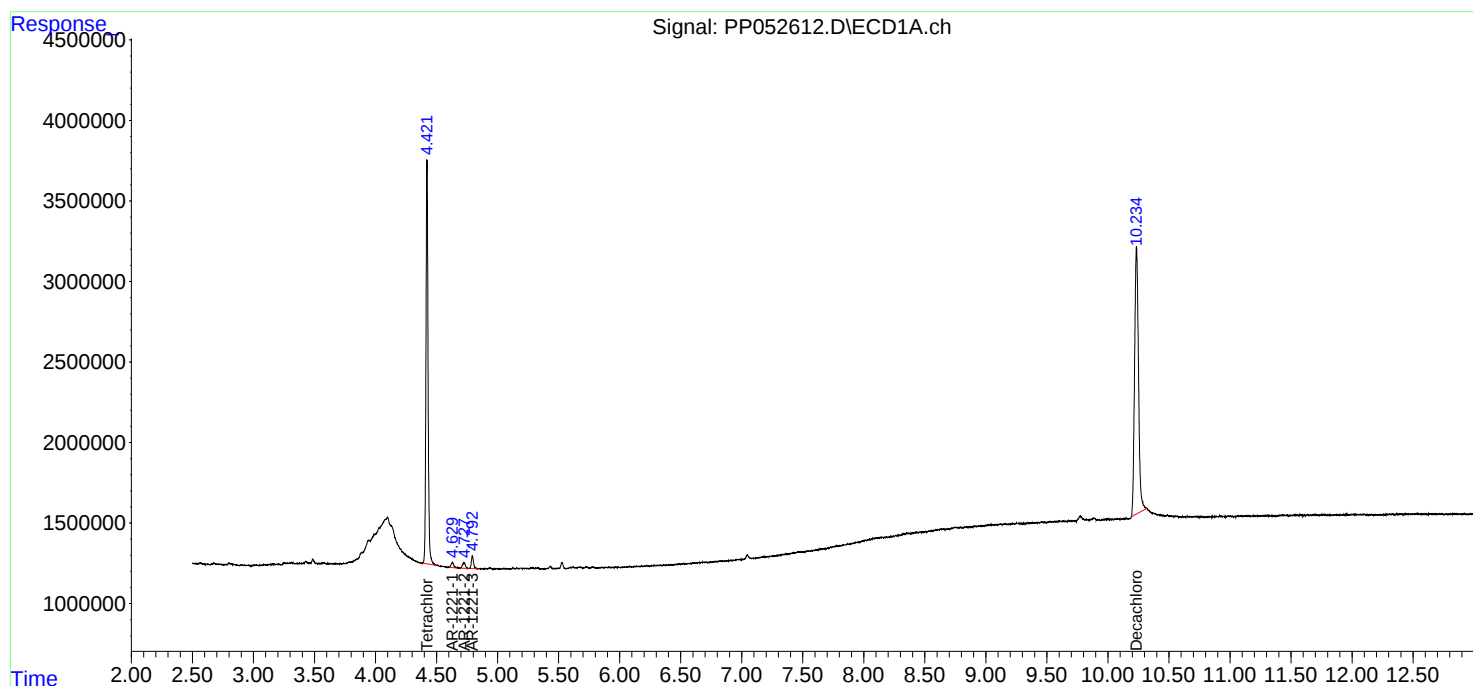


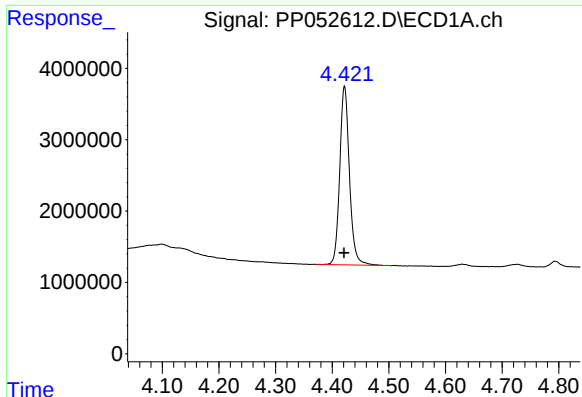

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 29847531
Conc: 18.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

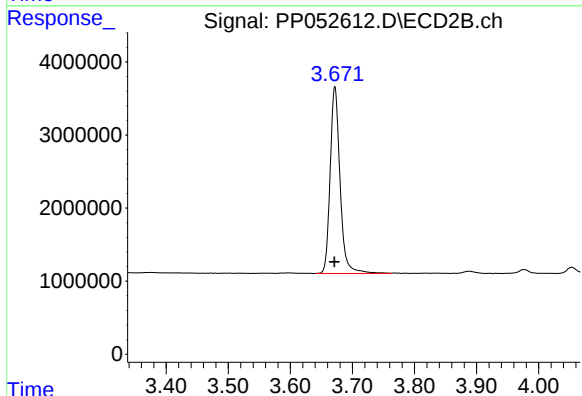


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 28310112
Conc: 21.25 ng/ml

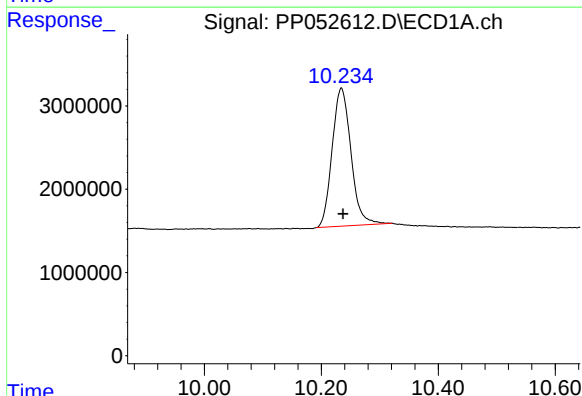


#2 Decachlorobiphenyl

R.T.: 10.234 min
Delta R.T.: -0.003 min
Response: 37008960
Conc: 23.09 ng/ml

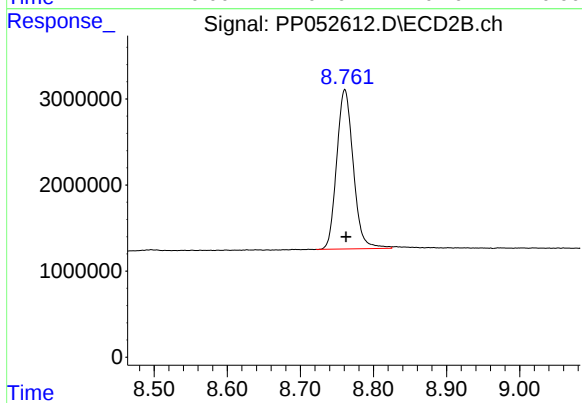

#2 Decachlorobiphenyl


R.T.: 8.761 min
Delta R.T.: -0.002 min
Response: 29168795
Conc: 23.47 ng/ml

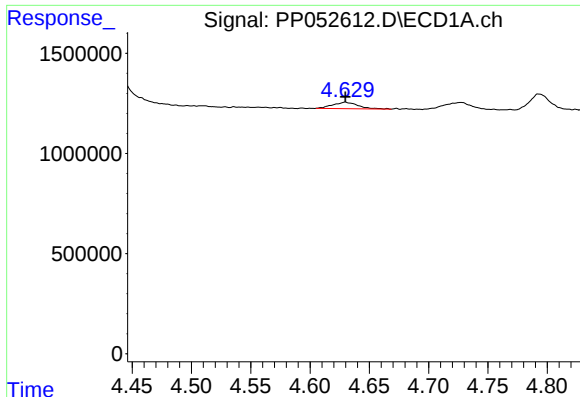

#8 AR-1221-1


R.T.: 4.630 min
Delta R.T.: 0.000 min
Response: 480302
Conc: 21.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

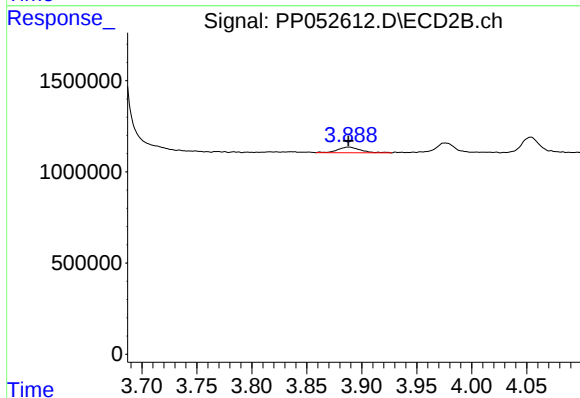


#8 AR-1221-1

R.T.: 3.888 min
Delta R.T.: 0.000 min
Response: 451305
Conc: 25.65 ng/ml

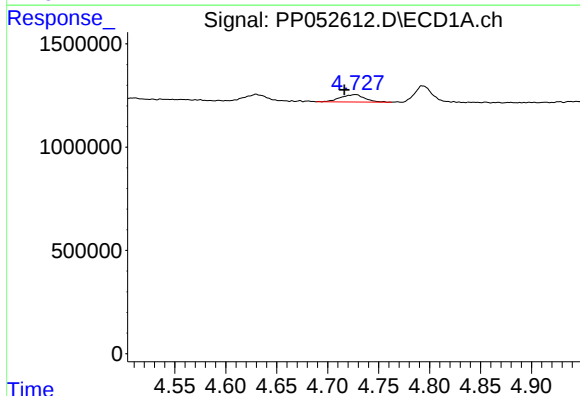


#9 AR-1221-2

R.T.: 4.727 min
Delta R.T.: 0.011 min
Response: 588710
Conc: 36.71 ng/ml

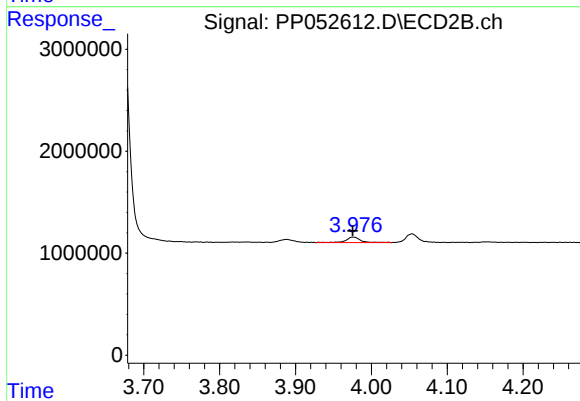

#9 AR-1221-2


R.T.: 3.976 min
Delta R.T.: 0.000 min
Response: 724081
Conc: 54.38 ng/ml

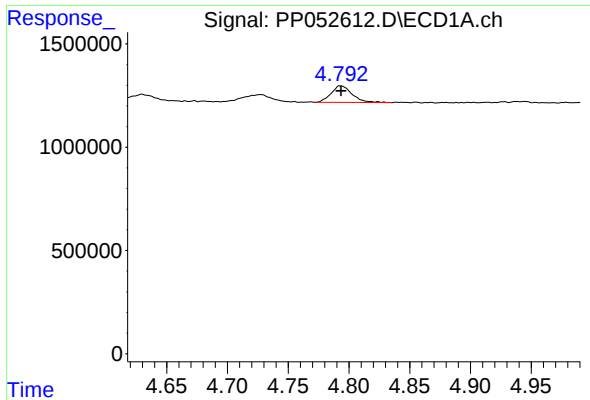

#10 AR-1221-3

R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 968173
Conc: 19.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

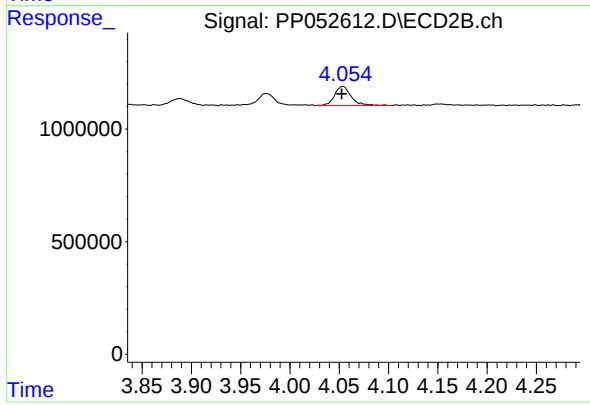

#10 AR-1221-3

R.T.: 4.054 min
Delta R.T.: 0.000 min
Response: 998868
Conc: 24.09 ng/ml