

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052613.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 11:08
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:54:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.422	3.672	30242374	28564580	18.279	21.439
2) SA Decachlor...	10.233	8.760	36759556	28934044	22.939	23.279
Target Compounds						
11) L3 AR-1232-1	4.794	4.053	793122	777253	21.363	24.513
12) L3 AR-1232-2	5.326	4.792	364356	552161	17.985	17.998
13) L3 AR-1232-3	5.618	4.972	708677	300768	23.320	18.716
14) L3 AR-1232-4	5.779	5.058	375151	255596	23.504	16.894 #
15) L3 AR-1232-5	5.869	5.230	357908	371581	26.433	21.751



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
Data File : PP052613.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 11:08
Operator : YP\AJ
Sample : N4955-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:54:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Oct 23 15:44:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

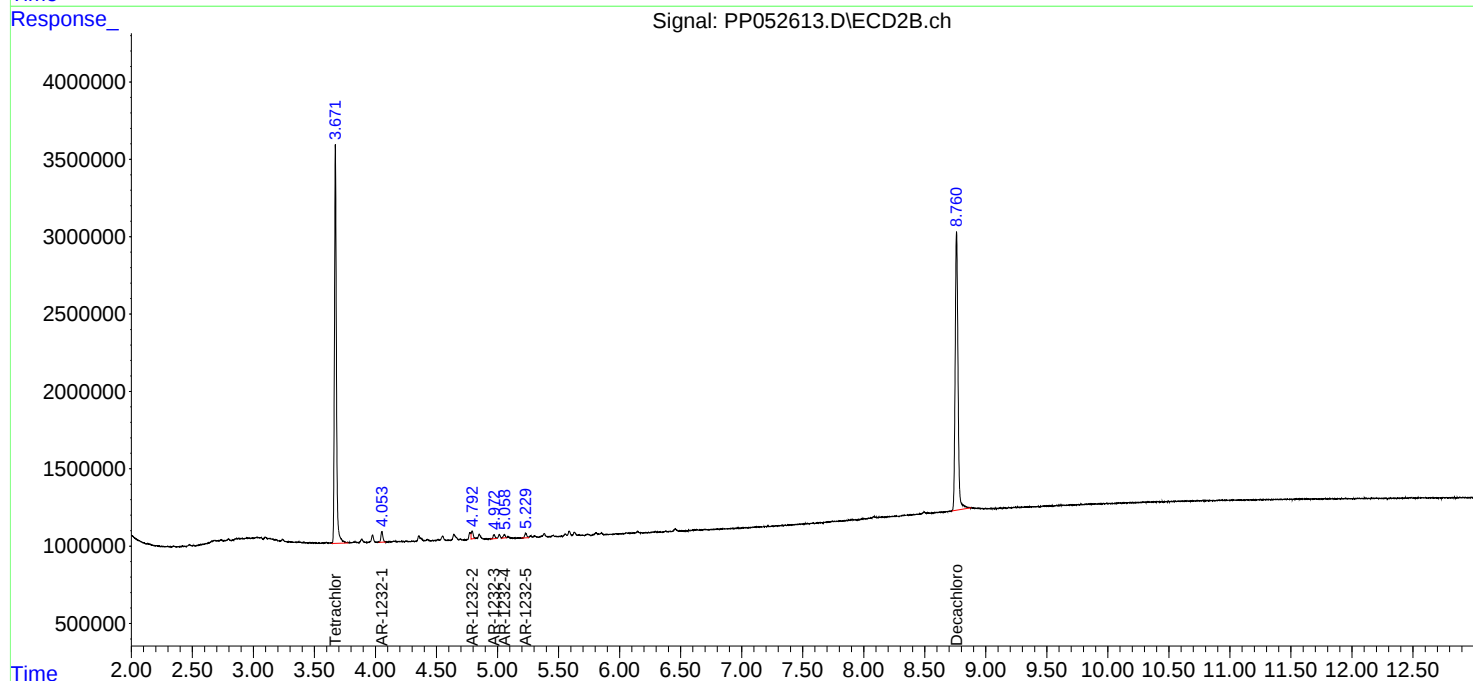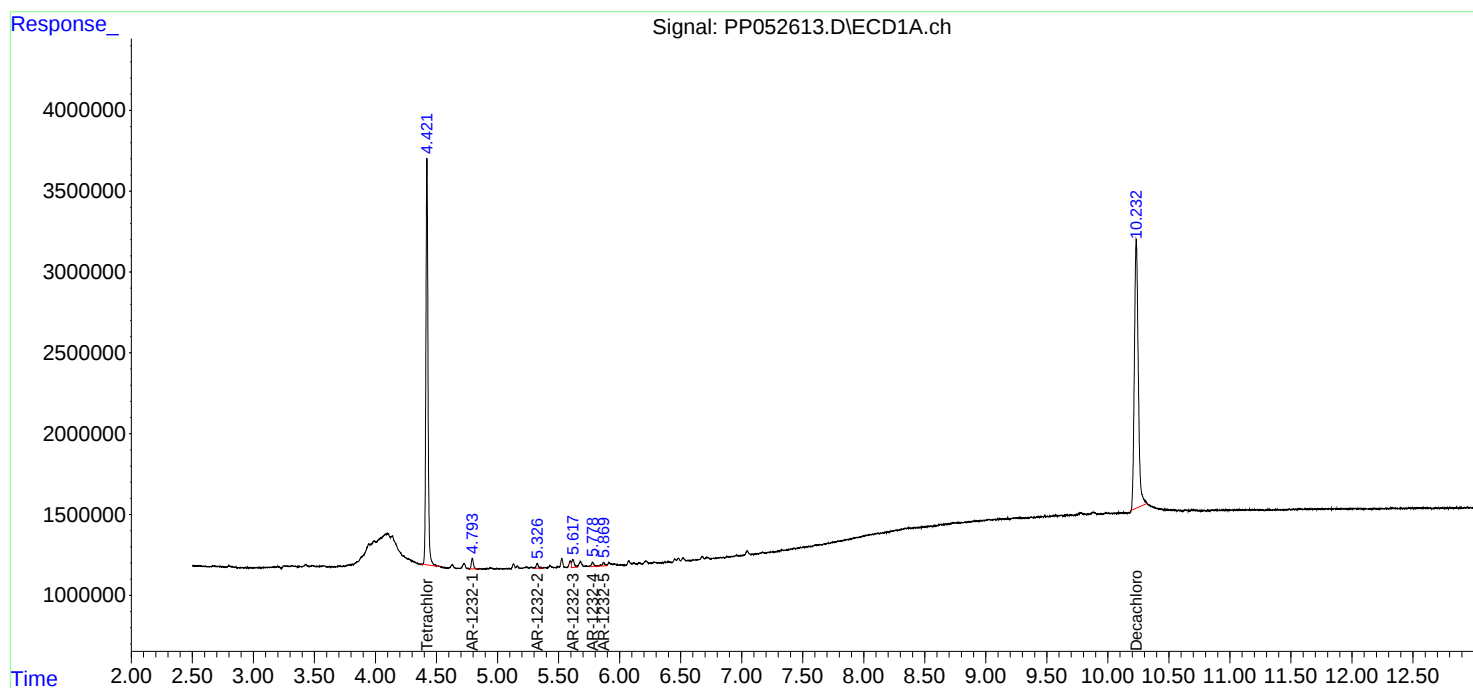


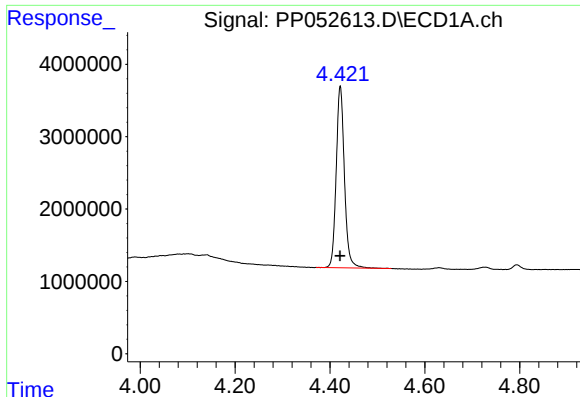

#1 Tetrachloro-m-xylene


R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 30242374
Conc: 18.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

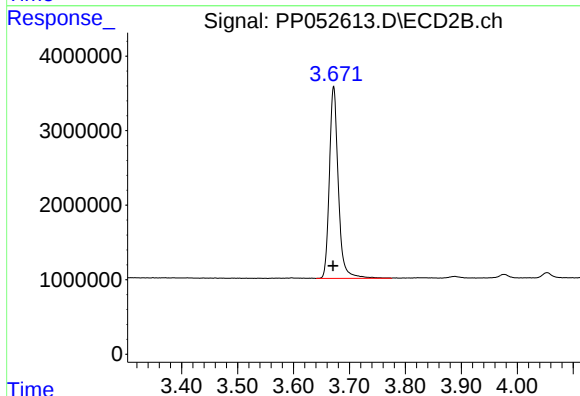


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.000 min
Response: 28564580
Conc: 21.44 ng/ml

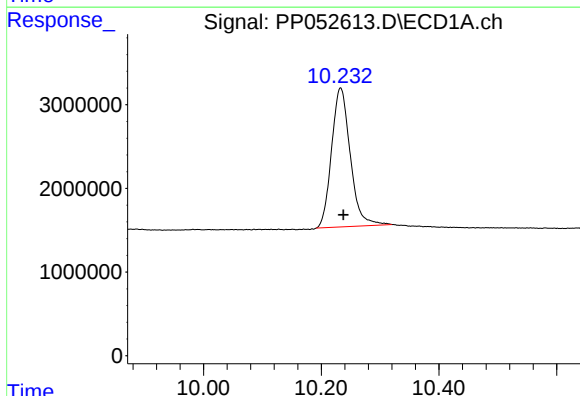


#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: -0.005 min
Response: 36759556
Conc: 22.94 ng/ml

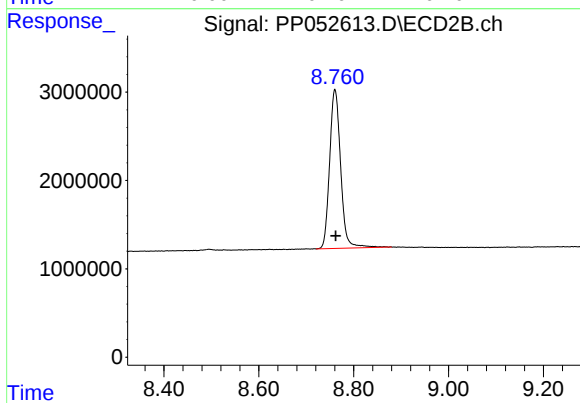

#2 Decachlorobiphenyl


R.T.: 8.760 min
Delta R.T.: -0.002 min
Response: 28934044
Conc: 23.28 ng/ml

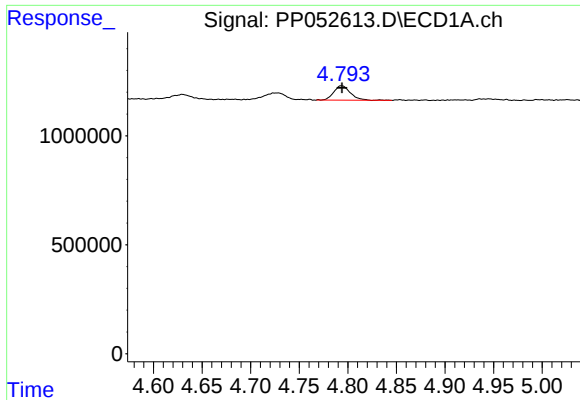

#11 AR-1232-1


R.T.: 4.794 min
Delta R.T.: 0.000 min
Response: 793122
Conc: 21.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

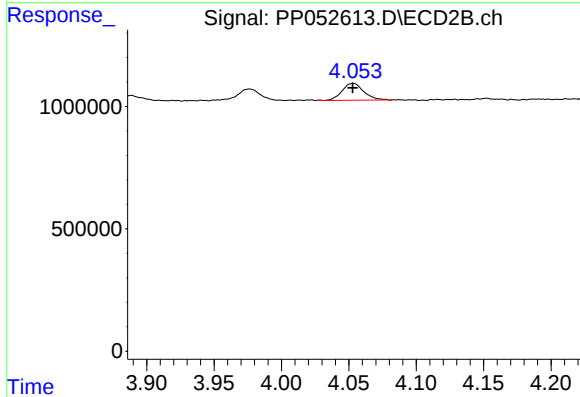


#11 AR-1232-1

R.T.: 4.053 min
Delta R.T.: 0.000 min
Response: 777253
Conc: 24.51 ng/ml

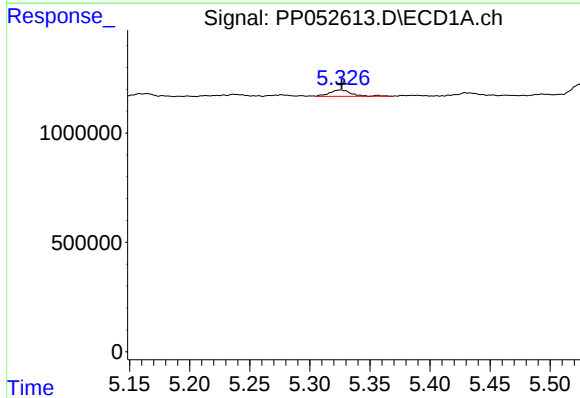


#12 AR-1232-2

R.T.: 5.326 min
Delta R.T.: -0.001 min
Response: 364356
Conc: 17.99 ng/ml

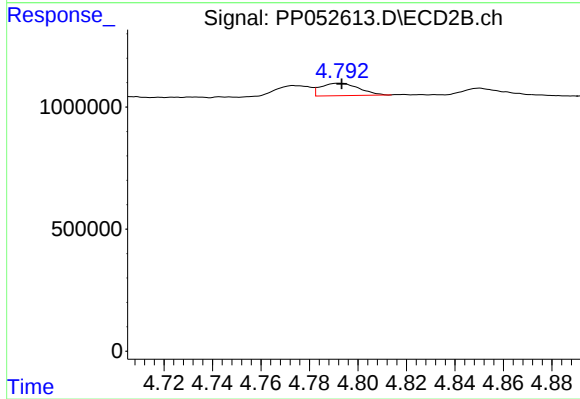

#12 AR-1232-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 552161
Conc: 18.00 ng/ml

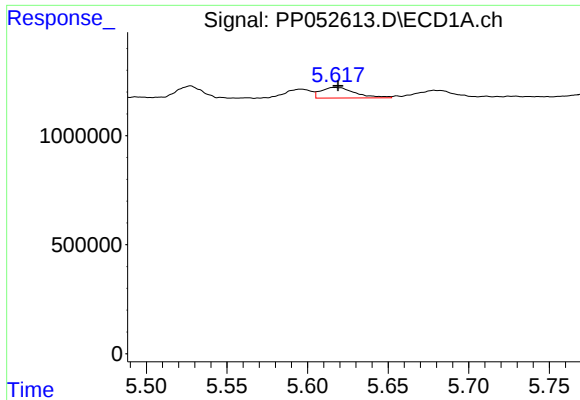

#13 AR-1232-3


R.T.: 5.618 min
Delta R.T.: -0.001 min
Response: 708677
Conc: 23.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

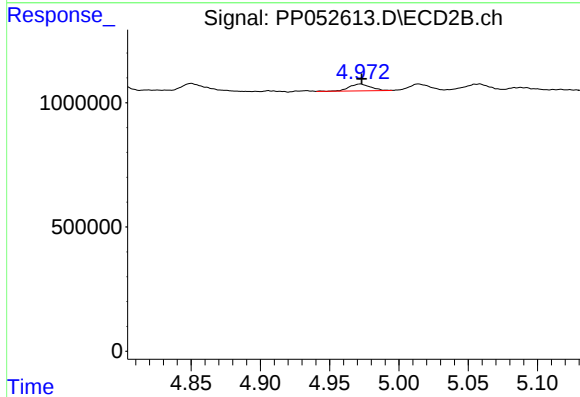


#13 AR-1232-3

R.T.: 4.972 min
Delta R.T.: -0.001 min
Response: 300768
Conc: 18.72 ng/ml

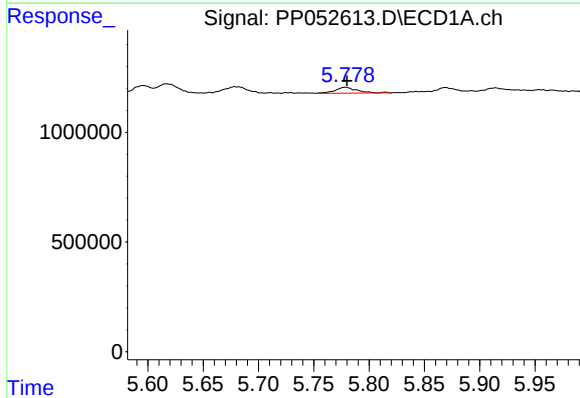


#14 AR-1232-4

R.T.: 5.779 min
Delta R.T.: -0.001 min
Response: 375151
Conc: 23.50 ng/ml

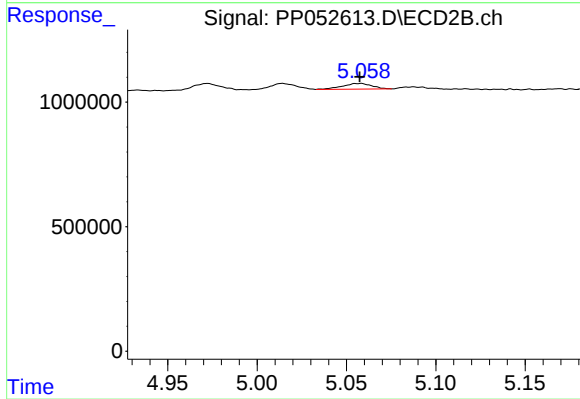

#14 AR-1232-4


R.T.: 5.058 min
Delta R.T.: 0.000 min
Response: 255596
Conc: 16.89 ng/ml

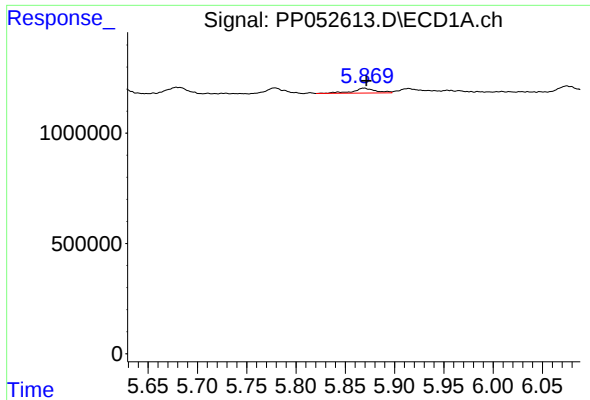

#15 AR-1232-5

R.T.: 5.869 min
Delta R.T.: -0.002 min
Response: 357908
Conc: 26.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

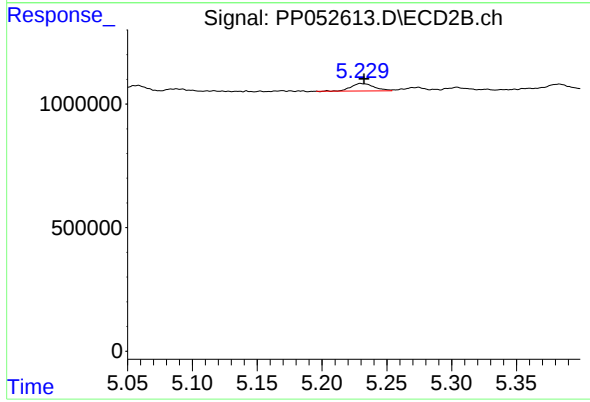

#15 AR-1232-5

R.T.: 5.230 min
Delta R.T.: -0.002 min
Response: 371581
Conc: 21.75 ng/ml