

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 17:44
 Operator : YP\AJ
 Sample : N4955-07
 Misc : AR1254 LOD 40 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 23:06:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.423	3.672	27366975	28090940	16.541	21.083 #
2) SA Decachlor...	10.235	8.760	31843196	28641324	19.871	23.044
Target Compounds						
26) L6 AR-1254-1	6.455	5.588	1735298	2450247	27.805	33.828
27) L6 AR-1254-2	6.674	5.738	2653740	2136792	27.630	33.273
28) L6 AR-1254-3	7.042	6.147	2600084	3118928	27.810	31.504
29) L6 AR-1254-4	7.329	6.379	1529248	1431105	24.762	27.779
30) L6 AR-1254-5	7.749	6.800	1958611	2461858	25.832	29.534



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
Data File : PP052637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 17:44
Operator : YP\AJ
Sample : N4955-07
Misc : AR1254 LOD 40 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 23:06:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Oct 23 15:44:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

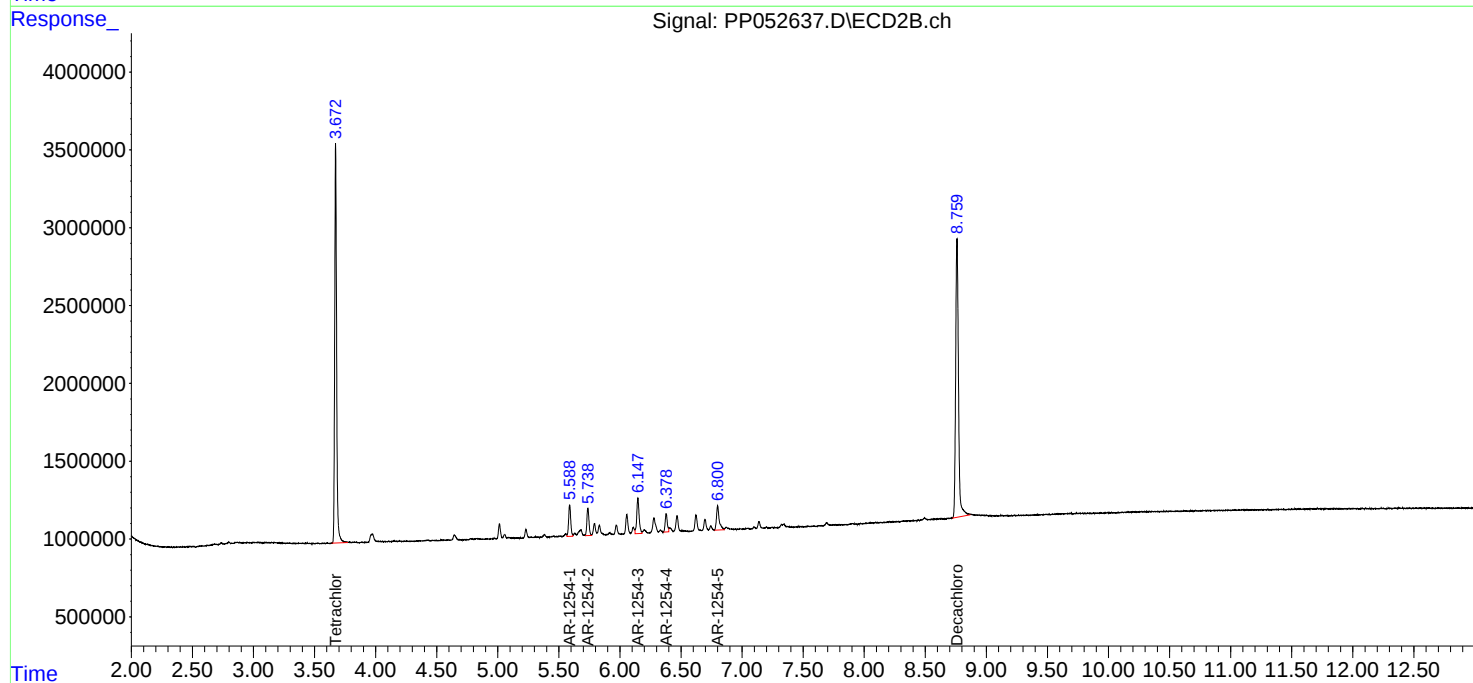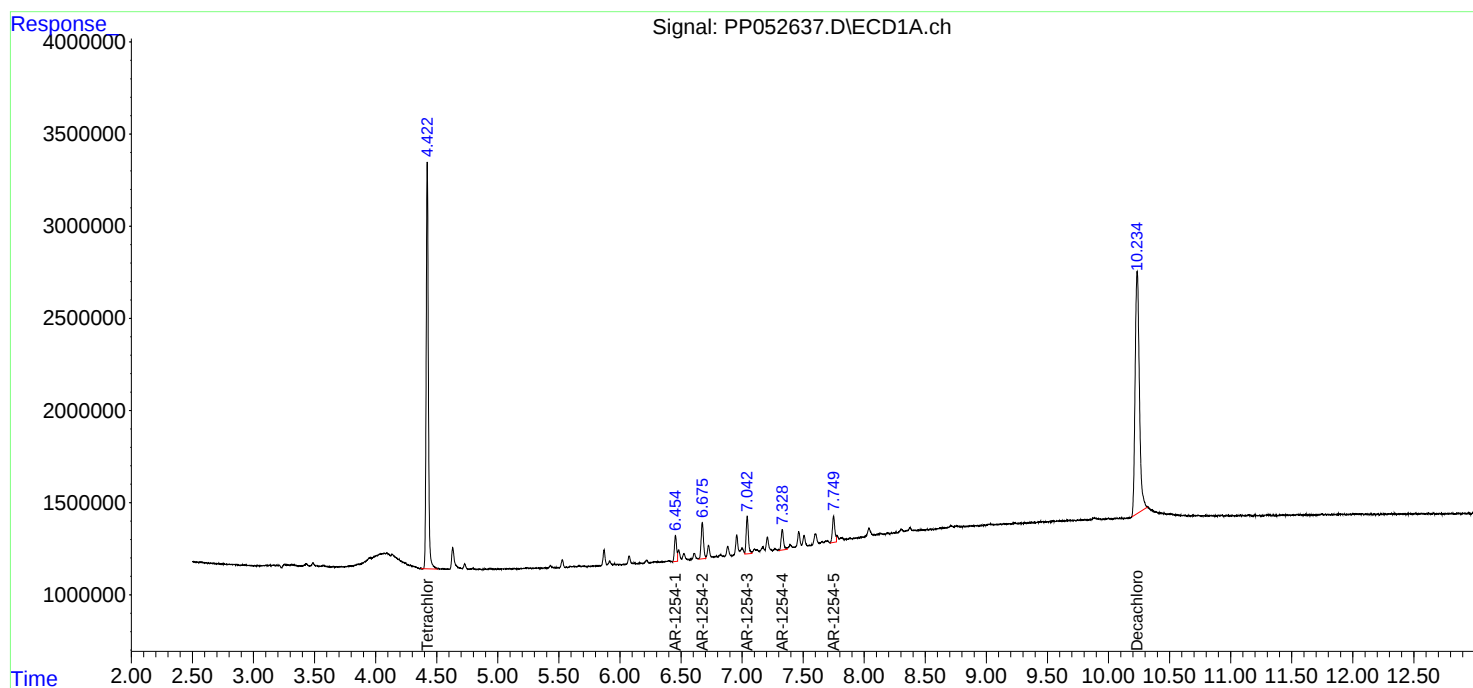


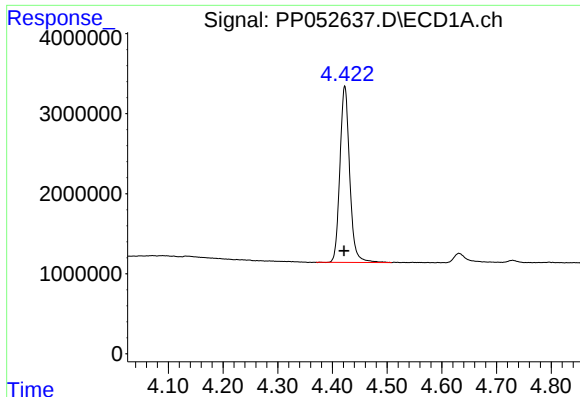

#1 Tetrachloro-m-xylene


R.T.: 4.423 min
Delta R.T.: 0.002 min
Response: 27366975
Conc: 16.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

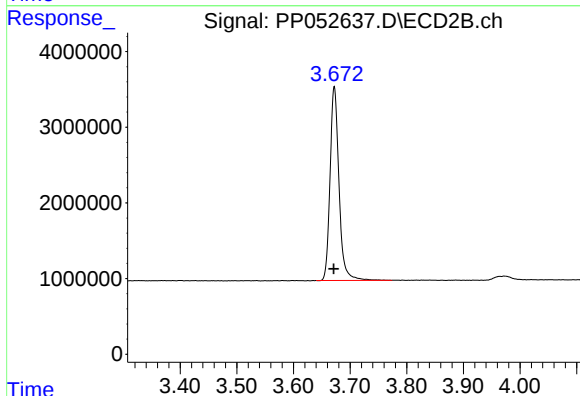


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: 0.001 min
Response: 28090940
Conc: 21.08 ng/ml

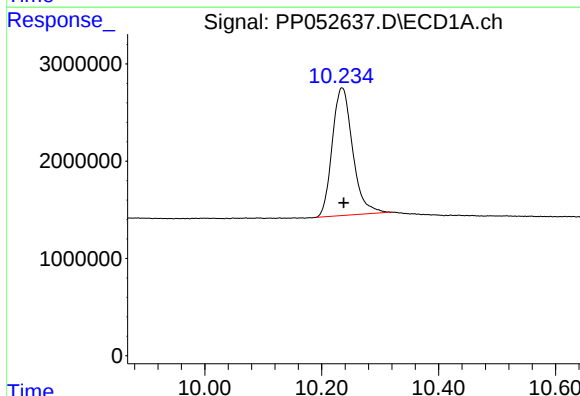


#2 Decachlorobiphenyl

R.T.: 10.235 min
Delta R.T.: -0.003 min
Response: 31843196
Conc: 19.87 ng/ml

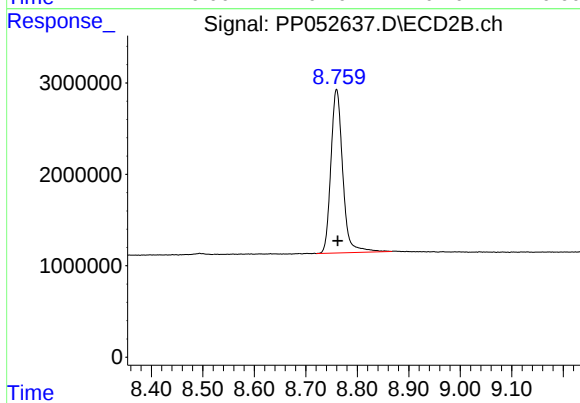

#2 Decachlorobiphenyl


R.T.: 8.760 min
Delta R.T.: -0.003 min
Response: 28641324
Conc: 23.04 ng/ml

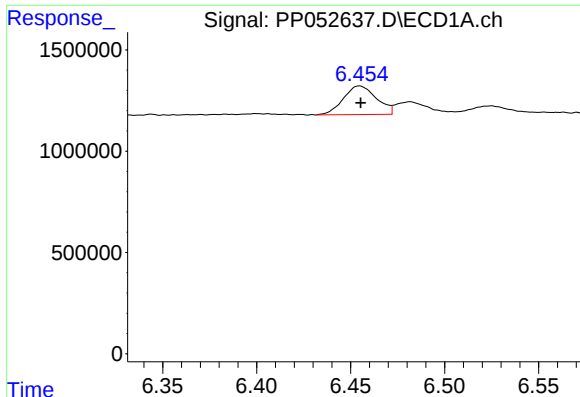

#26 AR-1254-1


R.T.: 6.455 min
Delta R.T.: 0.000 min
Response: 1735298
Conc: 27.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

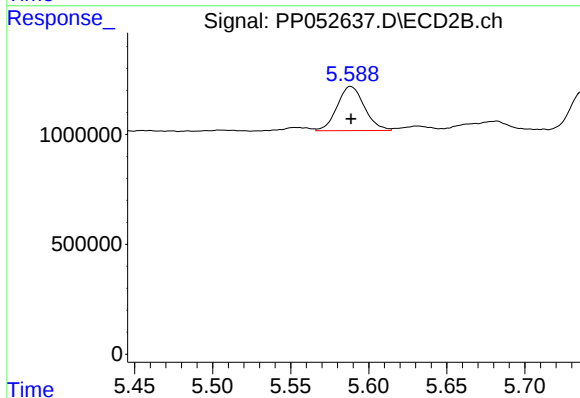


#26 AR-1254-1

R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 2450247
Conc: 33.83 ng/ml

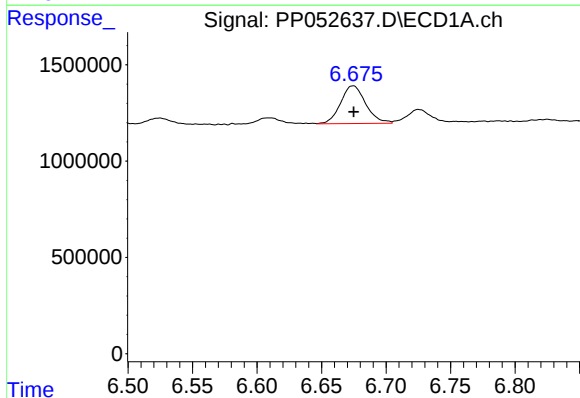


#27 AR-1254-2

R.T.: 6.674 min
Delta R.T.: 0.000 min
Response: 2653740
Conc: 27.63 ng/ml

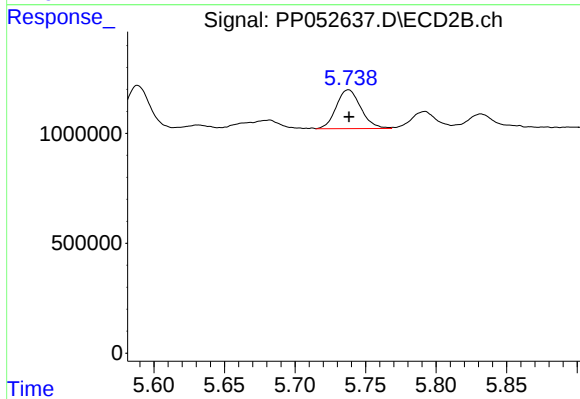

#27 AR-1254-2


R.T.: 5.738 min
Delta R.T.: 0.000 min
Response: 2136792
Conc: 33.27 ng/ml

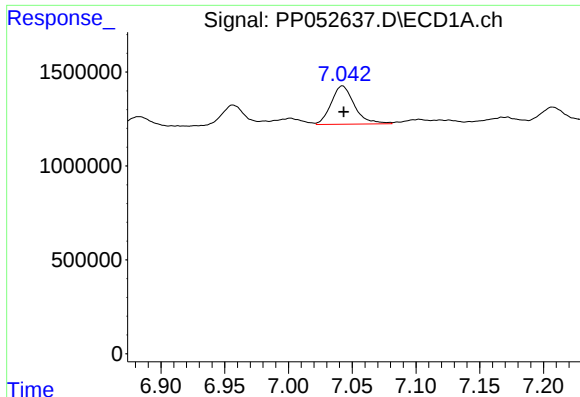

#28 AR-1254-3


R.T.: 7.042 min
Delta R.T.: -0.001 min
Response: 2600084
Conc: 27.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

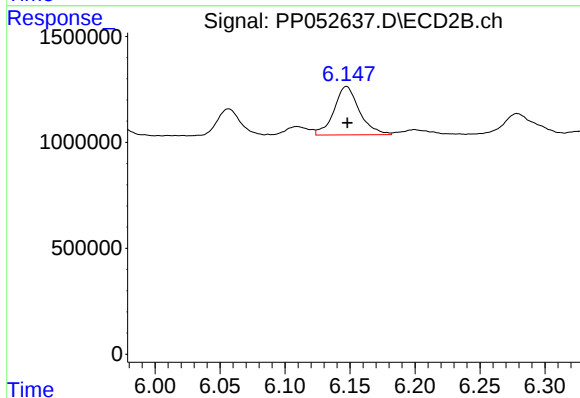


#28 AR-1254-3

R.T.: 6.147 min
Delta R.T.: 0.000 min
Response: 3118928
Conc: 31.50 ng/ml

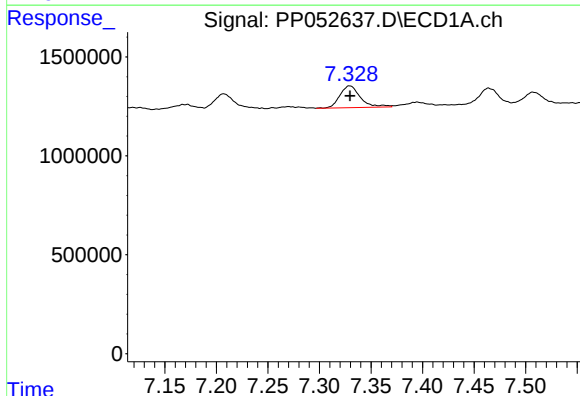


#29 AR-1254-4

R.T.: 7.329 min
Delta R.T.: 0.000 min
Response: 1529248
Conc: 24.76 ng/ml

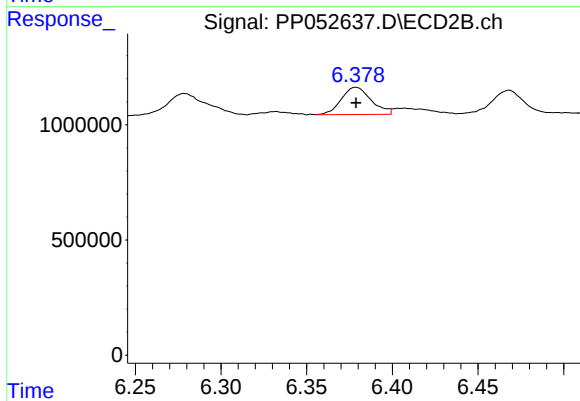

#29 AR-1254-4


R.T.: 6.379 min
Delta R.T.: 0.000 min
Response: 1431105
Conc: 27.78 ng/ml

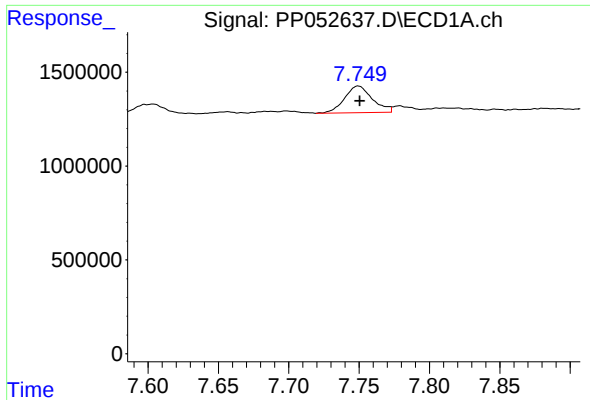

#30 AR-1254-5

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 1958611
Conc: 25.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT4-2022

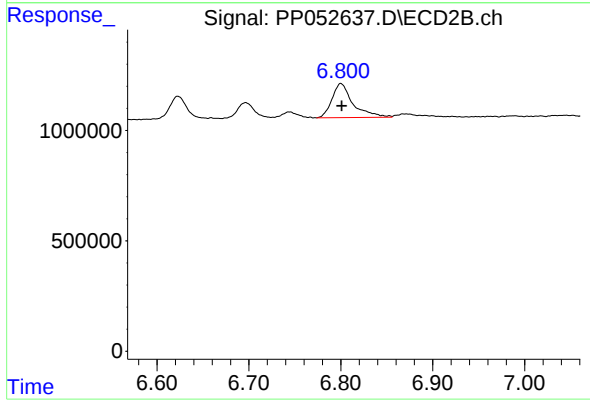

#30 AR-1254-5

R.T.: 6.800 min
Delta R.T.: 0.000 min
Response: 2461858
Conc: 29.53 ng/ml