

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
 Data File : PP052684.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2022 06:42
 Operator : YP\AJ
 Sample : N5253-03
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 124055

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/25/2022
 Supervised By :Ankita Jodhani 10/25/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 11:04:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sun Oct 23 15:44:19 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.671	16699277	16930928	10.094	12.707 #
2) SA Decachlor...	10.233	8.760	8866082	7874896	5.533	6.336m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102422\
Data File : PP052684.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2022 06:42
Operator : YP\AJ
Sample : N5253-03
Misc :
ALS Vial : 63 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
124055


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 11:04:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102122.M
Quant Title : GC EXTRACTABLES
QLast Update : Sun Oct 23 15:44:19 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

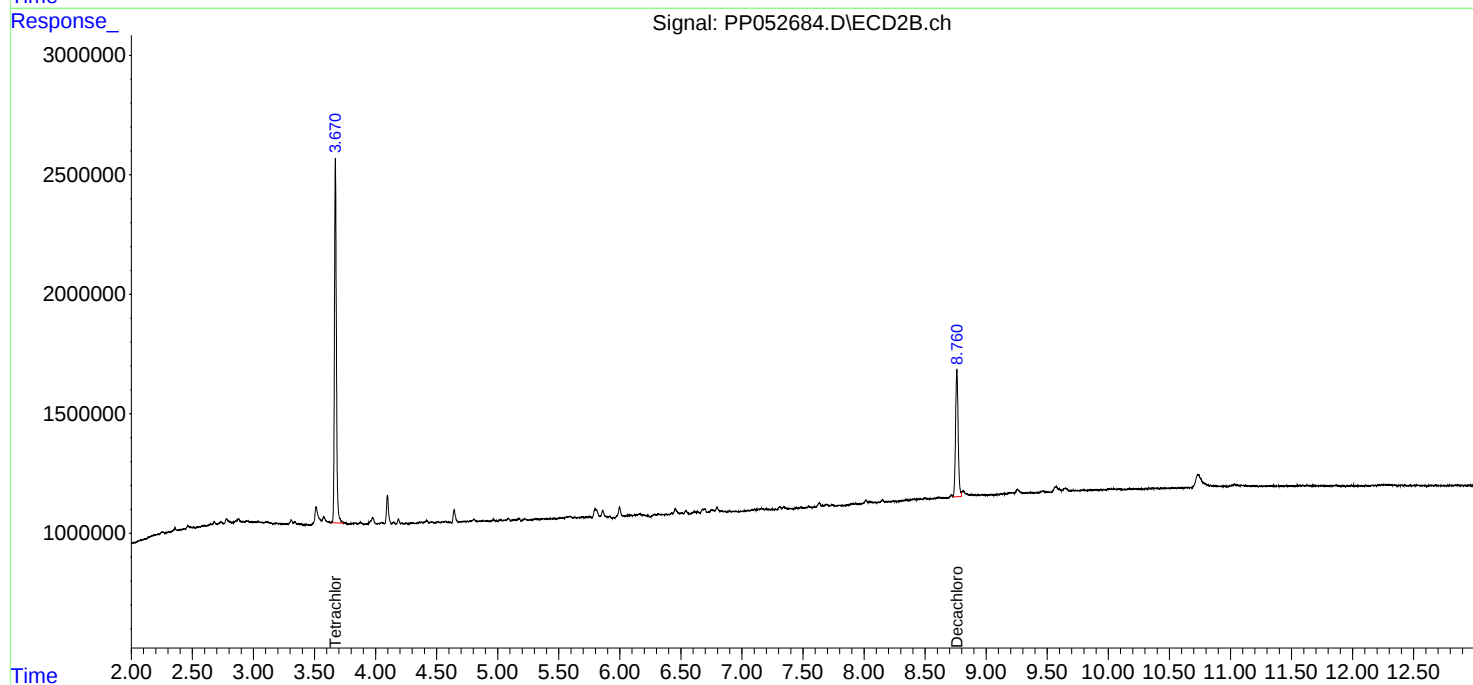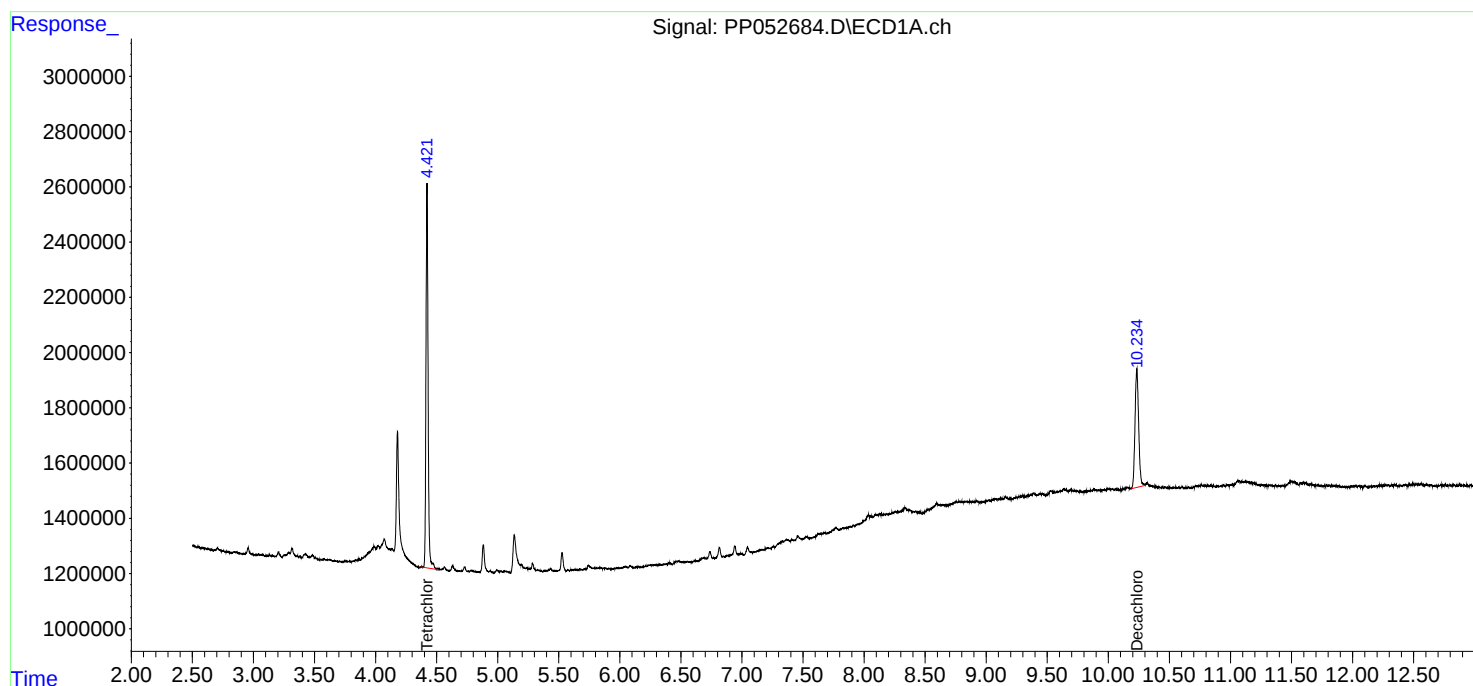

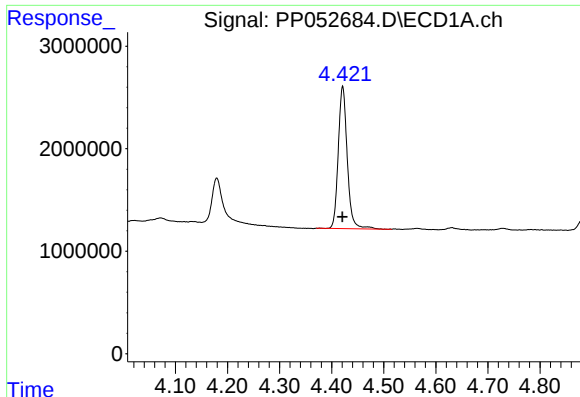


#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: 0.000 min
Response: 16699277
Conc: 10.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
124055


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2022
Supervised By :Ankita Jodhani 10/25/2022

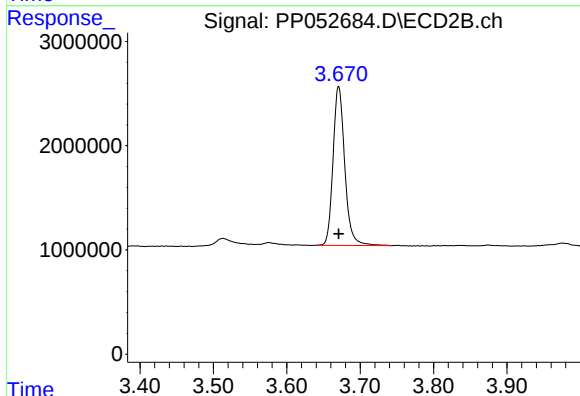


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: 0.000 min
Response: 16930928
Conc: 12.71 ng/ml

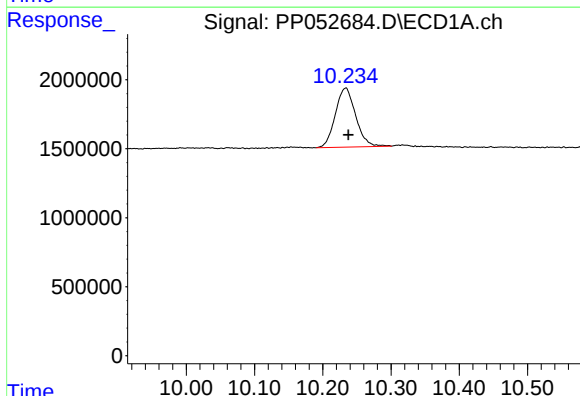

#2 Decachlorobiphenyl

R.T.: 10.233 min
Delta R.T.: -0.004 min
Response: 8866082
Conc: 5.53 ng/ml

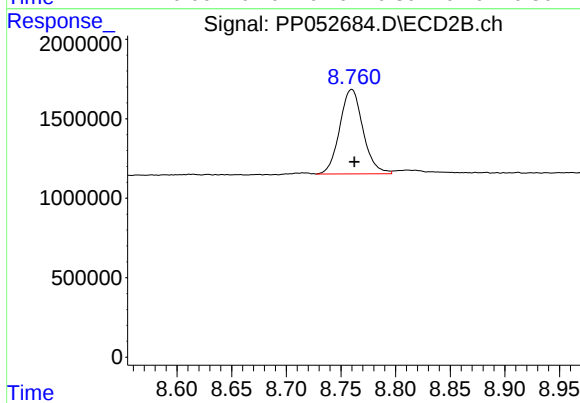

#2 Decachlorobiphenyl

R.T.: 8.760 min
Delta R.T.: -0.003 min
Response: 7874896
Conc: 6.34 ng/ml m