

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102423\
 Data File : PP061212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 11:47
 Operator : YP\AJ
 Sample : 04909-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LCOL-12RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/25/2023
 Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 12:23:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.567	3.699	114.3E6	23814966	51.996m	17.615m#
2) SA Decachlor...	10.515	8.767	25407178	12164244	16.224m	8.090m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102423\
Data File : PP061212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 11:47
Operator : YP\AJ
Sample : 04909-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LCOL-12RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 12:23:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

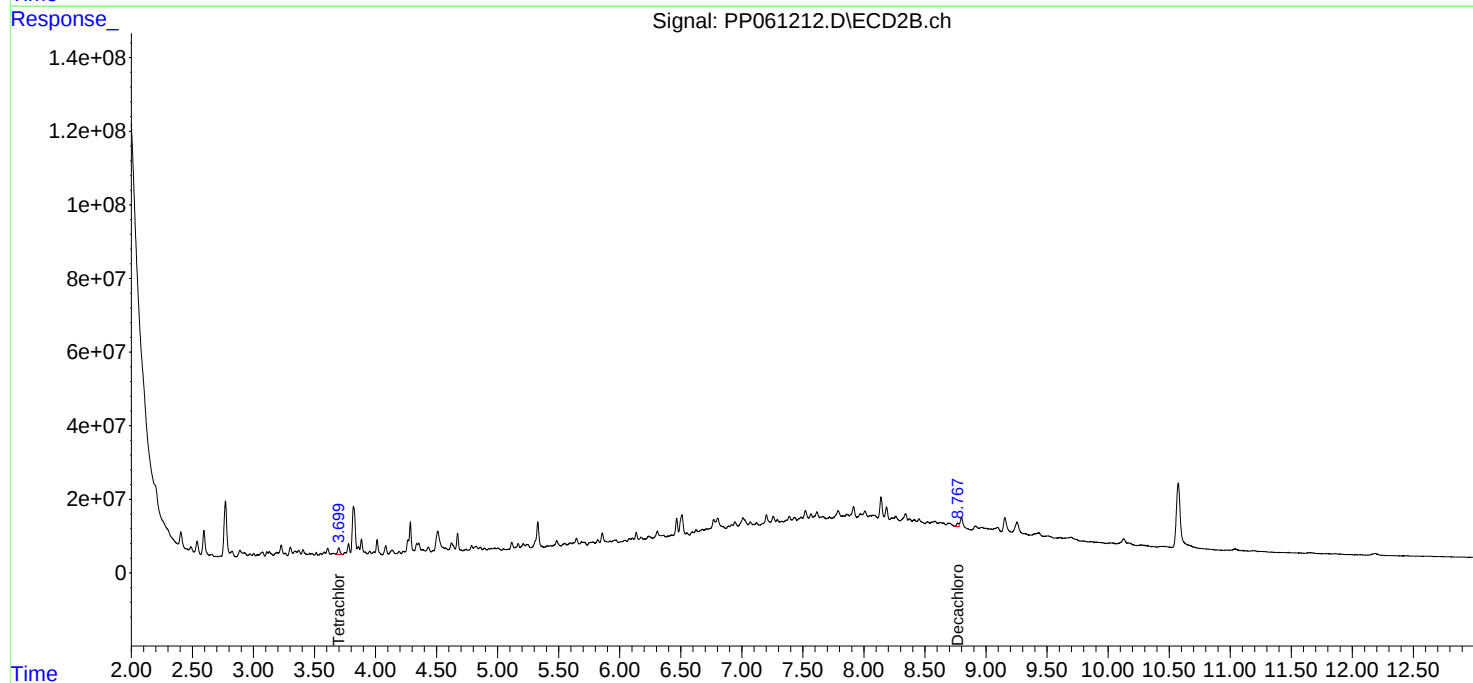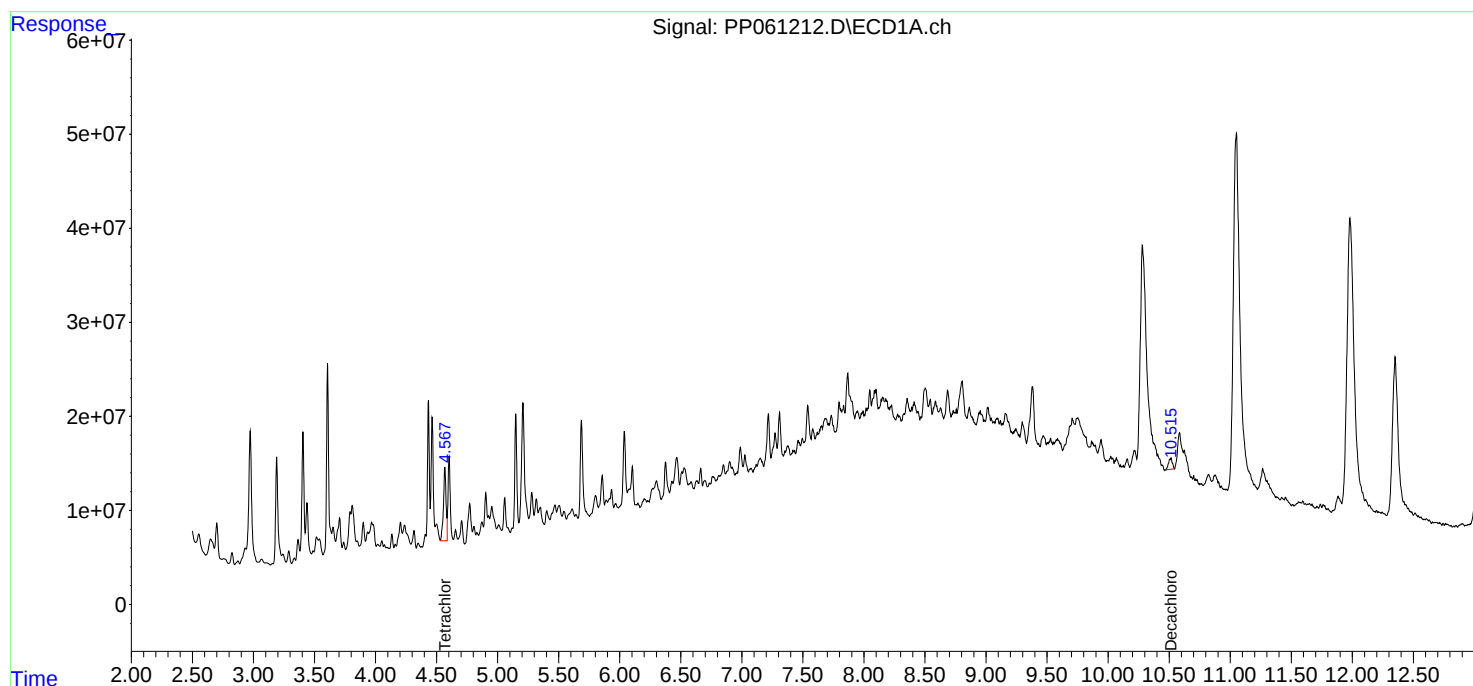

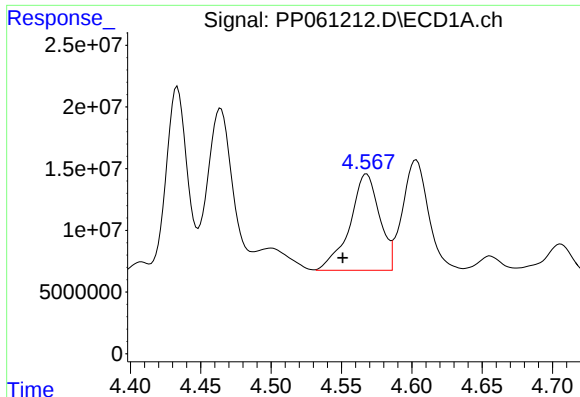

#1 Tetrachloro-m-xylene

R.T.: 4.567 min
Delta R.T.: 0.016 min
Response: 114305532
Conc: 52.00 ng/ml

Instrument :

ECD_P


ClientSampleId :

LCOL-12RE

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

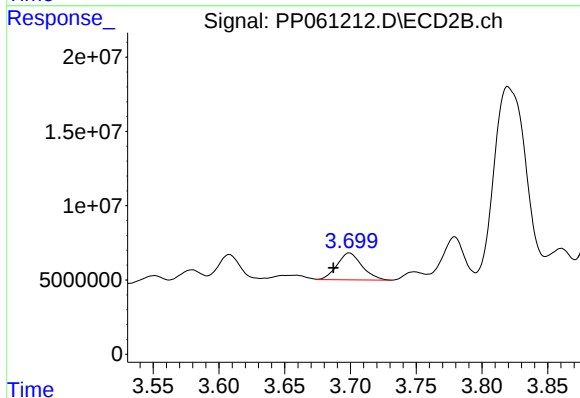


#1 Tetrachloro-m-xylene

R.T.: 3.699 min
Delta R.T.: 0.012 min
Response: 23814966
Conc: 17.61 ng/ml m

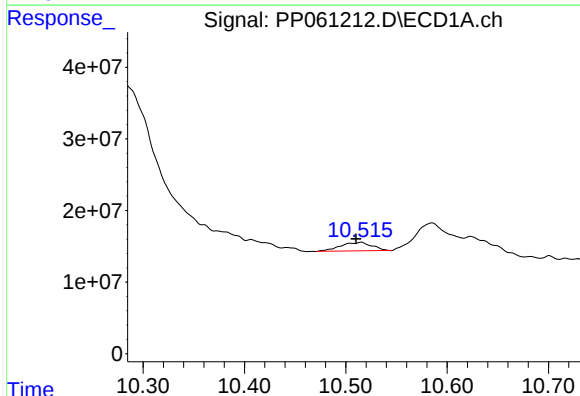

#2 Decachlorobiphenyl

R.T.: 10.515 min
Delta R.T.: 0.005 min
Response: 25407178
Conc: 16.22 ng/ml m

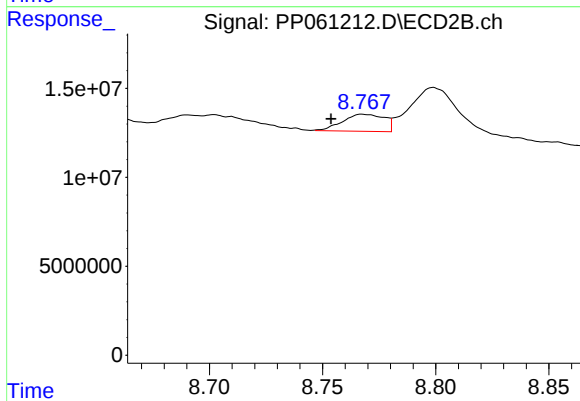

#2 Decachlorobiphenyl

R.T.: 8.767 min
Delta R.T.: 0.013 min
Response: 12164244
Conc: 8.09 ng/ml m