

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102423\
 Data File : PP061227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 18:13
 Operator : YP\AJ
 Sample : 05012-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BU-03-10232023

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/25/2023
 Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:16:50 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Oct 14 13:32:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.561	3.696	42410895	27006667	19.292	19.975
2) SA Decachlor...	10.532	8.766	32605046	24064972	20.821m	16.006

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102423\
Data File : PP061227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 18:13
Operator : YP\AJ
Sample : 05012-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BU-03-10232023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:16:50 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP101323.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Oct 14 13:32:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

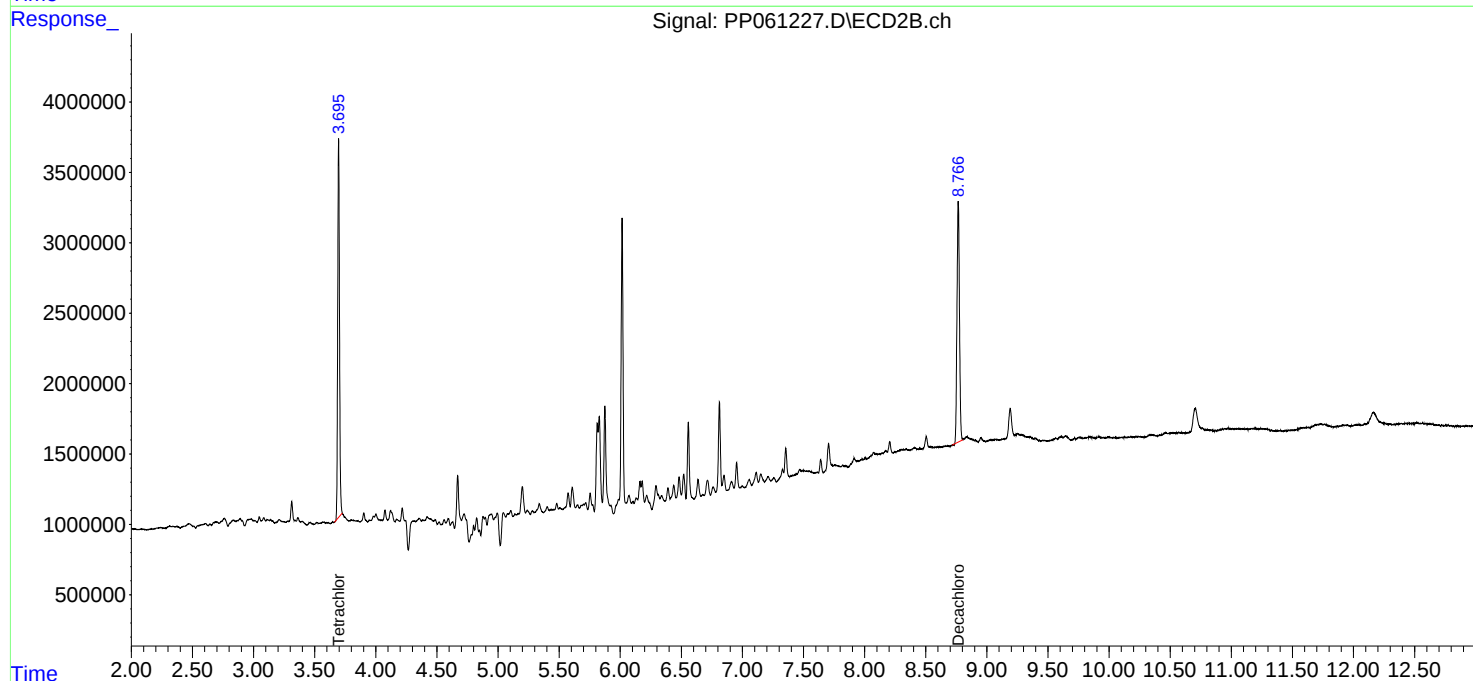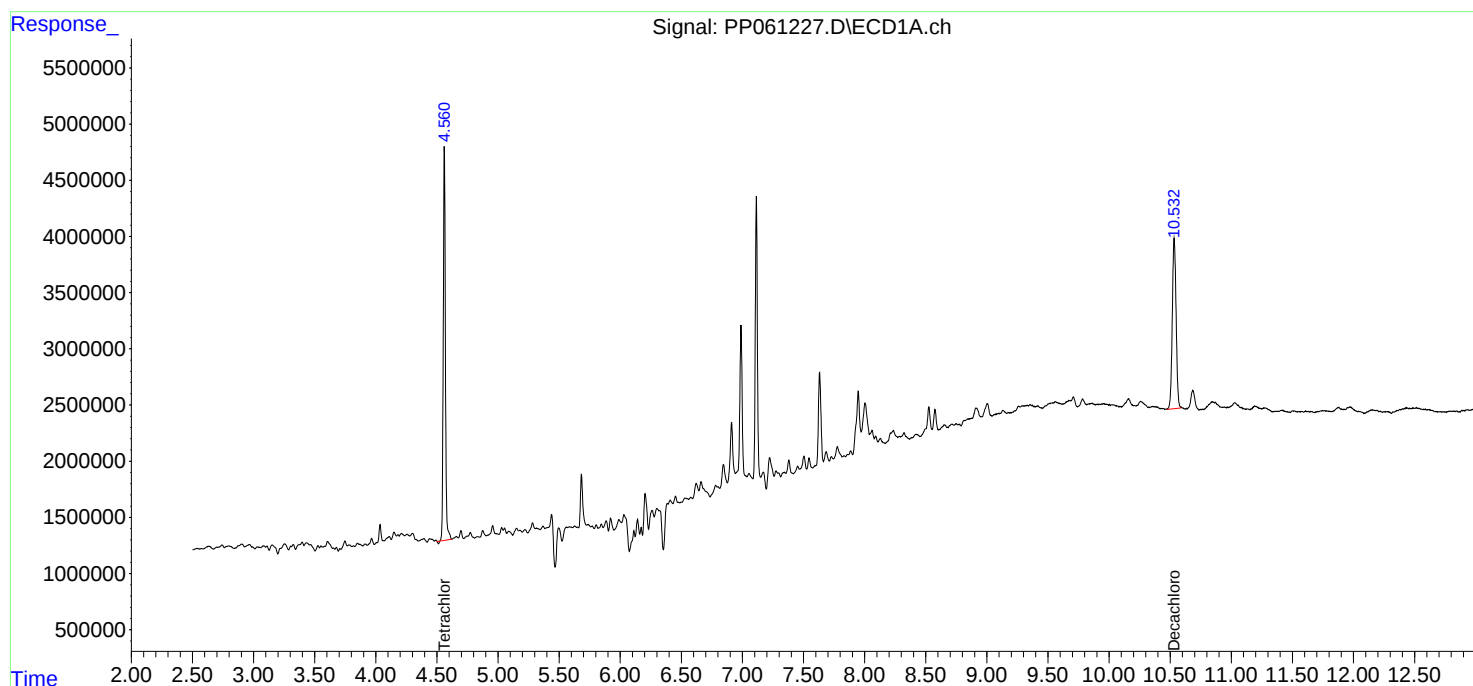

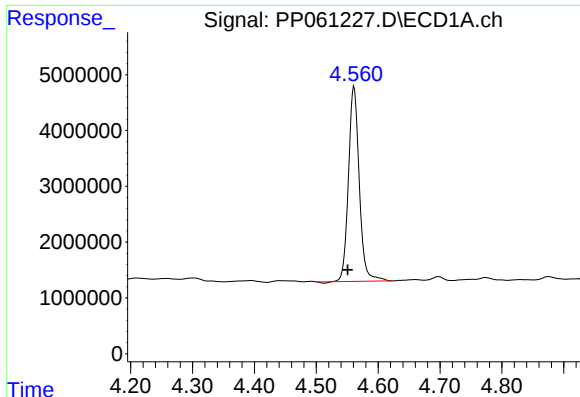


#1 Tetrachloro-m-xylene

R.T.: 4.561 min
Delta R.T.: 0.010 min
Response: 42410895
Conc: 19.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
BU-03-10232023


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

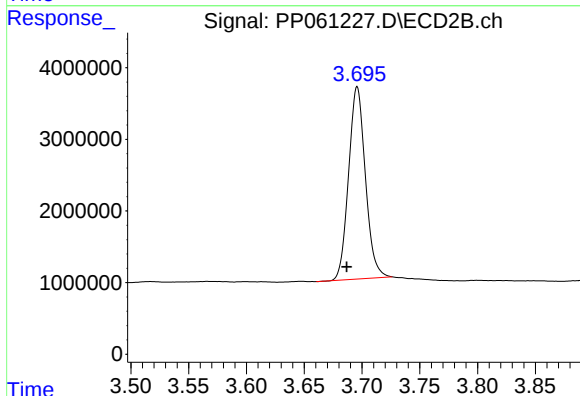


#1 Tetrachloro-m-xylene

R.T.: 3.696 min
Delta R.T.: 0.009 min
Response: 27006667
Conc: 19.98 ng/ml

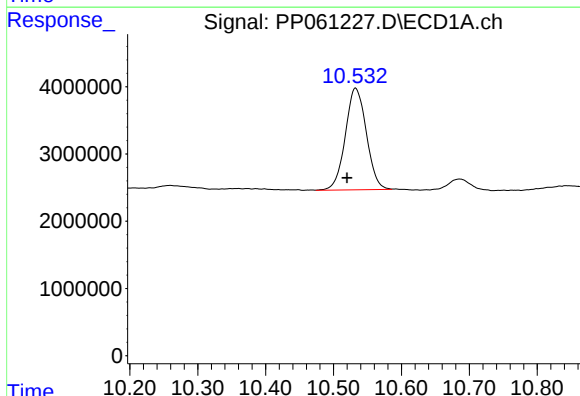

#2 Decachlorobiphenyl

R.T.: 10.532 min
Delta R.T.: 0.012 min
Response: 32605046
Conc: 20.82 ng/ml m

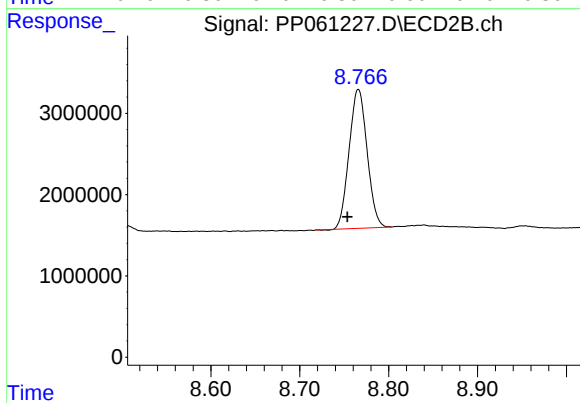

#2 Decachlorobiphenyl

R.T.: 8.766 min
Delta R.T.: 0.012 min
Response: 24064972
Conc: 16.01 ng/ml