

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102424\
 Data File : PP068202.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 13:46
 Operator : YP\AJ
 Sample : P4510-07 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FDA886K-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/25/2024
 Supervised By :Ankita Jodhani 10/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:41:08 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	4.050	1217414	1029840	1.315	1.019
2) SA Decachlor...	10.670	9.209	1475563	1264465	1.282	1.128m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102424\
Data File : PP068202.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 13:46
Operator : YP\AJ
Sample : P4510-07 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FDA886K-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:41:08 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

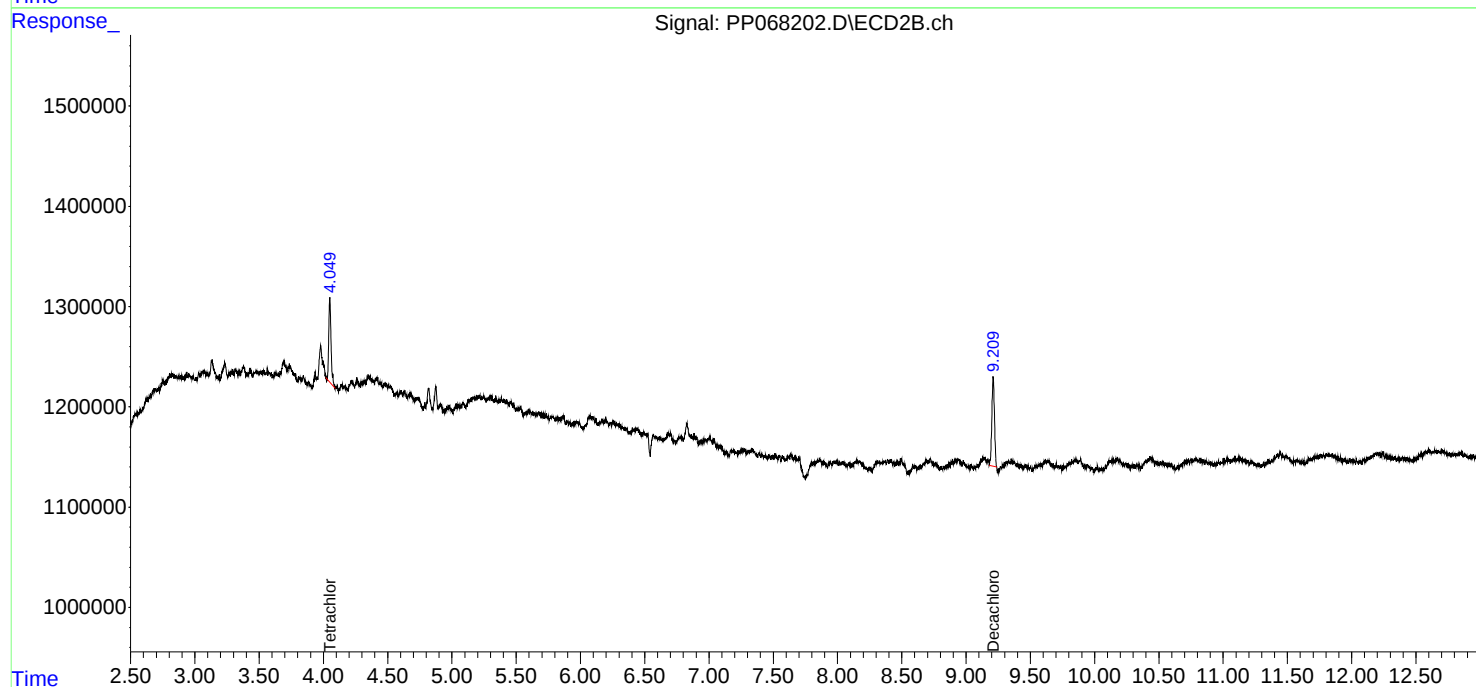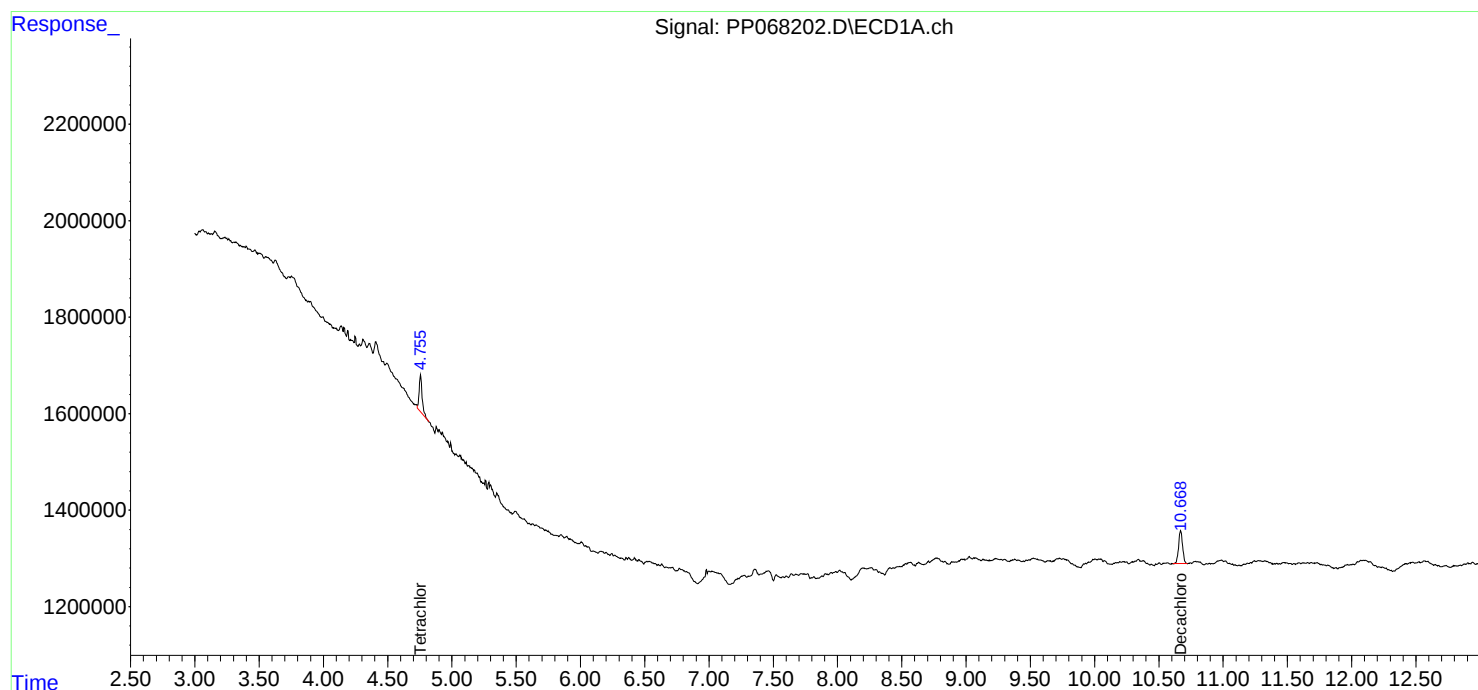

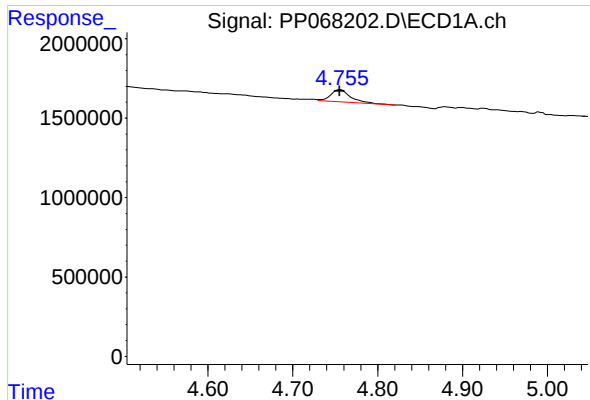

#1 Tetrachloro-m-xylene

R.T.: 4.756 min
Delta R.T.: 0.001 min
Response: 1217414
Conc: 1.32 ng/ml

Instrument :

ECD_P


ClientSampleId :

FDA886K-1-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

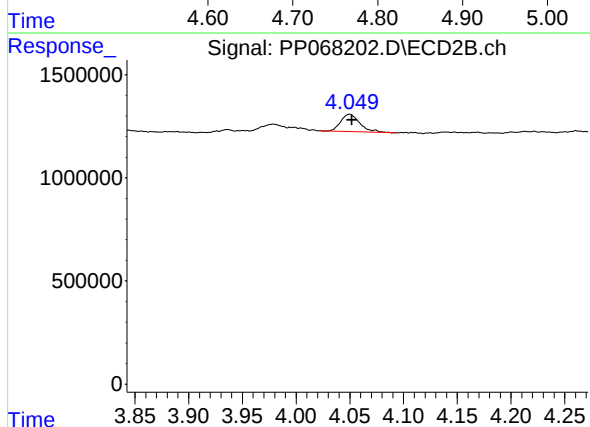


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 1029840
Conc: 1.02 ng/ml

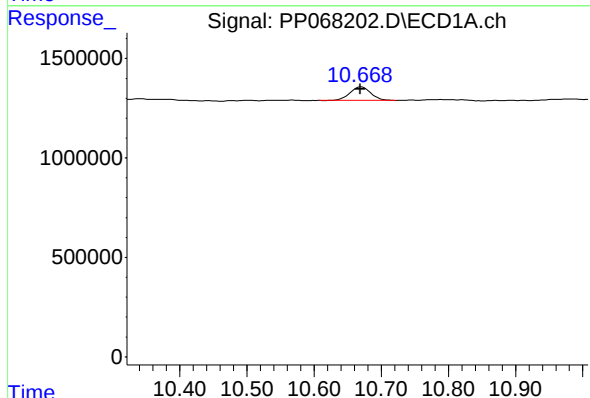

#2 Decachlorobiphenyl

R.T.: 10.670 min
Delta R.T.: 0.000 min
Response: 1475563
Conc: 1.28 ng/ml

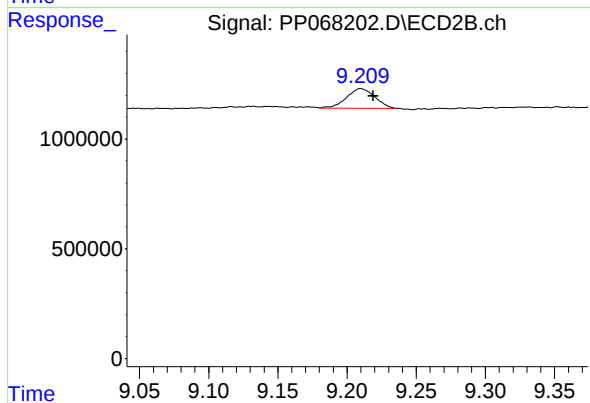

#2 Decachlorobiphenyl

R.T.: 9.209 min
Delta R.T.: -0.010 min
Response: 1264465
Conc: 1.13 ng/ml m