

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102424\
 Data File : PP068213.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 17:23
 Operator : YP\AJ
 Sample : P4510-13 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HID111K-2-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/25/2024
 Supervised By :Ankita Jodhani 10/25/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:47:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 09 05:48:32 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.755	4.050	1504071	1488552	1.625	1.473
2) SA Decachlor...	10.668	9.213	1934498	1666983	1.680m	1.486

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102424\
Data File : PP068213.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 17:23
Operator : YP\AJ
Sample : P4510-13 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HID111K-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:47:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP100824.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 09 05:48:32 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

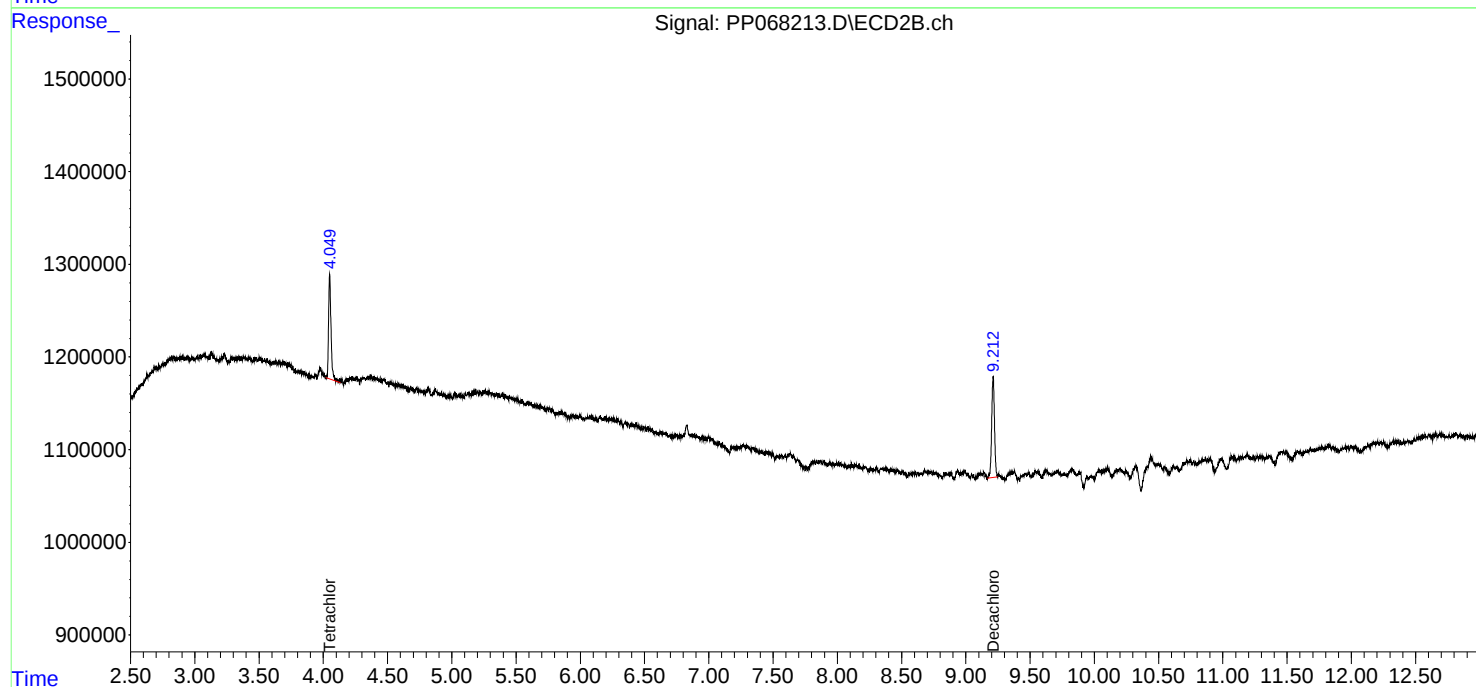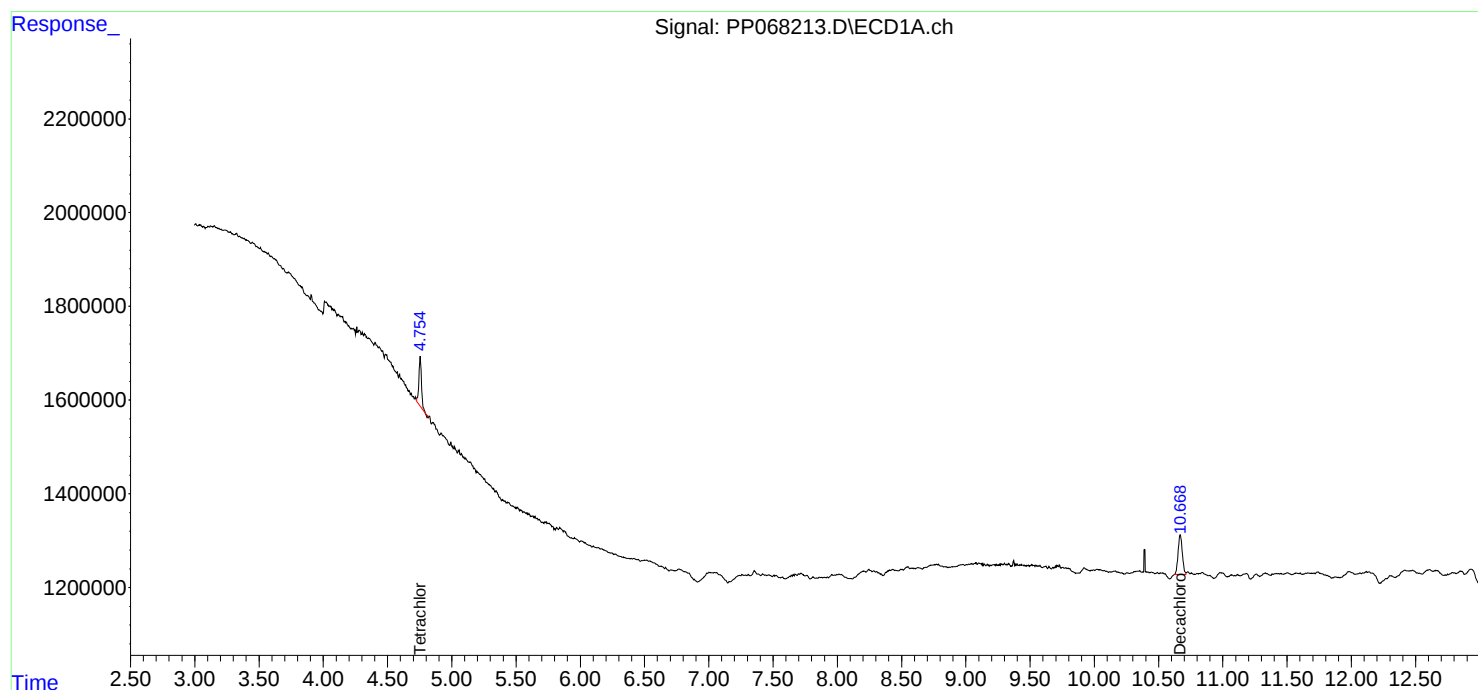

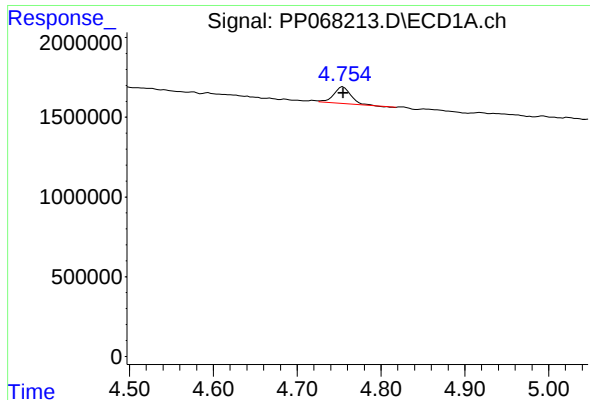


#1 Tetrachloro-m-xylene

R.T.: 4.755 min
Delta R.T.: 0.000 min
Response: 1504071
Conc: 1.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
HID111K-2-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/25/2024
Supervised By :Ankita Jodhani 10/25/2024

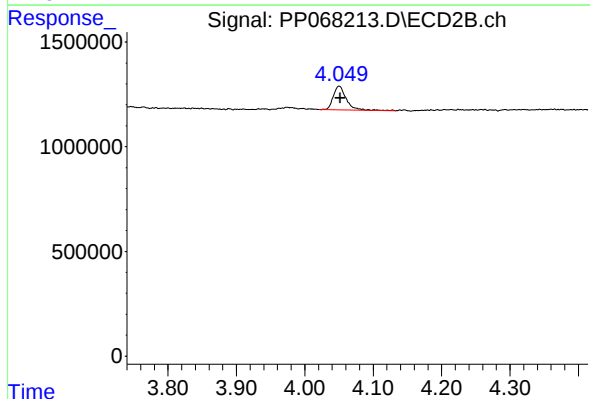


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.002 min
Response: 1488552
Conc: 1.47 ng/ml

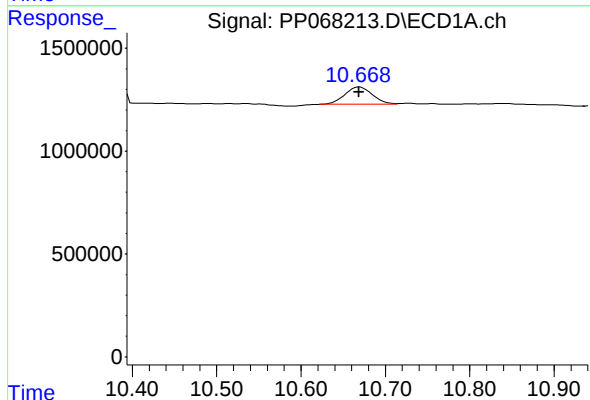

#2 Decachlorobiphenyl

R.T.: 10.668 min
Delta R.T.: -0.001 min
Response: 1934498
Conc: 1.68 ng/ml m

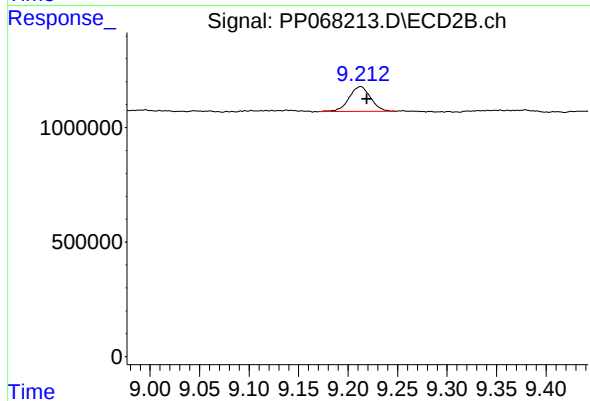

#2 Decachlorobiphenyl

R.T.: 9.213 min
Delta R.T.: -0.006 min
Response: 1666983
Conc: 1.49 ng/ml