

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102425\
 Data File : PP076052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2025 22:13
 Operator : YP\AJ
 Sample : Q3427-01 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/27/2025
 Supervised By :mohammad ahmed 10/28/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 23:41:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.642	3.778	3098463	4930795	2.168	0.745m#
2) SA Decachlor...	10.411	8.779	2374056	11814735	2.205m	1.437m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102425\
Data File : PP076052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2025 22:13
Operator : YP\AJ
Sample : Q3427-01 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2025
Supervised By :mohammad ahmed 10/28/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 23:41:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

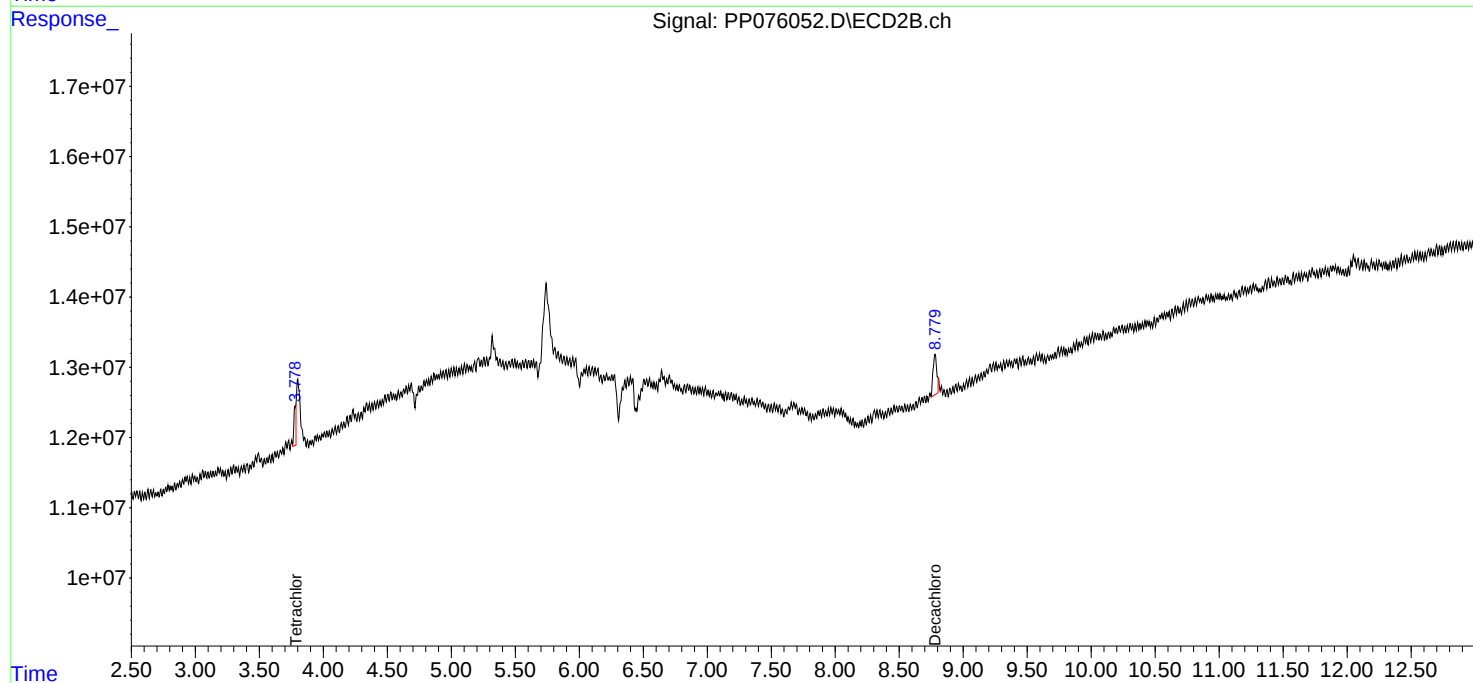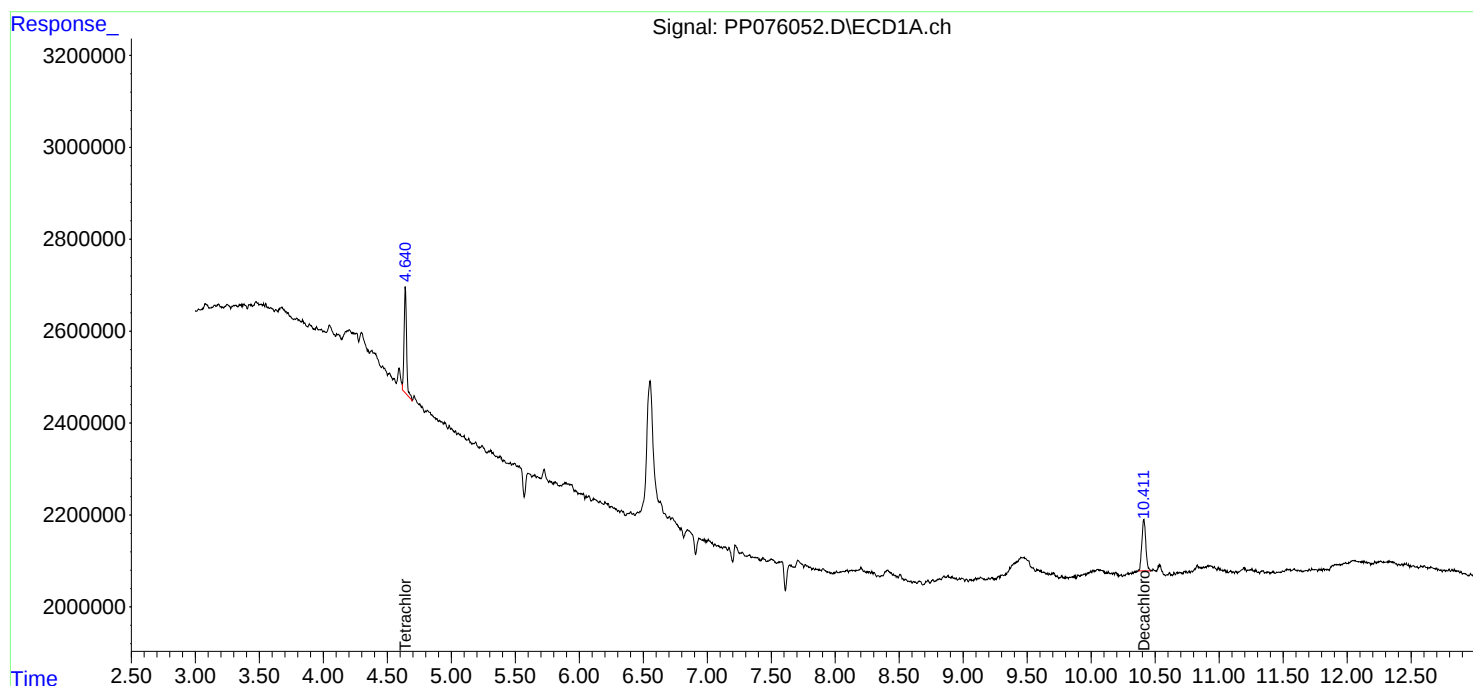

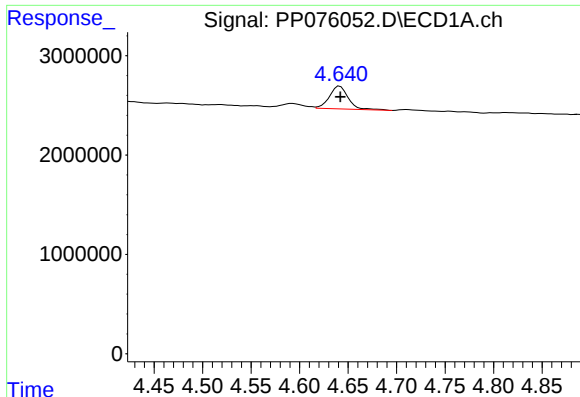


#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 3098463
Conc: 2.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/27/2025
Supervised By :mohammad ahmed 10/28/2025

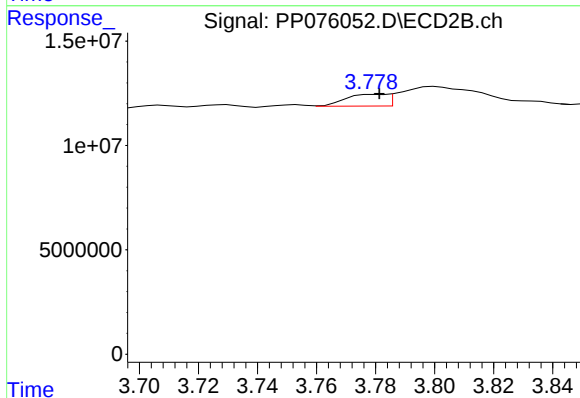


#1 Tetrachloro-m-xylene

R.T.: 3.778 min
Delta R.T.: -0.004 min
Response: 4930795
Conc: 0.75 ng/ml m

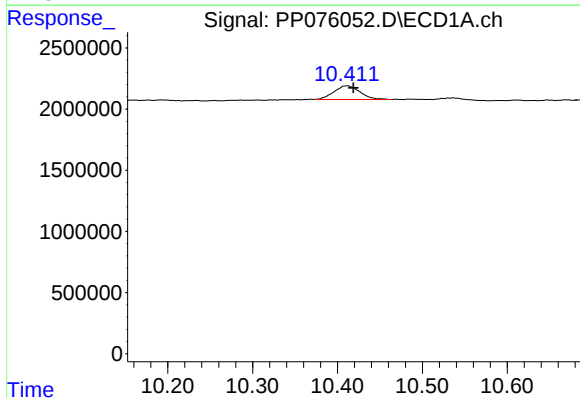

#2 Decachlorobiphenyl

R.T.: 10.411 min
Delta R.T.: -0.008 min
Response: 2374056
Conc: 2.21 ng/ml m

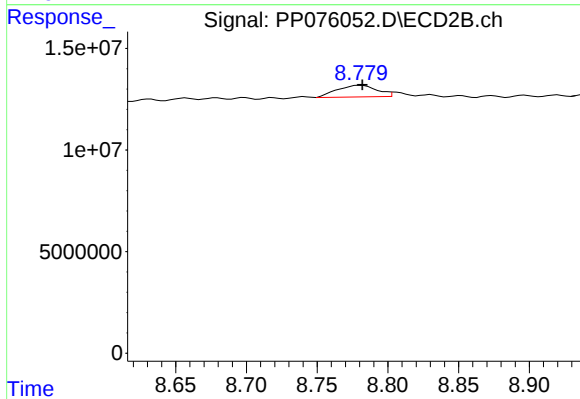

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: -0.003 min
Response: 11814735
Conc: 1.44 ng/ml m