

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102618\
 Data File : PS002162.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2018 09:26
 Operator : EI\SJ
 Sample : J5683-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 29 09:07:56 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
 Quant Title : 8080.M
 QLast Update : Sat Oct 27 01:34:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.468	10.931	109.1E6	109.1E6	346.676	303.858
Target Compounds							
1) T	Dalapon	2.938	2.362	28010671	51385780	61.070	113.809 #
2) T	3,5-DICHL...	0.000	9.092	0	3796325	N.D.	8.559 #
3) T	4-Nitroph...	0.000	10.088	0	8309389	N.D.	46.601 #
6) T	MCP	0.000	11.435	0	675739	N.D.	0.785 #
7) T	MCPA	0.000	11.829	0	2158998	N.D.	1.595 #
8) T	DICHLORPROP	0.000	12.285	0	729291	N.D.	2.271 #
9) T	2,4-D	0.000	12.798	0	902937	N.D.	2.120 #
10) T	Pentachlo...	0.000	13.280	0	5518242	N.D.	1.175 #
11) T	2,4,5-TP ...	0.000	14.001	0	647470	N.D.	0.354 #
12) T	2,4,5-T	0.000	14.587	0	640053	N.D.	0.427 #
13) T	2,4-DB	0.000	15.133	0	186370	N.D.	0.841 #
15) T	Picloram	0.000	16.795	0	1172910	N.D.	0.518 #
16) T	DCPA	0.000	16.806	0	647176	N.D.	0.273 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS102618\
Data File : PS002162.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2018 09:26
Operator : EI\SJ
Sample : J5683-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 29 09:07:56 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102618.M
Quant Title : 8080.M
QLast Update : Sat Oct 27 01:34:10 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

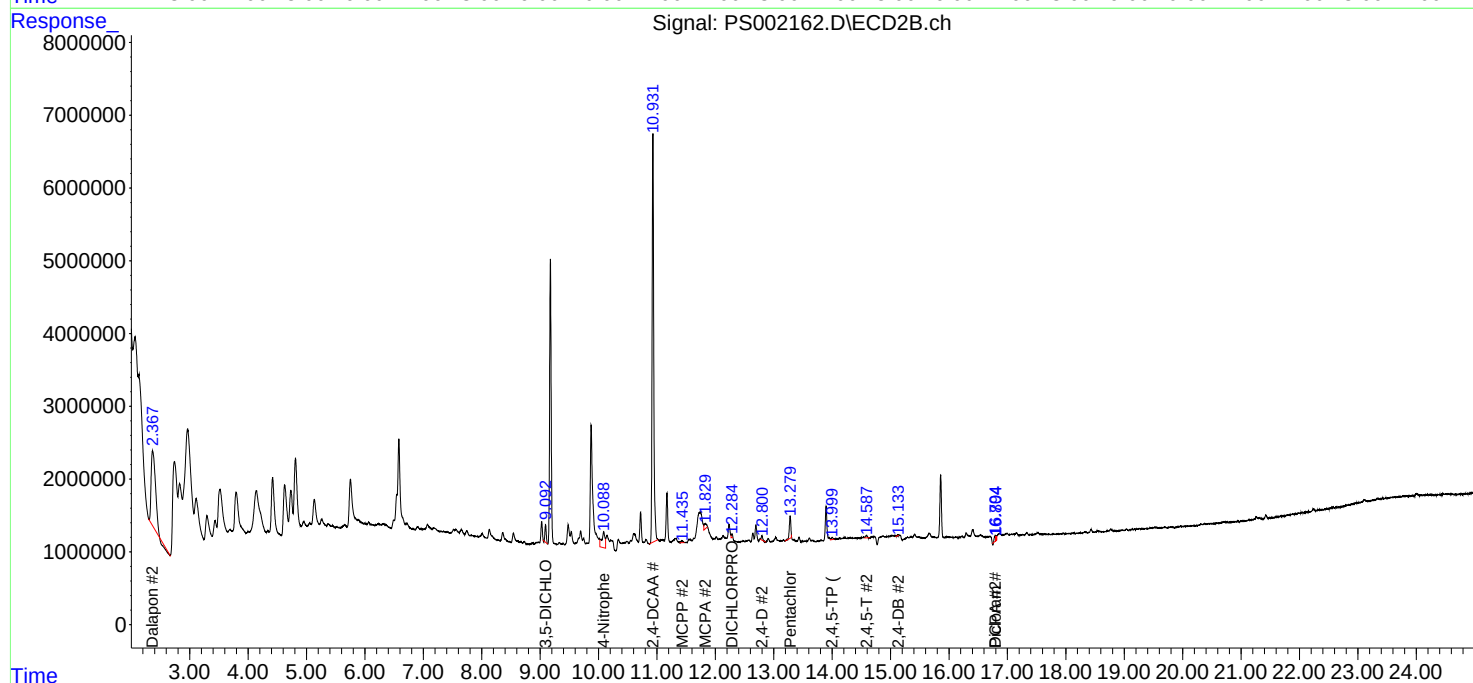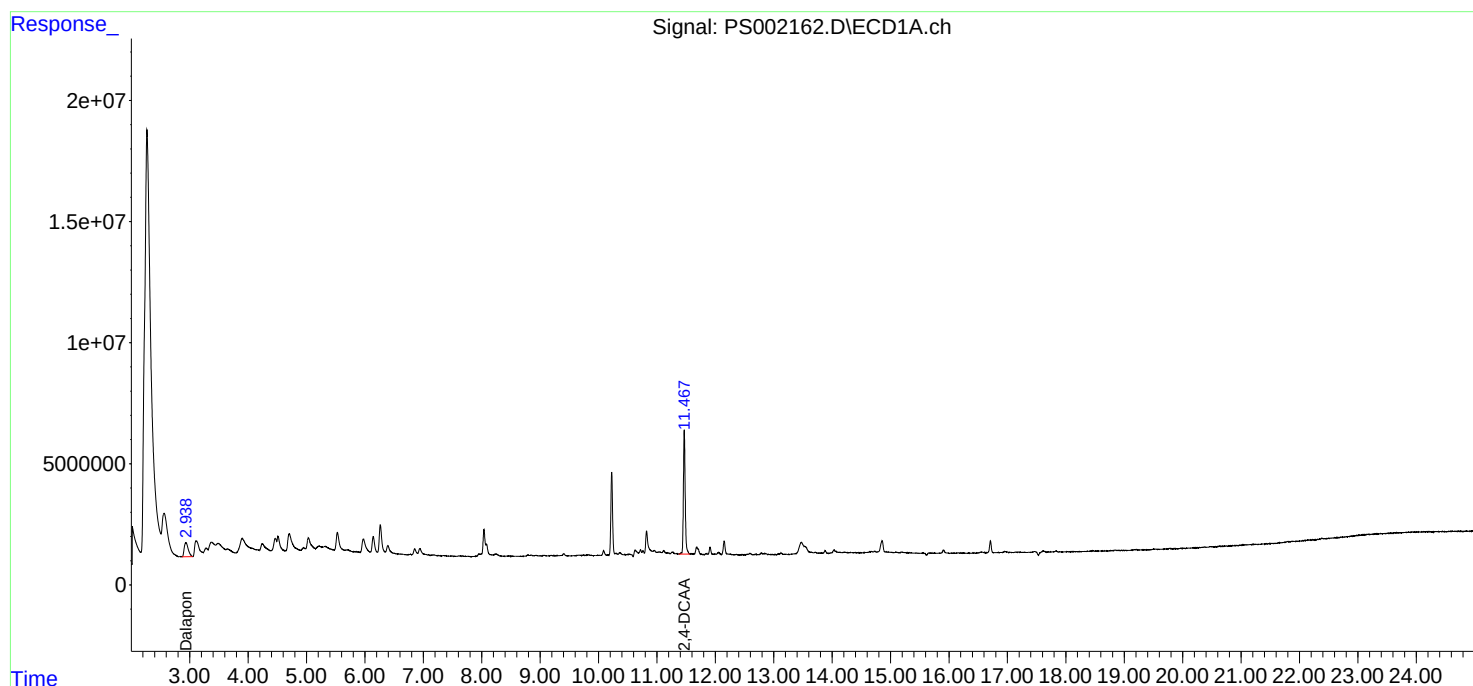


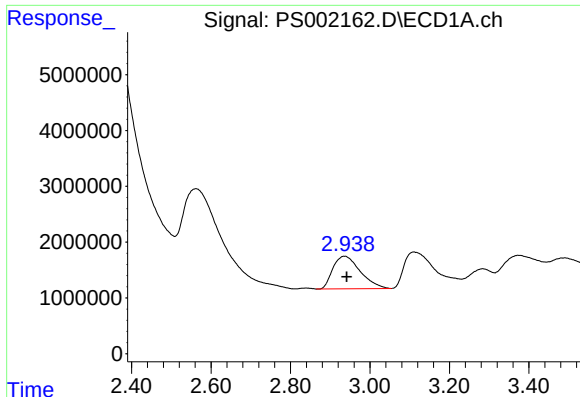

#1 Dalapon


R.T.: 2.938 min
Delta R.T.: -0.004 min
Response: 28010671
Conc: 61.07 ng/ml

Instrument :
ECD_P
ClientSampleId :

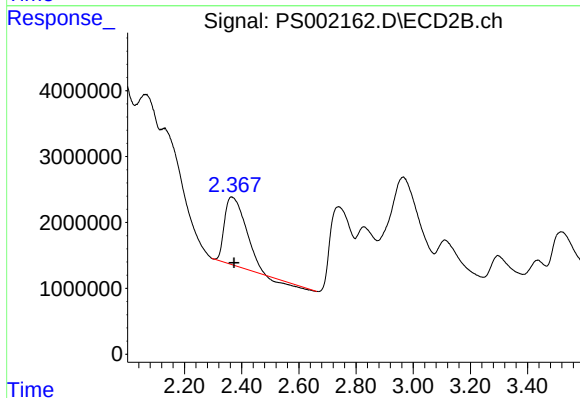


#1 Dalapon

R.T.: 2.362 min
Delta R.T.: -0.011 min
Response: 51385780
Conc: 113.81 ng/ml

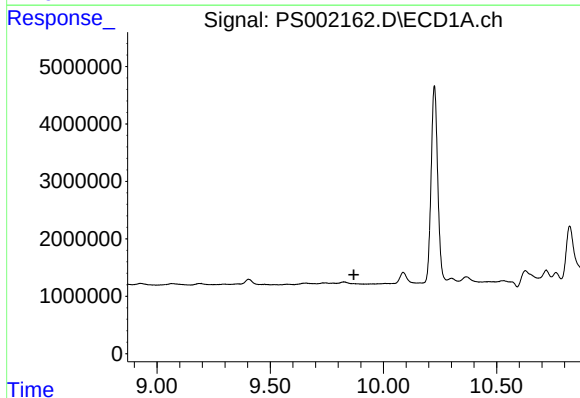


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.870 min
Response: 0
Conc: N.D.

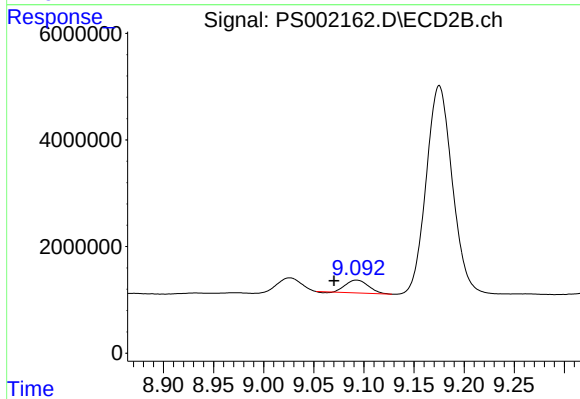

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.092 min
Delta R.T.: 0.022 min
Response: 3796325
Conc: 8.56 ng/ml

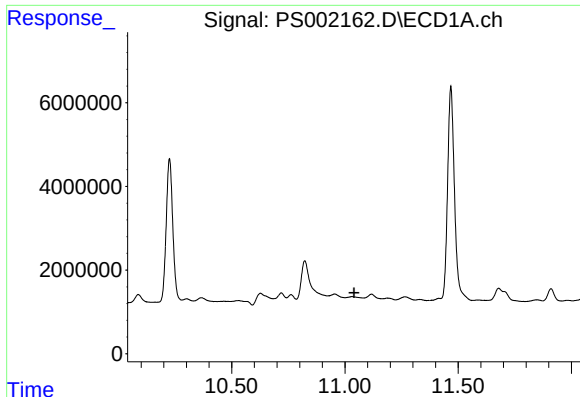

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.040 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

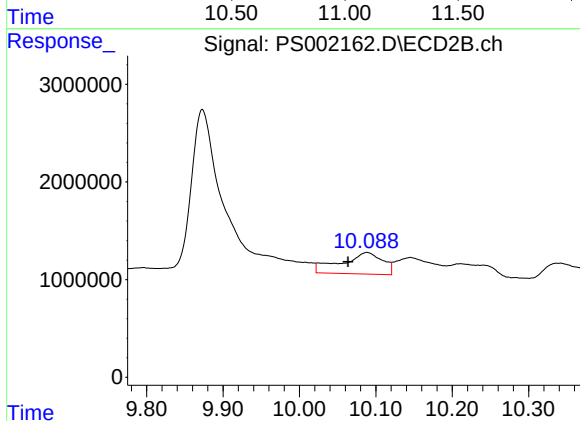


#3 4-Nitrophenol

R.T.: 10.088 min
Delta R.T.: 0.025 min
Response: 8309389
Conc: 46.60 ng/ml

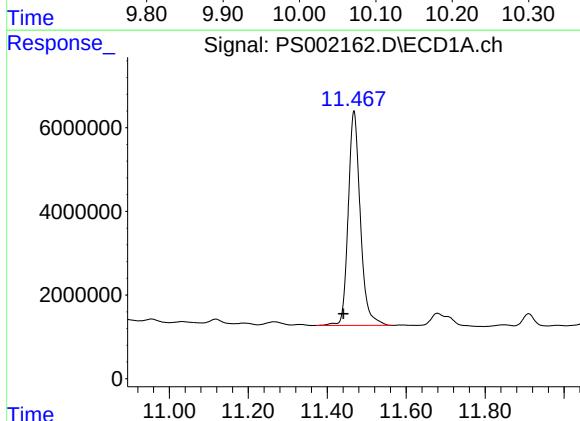


#4 2,4-DCAA

R.T.: 11.468 min
Delta R.T.: 0.027 min
Response: 109094109
Conc: 346.68 ng/ml

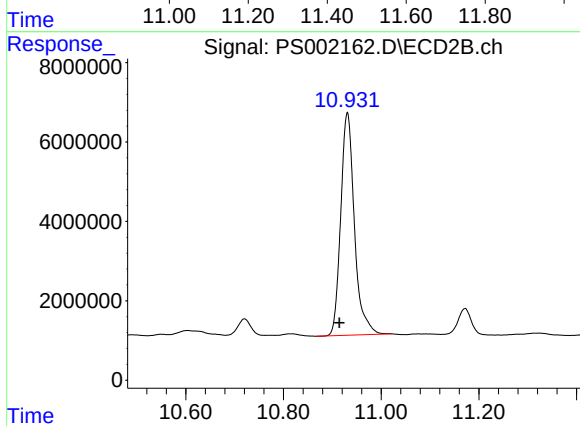

#4 2,4-DCAA


R.T.: 10.931 min
Delta R.T.: 0.017 min
Response: 109114906
Conc: 303.86 ng/ml

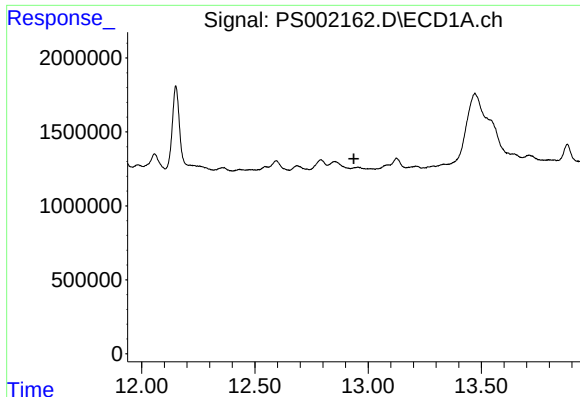

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

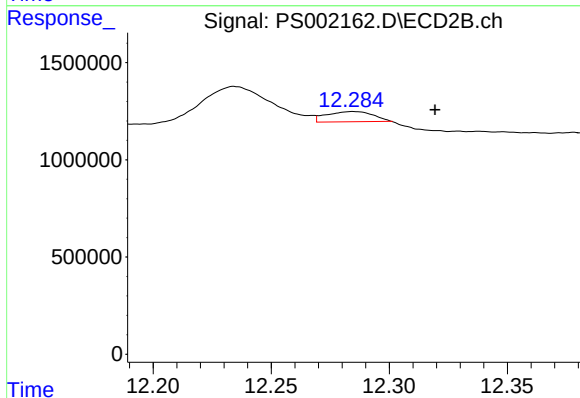


#8 DICHLORPROP

R.T.: 12.285 min
Delta R.T.: -0.035 min
Response: 729291
Conc: 2.27 ng/ml

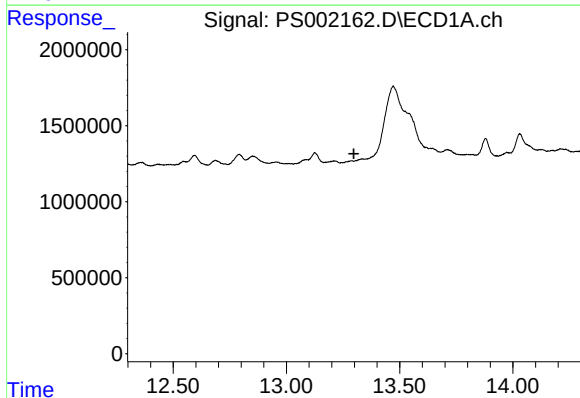


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

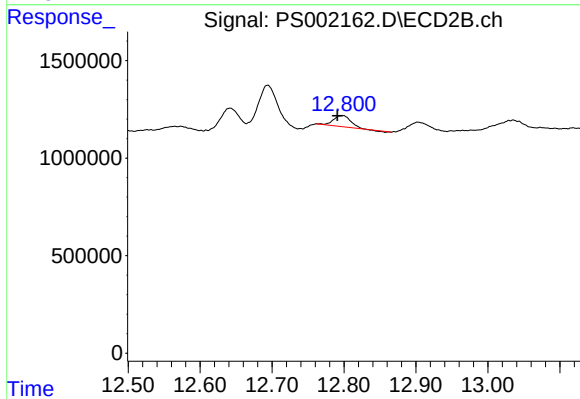

#9 2,4-D


R.T.: 12.798 min
Delta R.T.: 0.007 min
Response: 902937
Conc: 2.12 ng/ml

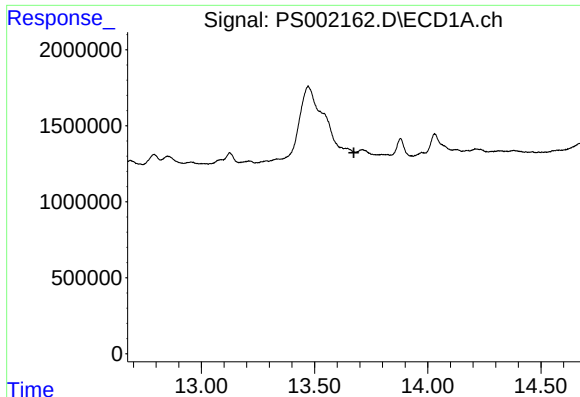

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

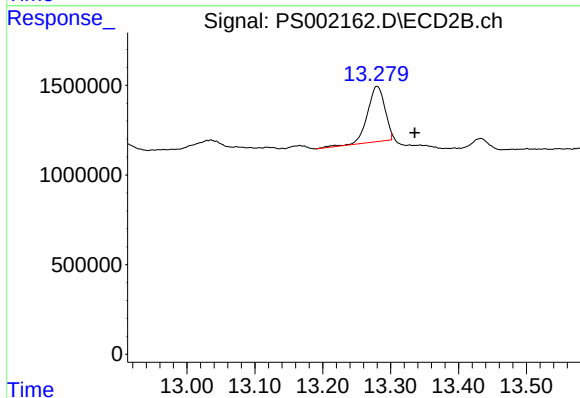


#10 Pentachlorophenol

R.T.: 13.280 min
Delta R.T.: -0.056 min
Response: 5518242
Conc: 1.17 ng/ml

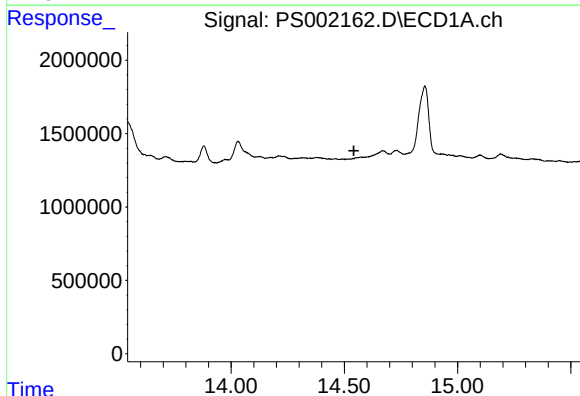


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.542 min
Response: 0
Conc: N.D.

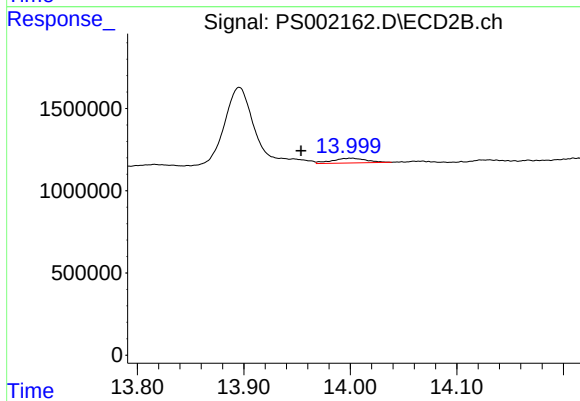

#11 2,4,5-TP (SILVEX)


R.T.: 14.001 min
Delta R.T.: 0.047 min
Response: 647470
Conc: 0.35 ng/ml

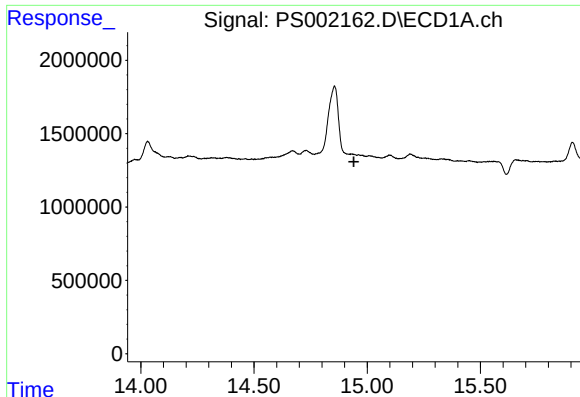

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.941 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

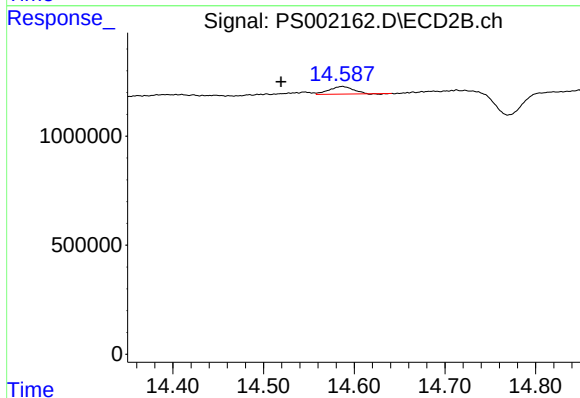


#12 2,4,5-T

R.T.: 14.587 min
Delta R.T.: 0.068 min
Response: 640053
Conc: 0.43 ng/ml

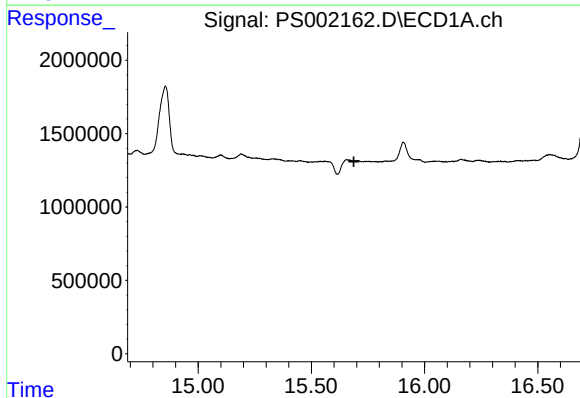


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.688 min
Response: 0
Conc: N.D.

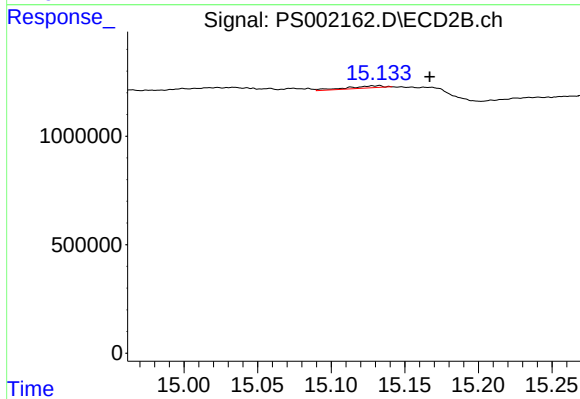

#13 2,4-DB


R.T.: 15.133 min
Delta R.T.: -0.034 min
Response: 186370
Conc: 0.84 ng/ml

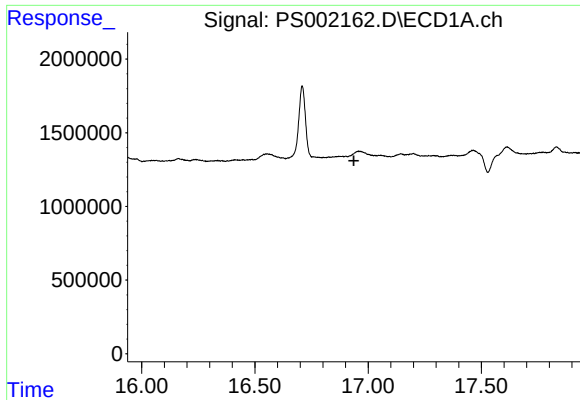

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.937 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

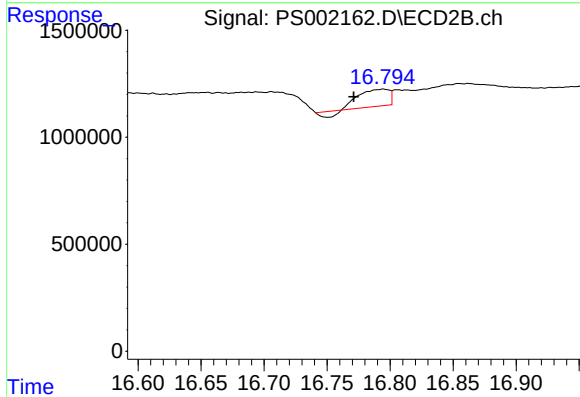


#15 Picloram

R.T.: 16.795 min
Delta R.T.: 0.023 min
Response: 1172910
Conc: 0.52 ng/ml

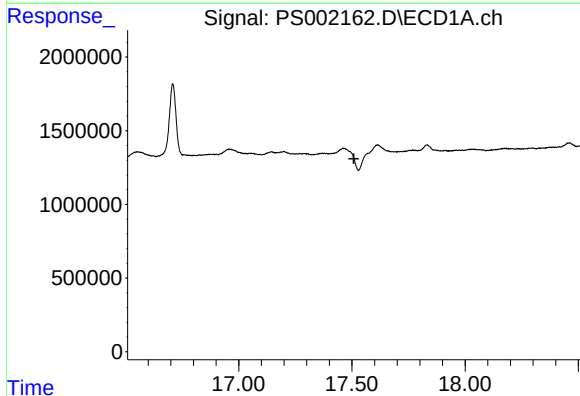

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.509 min
Response: 0
Conc: N.D.

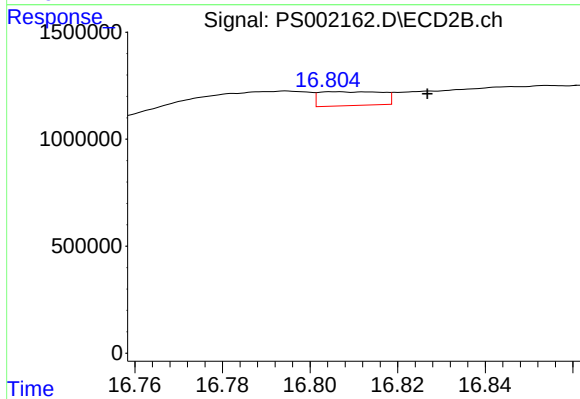

#16 DCPA

R.T.: 16.806 min
Delta R.T.: -0.021 min
Response: 647176
Conc: 0.27 ng/ml