

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102620\
Data File : PP030846.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2020 9:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:45:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 26 04:46:19 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.804	4.081	1346083	1239100	20.080	19.928
2) SA Decachlor...	10.690	9.418	796311	805218	21.681	20.352

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP102620\
Data File : PP030846.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 26 Oct 2020 9:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:45:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\AR1232PP102520.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Oct 26 04:46:19 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

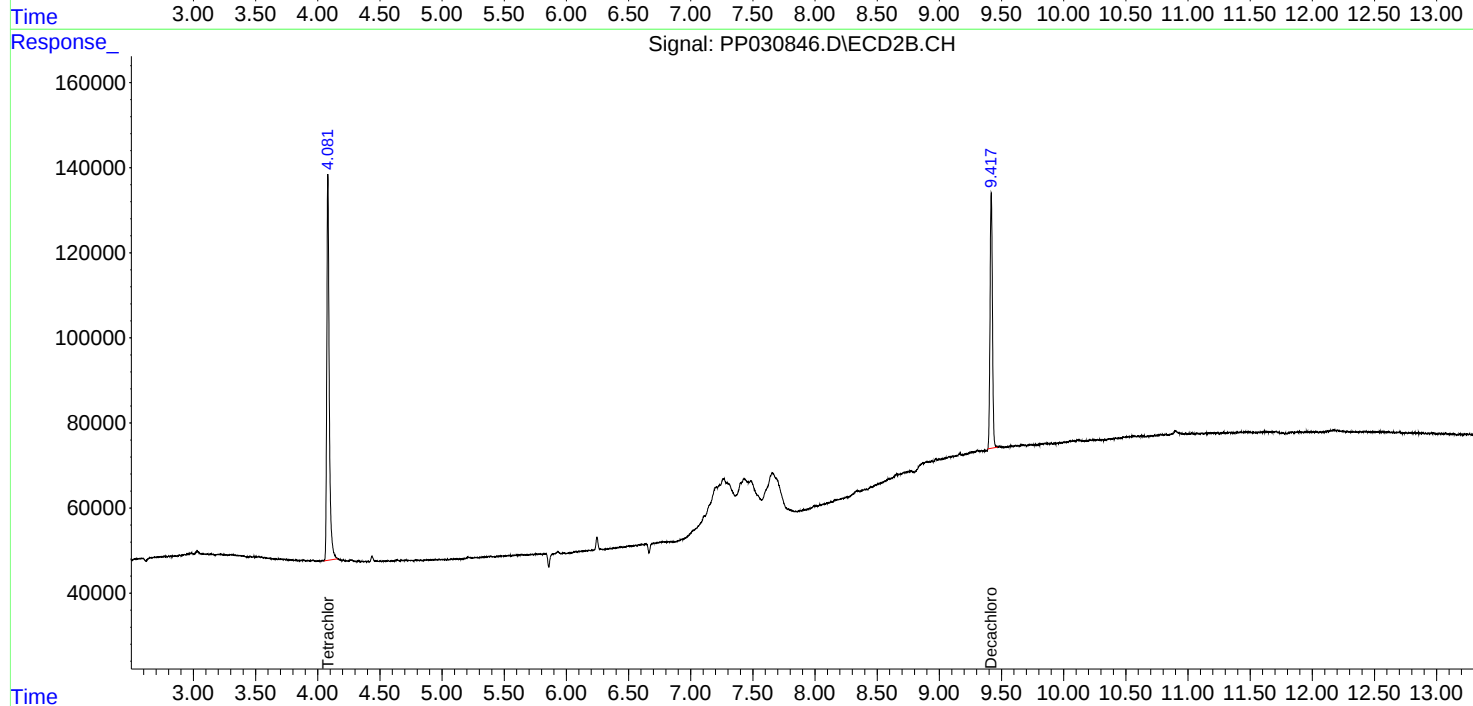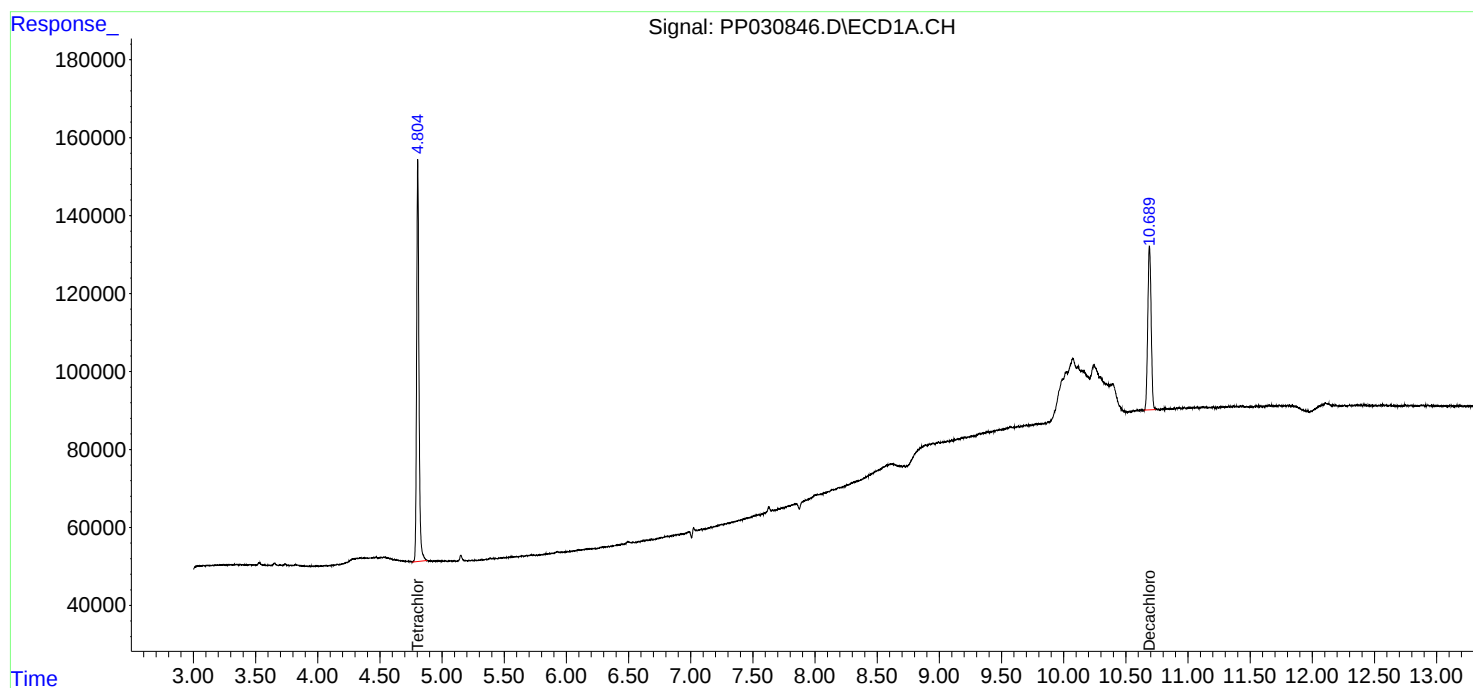


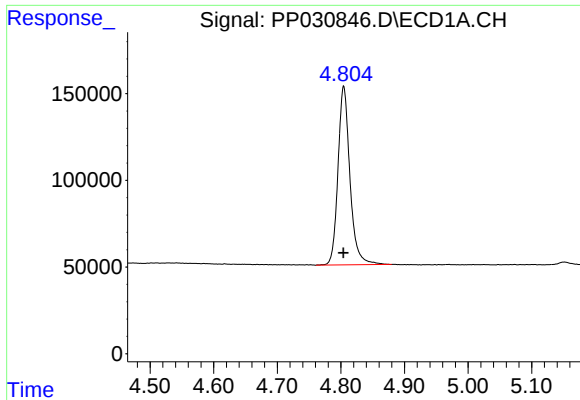

#1 Tetrachloro-m-xylene


R.T.: 4.804 min
Delta R.T.: 0.000 min
Response: 1346083
Conc: 20.08 ng/ml

Instrument :
ECD_P
ClientSampleId :

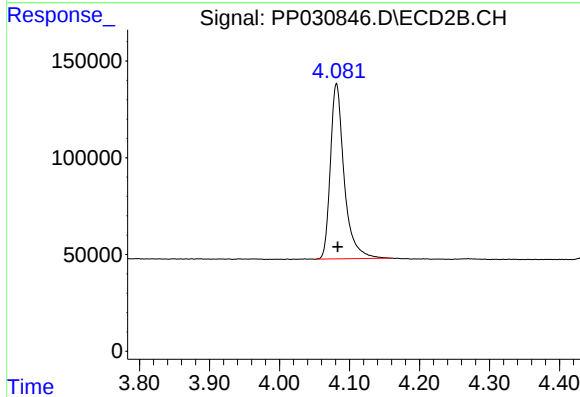


#1 Tetrachloro-m-xylene

R.T.: 4.081 min
Delta R.T.: -0.002 min
Response: 1239100
Conc: 19.93 ng/ml

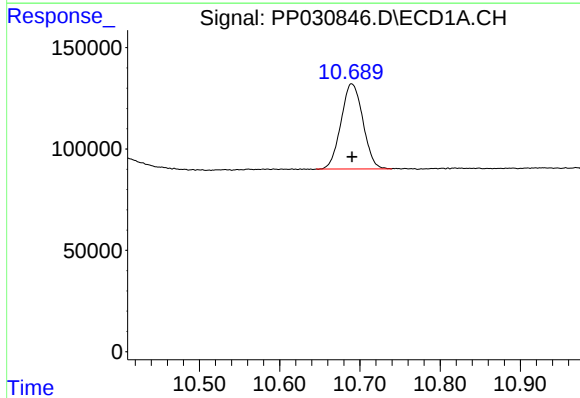

#2 Decachlorobiphenyl

R.T.: 10.690 min
Delta R.T.: 0.000 min
Response: 796311
Conc: 21.68 ng/ml

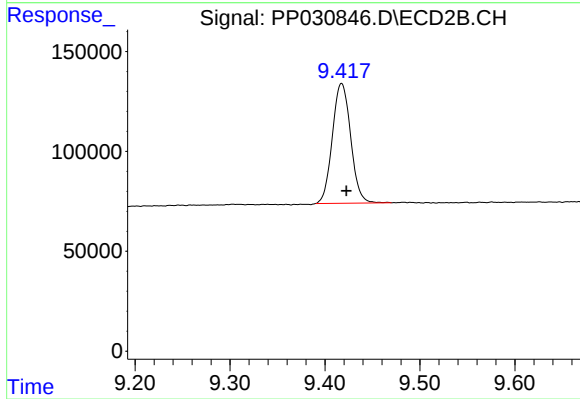

#2 Decachlorobiphenyl

R.T.: 9.418 min
Delta R.T.: -0.005 min
Response: 805218
Conc: 20.35 ng/ml